
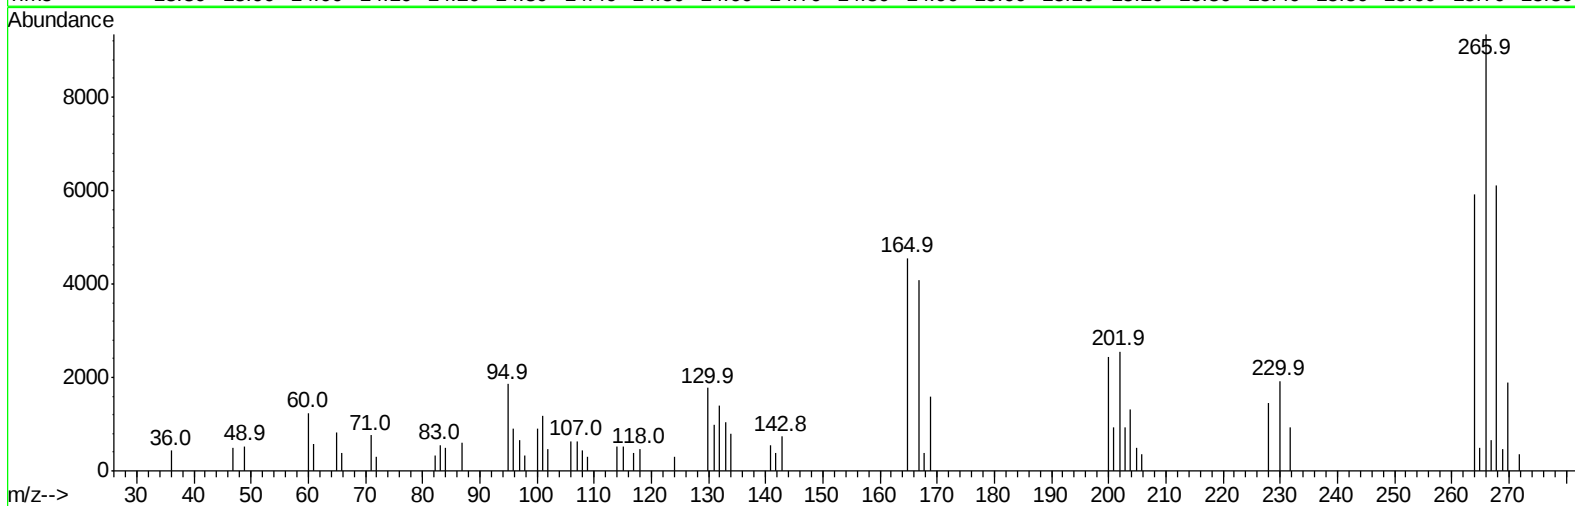


Data Path : Z:\HPCHEM1\BNA F\Data\BF052717\
Data File : BF095502.D
Acq On : 27 May 2017 17:31
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 00:48:43 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 26 16:50:16 2017
Response via : Initial Calibration

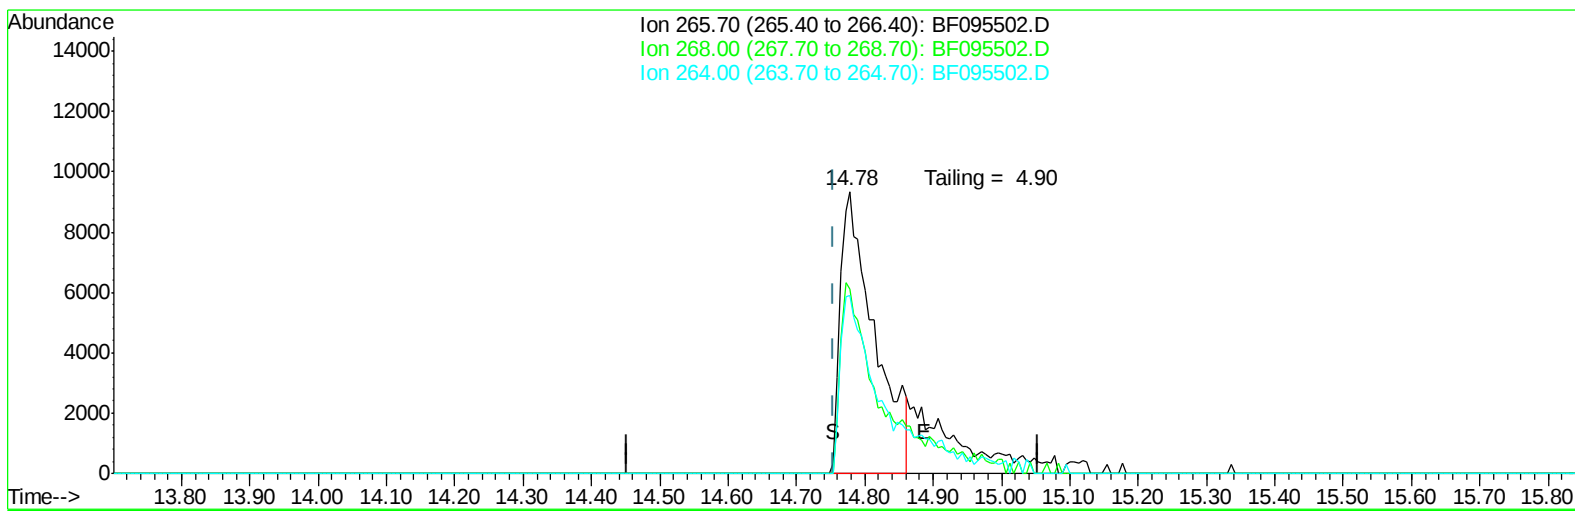

TIC: BF095502.D

(69) Pentachlorophenol (C)



14.777min (+0.024) 0.00ng

response 29122

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.31
264.00	64.60	63.26
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF052717\
Data File : BF095502.D
Acq On : 27 May 2017 17:31
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 00:48:43 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 26 16:50:16 2017
Response via : Initial Calibration

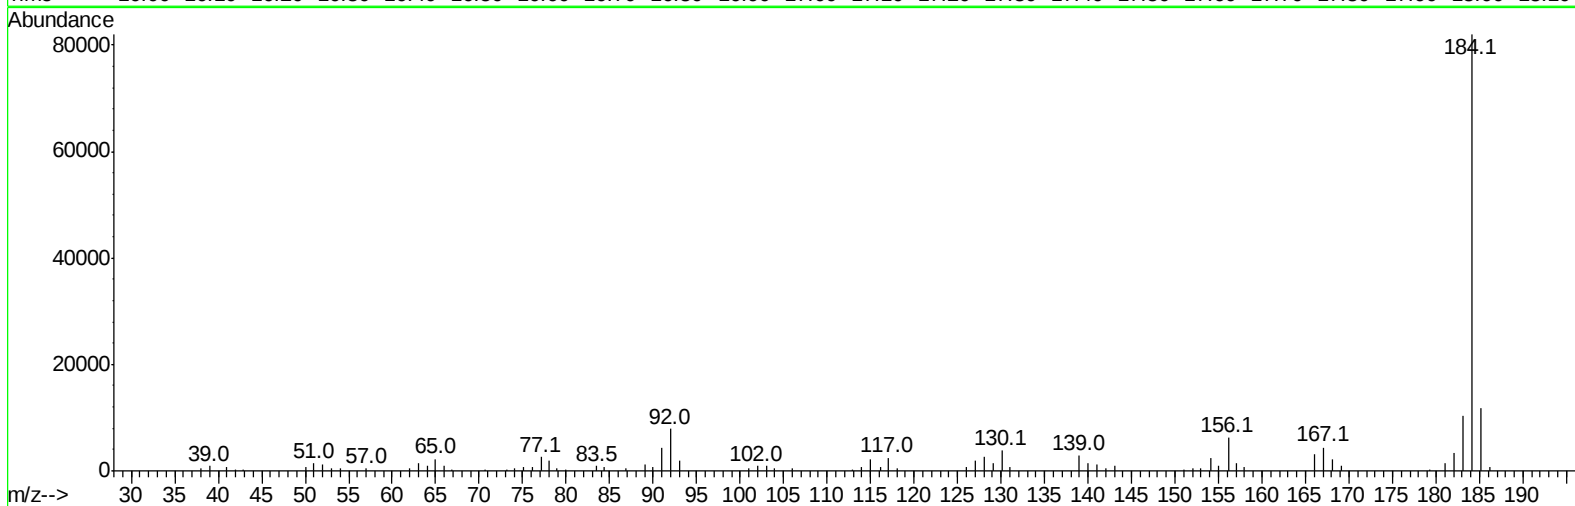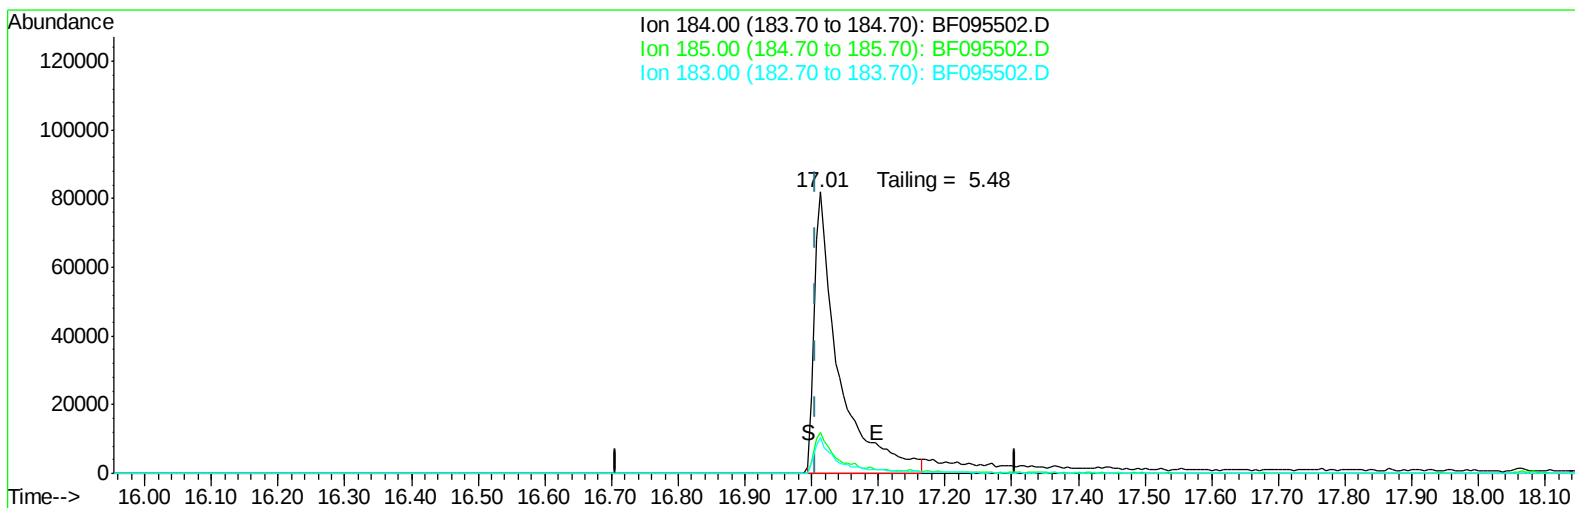

TIC: BF095502.D

(76) Benzidine

17.012min (+0.006) 0.00ng

response 202744

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.52#
183.00	12.20	12.66
0.00	0.00	0.00