

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052717\
 Data File : BF095506.D
 Acq On : 27 May 2017 20:11
 Operator : SJ/MA
 Sample : I3306-09
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DSK-MW-LW

Quant Time: May 29 02:37:30 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 26 16:50:16 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	77429	20.00	ng	0.00
21) Naphthalene-d8	9.77	136	359330	20.00	ng	0.01
38) Acenaphthene-d10	12.60	164	168956	20.00	ng	0.00
63) Phenanthrene-d10	15.00	188	300541	20.00	ng	0.00
75) Chrysene-d12	18.68	240	246393	20.00	ng	0.00
86) Perylene-d12	20.36	264	159591	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.72	112	353038	76.02	ng	0.01
7) Phenol-d6	7.31	99	265325	47.61	ng	0.02
23) Nitrobenzene-d5	8.64	82	521050	91.44	ng	-0.01
41) 2,4,6-Tribromophenol	13.89	330	195490	141.28	ng	-0.01
44) 2-Fluorobiphenyl	11.53	172	1108369	94.42	ng	0.00
78) Terphenyl-d14	17.32	244	831028	74.29	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052717\
Data File : BF095506.D
Acq On : 27 May 2017 20:11
Operator : SJ/MA
Sample : I3306-09
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSK-MW-LW

Quant Time: May 29 02:37:30 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 26 16:50:16 2017
Response via : Initial Calibration

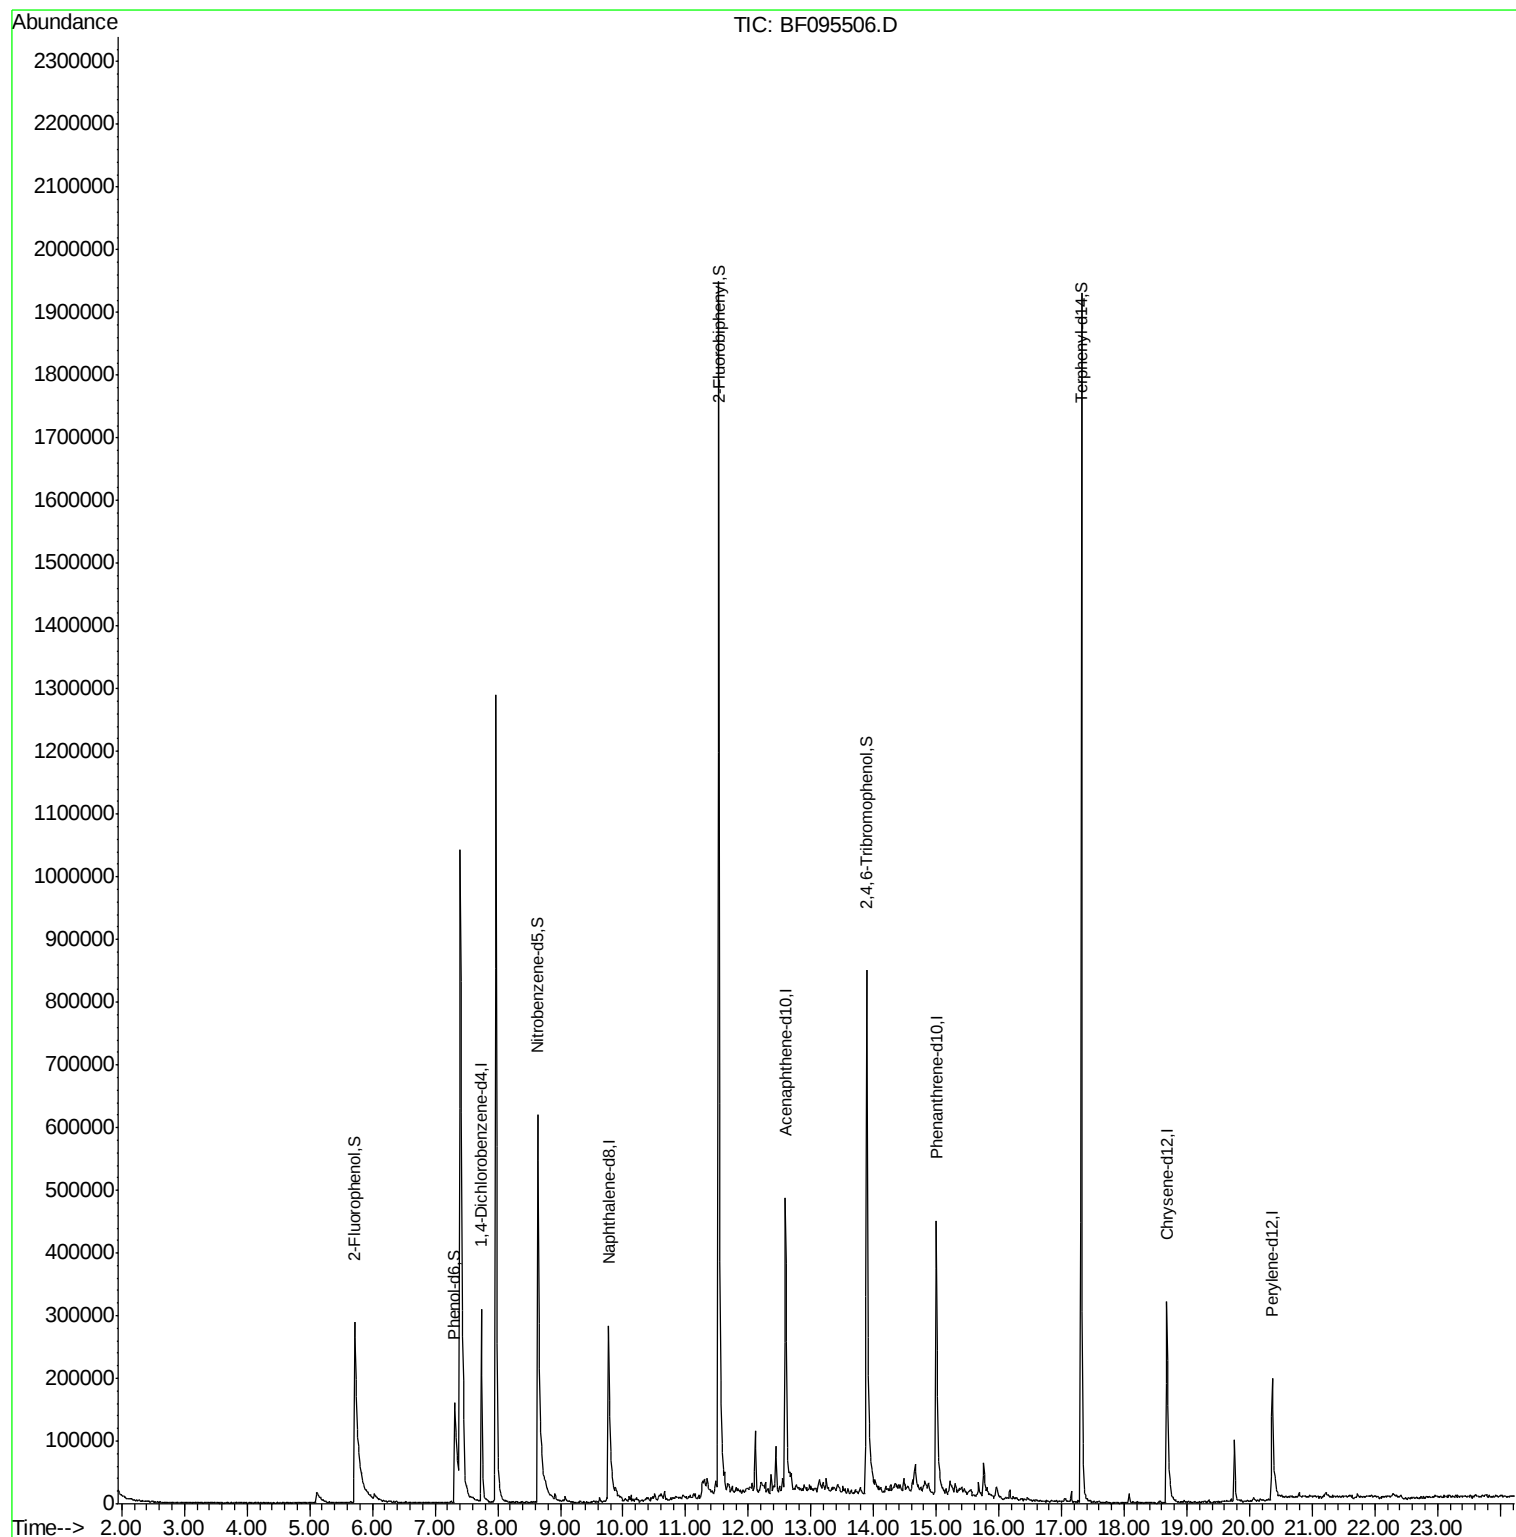

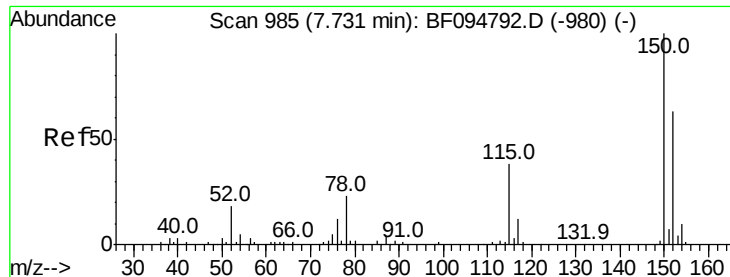


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.74 min Scan# 987
Delta R.T. 0.00 min
Lab File: BF095506.D
Acq: 27 May 2017 20:11

Instrument :
BNA_F
ClientSampleId :
DSK-MW-LW

Tot Ion:152 Resp: 77429
Ion Ratio Lower Upper
152 100
150 158.7 126.2 189.2
115 57.4 52.2 78.2

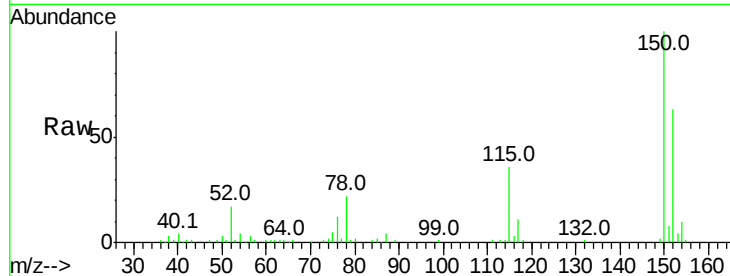


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

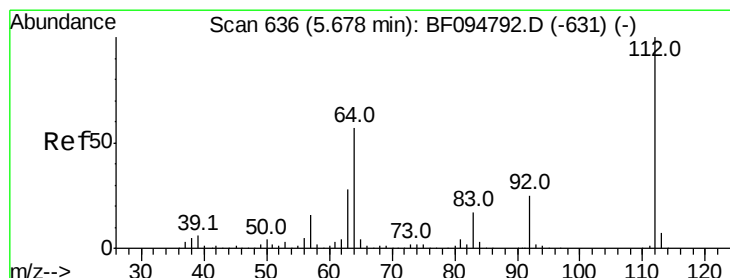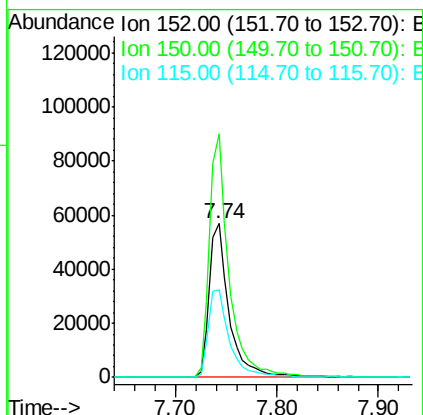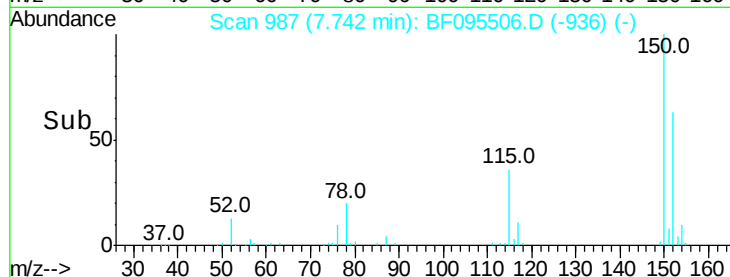



#5


2-Fluorophenol
Concen: 76.02 ng
RT: 5.72 min Scan# 643
Delta R.T. 0.01 min
Lab File: BF095506.D
Acq: 27 May 2017 20:11

Tgt Ion:112 Resp: 353038
Ion Ratio Lower Upper
112 100
64 56.3 46.0 69.0
63 26.3 23.4 35.0

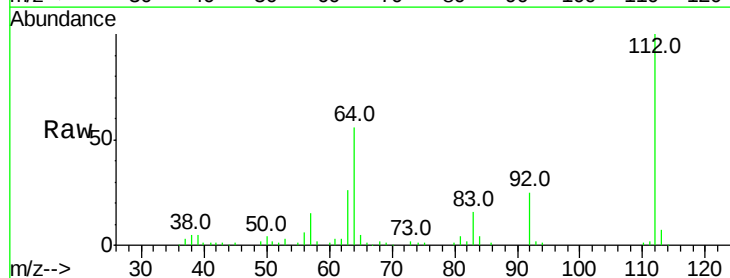

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

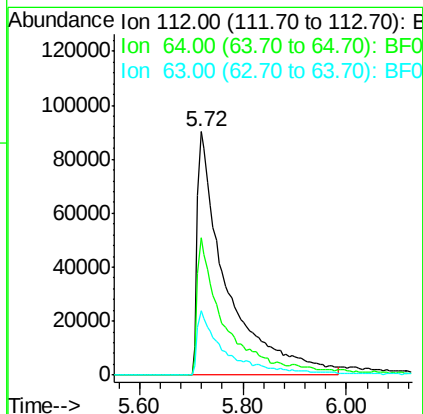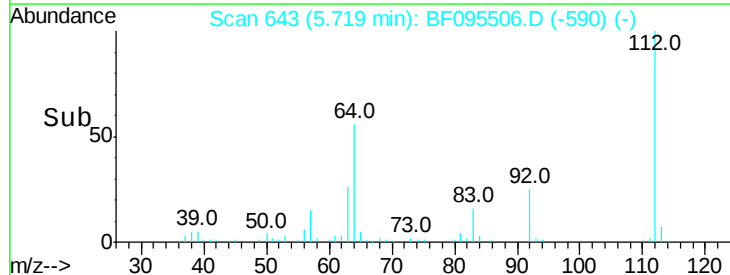

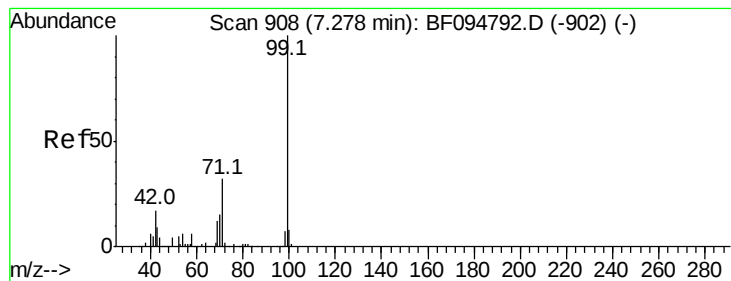

#7

Phenol-d6

Concen: 47.61 ng

RT: 7.31 min Scan# 914

Delta R.T. 0.02 min

Lab File: BF095506.D

Acq: 27 May 2017 20:11

Instrument :

BNA_F

ClientSampleId :

DSK-MW-LW





Tot Ion: 99 Resp: 265325

Ion Ratio Lower Upper

99 100

42 16.1 13.5 20.3

71 31.3 24.5 36.7

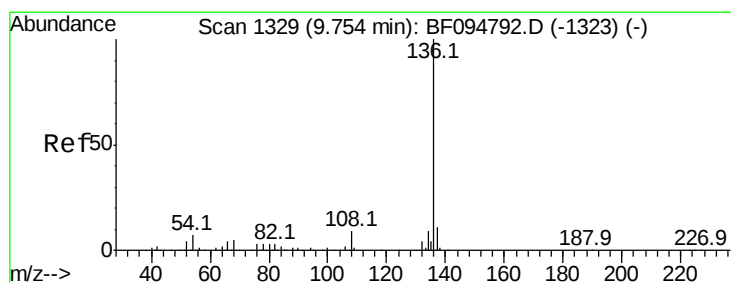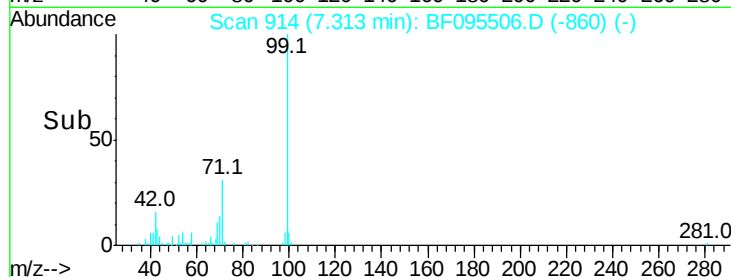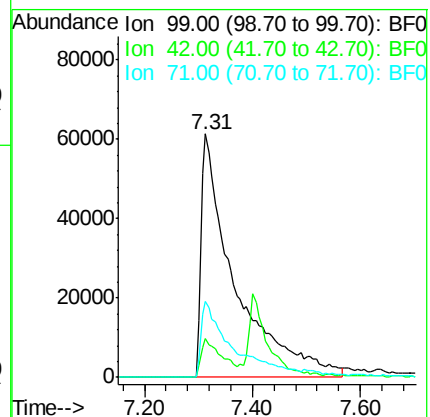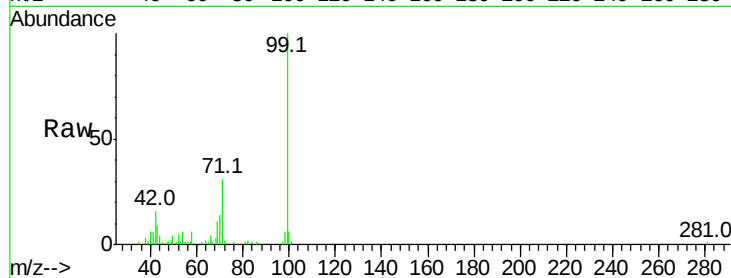

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.77 min Scan# 1332

Delta R.T. 0.01 min

Lab File: BF095506.D

Acq: 27 May 2017 20:11

Tgt Ion: 136 Resp: 359330




Ion Ratio Lower Upper


136 100

137 11.0 8.5 12.7

54 7.2 4.9 7.3

68 5.1 4.1 6.1

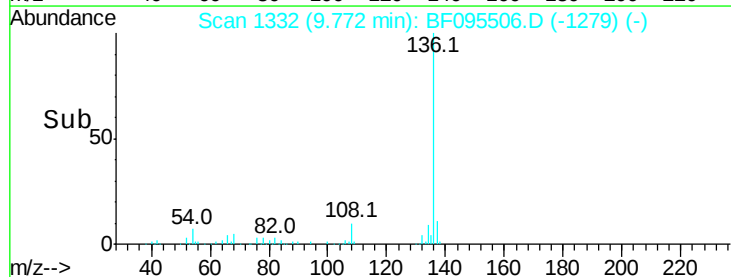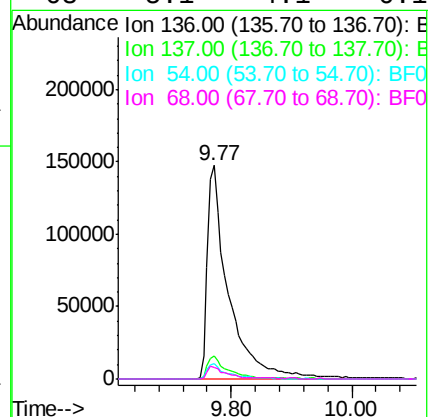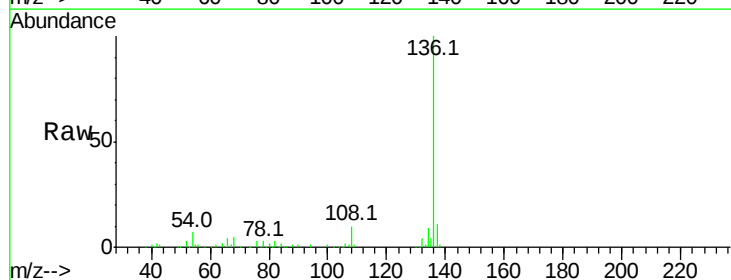

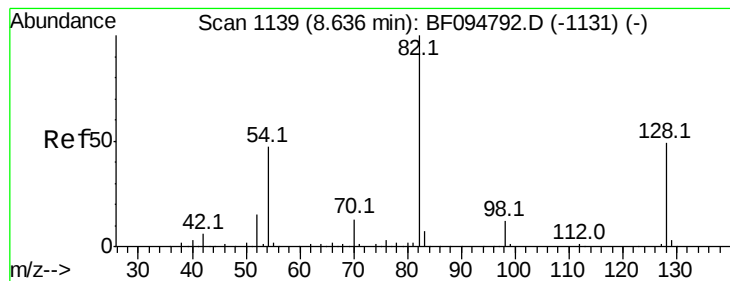

#23

Nitrobenzene-d5

Concen: 91.44 ng

RT: 8.64 min Scan# 1140

Delta R.T. -0.01 min

Lab File: BF095506.D

Acq: 27 May 2017 20:11

Instrument :

BNA_F

ClientSampleId :

DSK-MW-LW





Tot Ion: 82 Resp: 521050

Ion Ratio Lower Upper

82 100

128 46.9 34.0 51.0

54 46.1 42.2 63.2

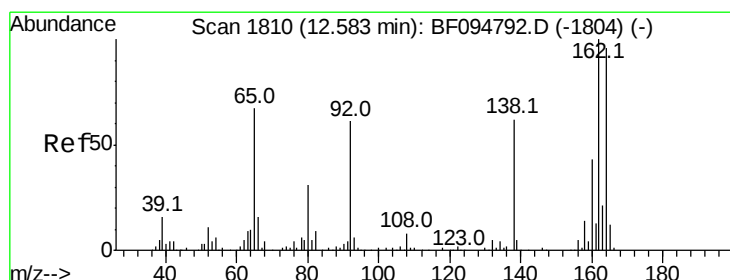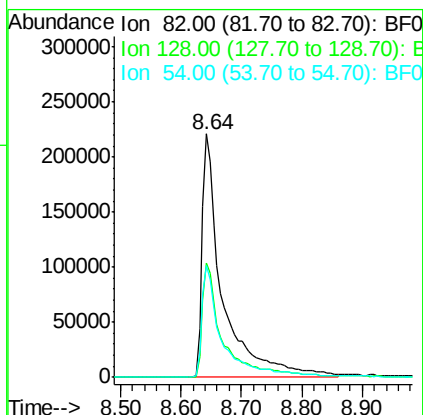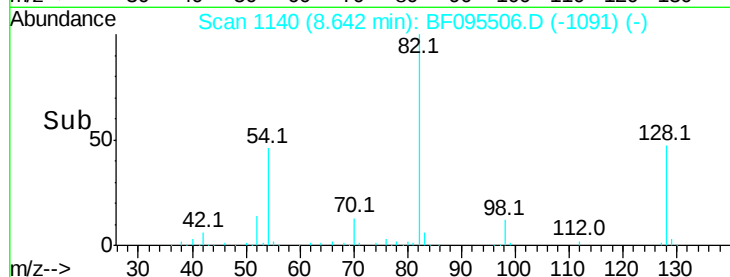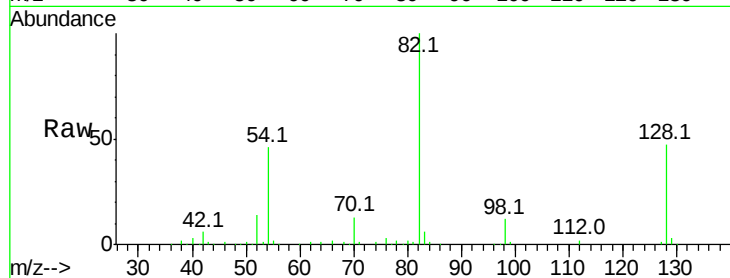

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 12.60 min Scan# 1812

Delta R.T. 0.00 min

Lab File: BF095506.D

Acq: 27 May 2017 20:11




Tgt Ion:164 Resp: 168956


Ion Ratio Lower Upper

164 100

162 107.1 82.6 123.8

160 44.8 36.2 54.2

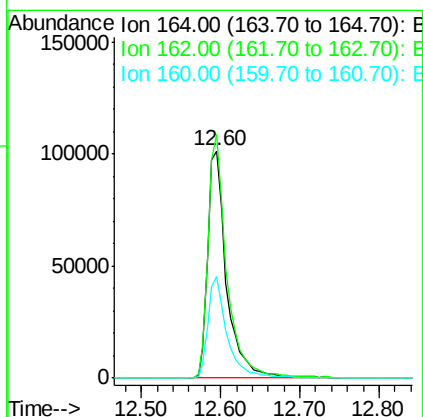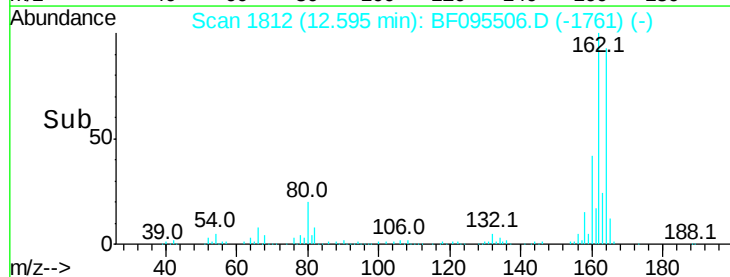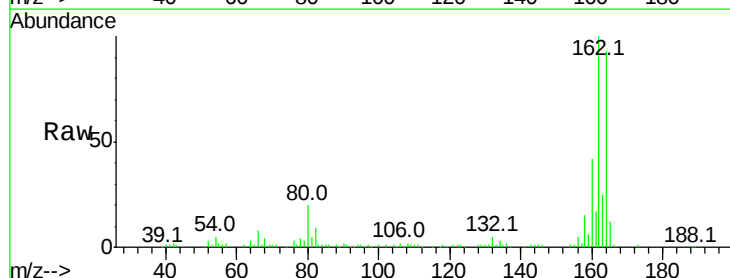


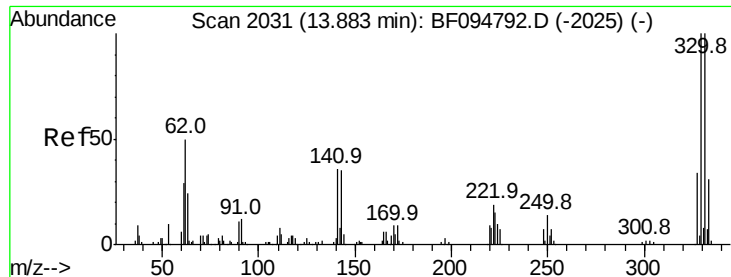




#41
 2,4,6-Tribromophenol
 Concen: 141.28 ng
 RT: 13.89 min Scan# 2032
 Delta R.T. -0.01 min
 Lab File: BF095506.D
 Acq: 27 May 2017 20:11

Instrument :
 BNA_F
 ClientSampleId :
 DSK-MW-LW

Tot Ion:330 Resp: 195490
 Ion Ratio Lower Upper
 330 100
 332 96.8 76.6 115.0
 141 39.8 31.4 47.2

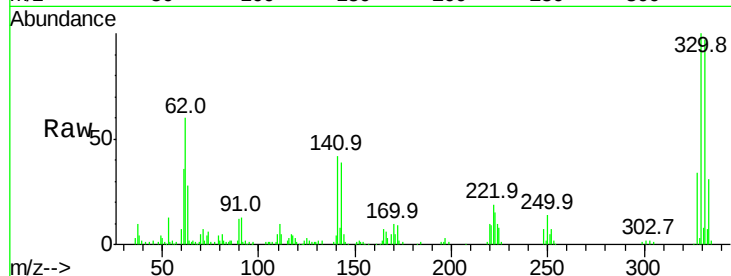


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

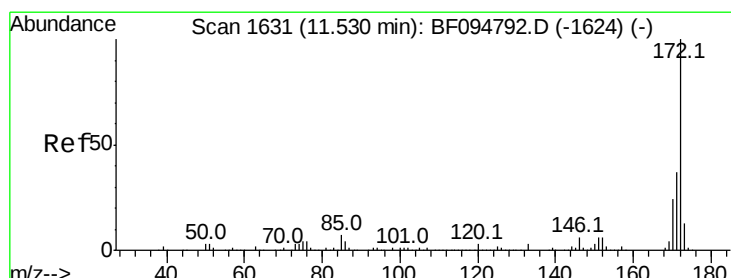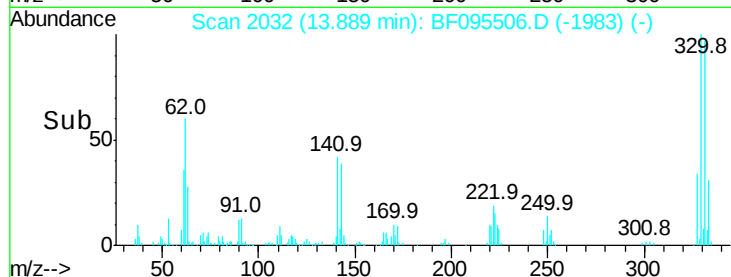
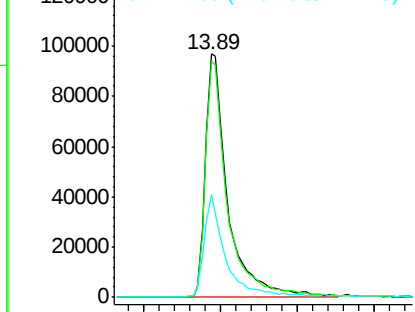



#44
 2-Fluorobiphenyl
 Concen: 94.42 ng
 RT: 11.53 min Scan# 1631
 Delta R.T. -0.01 min
 Lab File: BF095506.D
 Acq: 27 May 2017 20:11

Tgt Ion:172 Resp: 1108369
 Ion Ratio Lower Upper
 172 100
 171 35.2 29.6 44.4
 170 23.6 19.8 29.8

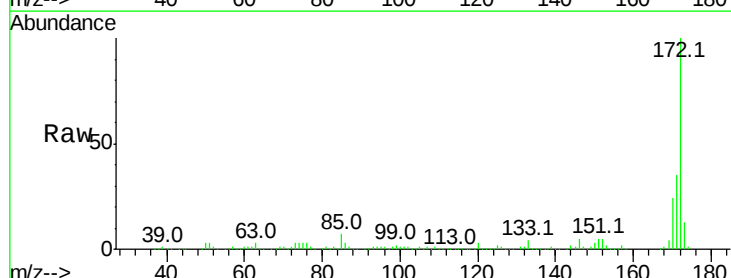

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

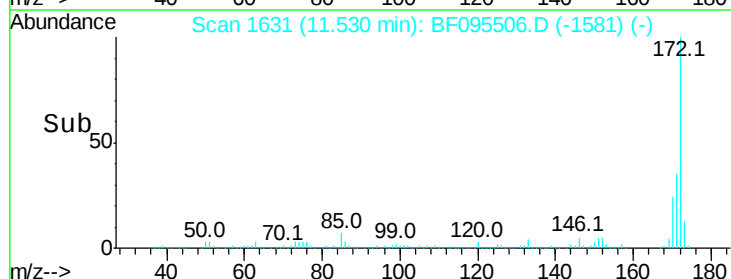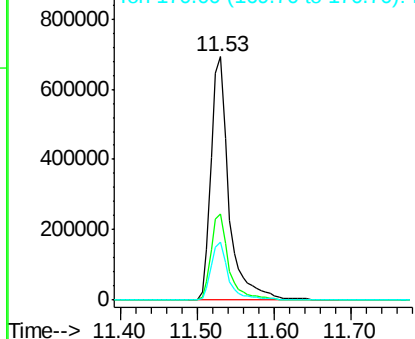


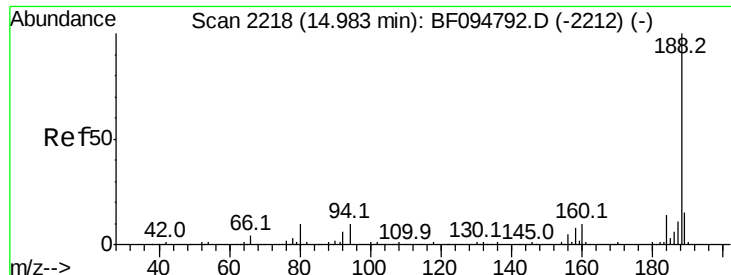




#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 15.00 min Scan# 2221
 Delta R.T. 0.00 min
 Lab File: BF095506.D
 Acq: 27 May 2017 20:11

Instrument :
 BNA_F
 ClientSampleId :
 DSK-MW-LW

Tot Ion:188 Resp: 300541
 Ion Ratio Lower Upper
 188 100
 94 10.8 9.4 14.2
 80 11.5 10.2 15.2

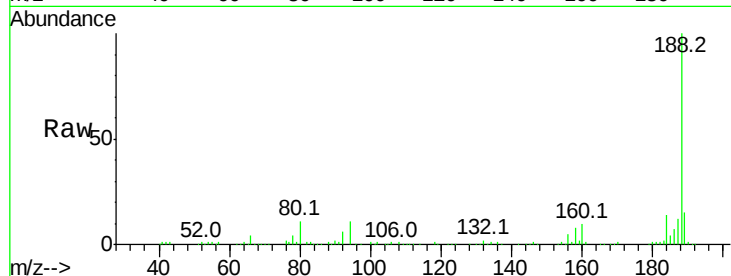


Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

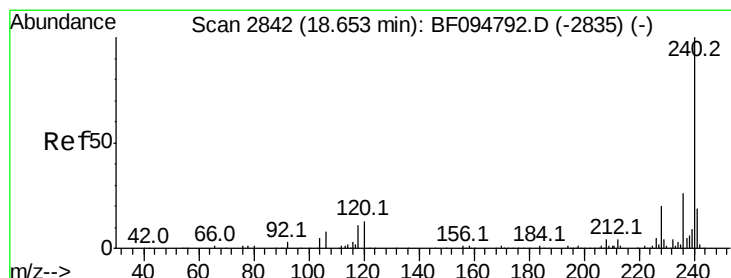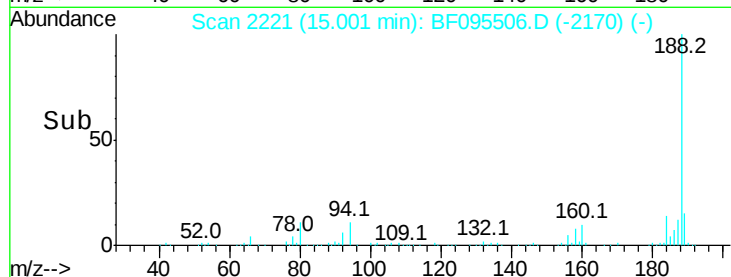
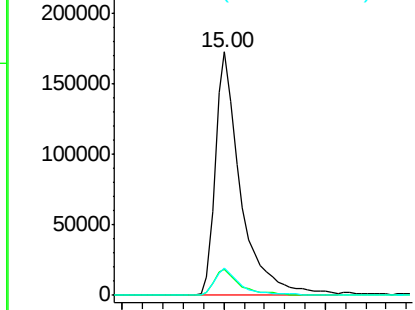



#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 18.68 min Scan# 2846
 Delta R.T. 0.00 min
 Lab File: BF095506.D
 Acq: 27 May 2017 20:11

Tgt Ion:240 Resp: 246393
 Ion Ratio Lower Upper
 240 100
 120 15.5 5.8 8.8#
 236 24.6 20.5 30.7

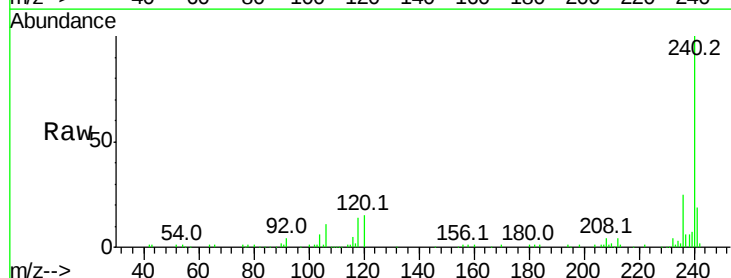

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

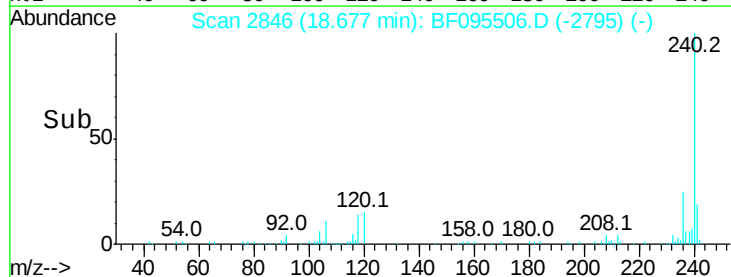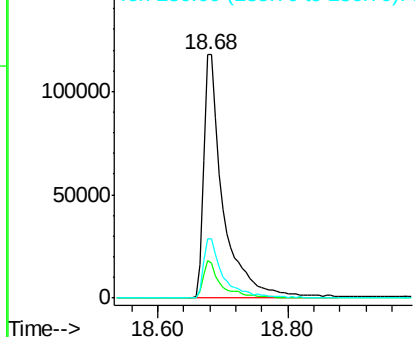

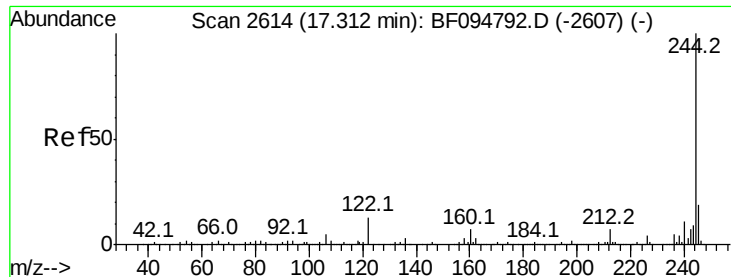

#78

Terphenyl-d14

Concen: 74.29 ng

RT: 17.32 min Scan# 2615

Delta R.T. -0.01 min

Lab File: BF095506.D

Acq: 27 May 2017 20:11

Instrument :

BNA_F

ClientSampleId :

DSK-MW-LW


Tot Ion:244 Resp: 831028

Ion Ratio Lower Upper

244 100

212 6.8 6.0 9.0




122 13.4 10.3 15.5

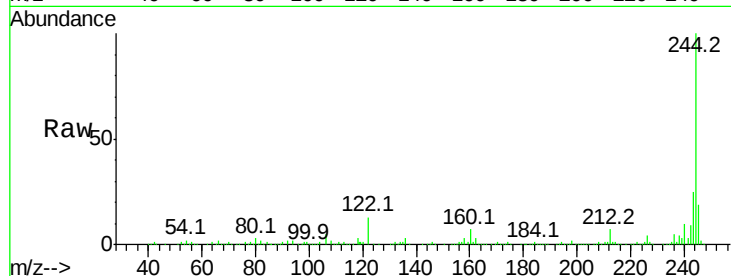

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

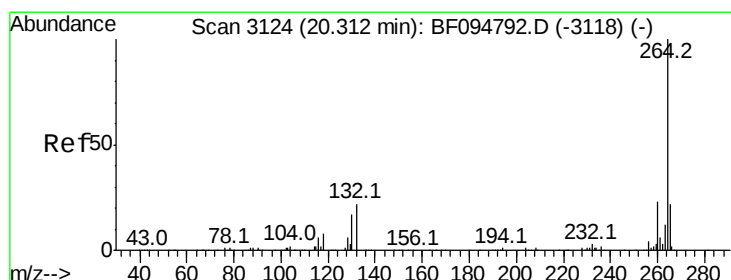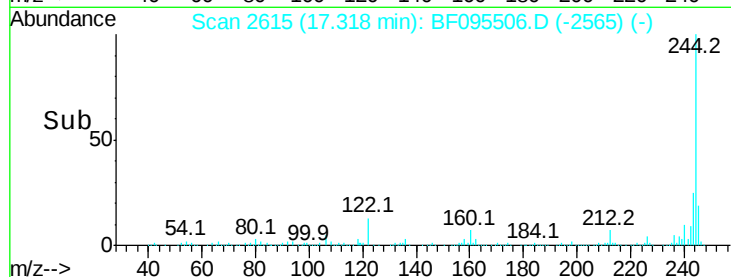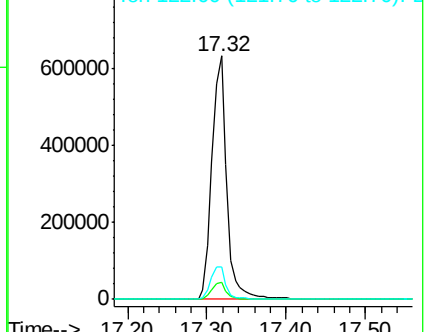

#86

Perylene-d12

Concen: 20.00 ng

RT: 20.36 min Scan# 3132

Delta R.T. 0.01 min

Lab File: BF095506.D

Acq: 27 May 2017 20:11


Tgt Ion:264 Resp: 159591

Ion Ratio Lower Upper

264 100

260 23.6 19.5 29.3

265 21.7 17.2 25.8

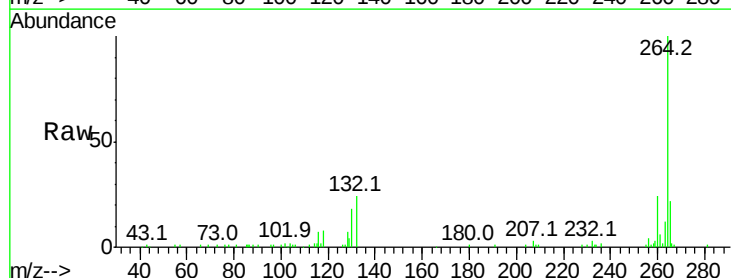

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

