

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052717\
 Data File : BF095505.D
 Acq On : 27 May 2017 19:39
 Operator : SJ/MA
 Sample : I3306-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DSK-MW-4S

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.119	537	541	547	rBV3	15381	39571	1.44%	0.229%
2	5.725	640	644	685	rBV	261129	1020342	37.07%	5.894%
3	7.319	911	915	926	rBV	142182	431963	15.69%	2.495%
4	7.407	926	930	960	rVB	997932	2227332	80.92%	12.865%
5	7.742	983	987	1004	rVB	342843	471916	17.15%	2.726%
6	7.972	1021	1026	1046	rBV	1398882	1961116	71.25%	11.328%
7	8.642	1136	1140	1158	rBV	543162	1239269	45.02%	7.158%
8	9.771	1328	1332	1359	rBV	213997	625443	22.72%	3.613%
9	11.530	1626	1631	1659	rBV	1428733	2641588	95.97%	15.258%
10	12.260	1751	1755	1767	rBV	15553	32762	1.19%	0.189%
11	12.601	1808	1813	1831	rBV2	382018	734276	26.68%	4.241%
12	13.895	2028	2033	2052	rBV	749790	1570036	57.04%	9.069%
13	15.006	2217	2222	2244	rBV	299118	656339	23.85%	3.791%
14	17.318	2609	2615	2629	rBV	2155212	2752410	100.00%	15.898%
15	18.677	2842	2846	2866	rBV	278113	526298	19.12%	3.040%
16	20.359	3128	3132	3147	rBV	180379	382072	13.88%	2.207%


Sum of corrected areas: 17312733

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052717\
Data File : BF095505.D
Acq On : 27 May 2017 19:39
Operator : SJ/MA
Sample : I3306-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSK-MW-4S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

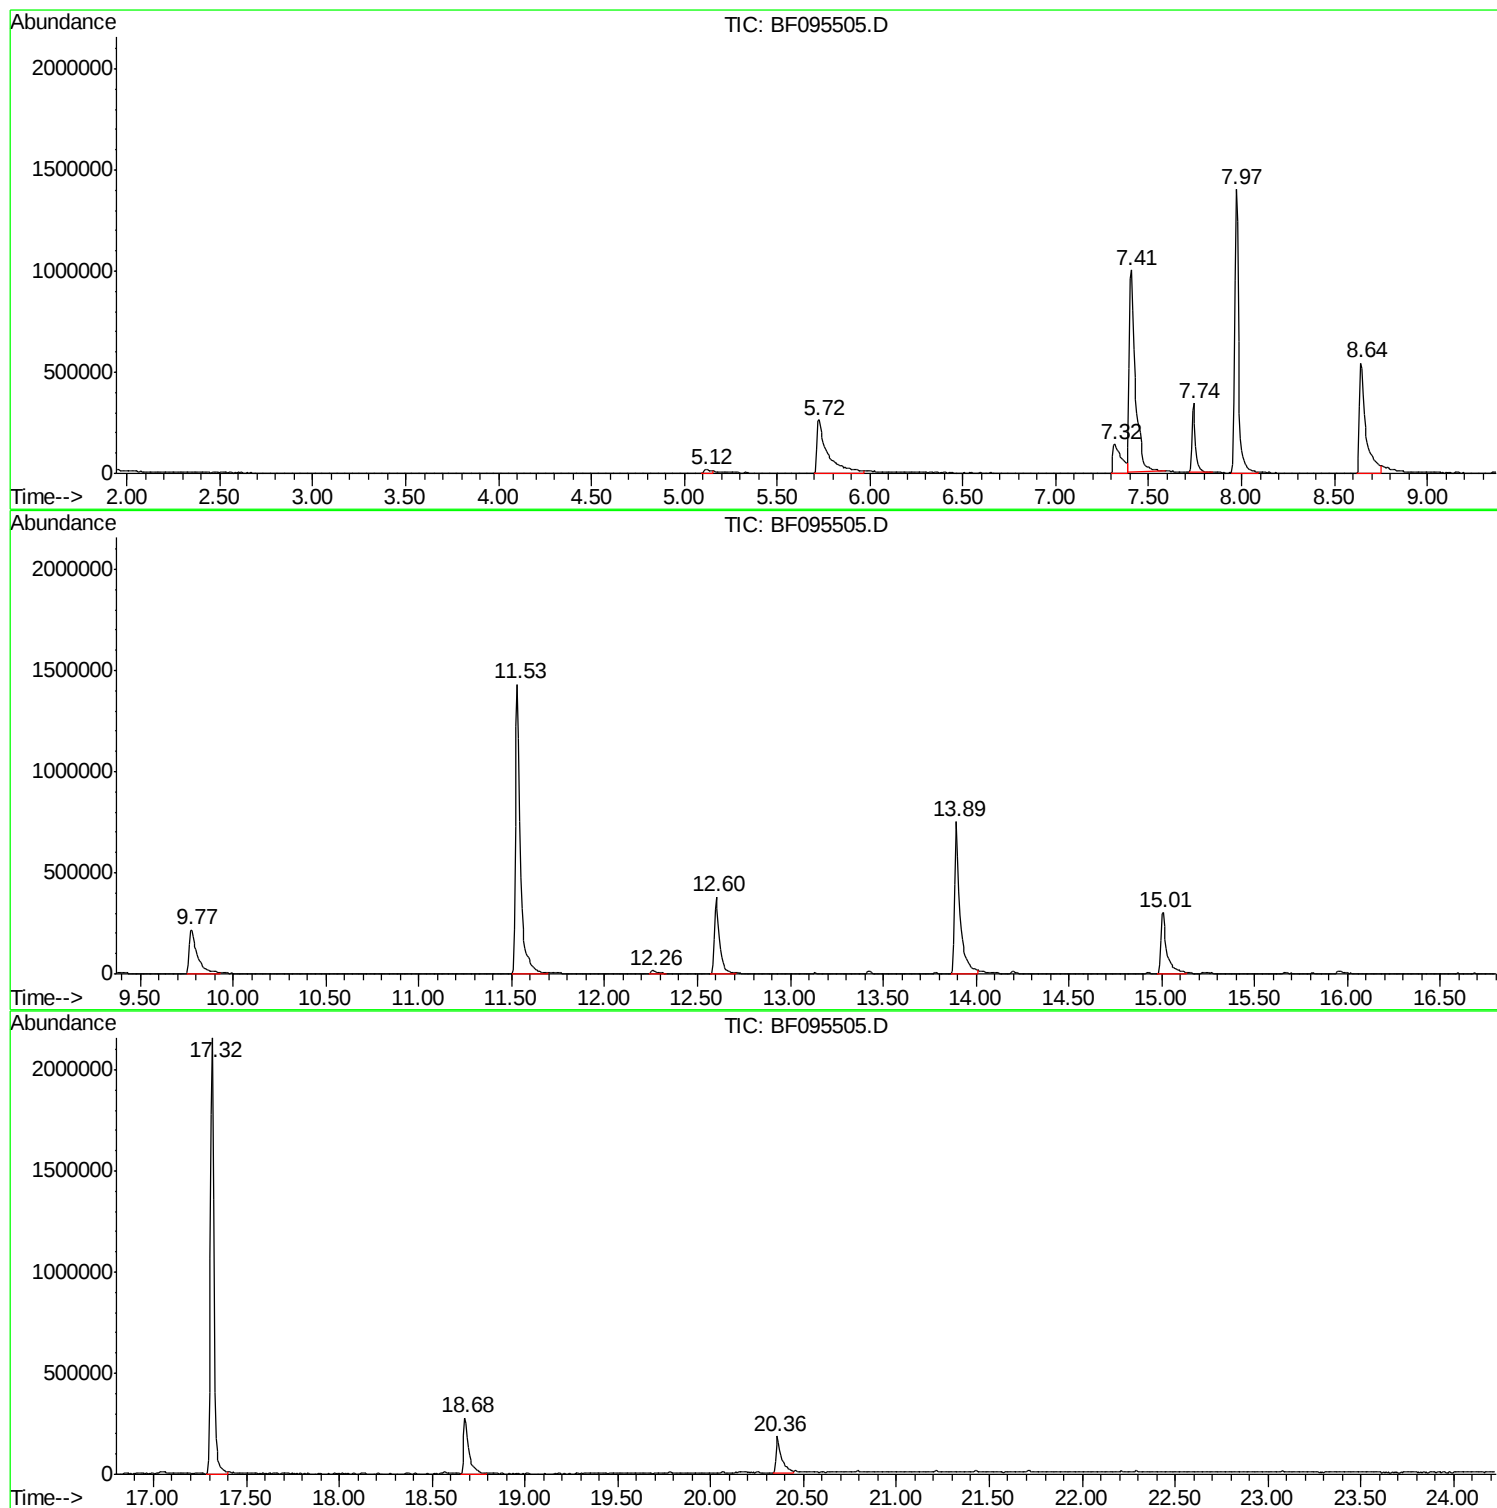

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052717\
Data File : BF095505.D
Acq On : 27 May 2017 19:39
Operator : SJ/MA
Sample : I3306-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSK-MW-4S










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.41 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.41	94.40 ng	2227330	1,4-Dichlorobenzene-d4	7.74

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

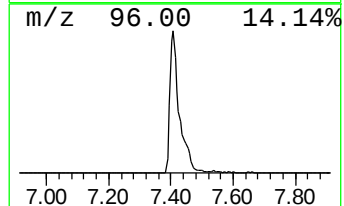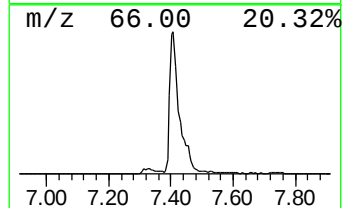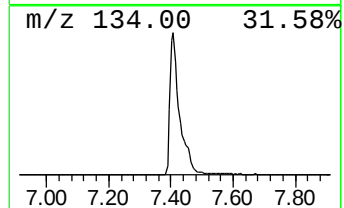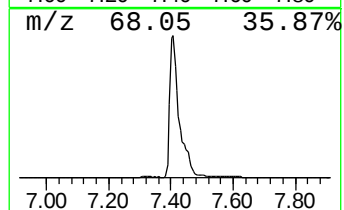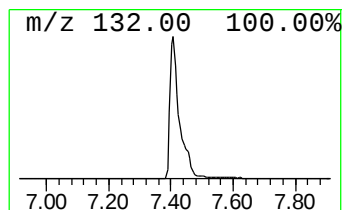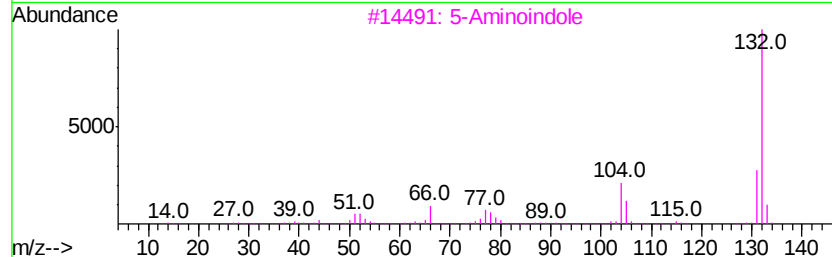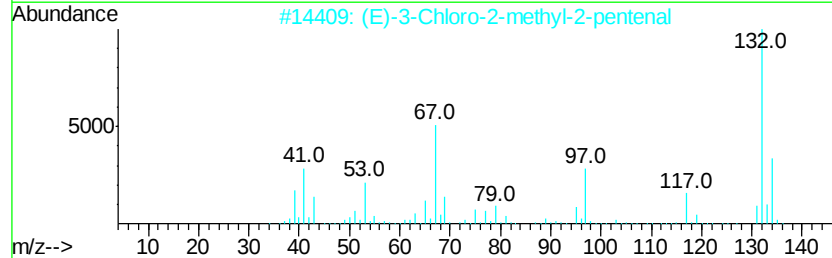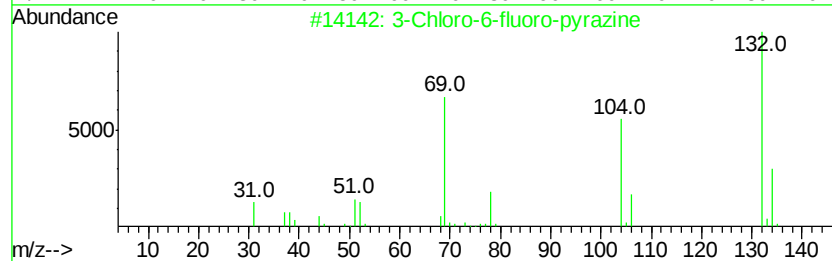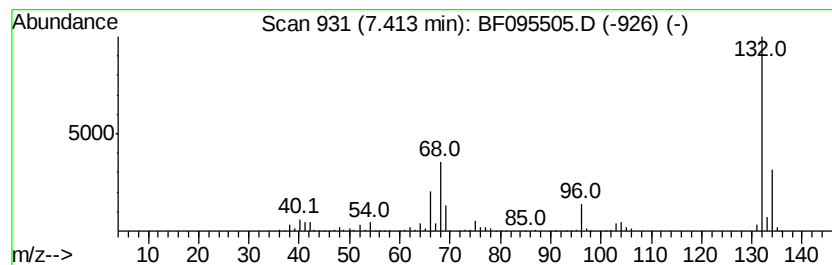

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052717\
Data File : BF095505.D
Acq On : 27 May 2017 19:39
Operator : SJ/MA
Sample : I3306-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSK-MW-4S

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.41	7.41	94.4	ng	2227330	1	7.74	471916	20.0