

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052717\
 Data File : BF095507.D
 Acq On : 27 May 2017 20:44
 Operator : SJ/MA
 Sample : I3306-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DSK-MW-LN

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.113	537	540	553	rBV3	12436	43993	1.43%	0.245%
2	5.719	640	643	667	rBV	282859	943823	30.76%	5.261%
3	6.019	691	694	709	rVB4	21168	52010	1.70%	0.290%
4	7.313	911	914	926	rBV	150499	450168	14.67%	2.509%
5	7.407	926	930	950	rVB	978780	2158174	70.35%	12.029%
6	7.742	983	987	1003	rVB	333026	476121	15.52%	2.654%
7	7.972	1021	1026	1051	rVB	1352070	1823993	59.45%	10.167%
8	8.642	1136	1140	1160	rBV	503382	1202769	39.20%	6.704%
9	9.772	1328	1332	1349	rBV	247295	615533	20.06%	3.431%
10	11.530	1626	1631	1659	rBV	1708923	3067947	100.00%	17.100%
11	12.601	1808	1813	1825	rBV2	400937	745547	24.30%	4.156%
12	13.895	2028	2033	2055	rBV	846874	1644932	53.62%	9.169%
13	15.001	2216	2221	2241	rBV	419663	744059	24.25%	4.147%
14	15.959	2379	2384	2392	rBV	35250	54556	1.78%	0.304%
15	17.318	2610	2615	2633	rBV	2243139	2858056	93.16%	15.931%
16	18.677	2842	2846	2863	rBV	323935	583045	19.00%	3.250%
17	20.359	3128	3132	3149	rBV	221370	475992	15.52%	2.653%


Sum of corrected areas: 17940718

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052717\
Data File : BF095507.D
Acq On : 27 May 2017 20:44
Operator : SJ/MA
Sample : I3306-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSK-MW-LN

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

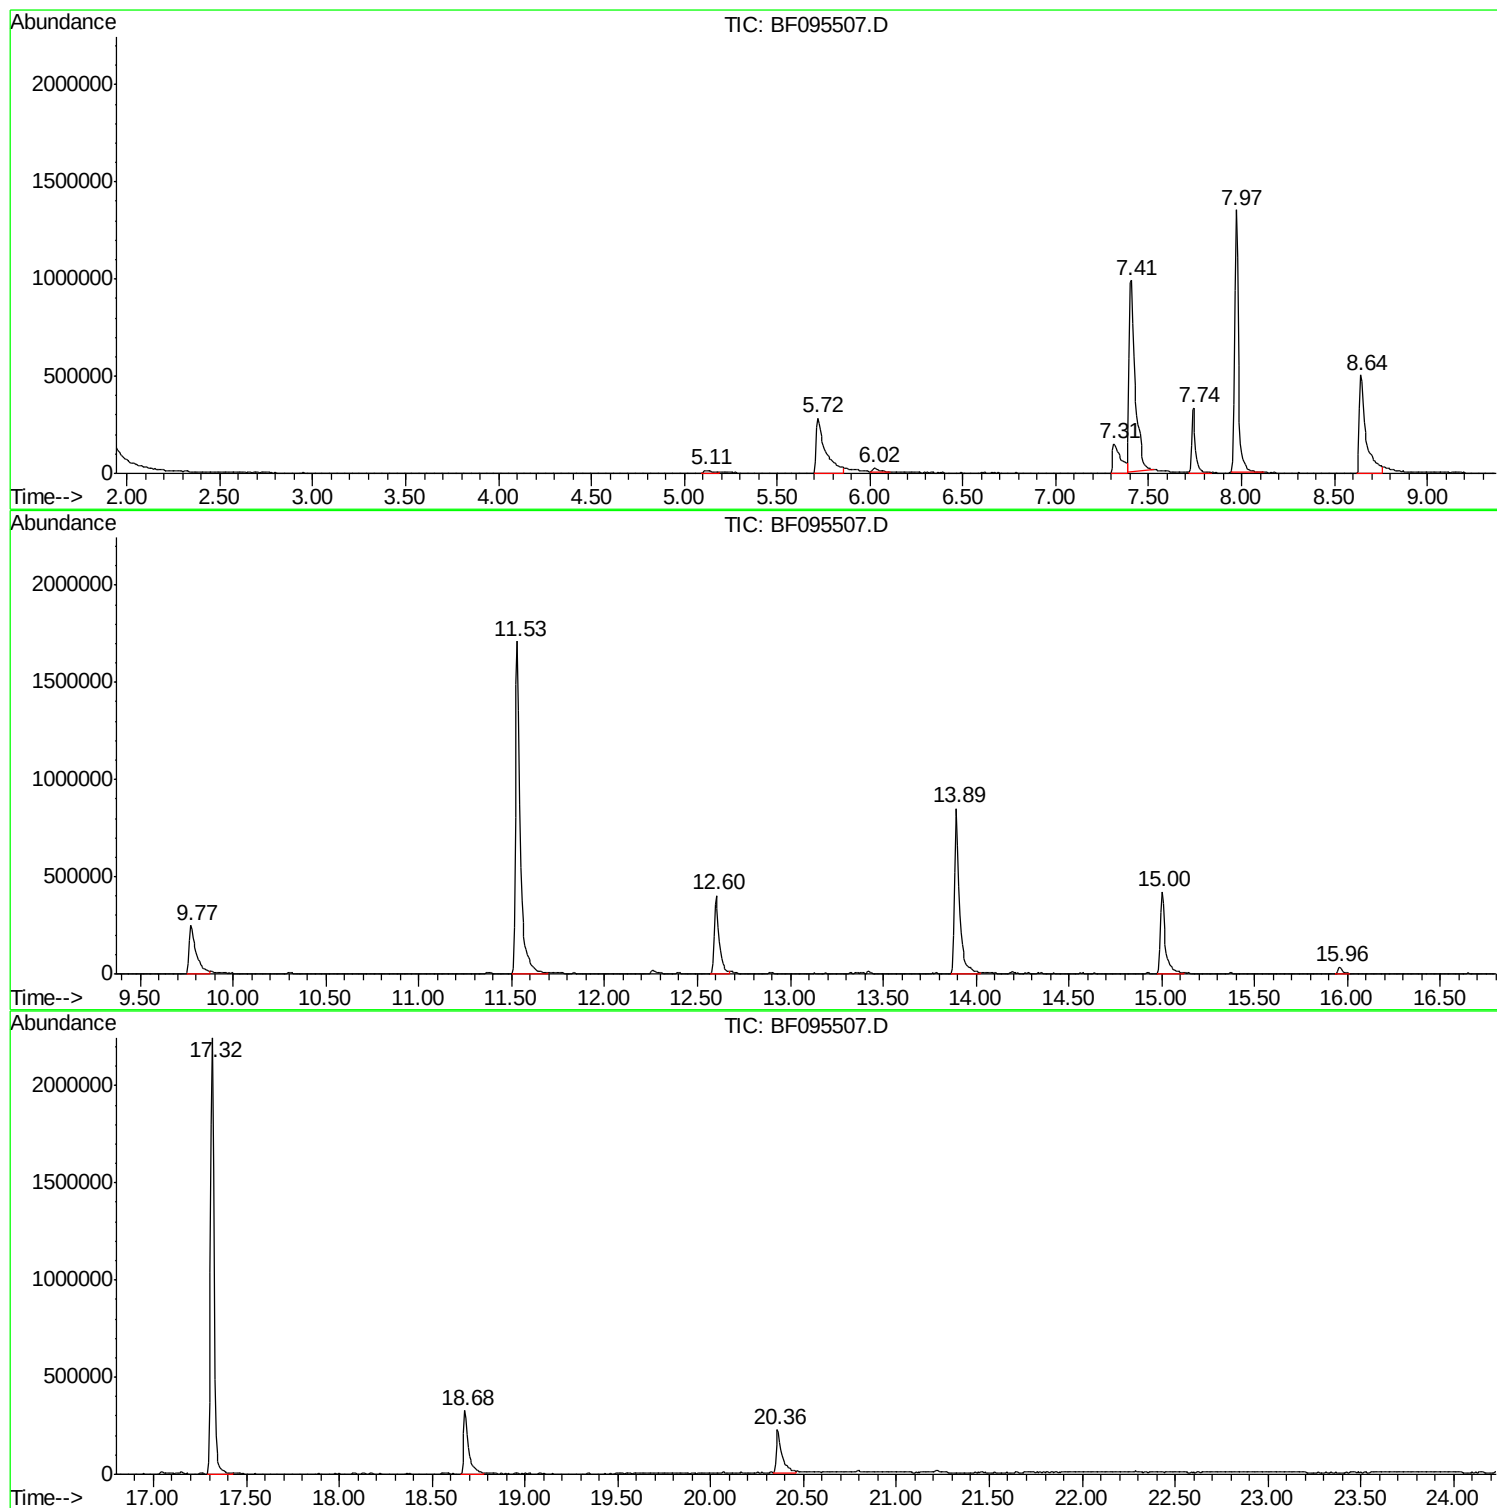

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052717\
Data File : BF095507.D
Acq On : 27 May 2017 20:44
Operator : SJ/MA
Sample : I3306-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSK-MW-LN










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.41 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.41	90.66 ng	2158170	1,4-Dichlorobenzene-d4	7.74

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	35
3		Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	12
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		Xenon	132	Xe	007440-63-3	9

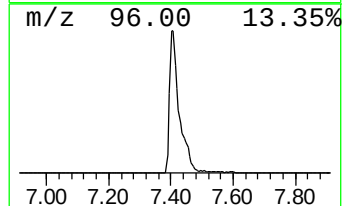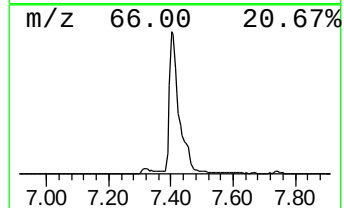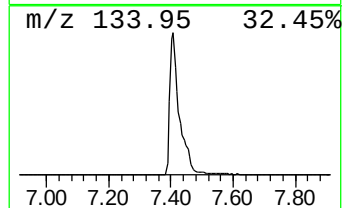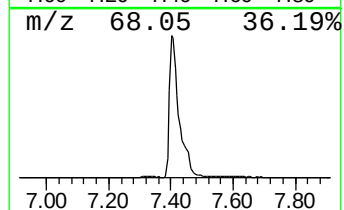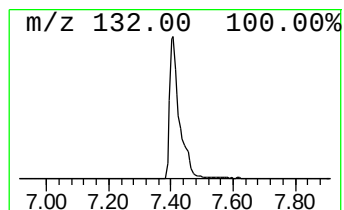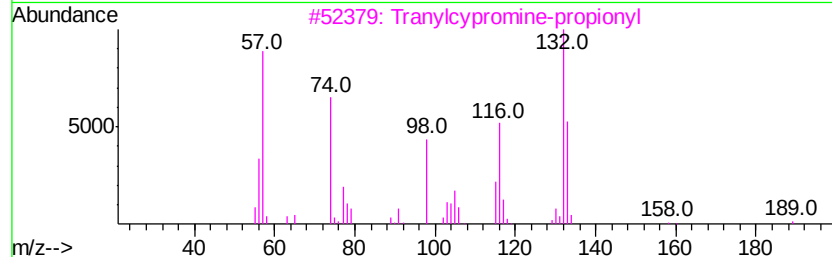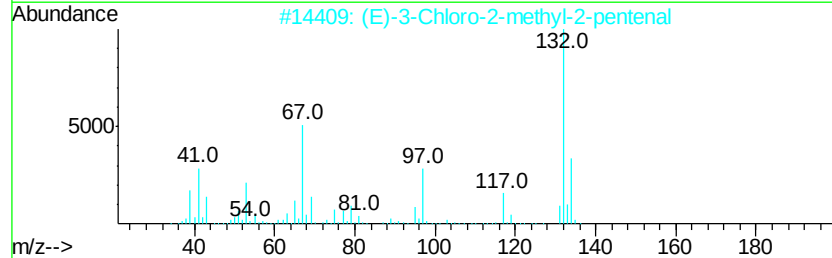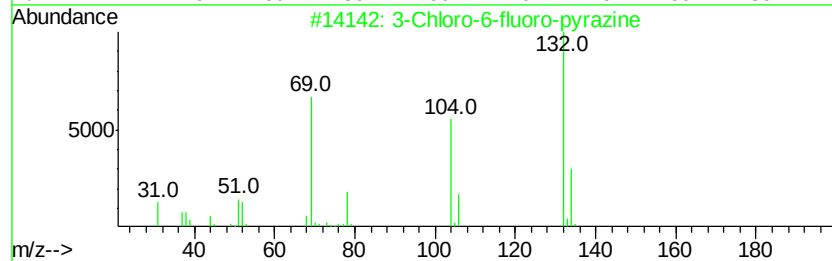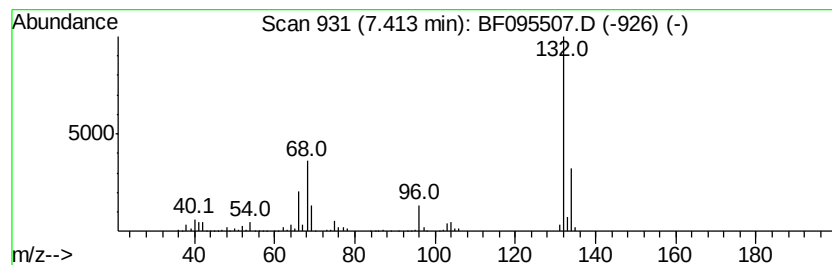

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052717\
Data File : BF095507.D
Acq On : 27 May 2017 20:44
Operator : SJ/MA
Sample : I3306-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSK-MW-LN

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.41	7.41	90.7	ng	2158170	1	7.74	476121	20.0