

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052717\
 Data File : BF095510.D
 Acq On : 27 May 2017 22:20
 Operator : SJ/MA
 Sample : I3306-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DSK-MW-6

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.719	640	643	674	rBV	295130	1051302	33.71%	5.446%
2	7.313	911	914	926	rBV	157660	476270	15.27%	2.467%
3	7.401	926	929	956	rVB	1087382	2410810	77.30%	12.489%
4	7.742	983	987	1003	rVB	359203	510489	16.37%	2.644%
5	7.972	1022	1026	1051	rBV	1543382	2125023	68.14%	11.008%
6	8.642	1136	1140	1158	rBV	646053	1418519	45.48%	7.348%
7	9.772	1328	1332	1355	rBV	260937	665407	21.34%	3.447%
8	11.530	1626	1631	1651	rBV	1828101	3118739	100.00%	16.156%
9	12.277	1747	1758	1770	rBV6	18323	60667	1.95%	0.314%
10	12.601	1808	1813	1832	rBV2	421763	843928	27.06%	4.372%
11	13.895	2027	2033	2054	rBV	847575	1747610	56.04%	9.053%
12	15.006	2217	2222	2251	rVB2	376233	780236	25.02%	4.042%
13	17.318	2609	2615	2634	rBV	2387031	3020076	96.84%	15.645%
14	18.683	2842	2847	2869	rBV	347478	650434	20.86%	3.369%
15	20.359	3128	3132	3145	rBV2	212499	424616	13.61%	2.200%


Sum of corrected areas: 19304126

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052717\
Data File : BF095510.D
Acq On : 27 May 2017 22:20
Operator : SJ/MA
Sample : I3306-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSK-MW-6

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

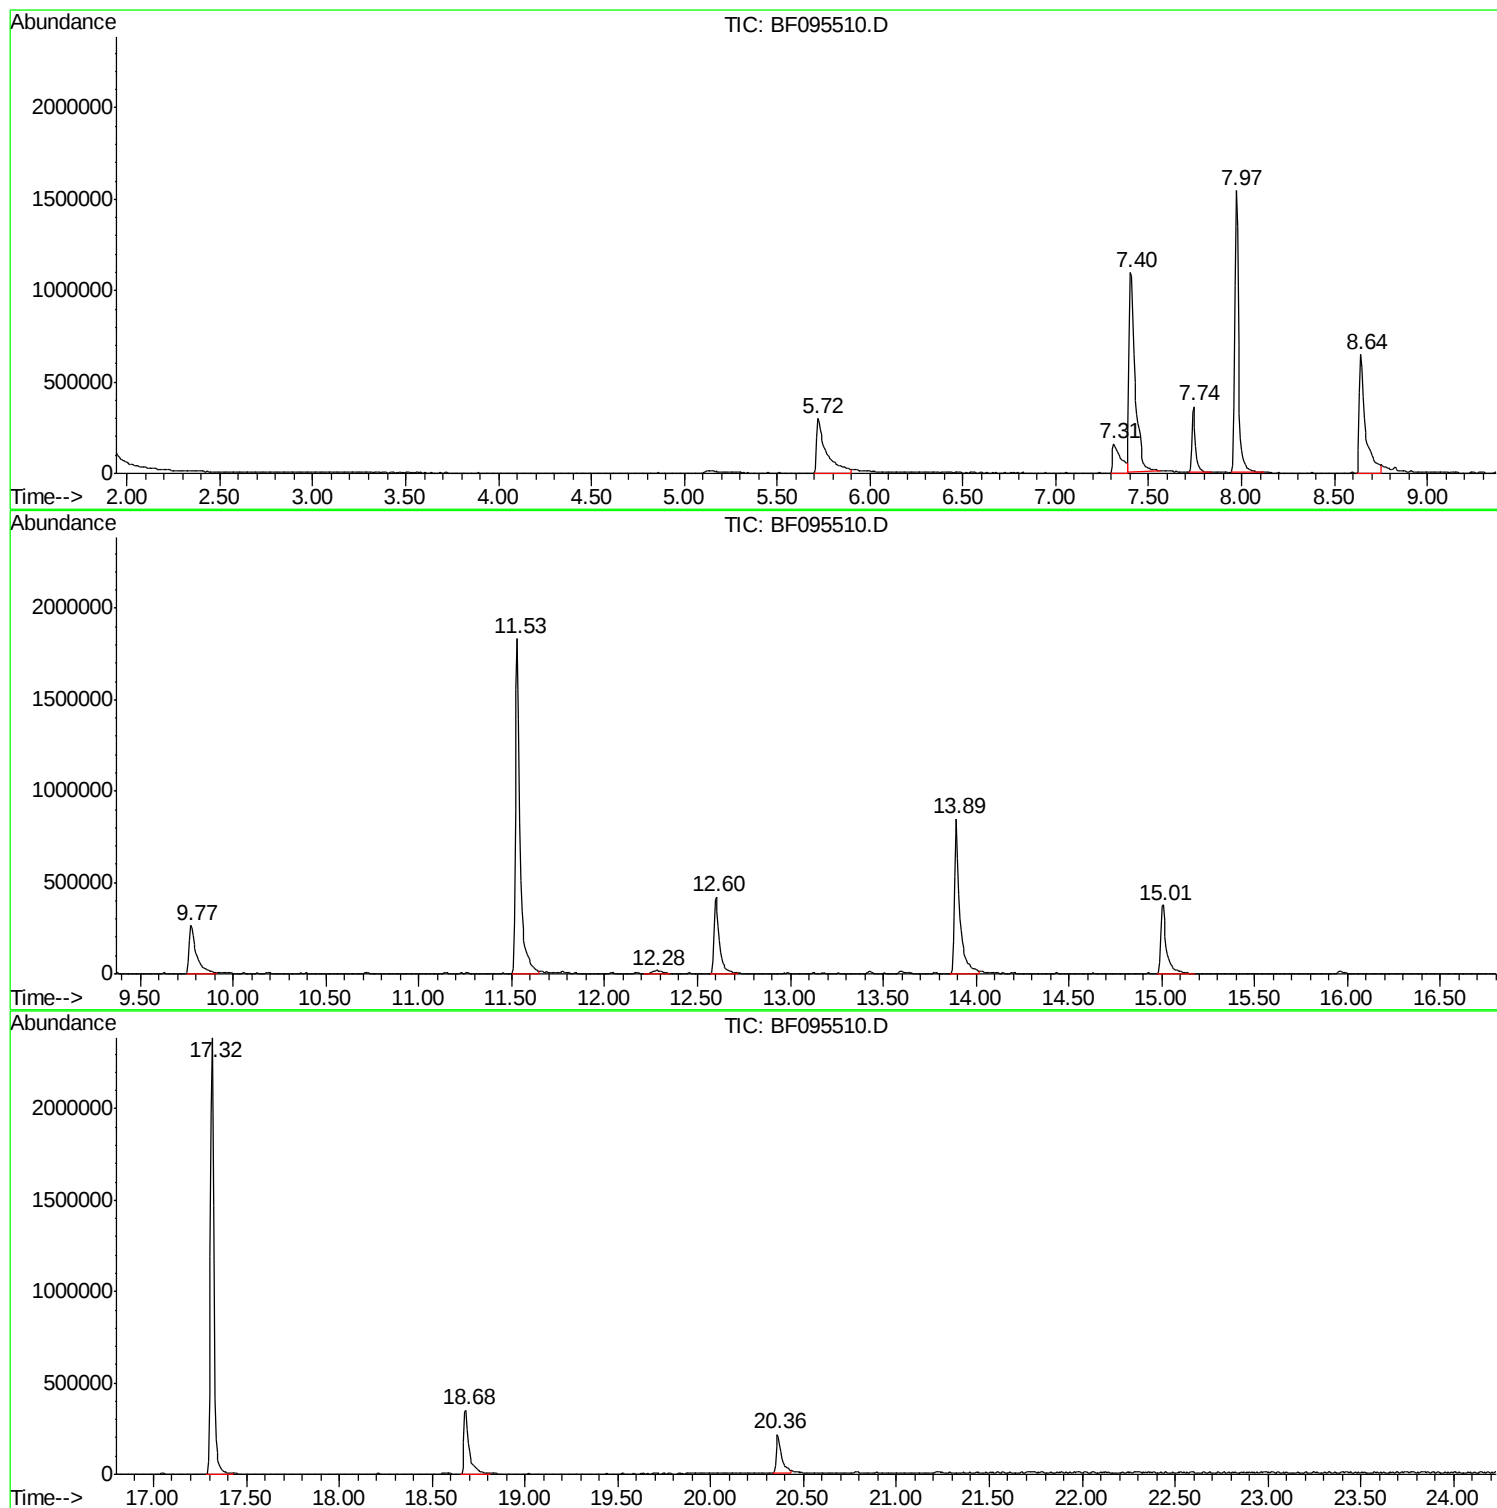

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052717\
Data File : BF095510.D
Acq On : 27 May 2017 22:20
Operator : SJ/MA
Sample : I3306-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSK-MW-6










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.40 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.40	94.45 ng	2410810	1,4-Dichlorobenzene-d4	7.74

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	10
3		4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

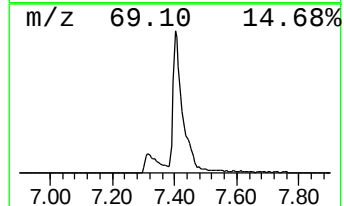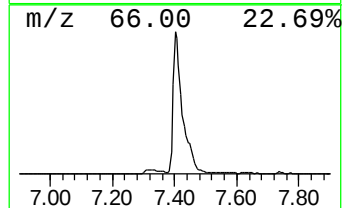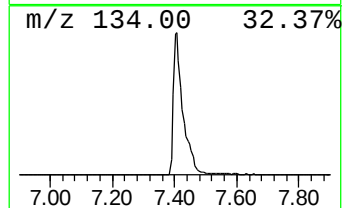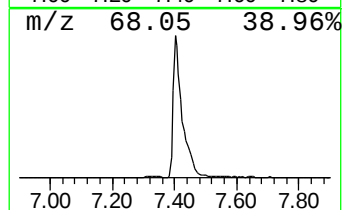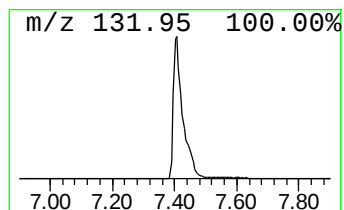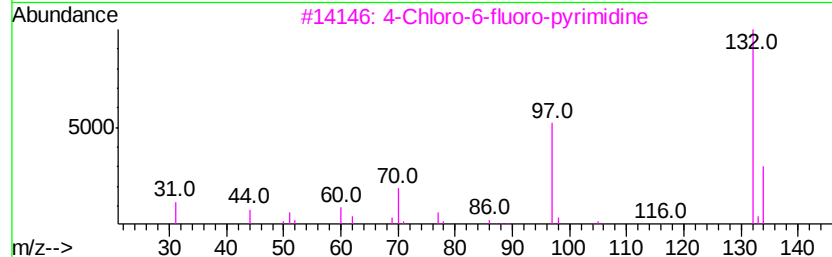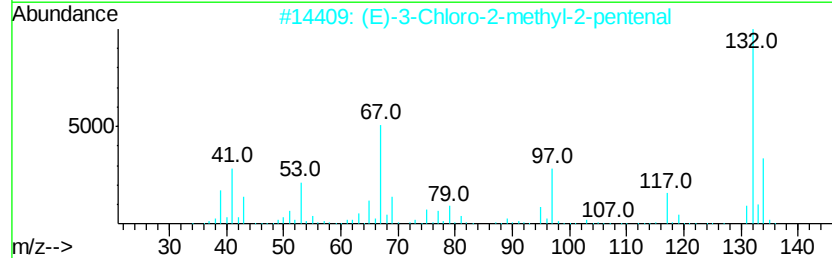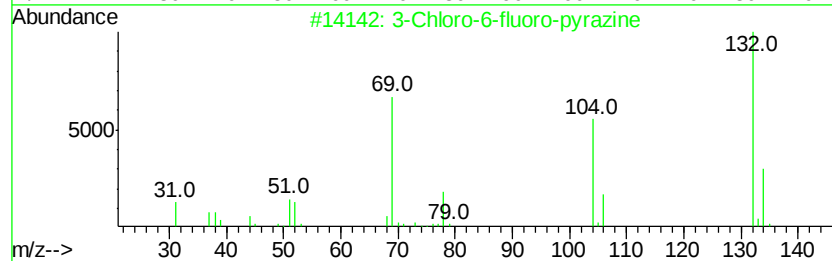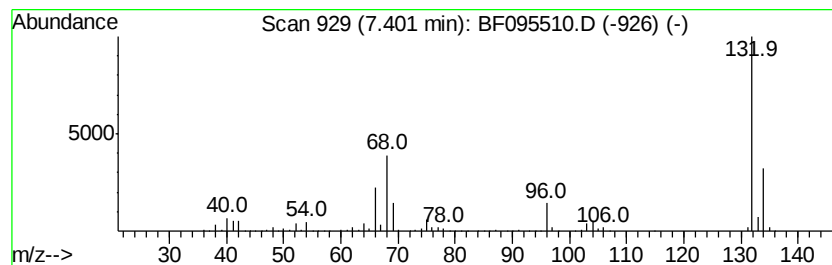

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052717\
Data File : BF095510.D
Acq On : 27 May 2017 22:20
Operator : SJ/MA
Sample : I3306-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSK-MW-6

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.40	7.40	94.5	ng	2410810	1	7.74	510489	20.0