


Data Path : Z:\HPCHEM1\BNA F\DATA\BF052717\
 Data File : BF095498.D
 Acq On : 27 May 2017 13:01
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF050217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 26 16:50:16 2017

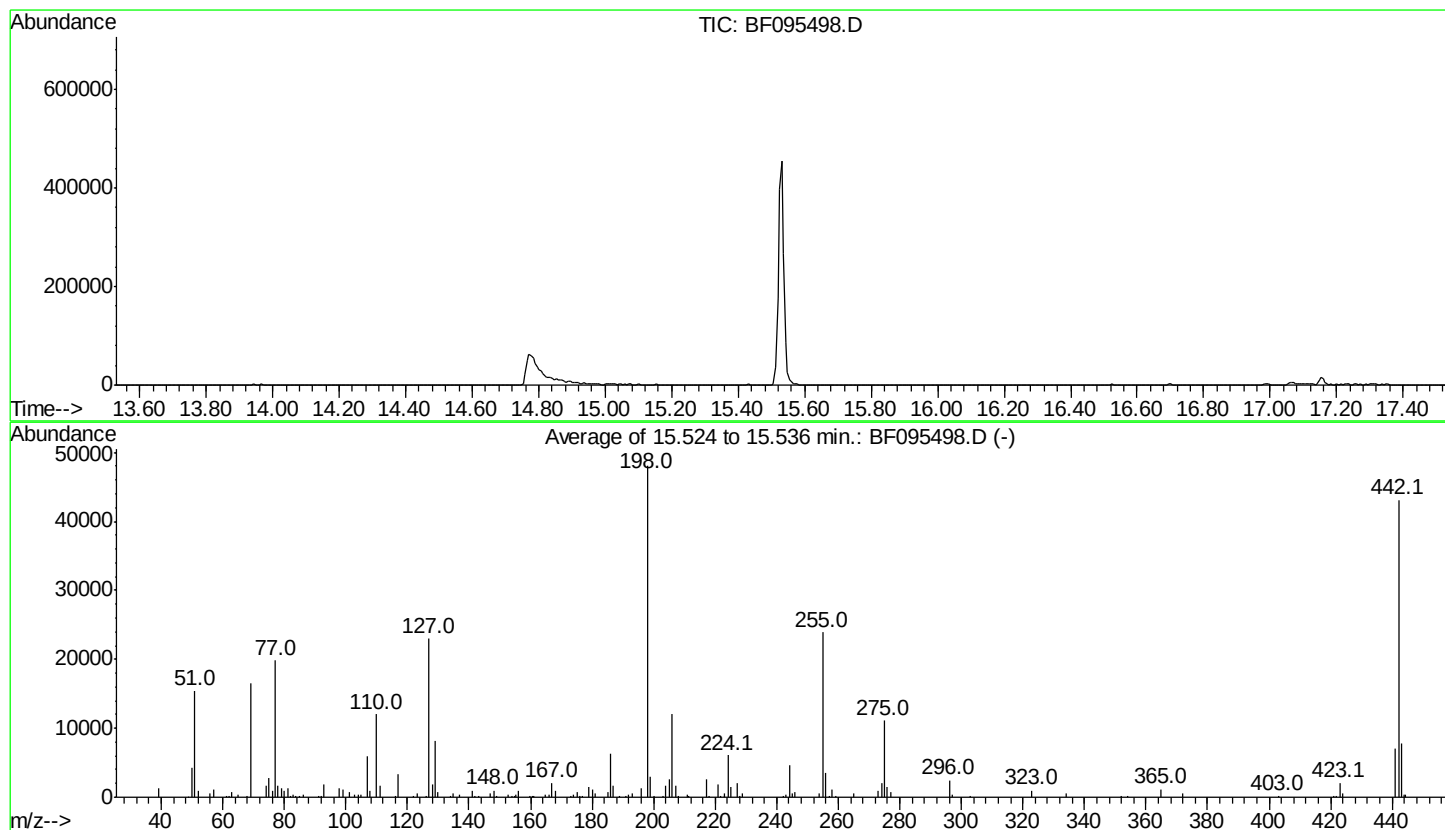

AutoFind: Scans 2310, 2311, 2312; Background Corrected with Scan 2304

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	15477	PASS
68	69	0.00	2	1.1	180	PASS
69	198	0.00	100	34.4	16544	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.8	22986	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48085	PASS
199	198	5	9	6.4	3058	PASS
275	198	10	60	23.1	11089	PASS
365	198	1	100	2.5	1182	PASS
441	442	0.01	24	16.5	7097	PASS
442	198	50	100	89.7	43130	PASS
443	442	15	24	18.1	7817	PASS