

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052722\
 Data File : BF128500.D
 Acq On : 27 May 2022 10:07
 Operator : CG\JU
 Sample : PB145062BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145062BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128500.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.469	534	541	544	rBV	5776899	6673297	80.56%	12.849%
2	6.463	703	710	713	rBV	4882551	6802752	82.13%	13.098%
3	6.839	770	774	777	rBV	1579324	1444331	17.44%	2.781%
4	7.404	863	870	873	rBV	3945514	4660744	56.27%	8.974%
5	8.116	986	991	995	rBV	2011786	1970987	23.79%	3.795%
6	9.198	1168	1175	1179	rBV	6759139	8283325	100.00%	15.949%
7	9.875	1284	1290	1294	rBV	2660480	2396856	28.94%	4.615%
8	10.669	1417	1425	1428	rBV	4377236	4798489	57.93%	9.239%
9	11.363	1537	1543	1546	rBV	2776755	2359580	28.49%	4.543%
10	11.522	1566	1570	1574	rVB	105522	93761	1.13%	0.181%
11	12.957	1809	1814	1818	rBV	6981465	8228074	99.33%	15.843%
12	14.004	1987	1992	1995	rBV	2209083	2036556	24.59%	3.921%
13	14.098	2001	2008	2017	rBV	460170	555218	6.70%	1.069%
14	15.468	2235	2241	2247	rBV	1308650	1632638	19.71%	3.144%




Sum of corrected areas: 51936608

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052722\
Data File : BF128500.D
Acq On : 27 May 2022 10:07
Operator : CG\JU
Sample : PB145062BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145062BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

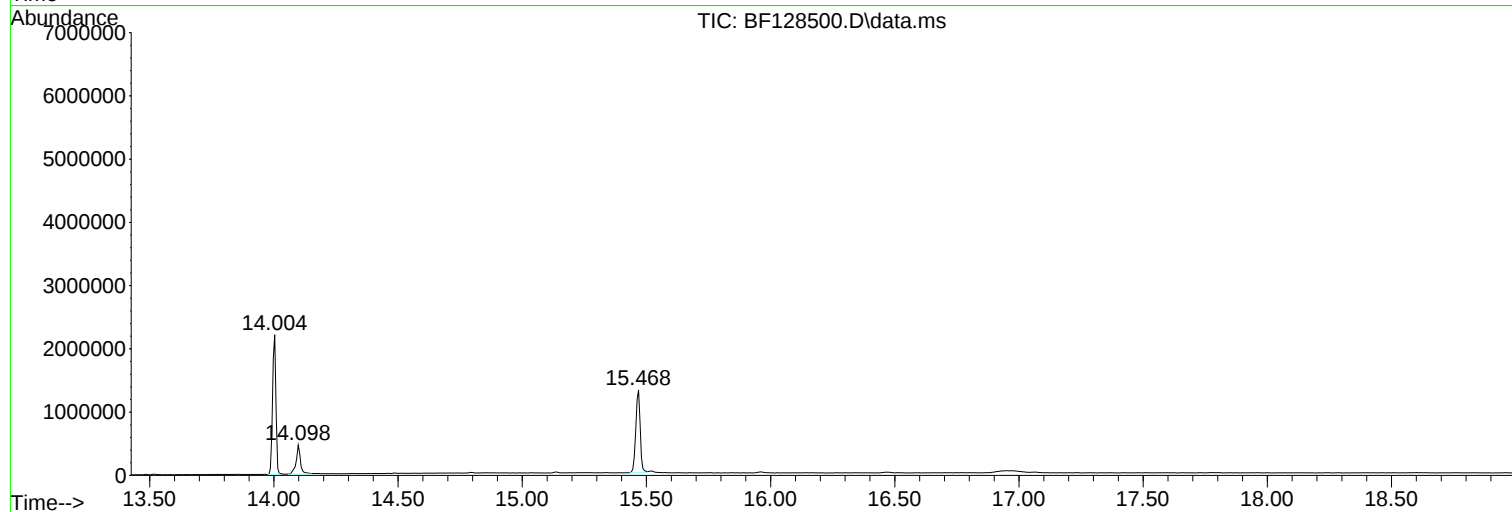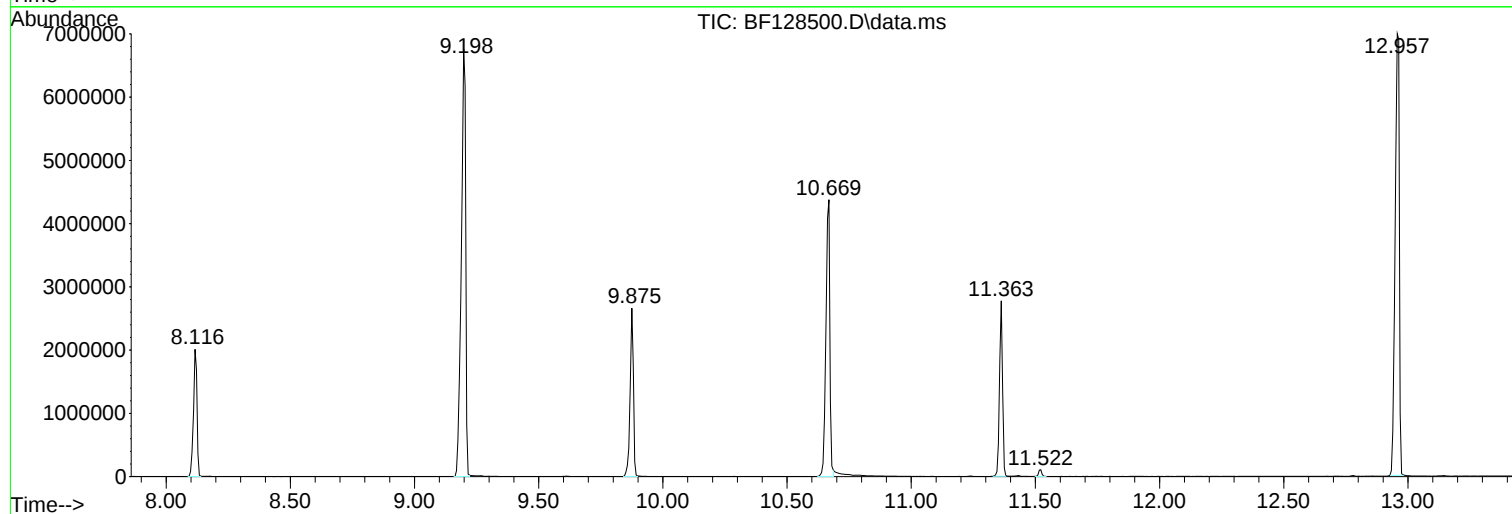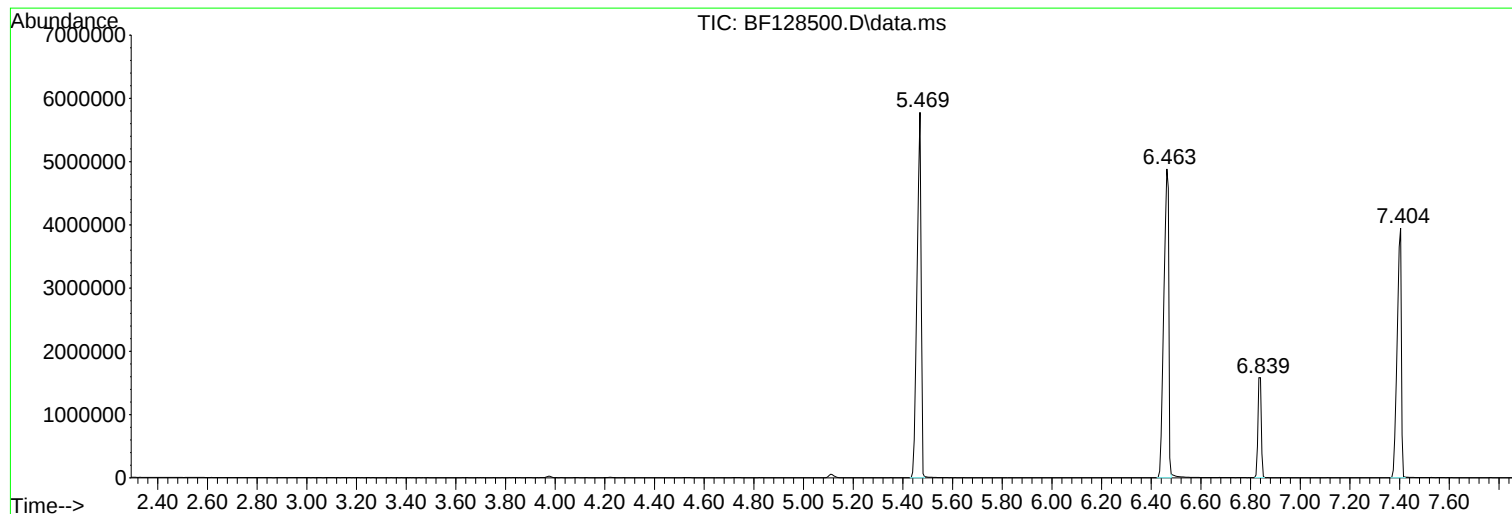

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052722\
Data File : BF128500.D
Acq On : 27 May 2022 10:07
Operator : CG\JU
Sample : PB145062BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB145062BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
14.098	5.45 ng	555218	Chrysene-d12	14.004	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Triphenylphosphine oxide	278	C18H15OP	000791-28-6	96
2	(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19NO3S	1000483-83-4	52
3	Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	42
4	Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	35
5	2-Phenyl-6-(trifluoromethyl)-1H-...	277	C15H10F3NO	1000387-59-3	9

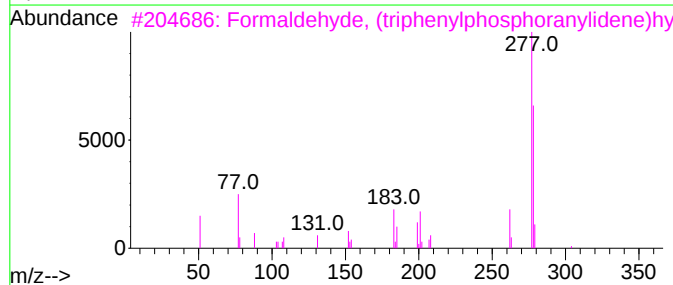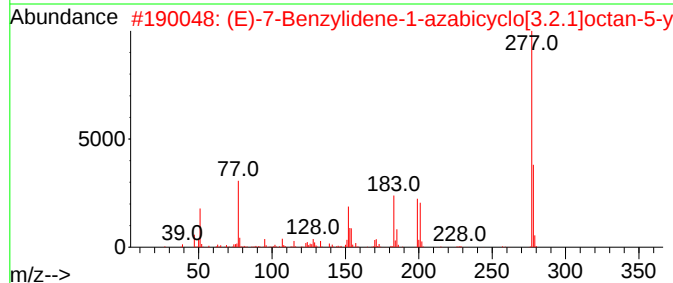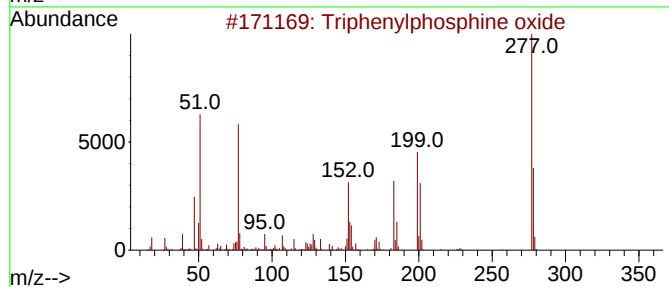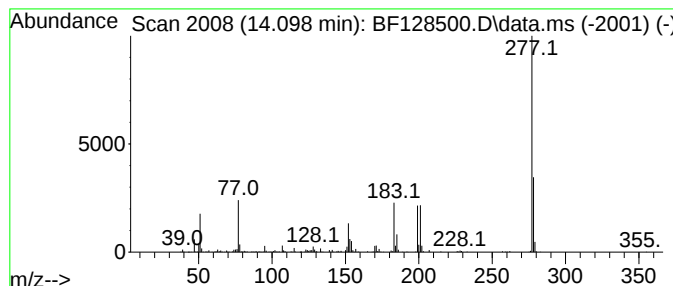

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052722\
Data File : BF128500.D
Acq On : 27 May 2022 10:07
Operator : CG\JU
Sample : PB145062BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145062BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.098	5.5	ng	555218	5	14.004	2036560	20.0