


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052722\
 Data File : BF128498.D
 Acq On : 27 May 2022 09:08
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 27 01:51:59 2022

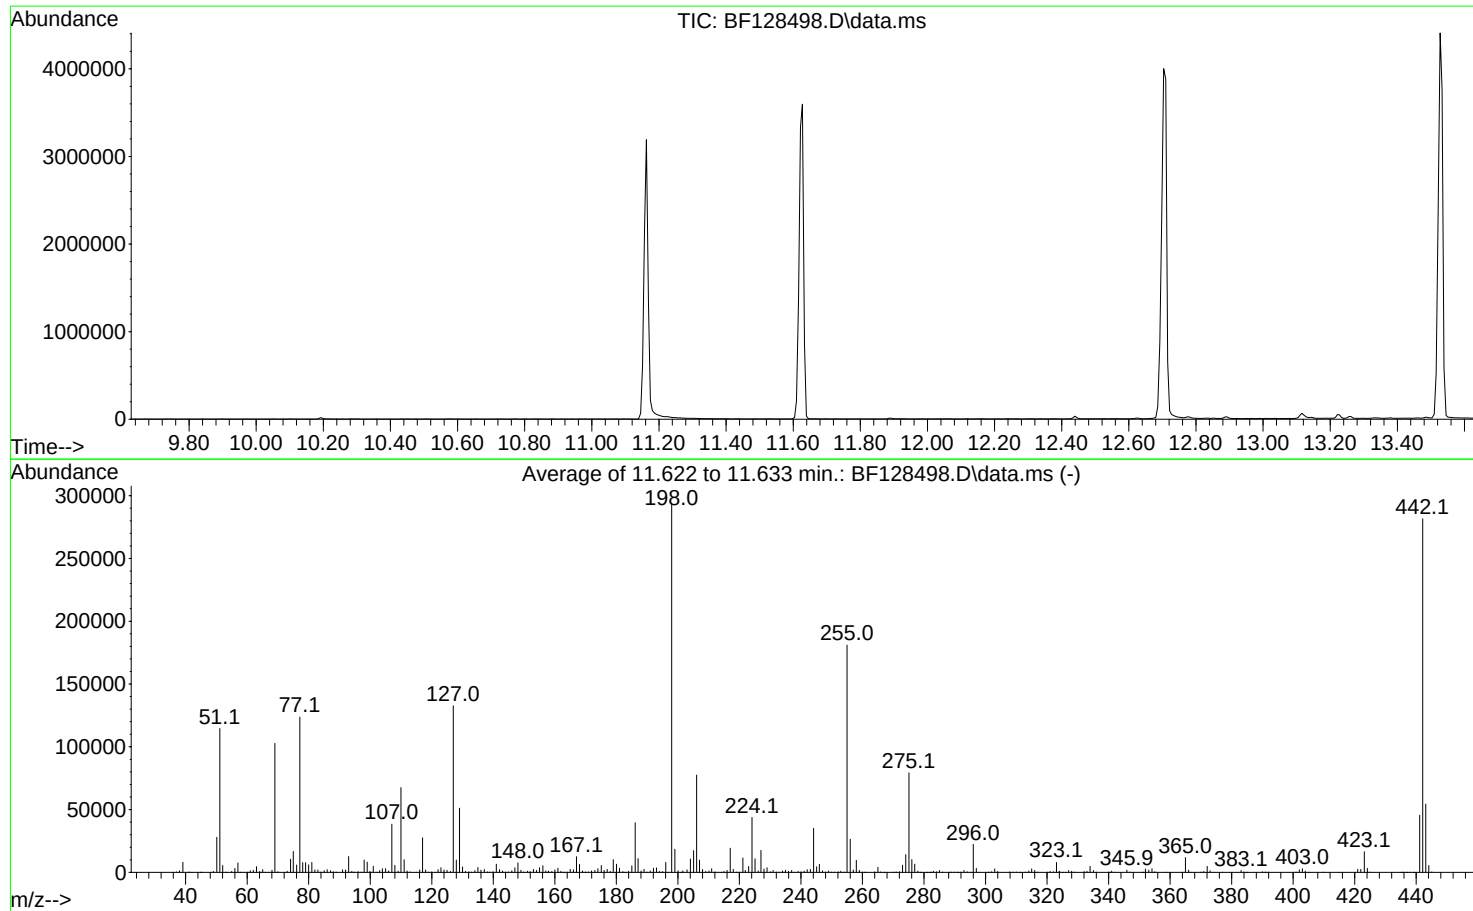

AutoFind: Scans 1587, 1588, 1589; Background Corrected with Scan 1580

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	114534	PASS
68	69	0.00	2	1.7	1766	PASS
69	198	0.00	100	35.1	102768	PASS
70	69	0.00	2	0.5	498	PASS
127	198	10	80	45.3	132608	PASS
197	198	0.00	2	0.1	180	PASS
198	198	100	100	100.0	292995	PASS
199	198	5	9	6.3	18536	PASS
275	198	10	60	27.1	79301	PASS
365	198	1	100	4.0	11731	PASS
441	198	0.01	100	15.5	45517	PASS
442	442	50	100	100.0	281621	PASS
443	442	15	24	19.3	54387	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/27/2022	BNA_F	<u>BF128498.D</u>
Compound Name	Response	Retention Time
DDT	787370	13.527
DDD	11611	13.227
DDE	2427	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14038	801408	1.75

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052722\
 Data File : BF128498.D
 Acq On : 27 May 2022 09:08
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 28 05:56:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 27 01:51:59 2022
 Response via : Initial Calibration

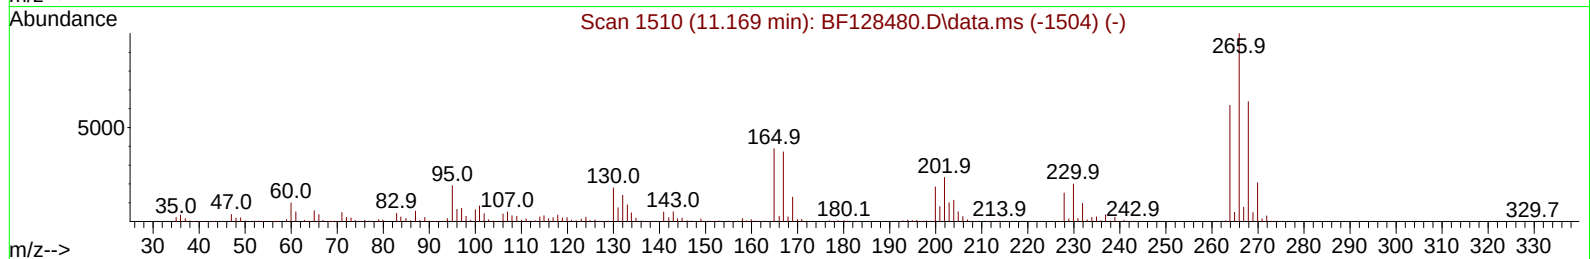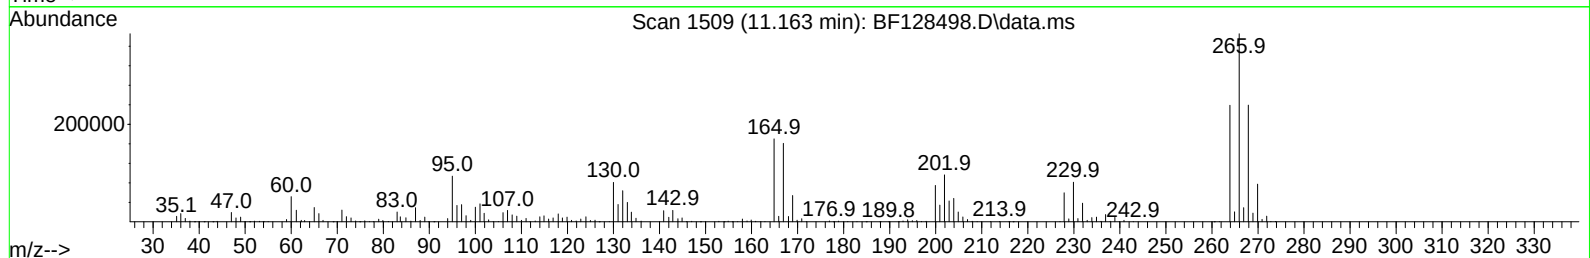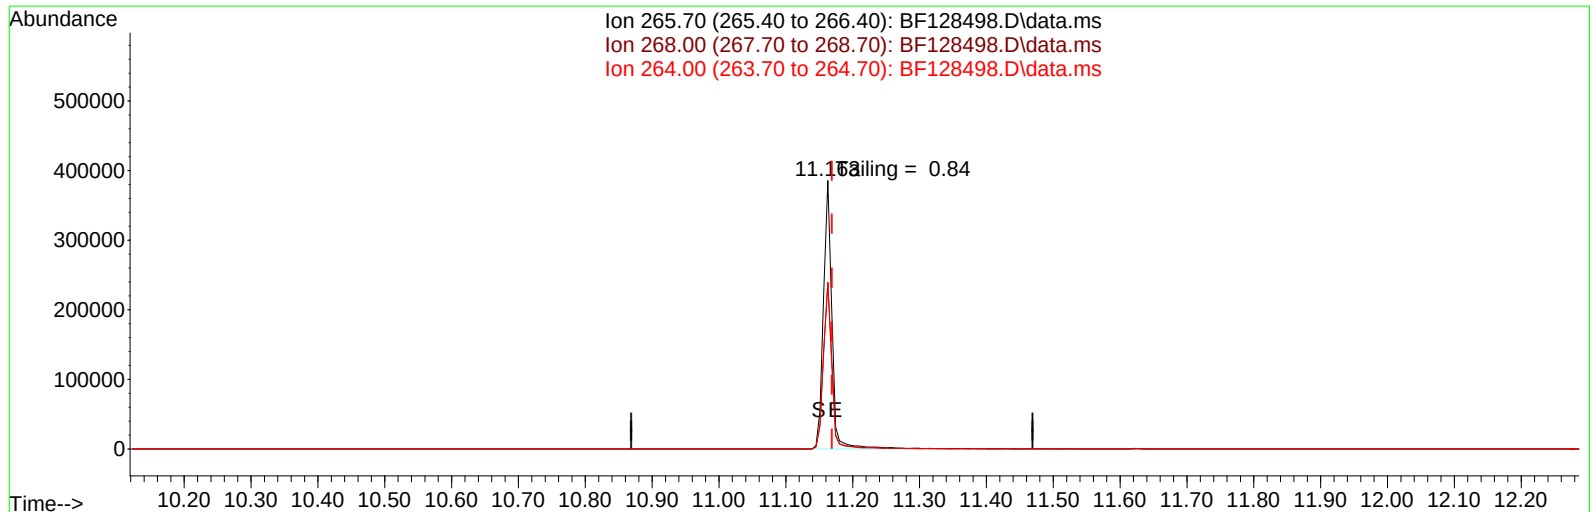

TIC: BF128498.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.006) 799718.01 ng




response 344736

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.02
264.00	61.80	61.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052722\
Data File : BF128498.D
Acq On : 27 May 2022 09:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 28 05:56:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration

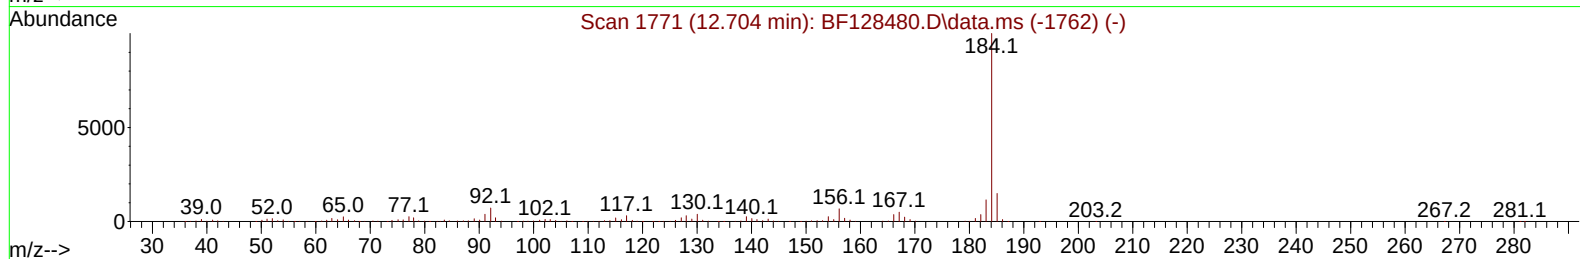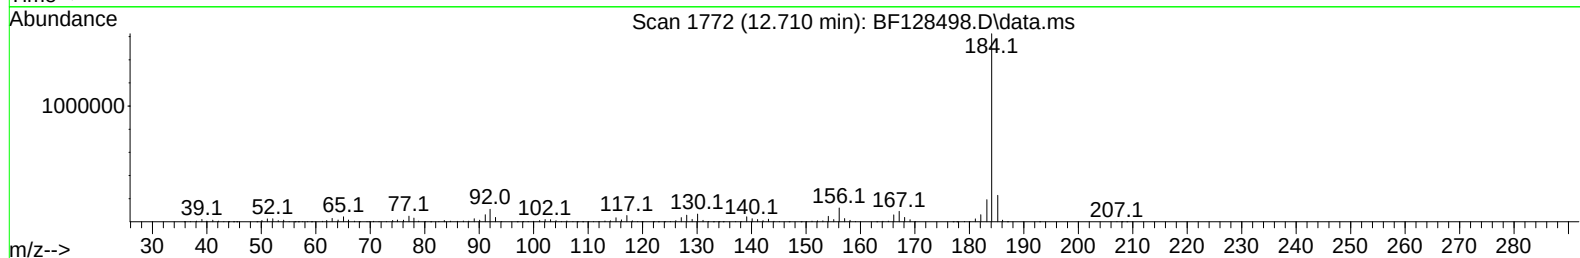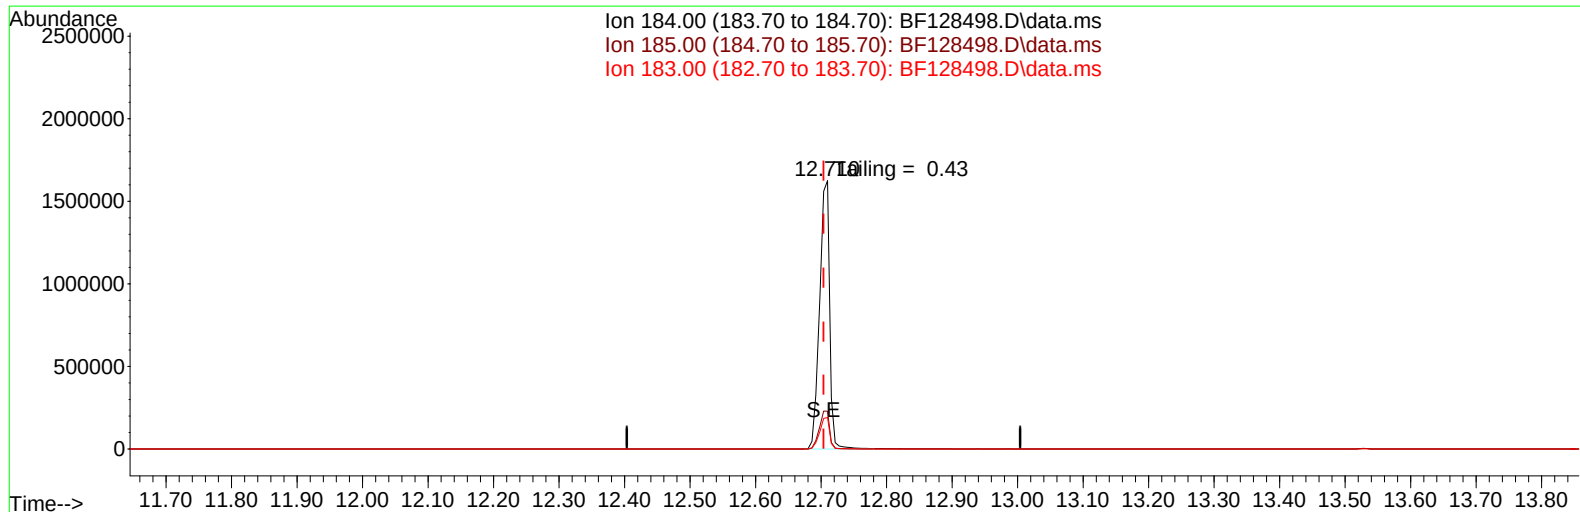

TIC: BF128498.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 236163.09 ng

response 1737670

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.09
183.00	11.60	11.74
0.00	0.00	0.00