


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052722\
 Data File : BF128513.D
 Acq On : 27 May 2022 16:49
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 27 01:51:59 2022

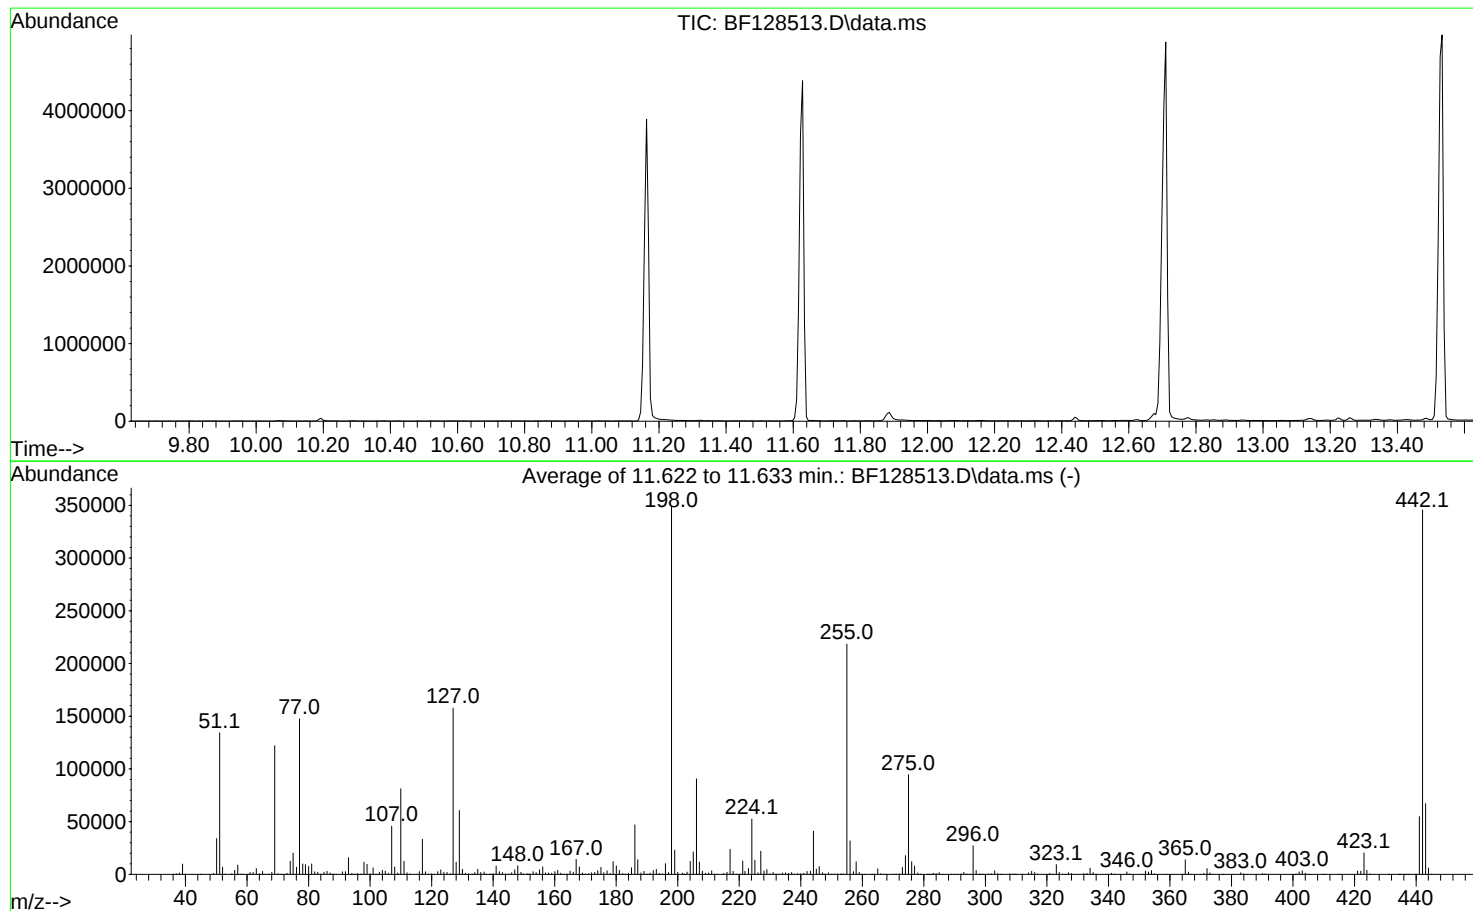

AutoFind: Scans 1587, 1588, 1589; Background Corrected with Scan 1580

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	134272	PASS
68	69	0.00	2	1.7	2050	PASS
69	198	0.00	100	35.0	122068	PASS
70	69	0.00	2	0.6	751	PASS
127	198	10	80	45.2	157667	PASS
197	198	0.00	2	0.5	1641	PASS
198	198	100	100	100.0	348885	PASS
199	198	5	9	6.6	23144	PASS
275	198	10	60	27.1	94568	PASS
365	198	1	100	4.0	13782	PASS
441	198	0.01	100	15.7	54856	PASS
442	442	50	100	100.0	345643	PASS
443	442	15	24	19.4	67096	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/27/2022	BNA_F	<u>BF128513.D</u>
Compound Name	Response	Retention Time
DDT	948724	13.533
DDD	10526	13.227
DDE	698	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11224	959948	1.17

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052722\
Data File : BF128513.D
Acq On : 27 May 2022 16:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 28 05:59:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration

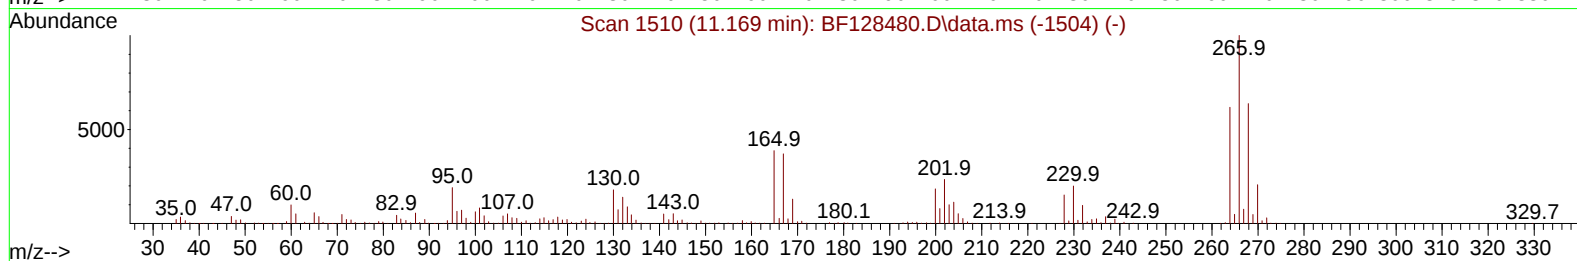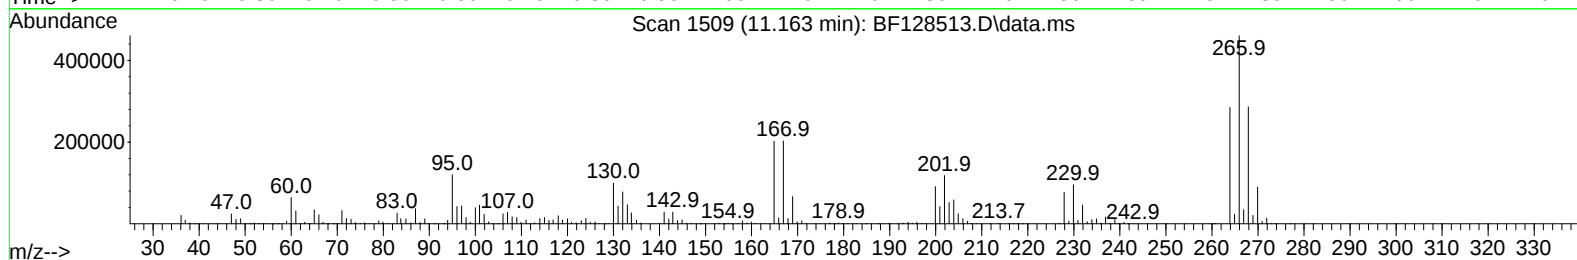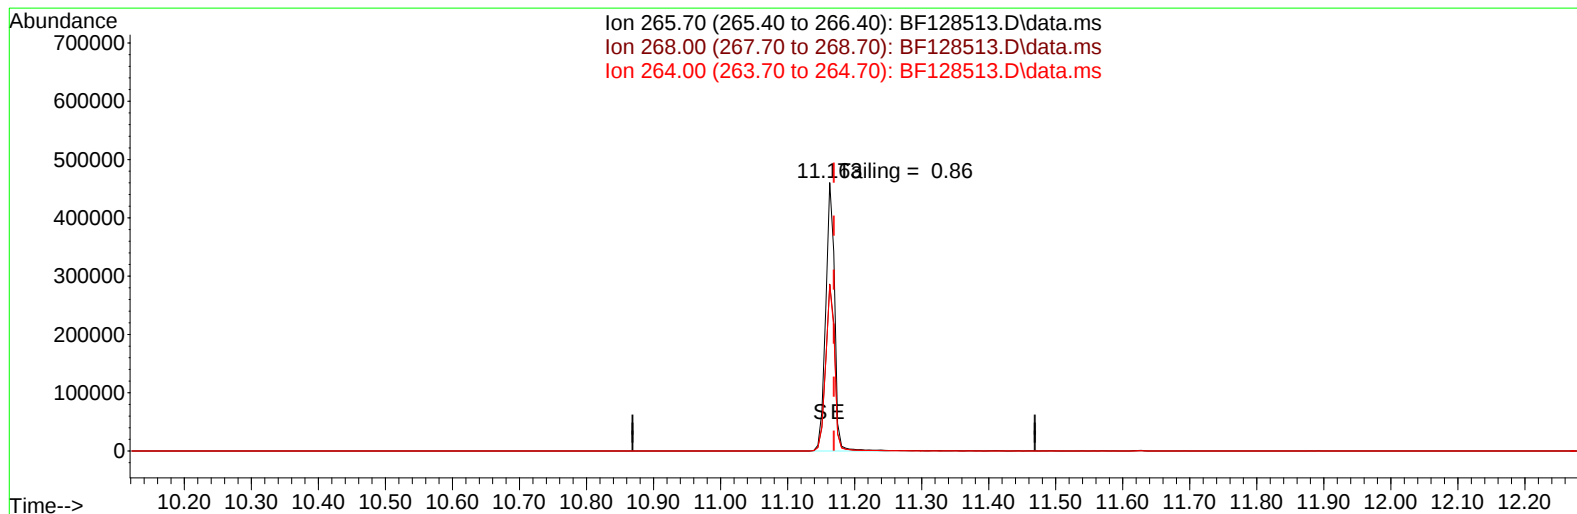

TIC: BF128513.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.006) 263935.14 ng




response 429409

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.22
264.00	61.80	61.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052722\
 Data File : BF128513.D
 Acq On : 27 May 2022 16:49
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: May 28 05:59:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 27 01:51:59 2022
 Response via : Initial Calibration

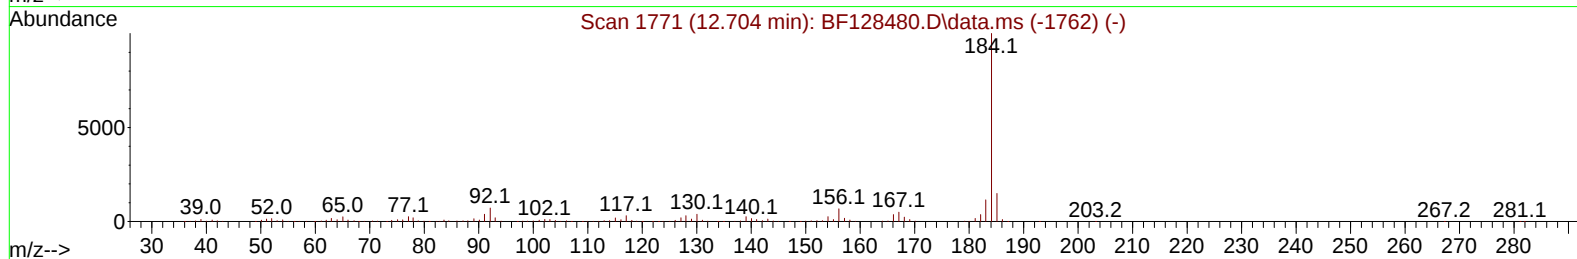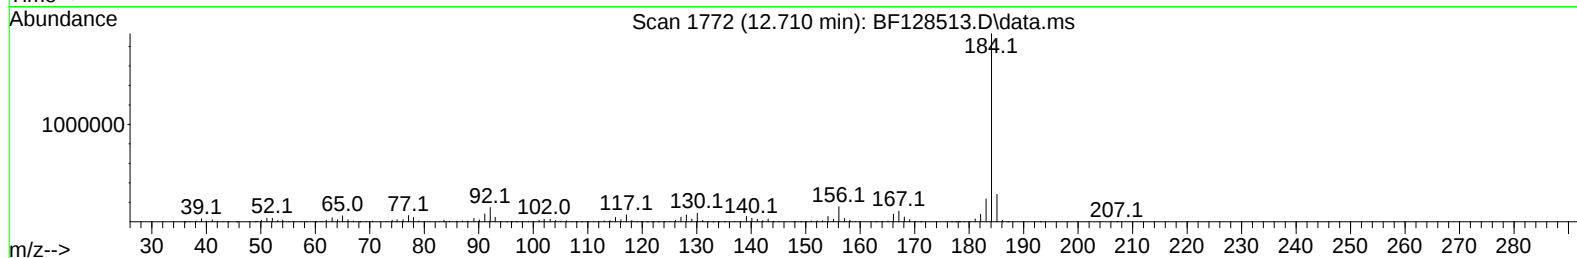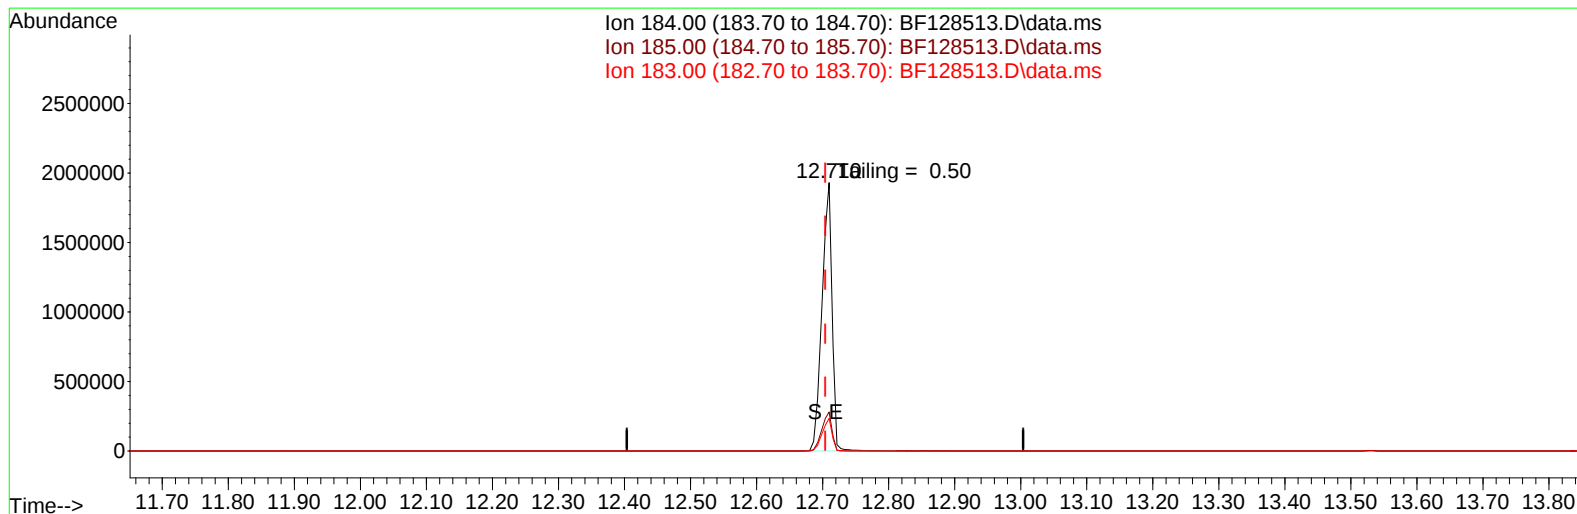

TIC: BF128513.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 61553.08 ng

response 2048711

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.55
183.00	11.60	12.18
0.00	0.00	0.00