
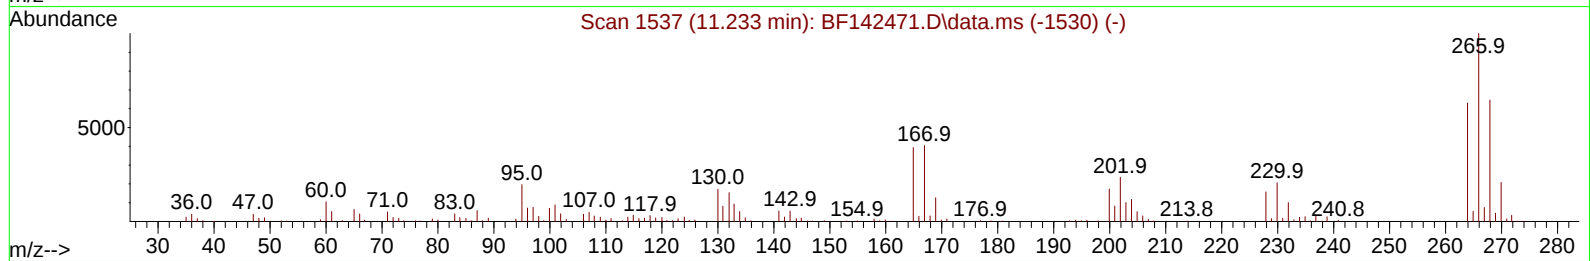
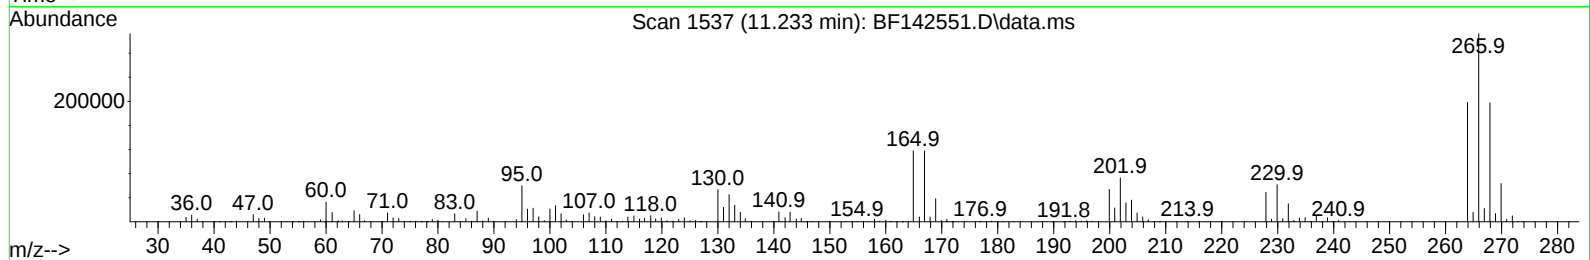


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052725\
Data File : BF142551.D
Acq On : 27 May 2025 09:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 11:46:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

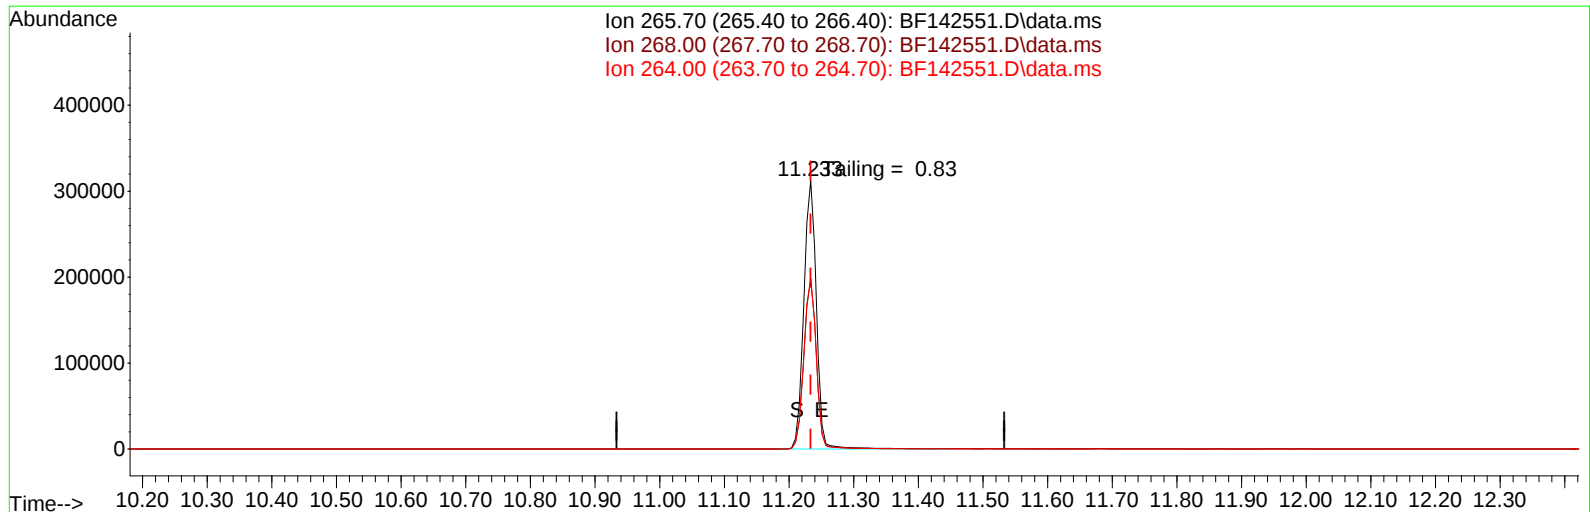

TIC: BF142551.D\data.ms

(70) Pentachlorophenol (C)




11.233min (+ 0.000) 96217.29 ng

response 423416

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	63.31
264.00	63.00	63.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052725\
Data File : BF142551.D
Acq On : 27 May 2025 09:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 27 11:46:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

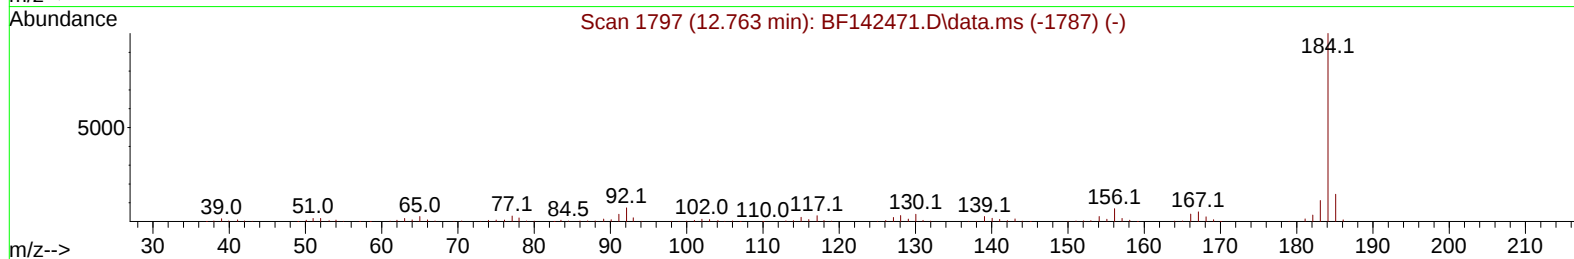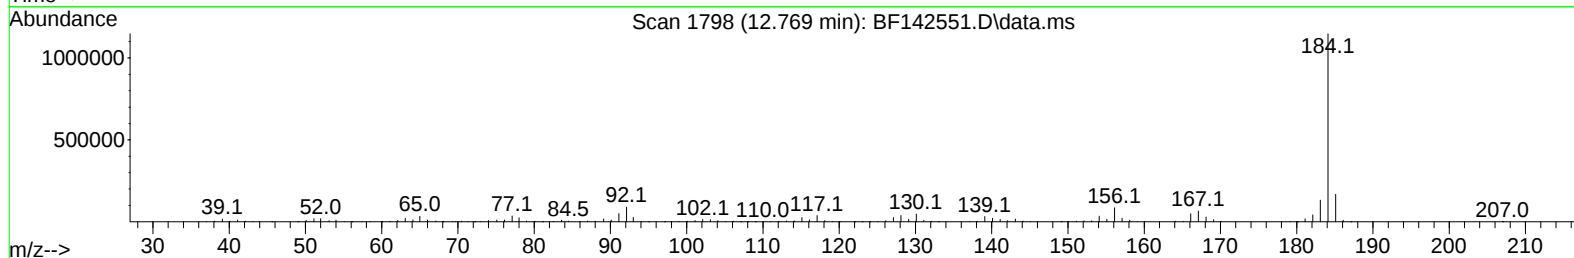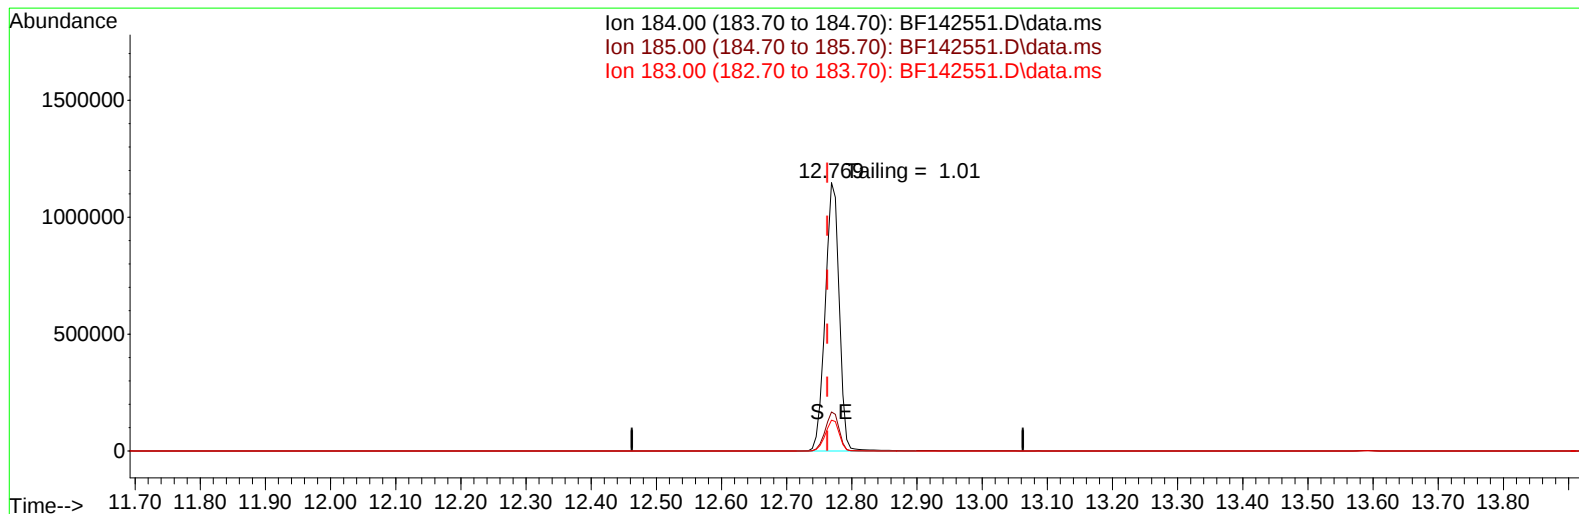

TIC: BF142551.D\data.ms

(77) Benzidine

12.769min (+ 0.006) 104012.72 ng

response 1726299

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.55
183.00	11.20	11.51
0.00	0.00	0.00