
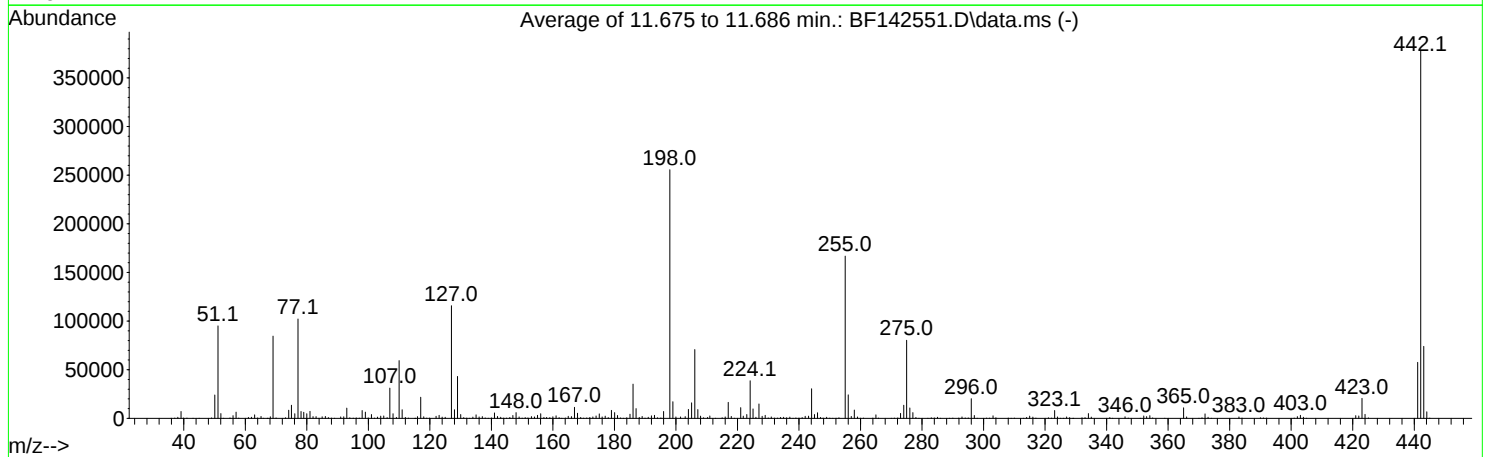


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052725\
Data File : BF142551.D
Acq On : 27 May 2025 09:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue May 20 16:26:47 2025

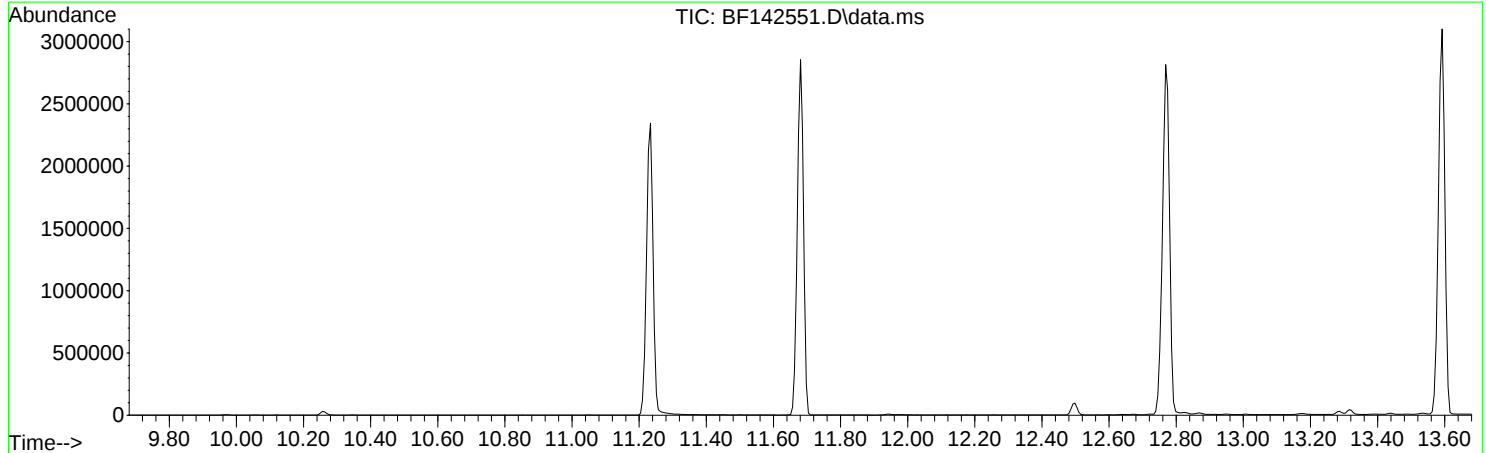




AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	95056	PASS
68	69	0.00	2	1.9	1592	PASS
69	198	0.00	100	33.1	84611	PASS
70	69	0.00	2	0.5	456	PASS
127	198	10	80	45.3	115752	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	255659	PASS
199	198	5	9	6.7	17178	PASS
275	198	10	60	31.4	80216	PASS
365	198	1	100	4.2	10786	PASS
441	198	0.01	100	22.5	57517	PASS
442	442	50	100	100.0	378197	PASS
443	442	15	24	19.6	73995	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052725\
Data File : BF142551.D
Acq On : 27 May 2025 09:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 27 11:46:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

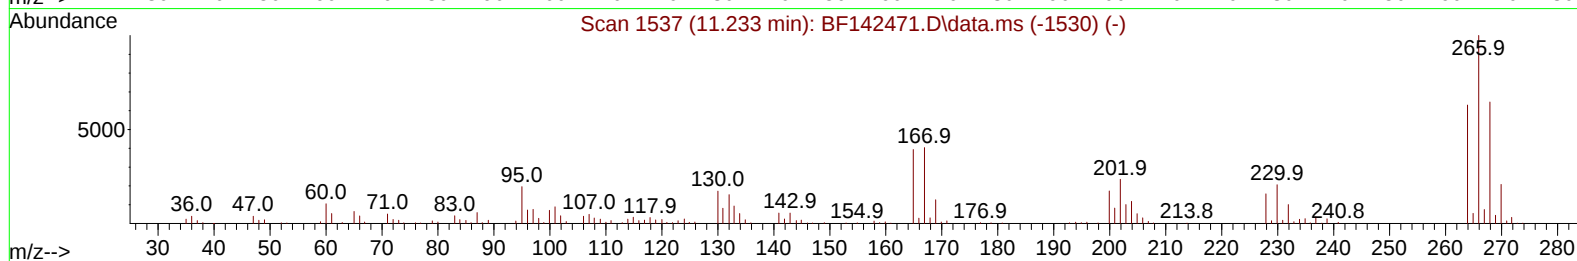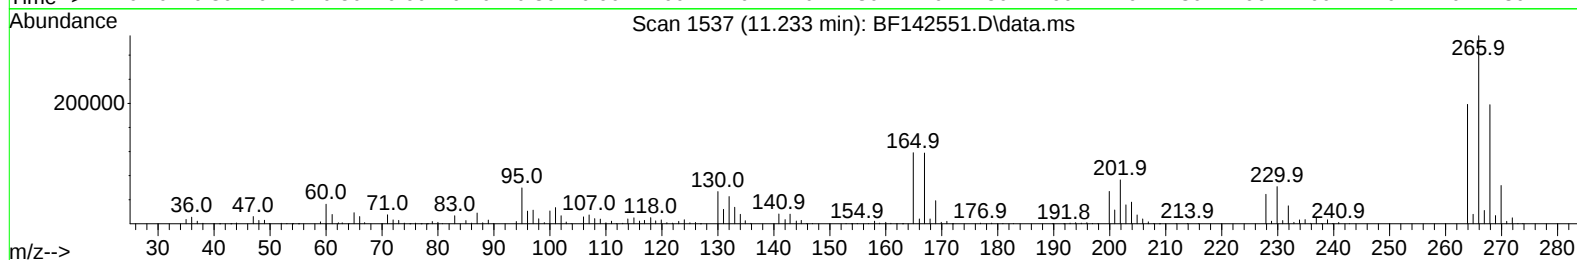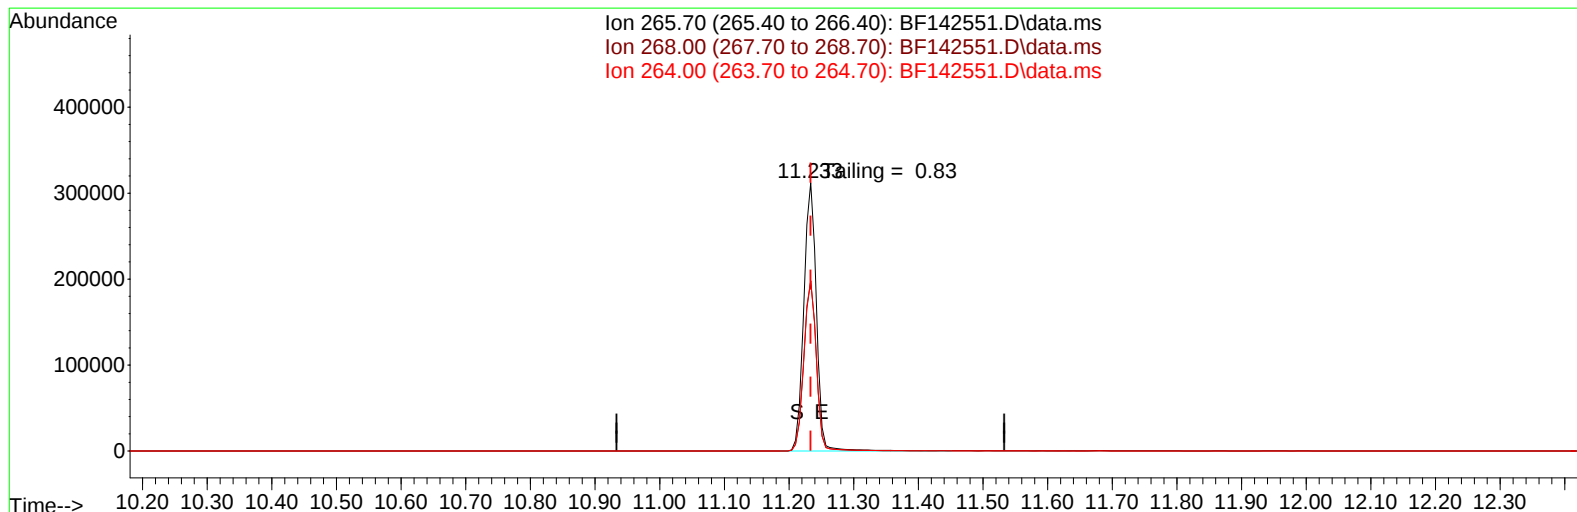

TIC: BF142551.D\data.ms

(70) Pentachlorophenol (C)

11.233min (+ 0.000) 96217.29 ng




response 423416

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	63.31
264.00	63.00	63.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052725\
Data File : BF142551.D
Acq On : 27 May 2025 09:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 27 11:46:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 20 16:26:47 2025
Response via : Initial Calibration

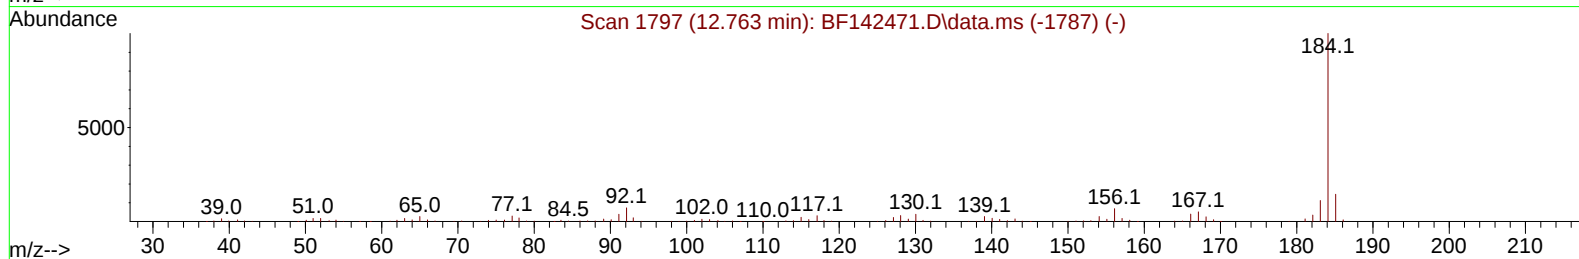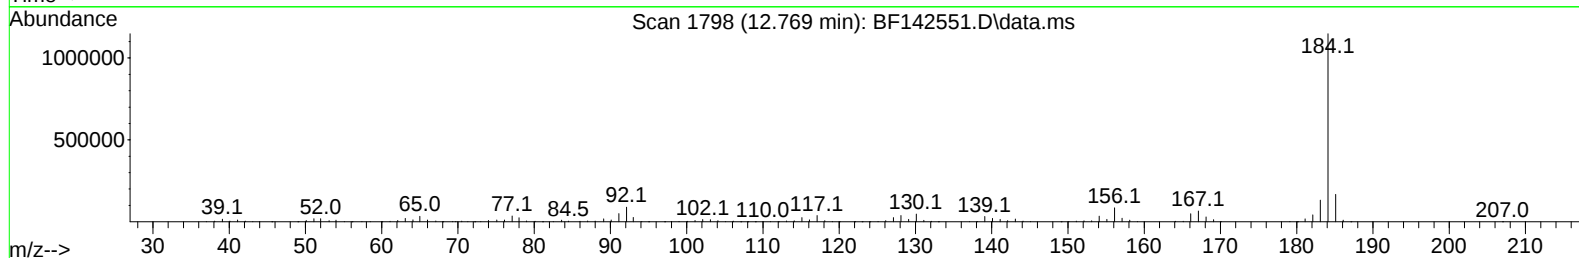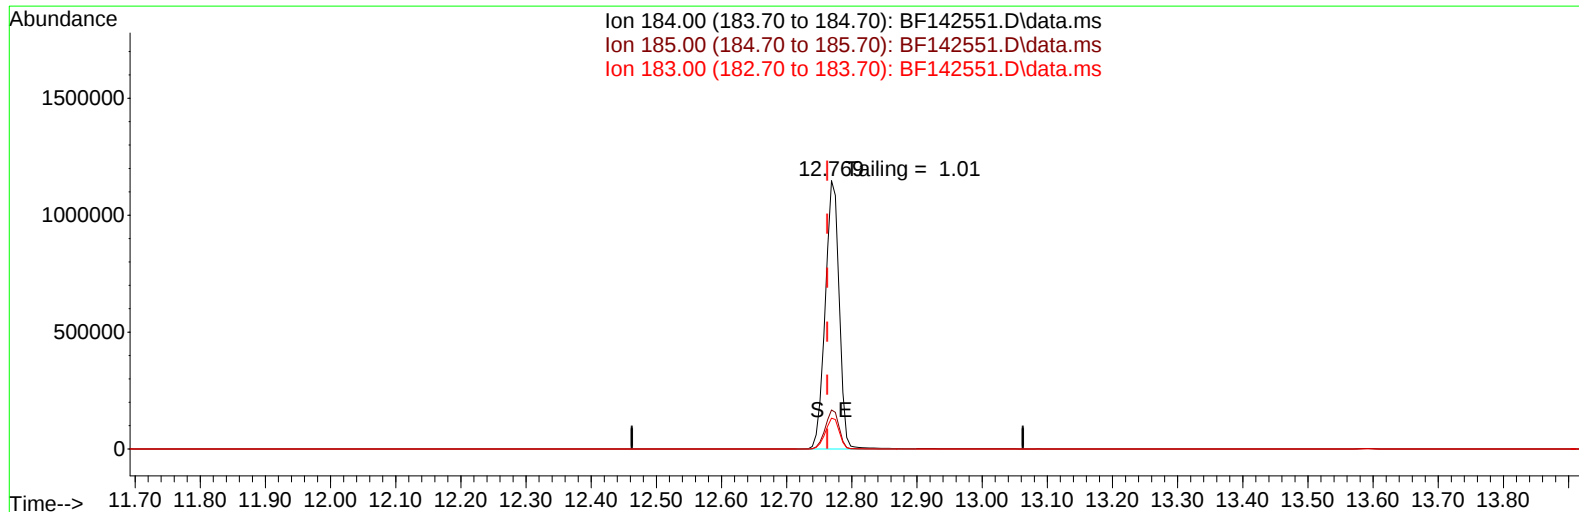

TIC: BF142551.D\data.ms

(77) Benzidine

12.769min (+ 0.006) 104012.72 ng

response 1726299

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.55
183.00	11.20	11.51
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/27/2025	BNA_F	<u>BF142551.D</u>
Compound Name	Response	Retention Time
DDT	843656	13.592
DDD	17595	13.316
DDE	1003	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18598	862254	2.16

Instrument :
BNA_F
ClientSampleId :
DFTPP