


Data Path : Z:\HPCHEM1\BNA F\Data\BF052815\
 Data File : BF079540.D
 Acq On : 28 May 2015 12:25
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 28 18:41:08 2015

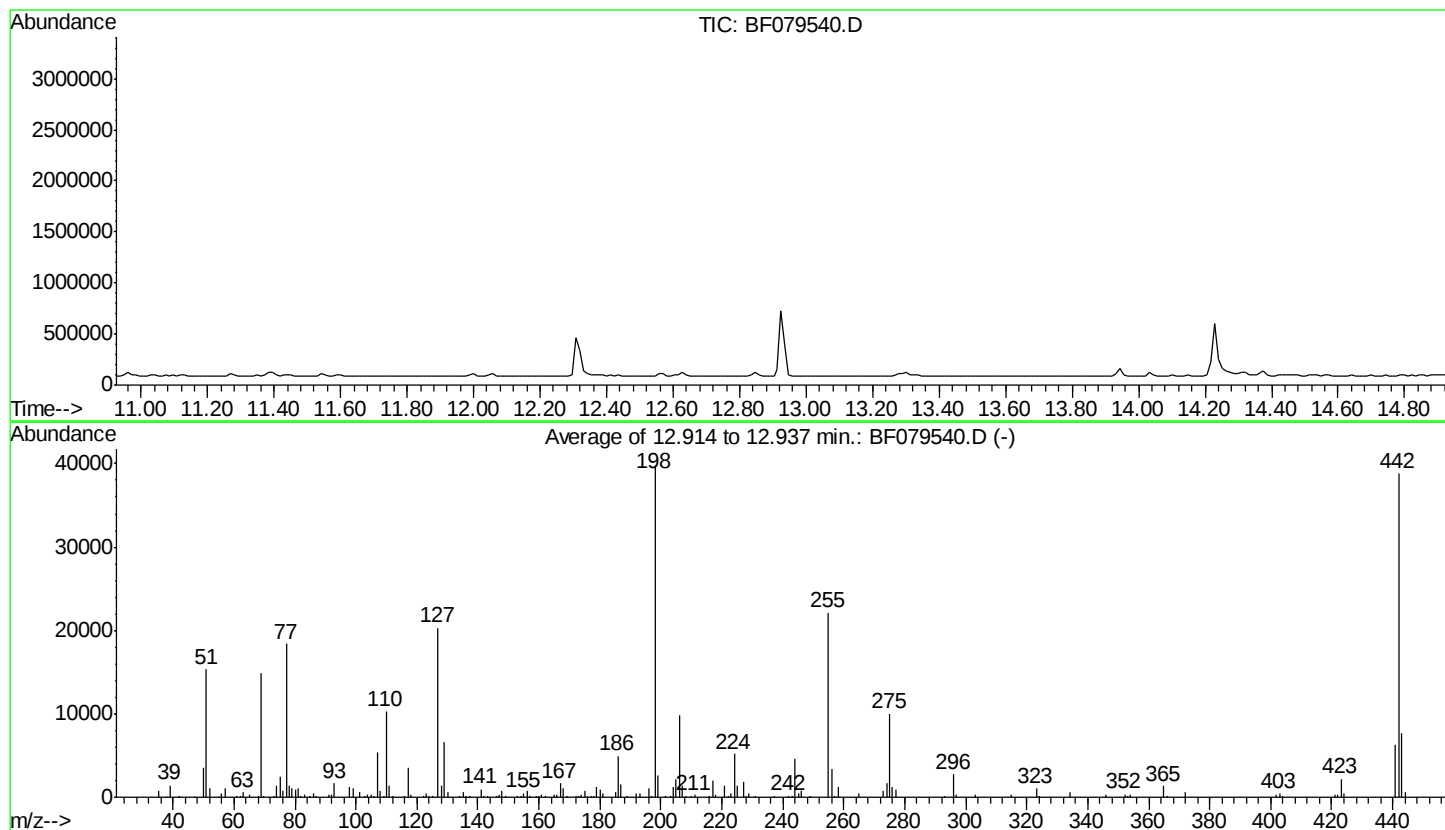

AutoFind: Scans 1026, 1027, 1028; Background Corrected with Scan 1023

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	15293	PASS
68	69	0.00	2	1.2	185	PASS
69	198	0.00	100	37.5	14913	PASS
70	69	0.00	2	0.9	141	PASS
127	198	10	80	51.1	20315	PASS
197	198	0.00	2	0.4	166	PASS
198	198	100	100	100.0	39763	PASS
199	198	5	9	6.6	2618	PASS
275	198	10	60	25.3	10041	PASS
365	198	1	100	3.4	1352	PASS
441	442	0.01	24	16.1	6240	PASS
442	198	50	100	97.5	38764	PASS
443	442	15	24	19.7	7633	PASS