
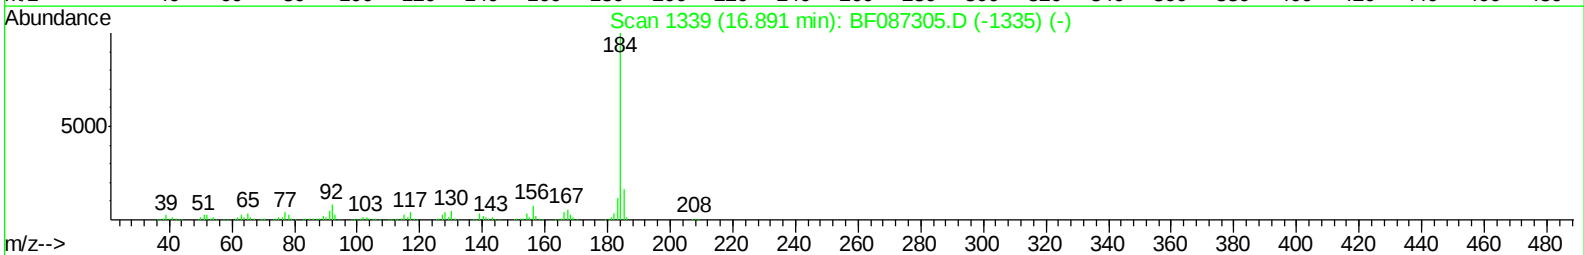
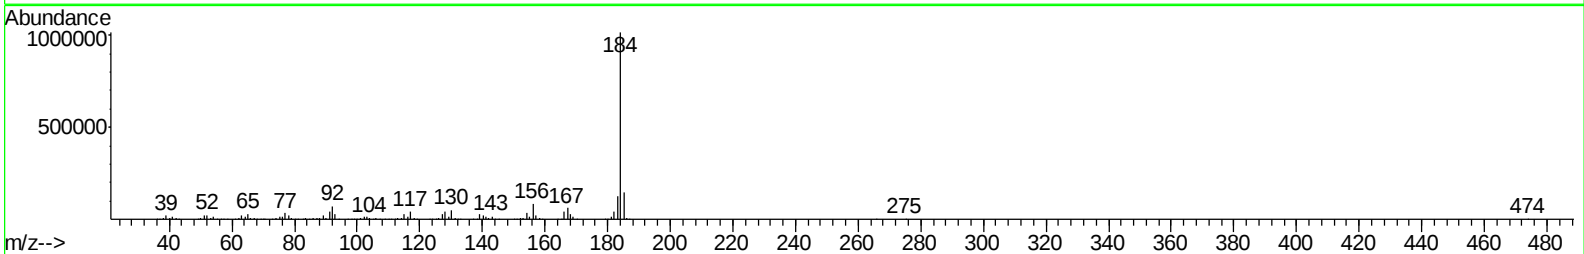


```
Data Path : Z:\HPCHEM1\BNA_F\Data\BF052816\  
Data File : BF087499.D  
Acq On    : 29 May 2016    2:36  
Operator  : UM/SJ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: May 30 05:12:11 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 16:26:52 2016
Response via : Initial Calibration

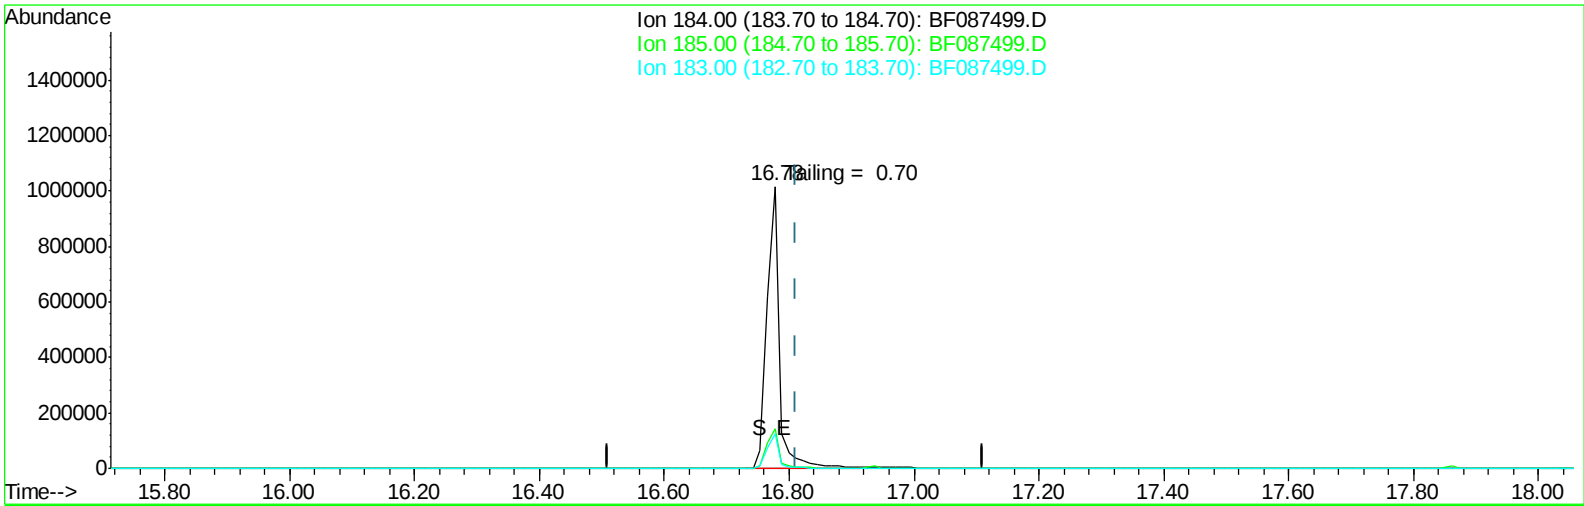

TIC: BF087499.D

(76) Benzidine




16.777min (-0.034) 0.00ng

```
response 1411228
```

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.17
183.00	12.20	12.39
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF052816\
Data File : BF087499.D
Acq On : 29 May 2016 2:36
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 05:12:11 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 16:26:52 2016
Response via : Initial Calibration

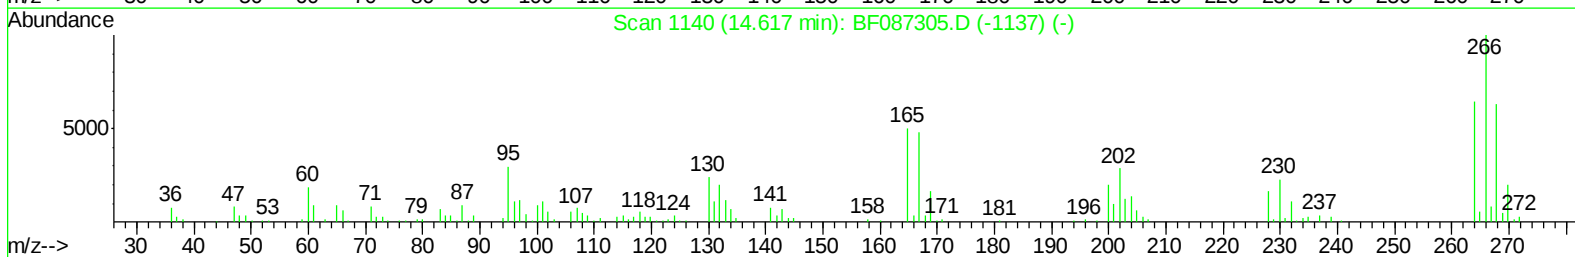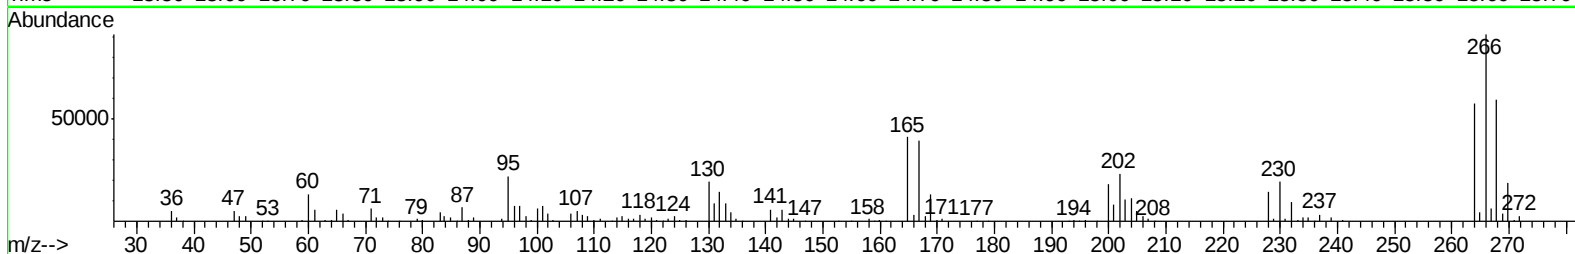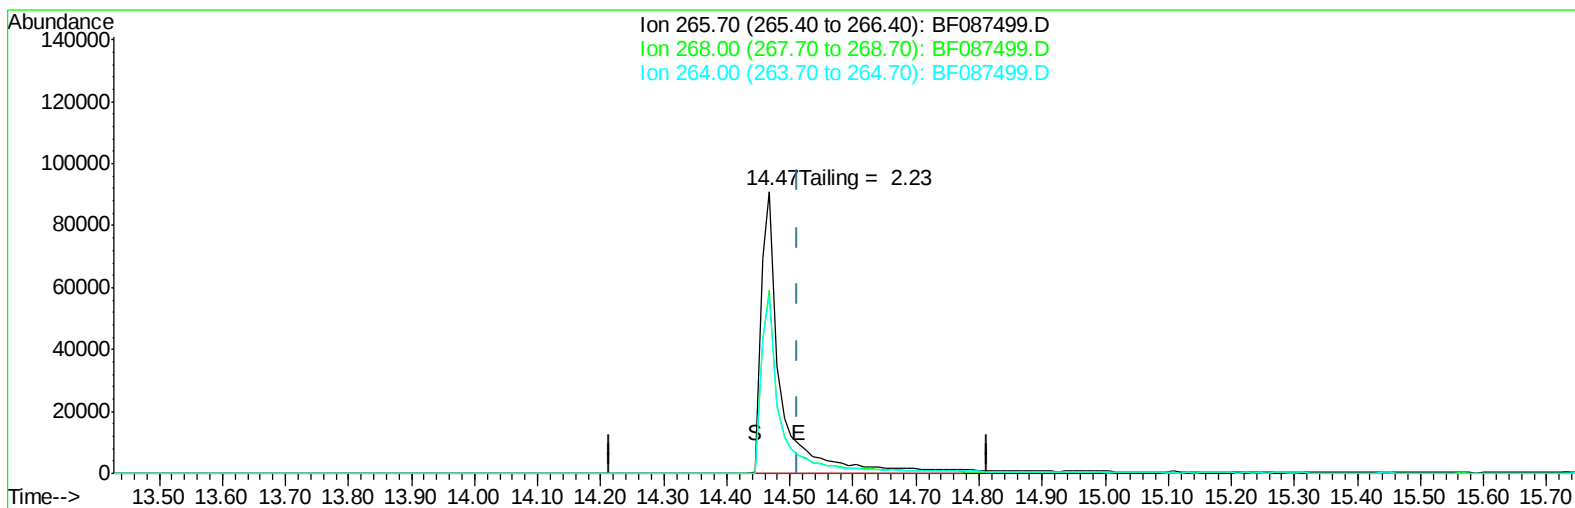

TIC: BF087499.D

(69) Pentachlorophenol (C)

14.468min (-0.046) 0.00ng

response 199379

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	65.10
264.00	66.10	63.18
0.00	0.00	0.00