

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052816\
 Data File : BF087481.D
 Acq On : 28 May 2016 15:56
 Operator : UM/SJ
 Sample : PB90943TB
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB90943TB

Quant Time: May 30 03:29:05 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 30 03:25:10 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	110217	20.00	ng	-0.01
21) Naphthalene-d8	9.50	136	454342	20.00	ng	-0.01
38) Acenaphthene-d10	12.32	164	218473	20.00	ng	-0.01
63) Phenanthrene-d10	14.72	188	433300	20.00	ng	-0.01
75) Chrysene-d12	18.43	240	361708	20.00	ng	0.00
86) Perylene-d12	20.10	264	227339	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	671950	107.13	ng	0.01
7) Phenol-d6	7.02	99	917877	108.30	ng	-0.02
23) Nitrobenzene-d5	8.38	82	574988	63.78	ng	-0.02
41) 2,4,6-Tribromophenol	13.62	330	191646	91.28	ng	-0.01
44) 2-Fluorobiphenyl	11.27	172	1009688	65.15	ng	-0.02
78) Terphenyl-d14	17.09	244	1033309	60.73	ng	0.00


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052816\
Data File : BF087481.D
Acq On : 28 May 2016 15:56
Operator : UM/SJ
Sample : PB90943TB
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB90943TB

Quant Time: May 30 03:29:05 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 30 03:25:10 2016
Response via : Initial Calibration

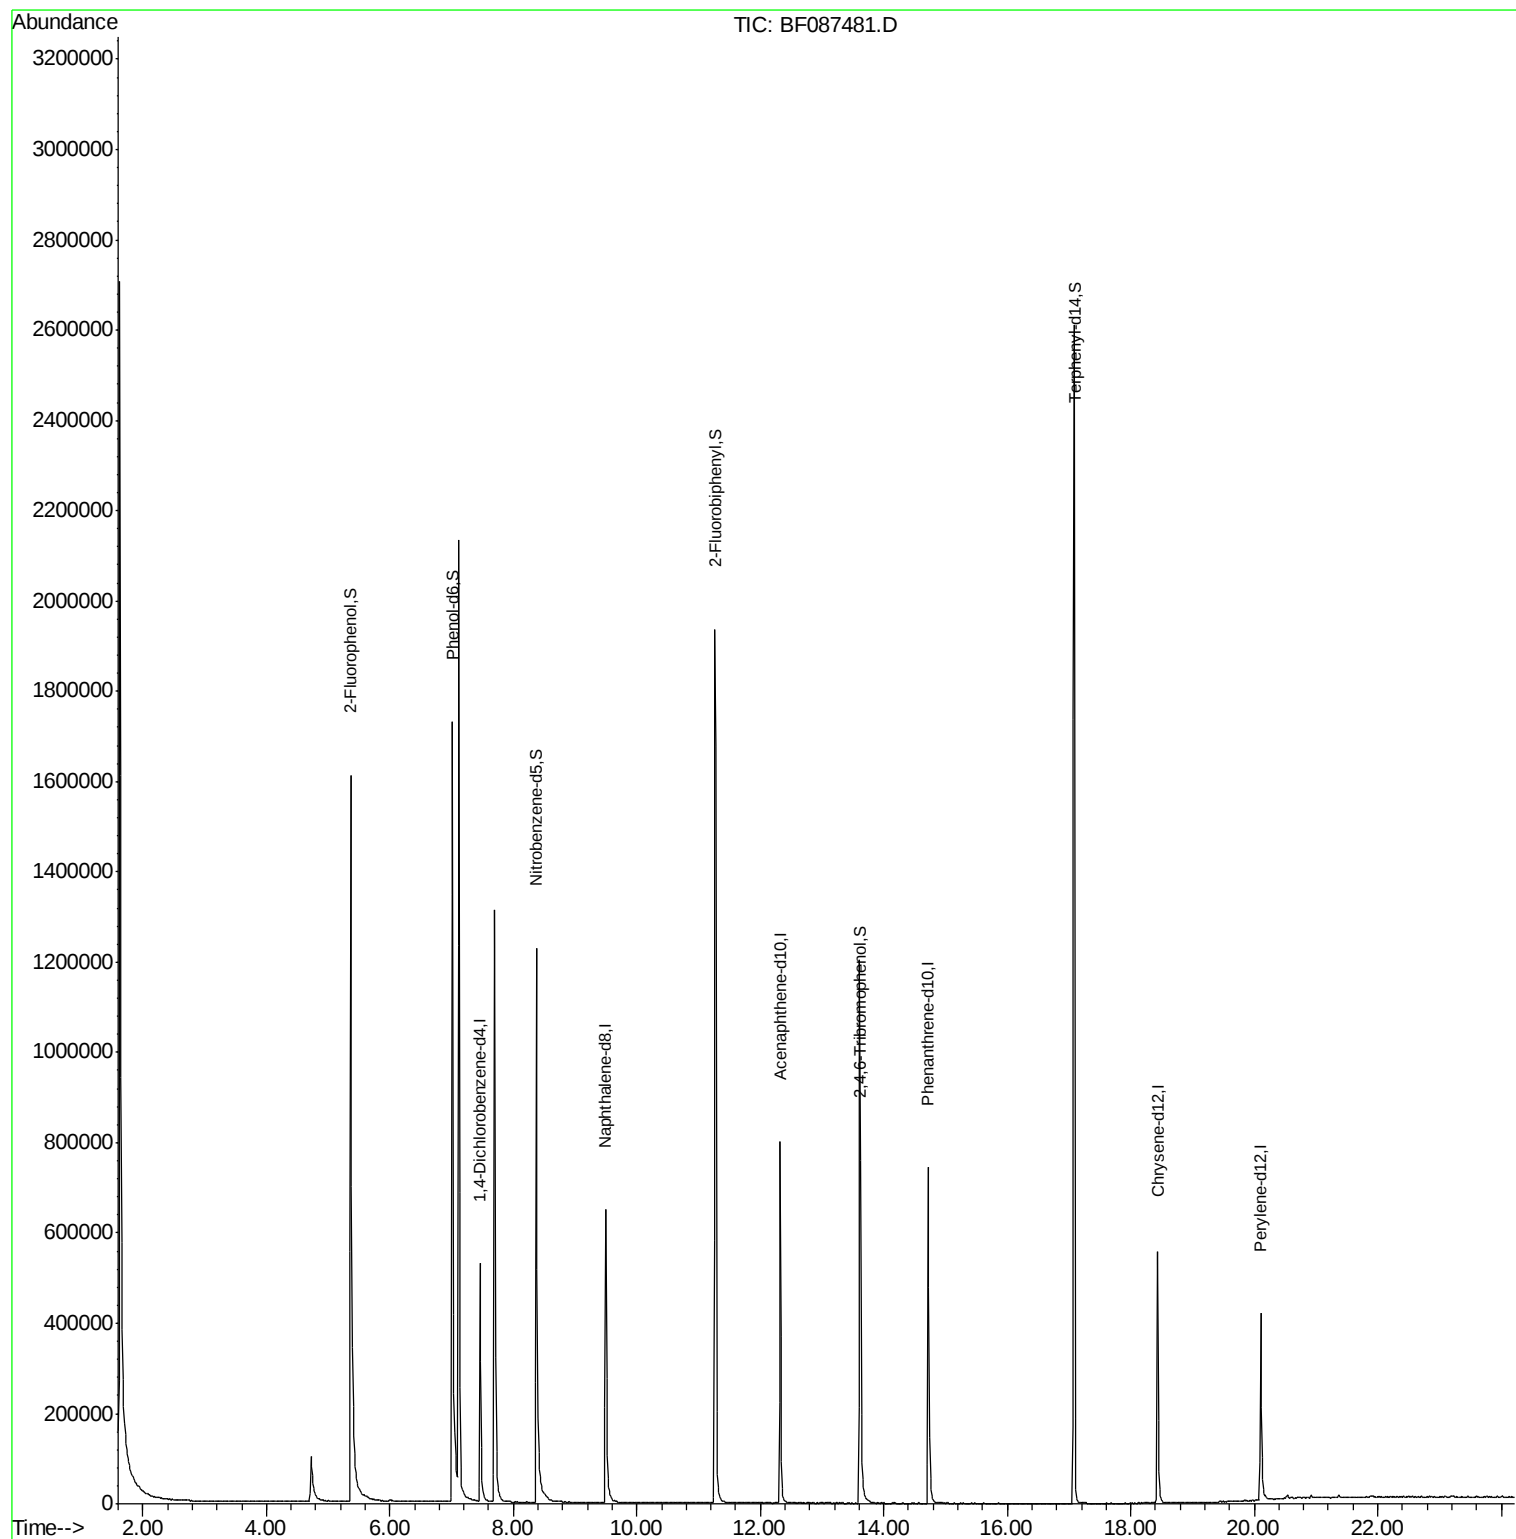




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.46 min Scan# 514
Delta R.T. -0.01 min
Lab File: BF087481.D
Acq: 28 May 2016 15:56

Instrument :
BNA_F
ClientSampleId :
PB90943TB

Tgt Ion:152 Resp: 110217
Ion Ratio Lower Upper
152 100
150 155.3 125.8 188.6
115 69.7 51.5 77.3

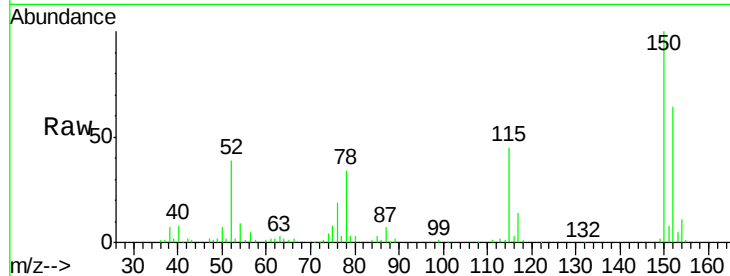


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

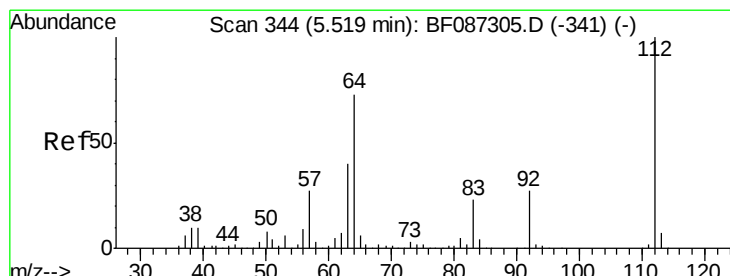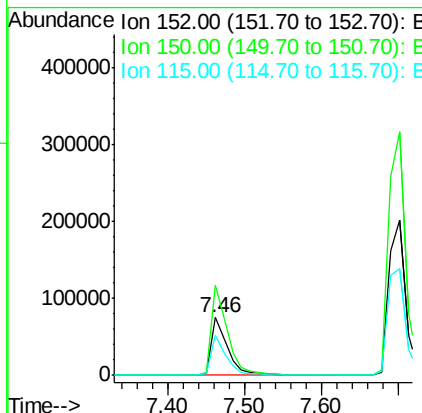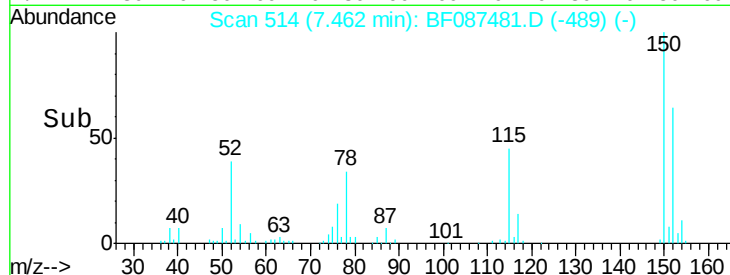



#5


2-Fluorophenol
Concen: 107.13 ng
RT: 5.37 min Scan# 331
Delta R.T. 0.01 min
Lab File: BF087481.D
Acq: 28 May 2016 15:56

Tgt Ion:112 Resp: 671950
Ion Ratio Lower Upper
112 100
64 70.8 52.1 78.1
63 39.8 25.7 38.5#

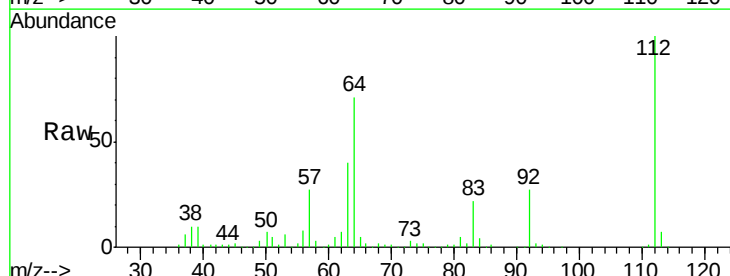

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

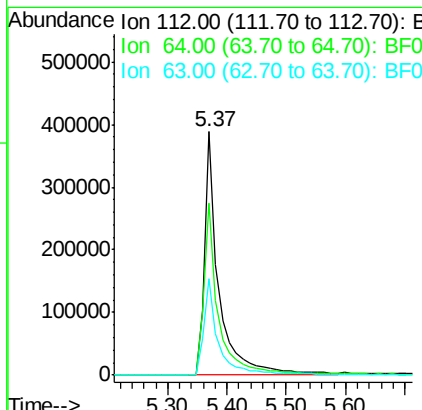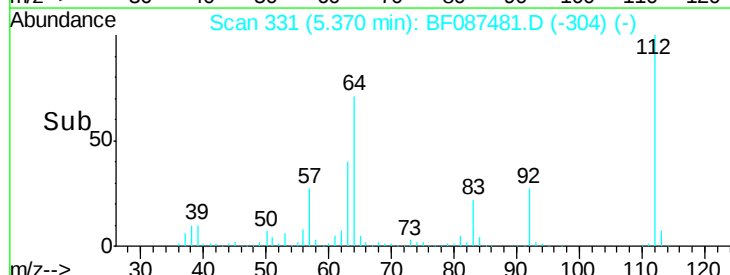

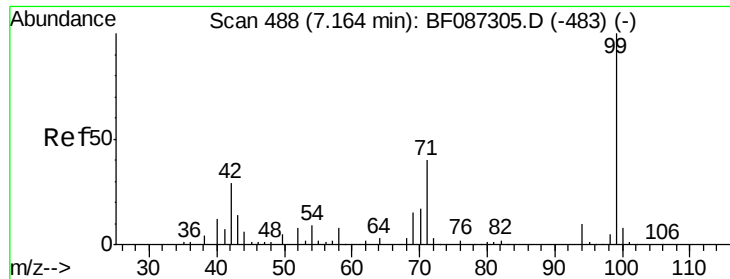

#7

Phenol-d6

Concen: 108.30 ng

RT: 7.02 min Scan# 475

Delta R.T. -0.02 min

Lab File: BF087481.D

Acq: 28 May 2016 15:56

Instrument :

BNA_F

ClientSampleId :

PB90943TB


Tgt Ion: 99 Resp: 917877

Ion Ratio Lower Upper

99 100

42 27.0 13.6 20.4#




71 38.2 24.6 36.8#

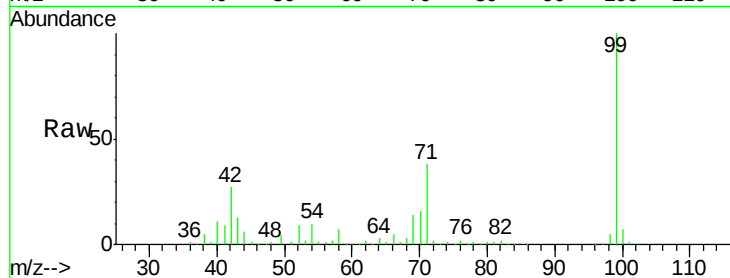

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

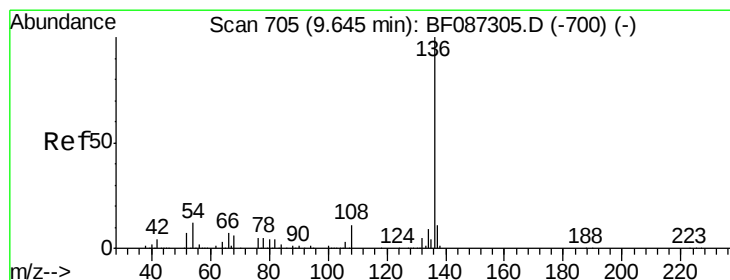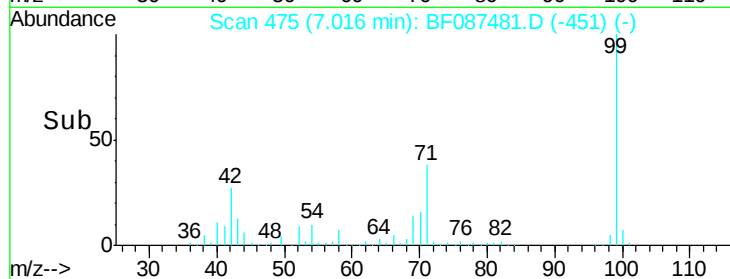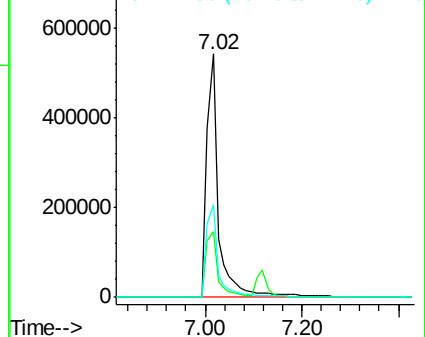

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.50 min Scan# 692

Delta R.T. -0.01 min

Lab File: BF087481.D

Acq: 28 May 2016 15:56

Tgt Ion: 136 Resp: 454342


Ion Ratio Lower Upper

136 100

137 10.8 8.8 13.2

54 10.9 5.0 7.4#

68 5.4 4.4 6.6


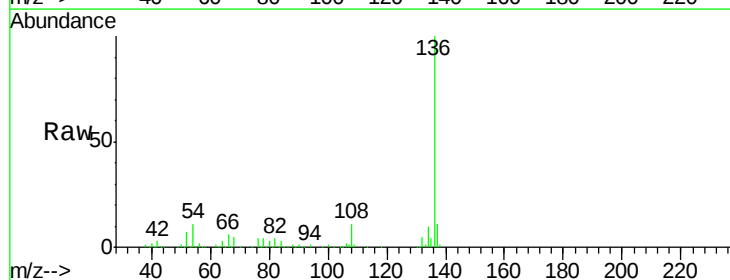



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



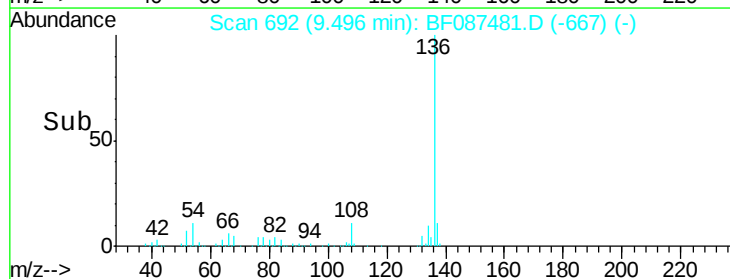
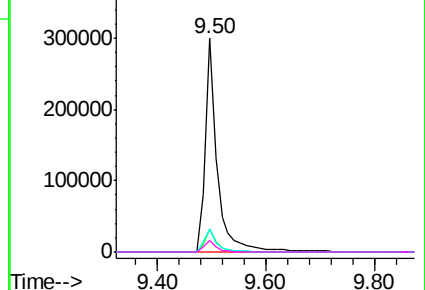


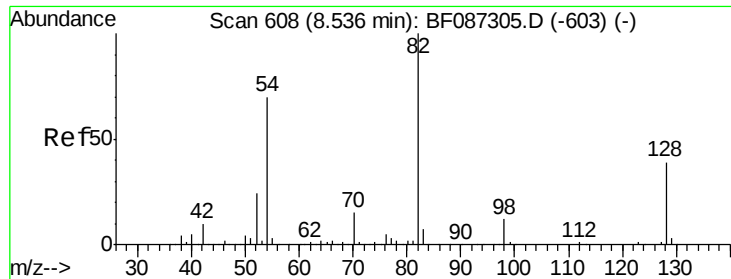

#23
 Nitrobenzene-d5
 Concen: 63.78 ng
 RT: 8.38 min Scan# 594
 Delta R.T. -0.02 min
 Lab File: BF087481.D
 Acq: 28 May 2016 15:56




Instrument :
 BNA_F
 ClientSampleId :
 PB90943TB


Tgt Ion: 82 Resp: 574988
 Ion Ratio Lower Upper
 82 100
 128 38.0 40.6 61.0#
 54 71.4 38.1 57.1#

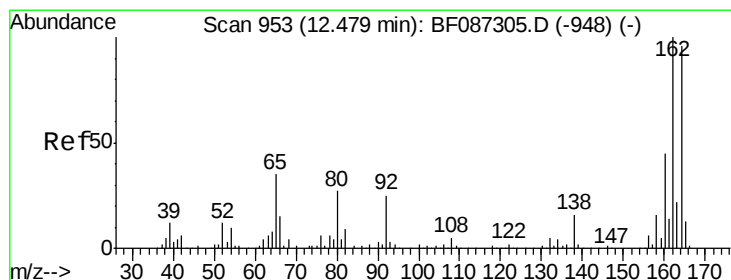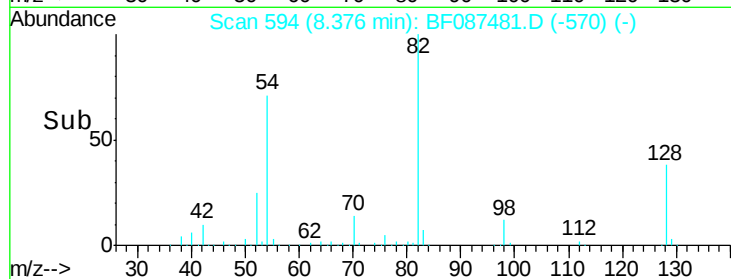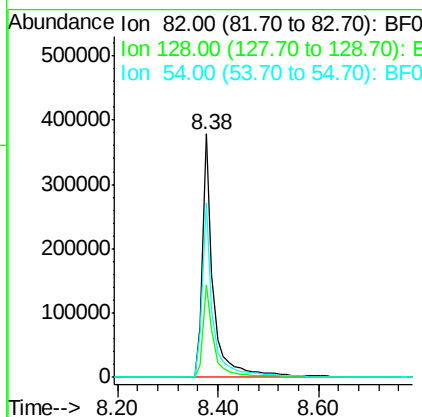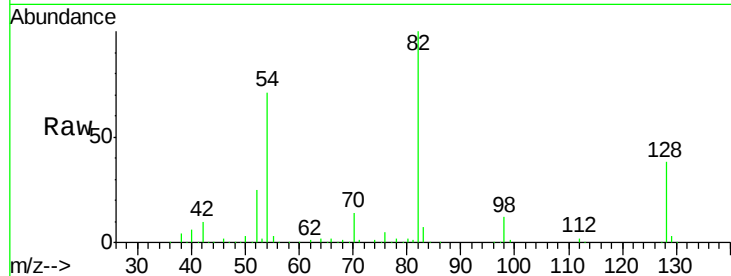

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 12.32 min Scan# 939
 Delta R.T. -0.01 min
 Lab File: BF087481.D
 Acq: 28 May 2016 15:56

Tgt Ion: 164 Resp: 218473
 Ion Ratio Lower Upper
 164 100
 162 102.3 82.8 124.2
 160 47.4 36.9 55.3

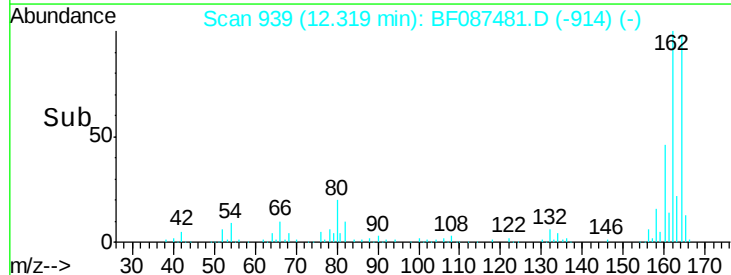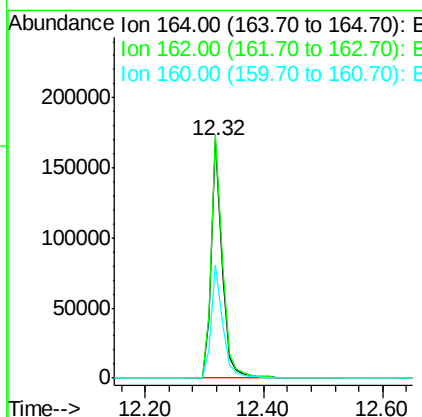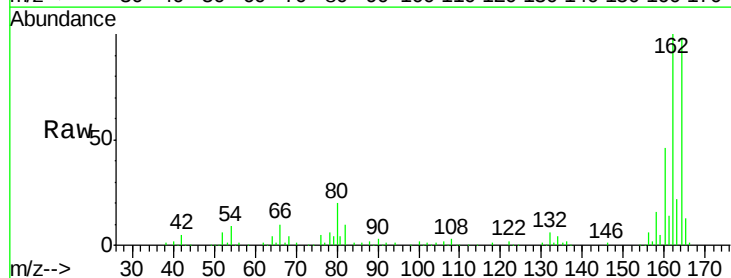


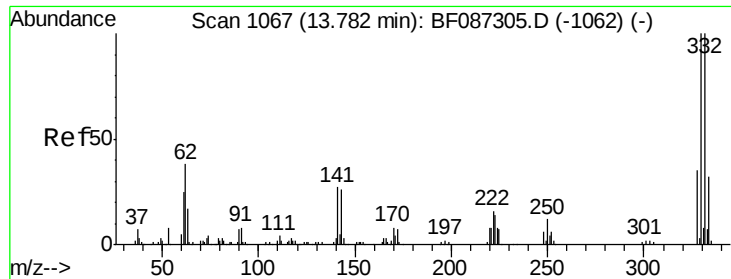




#41
 2,4,6-Tribromophenol
 Concen: 91.28 ng
 RT: 13.62 min Scan# 1053
 Delta R.T. -0.01 min
 Lab File: BF087481.D
 Acq: 28 May 2016 15:56

Instrument :
 BNA_F
 ClientSampleId :
 PB90943TB

Tgt Ion:330 Resp: 191646
 Ion Ratio Lower Upper
 330 100
 332 96.7 79.0 118.4
 141 43.7 31.2 46.8

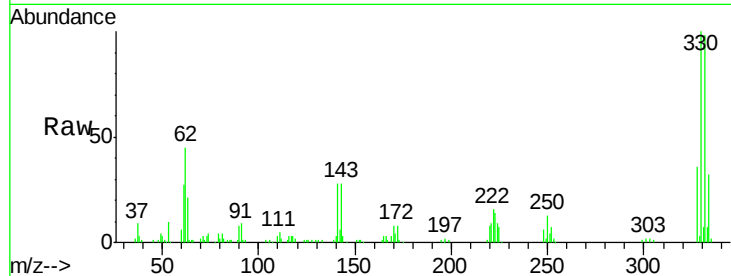


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

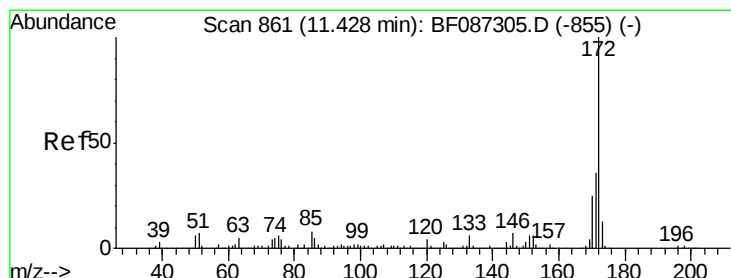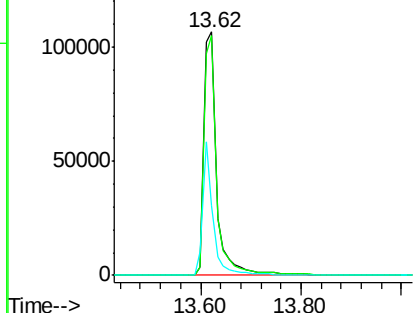
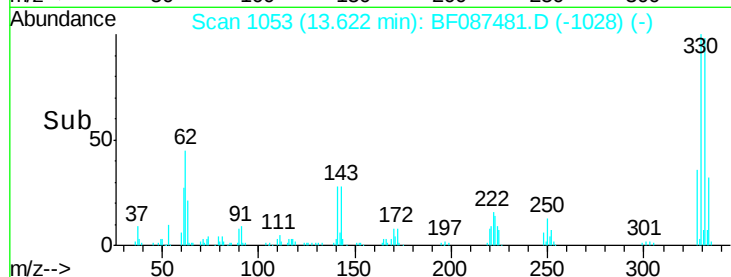



#44
 2-Fluorobiphenyl
 Concen: 65.15 ng
 RT: 11.27 min Scan# 847
 Delta R.T. -0.02 min
 Lab File: BF087481.D
 Acq: 28 May 2016 15:56

Tgt Ion:172 Resp: 1009688
 Ion Ratio Lower Upper
 172 100
 171 35.4 29.0 43.6
 170 23.8 19.8 29.8

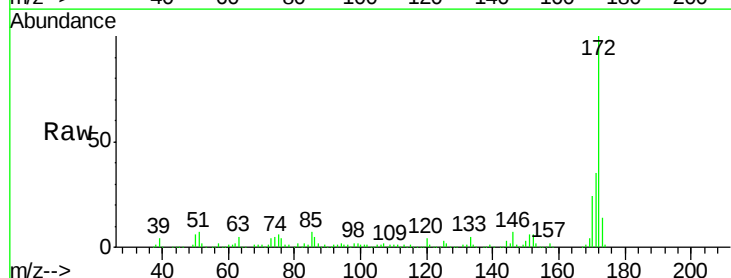

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

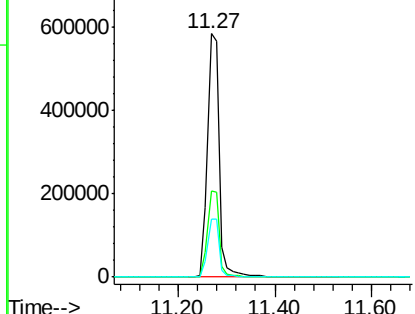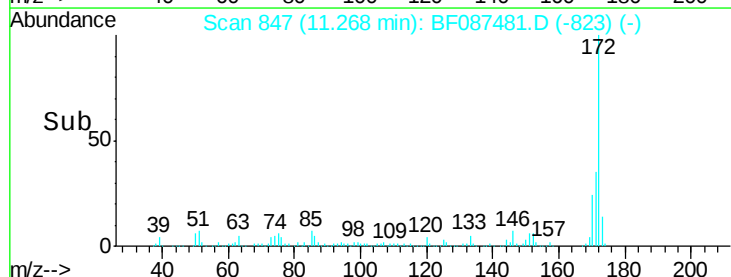


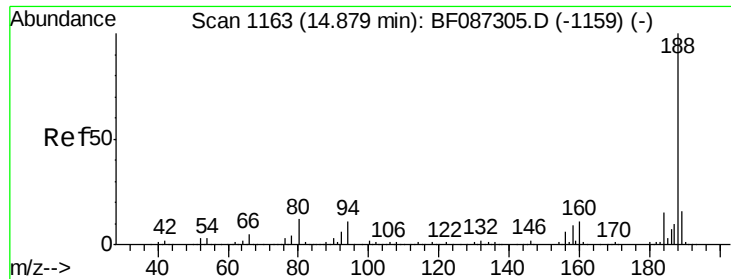




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 14.72 min Scan# 1149
Delta R.T. -0.01 min
Lab File: BF087481.D
Acq: 28 May 2016 15:56

Instrument :
BNA_F
ClientSampleId :
PB90943TB

Tgt Ion:188 Resp: 433300
Ion Ratio Lower Upper
188 100
94 10.5 6.8 10.2#
80 11.4 7.1 10.7#

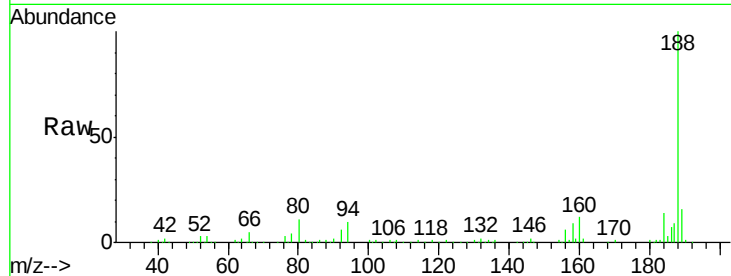


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

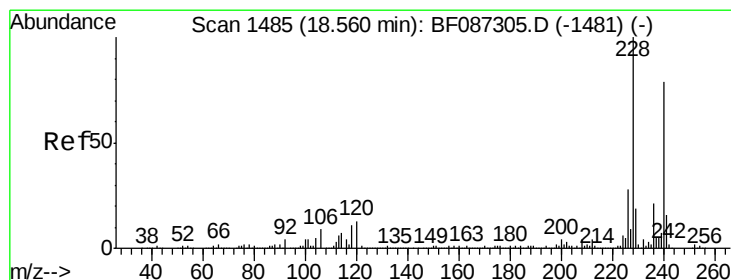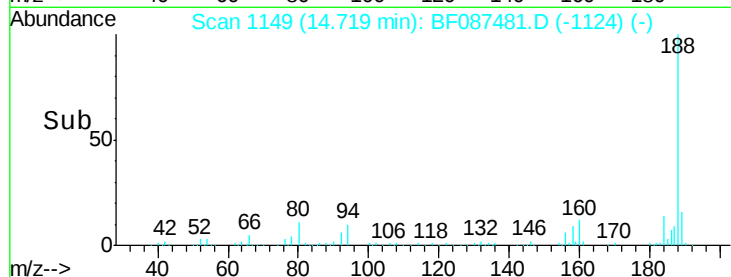
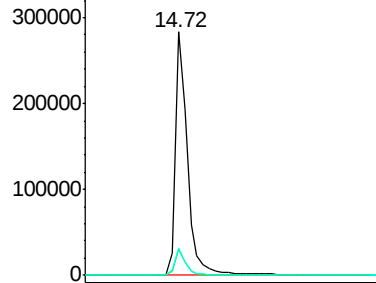


#75
Chrysene-d12
Concen: 20.00 ng
RT: 18.43 min Scan# 1474
Delta R.T. -0.00 min
Lab File: BF087481.D
Acq: 28 May 2016 15:56

Tgt Ion:240 Resp: 361708
Ion Ratio Lower Upper
240 100
120 9.0 11.2 16.8#
236 26.0 21.2 31.8

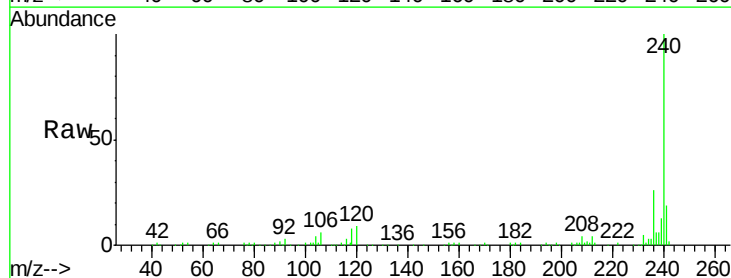

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

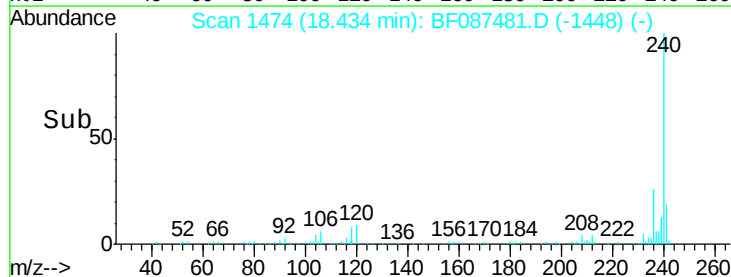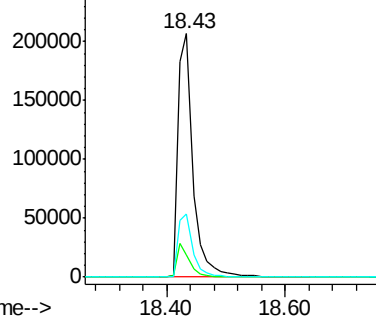



#78

Terphenyl-d14

Concen: 60.73 ng

RT: 17.09 min Scan# 1356

Delta R.T. -0.00 min

Lab File: BF087481.D

Acq: 28 May 2016 15:56

Instrument :

BNA_F

ClientSampleId :

PB90943TB


Tgt Ion:244 Resp: 1033309

Ion Ratio Lower Upper




244 100

212 7.8 6.2 9.2

122 9.7 12.0 18.0#

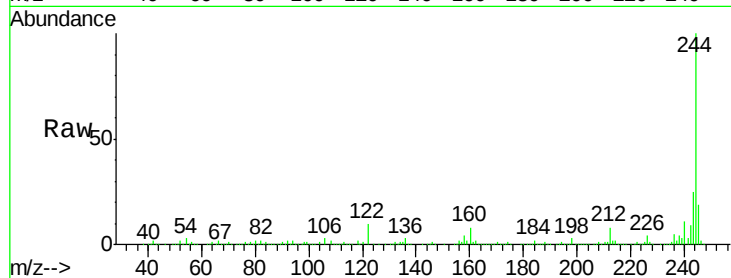

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

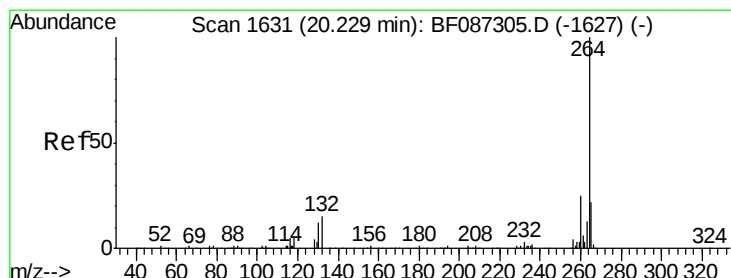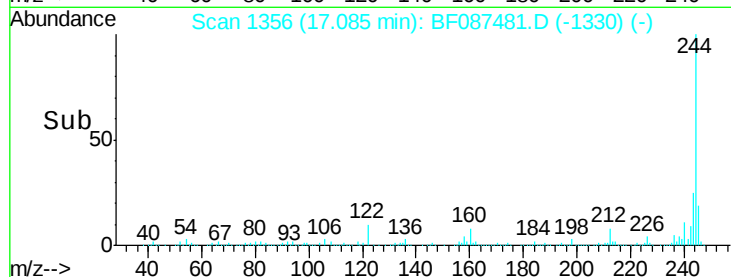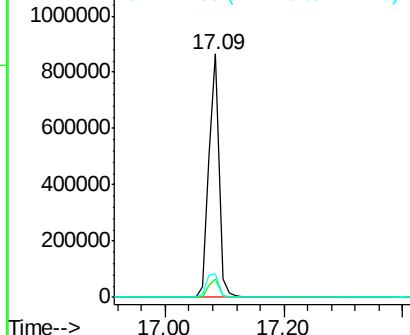

#86

Perylene-d12

Concen: 20.00 ng

RT: 20.10 min Scan# 1620

Delta R.T. -0.00 min

Lab File: BF087481.D

Acq: 28 May 2016 15:56


Tgt Ion:264 Resp: 227339

Ion Ratio Lower Upper

264 100

260 24.2 19.5 29.3

265 21.9 17.3 25.9

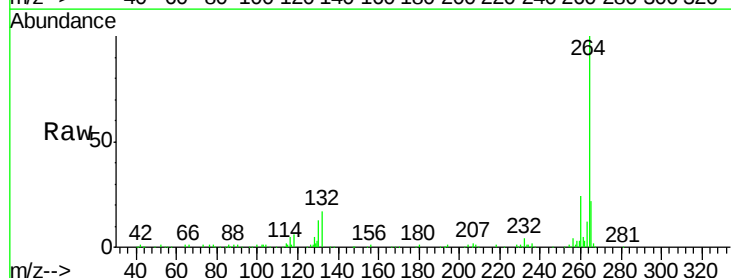

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

