

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052816\
 Data File : BF087495.D
 Acq On : 29 May 2016 00:03
 Operator : UM/SJ
 Sample : H3276-08
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-06


Quant Time: May 30 04:04:21 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 30 03:48:52 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	110900	20.00	ng	-0.01
21) Naphthalene-d8	9.50	136	452508	20.00	ng	-0.01
38) Acenaphthene-d10	12.32	164	20484			

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052816\
Data File : BF087495.D
Acq On : 29 May 2016 00:03
Operator : UM/SJ
Sample : H3276-08
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-06

Quant Time: May 30 04:04:21 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 30 03:48:52 2016
Response via : Initial Calibration

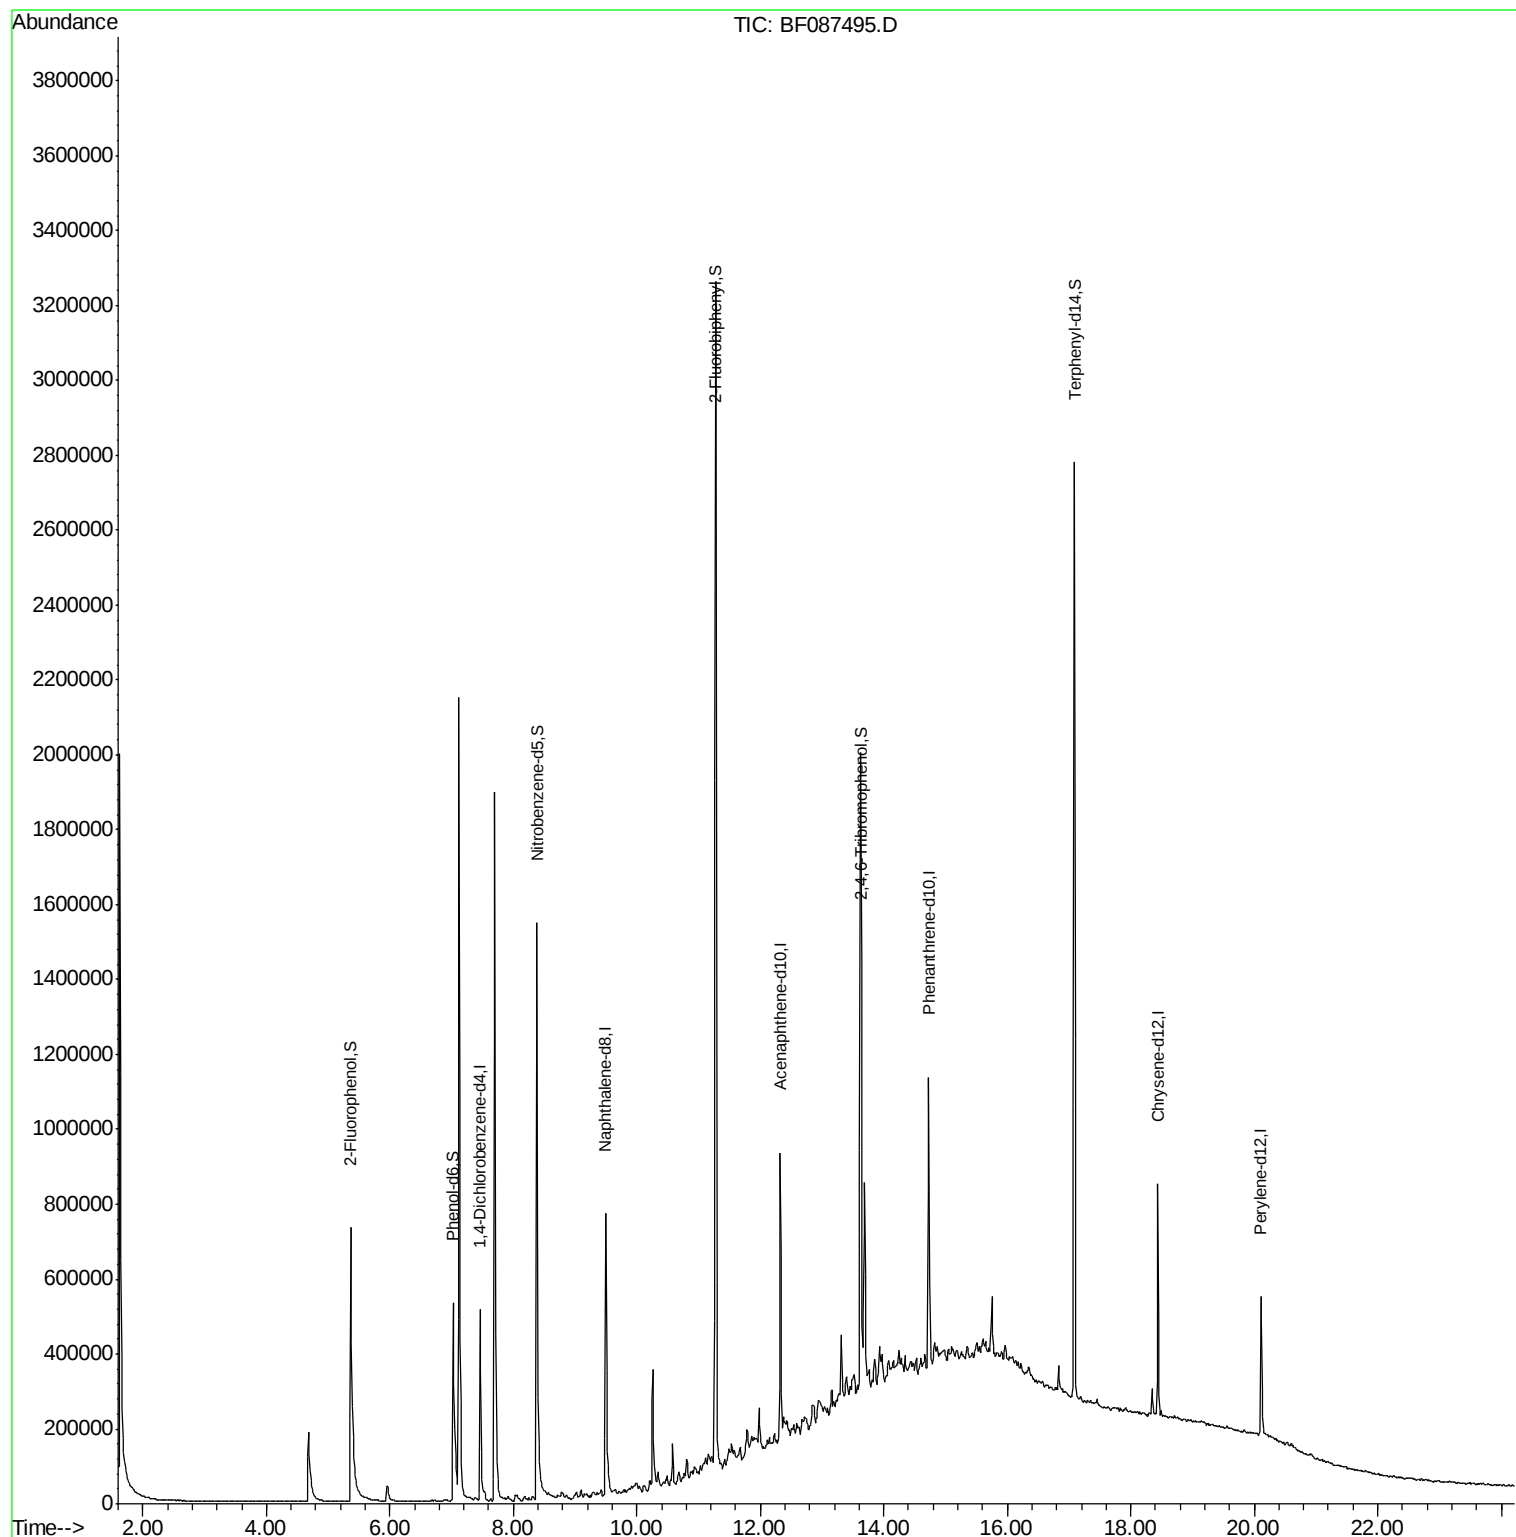



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.46 min Scan# 514

Delta R.T. -0.01 min

Lab File: BF087495.D

Acq: 29 May 2016 00:03

Instrument :

BNA_F

ClientSampleId :

MW-06

Tgt



#7

Phenol-d6

Concen: 41.33 ng

RT: 7.03 min Scan# 476

Delta R.T. -0.01 min

Lab File: BF087495.D

Acq: 29 May 2016 00:03

Instrument :


BNA_F




#23
 Nitrobenzene-d5
 Concen: 87.01 ng
 RT: 8.39 min Scan# 595
 Delta R.T. -0.01 min
 Lab File: BF087495.D
 Acq: 29 May 2016 00:03

Instrument :
 BNA_F
 ClientSampleId :
 MW-06

Tgt Ion: 82 Resp: 781193
 Ion Ratio Lower Upper
 82 100
 128 42.2 40.6 61.0
 54 66.6 38.1 57.1#

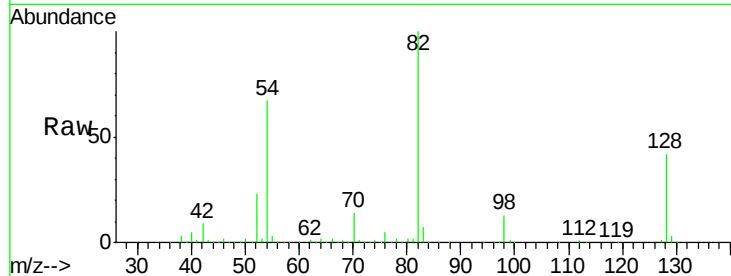

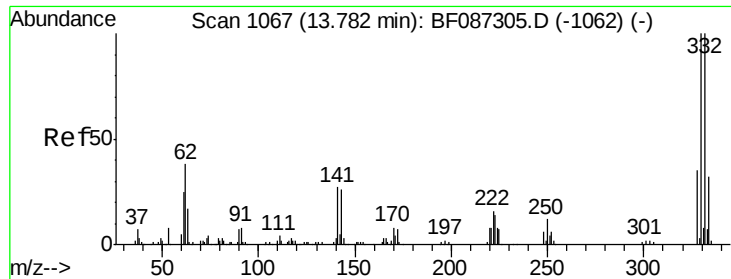

#41

2,4,6-Tribromophenol

Concen: 144.86 ng

RT: 13.63 min Scan# 1054


Delta R.T. 0.00 min

Lab File: BF087495.D

Acq: 29 May 2016 00:03

Instrument :


BNA_F

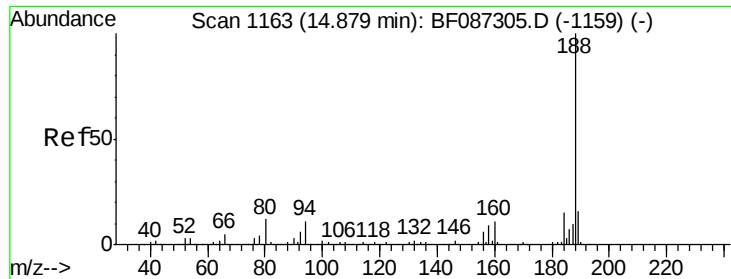


#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 14.73 min Scan# 1150
Delta R.T. 0.00 min
Lab File: BF087495.D
Acq: 29 May 2016 00:03

Instrument :
BNA_F
ClientSampleId :
MW-06

Tgt Ion:188 Resp: 381087
Ion Ratio Lower Upper
188 100
94 9.1 6.8 10.2
80 9.3 7.1 10.7

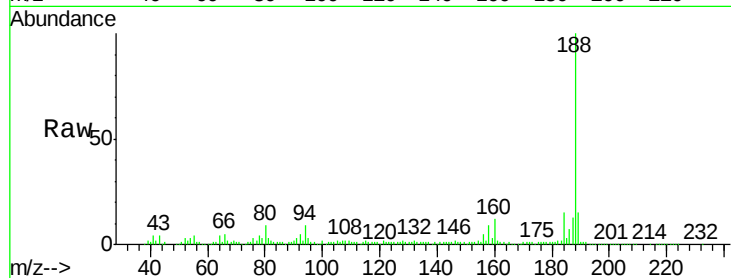

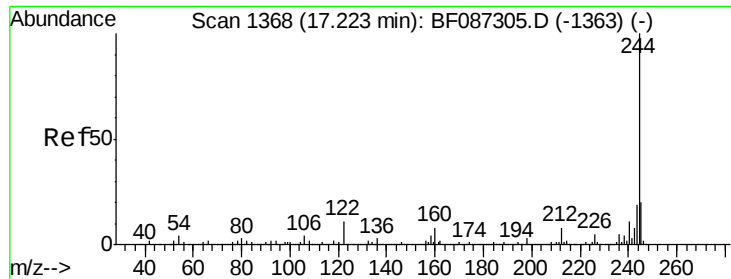

#78

Terphenyl-d14

Concen: 77.86 ng

RT: 17.09 min Scan# 1356

Delta R.T. 0.00 min

Lab File: BF087495.D

Acq: 29 May 2016 00:03

Instrument :

BNA_F