

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052816\
 Data File : BF087496.D
 Acq On : 29 May 2016 00:37
 Operator : UM/SJ
 Sample : H3276-09
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FIELDBLANK

Quant Time: May 30 04:07:43 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 30 03:48:52 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	107097	20.00	ng	-0.01
21) Naphthalene-d8	9.50	136	438882	20.00	ng	-0.01
38) Acenaphthene-d10	12.32	164	212835	20.00	ng	-0.01
63) Phenanthrene-d10	14.72	188	415228	20.00	ng	-0.01
75) Chrysene-d12	18.43	240	324855	20.00	ng	0.00
86) Perylene-d12	20.10	264	226523	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	406214	66.65	ng	0.01
7) Phenol-d6	7.03	99	346077	42.02	ng	-0.01
23) Nitrobenzene-d5	8.39	82	786311	90.30	ng	-0.01
41) 2,4,6-Tribromophenol	13.62	330	288959	141.28	ng	-0.01
44) 2-Fluorobiphenyl	11.28	172	1364737	90.40	ng	-0.01
78) Terphenyl-d14	17.09	244	1337908	87.56	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052816\
Data File : BF087496.D
Acq On : 29 May 2016 00:37
Operator : UM/SJ
Sample : H3276-09
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FIELDBLANK

Quant Time: May 30 04:07:43 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 30 03:48:52 2016
Response via : Initial Calibration

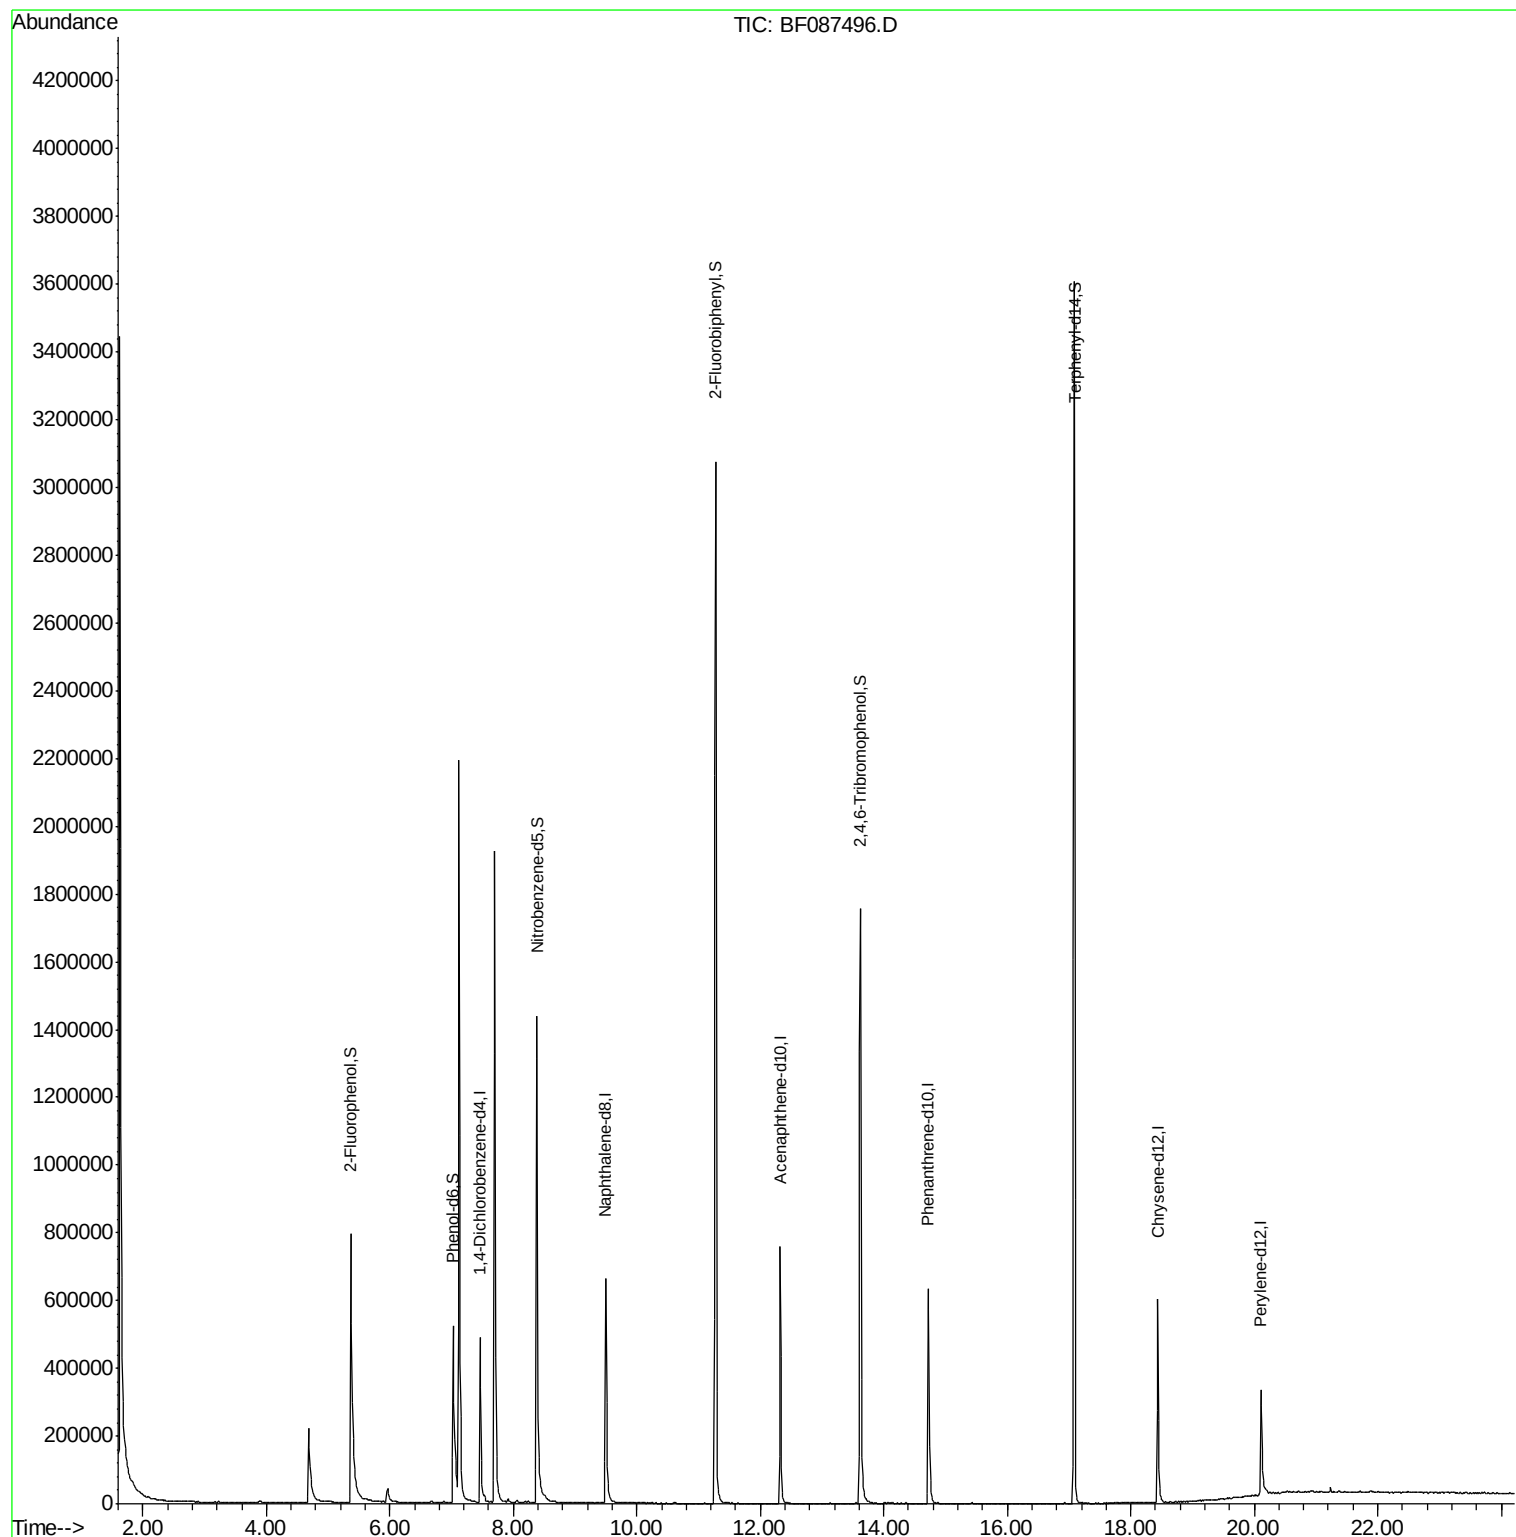







#1

1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.46 min Scan# 514
 Delta R.T. -0.01 min
 Lab File: BF087496.D
 Acq: 29 May 2016 00:37

Instrument :
 BNA_F
 ClientSampleId :
 FIELDBLANK




Tgt Ion:152 Resp: 107097
 Ion Ratio Lower Upper
 152 100
 150 162.3 125.8 188.6
 115 73.6 51.5 77.3

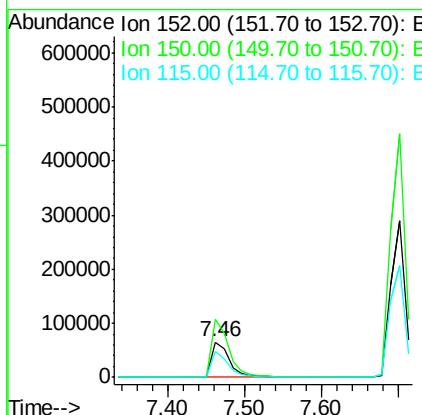


#5

2-Fluorophenol
 Concen: 66.65 ng
 RT: 5.37 min Scan# 331
 Delta R.T. 0.01 min
 Lab File: BF087496.D
 Acq: 29 May 2016 00:37

Tgt Ion:112 Resp: 406214
 Ion Ratio Lower Upper
 112 100
 64 74.7 52.1 78.1
 63 42.1 25.7 38.5#

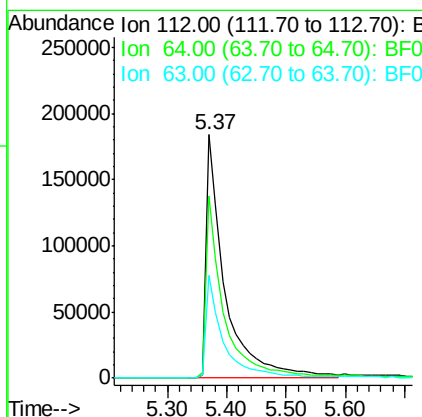

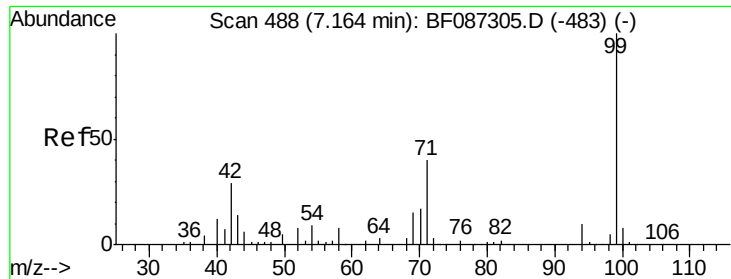

#7

Phenol-d6

Concen: 42.02 ng

RT: 7.03 min Scan# 476

Delta R.T. -0.01 min

Lab File: BF087496.D

Acq: 29 May 2016 00:37

Instrument :

BNA_F

ClientSampleId :

FIELDBLANK





Tgt Ion: 99 Resp: 346077

Ion Ratio Lower Upper

99 100

42 28.6 13.6 20.4#

71 38.7 24.6 36.8#

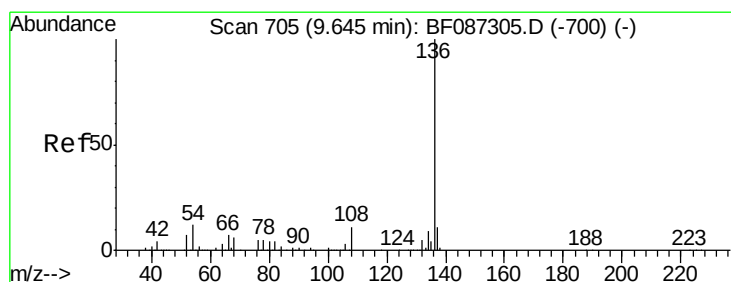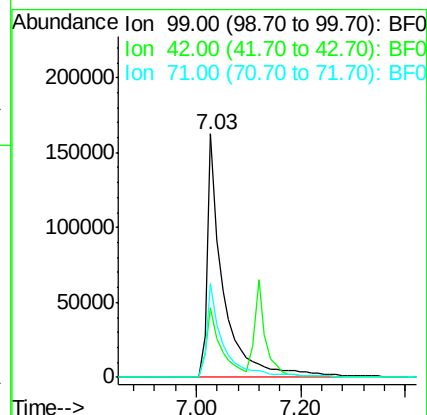

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.50 min Scan# 692

Delta R.T. -0.01 min

Lab File: BF087496.D

Acq: 29 May 2016 00:37

Tgt Ion: 136 Resp: 438882




Ion Ratio Lower Upper


136 100

137 10.8 8.8 13.2

54 11.5 5.0 7.4#

68 5.5 4.4 6.6


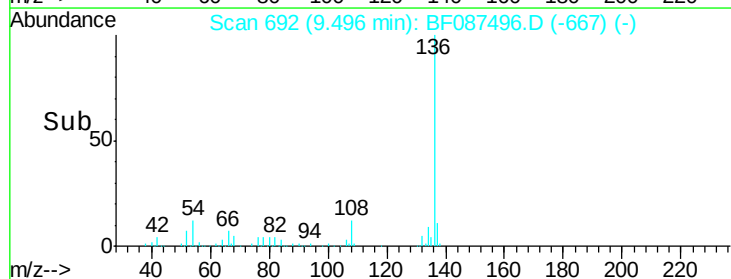
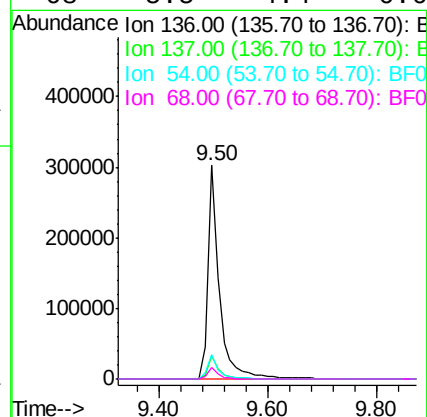
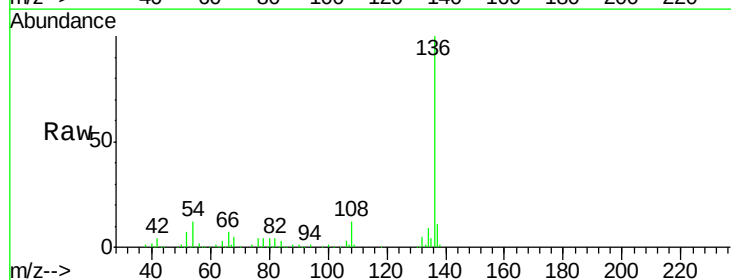




#23
 Nitrobenzene-d5
 Concen: 90.30 ng
 RT: 8.39 min Scan# 595
 Delta R.T. -0.01 min
 Lab File: BF087496.D
 Acq: 29 May 2016 00:37




Instrument :
 BNA_F
 ClientSampleId :
 FIELDBLANK


Tgt Ion: 82 Resp: 786311
 Ion Ratio Lower Upper
 82 100
 128 42.7 40.6 61.0
 54 65.7 38.1 57.1#

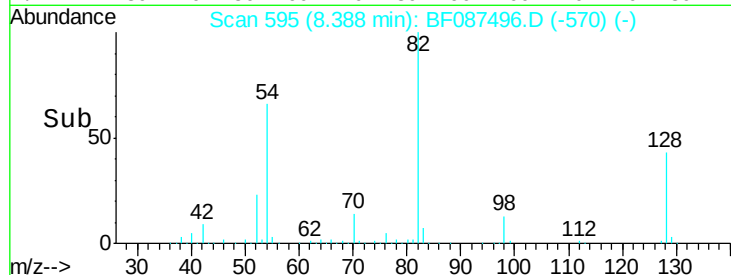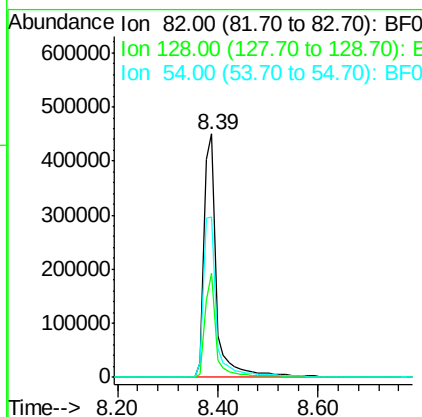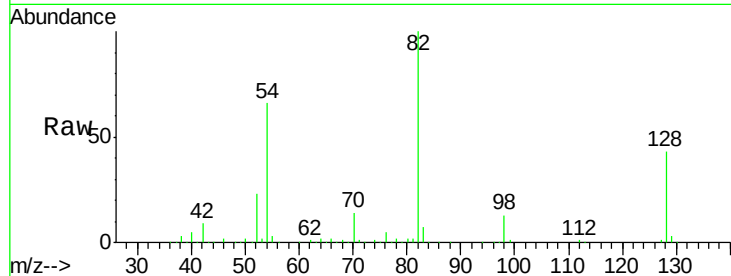

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 12.32 min Scan# 939
 Delta R.T. -0.01 min
 Lab File: BF087496.D
 Acq: 29 May 2016 00:37

Tgt Ion: 164 Resp: 212835
 Ion Ratio Lower Upper
 164 100
 162 101.5 82.8 124.2
 160 47.0 36.9 55.3

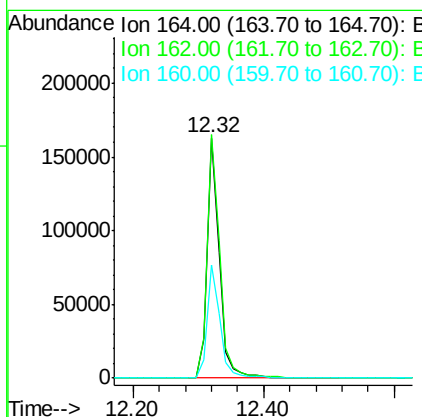


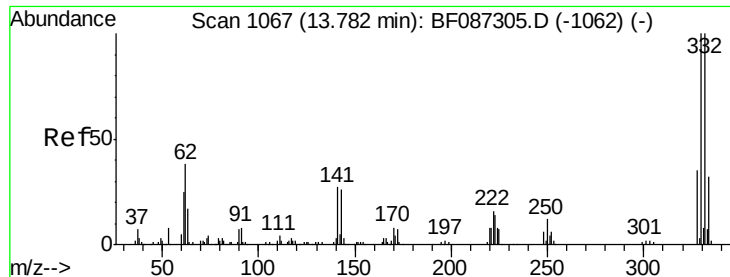




#41
 2,4,6-Tribromophenol
 Concen: 141.28 ng
 RT: 13.62 min Scan# 1053
 Delta R.T. -0.01 min
 Lab File: BF087496.D
 Acq: 29 May 2016 00:37

Instrument :
 BNA_F
 ClientSampleId :
 FIELDBLANK

Tgt Ion:330 Resp: 288959
 Ion Ratio Lower Upper
 330 100
 332 96.5 79.0 118.4
 141 43.5 31.2 46.8

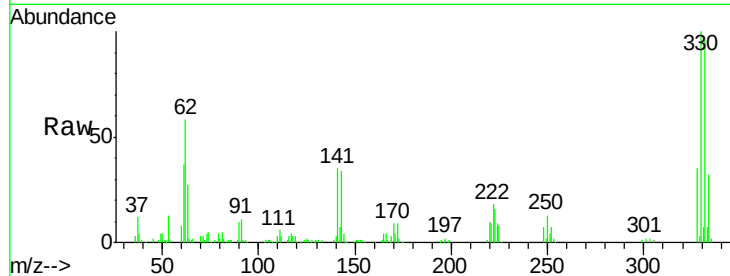


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

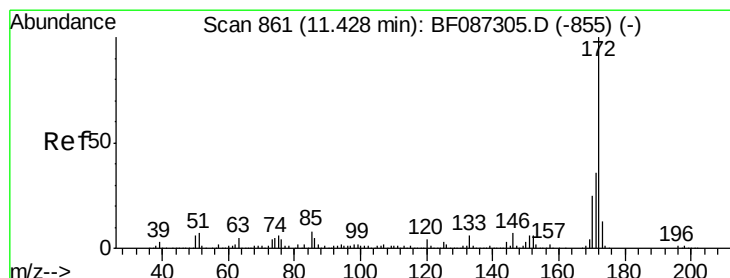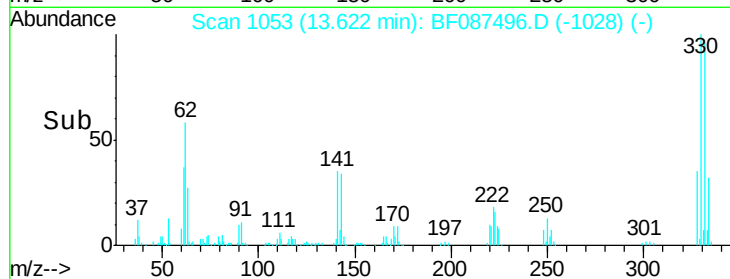
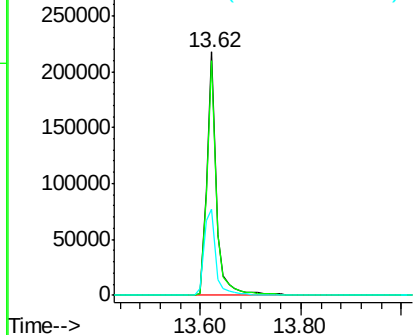



#44
 2-Fluorobiphenyl
 Concen: 90.40 ng
 RT: 11.28 min Scan# 848
 Delta R.T. -0.01 min
 Lab File: BF087496.D
 Acq: 29 May 2016 00:37

Tgt Ion:172 Resp: 1364737
 Ion Ratio Lower Upper
 172 100
 171 36.3 29.0 43.6
 170 24.1 19.8 29.8

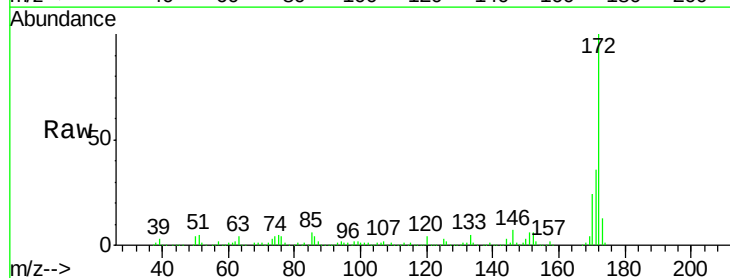

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

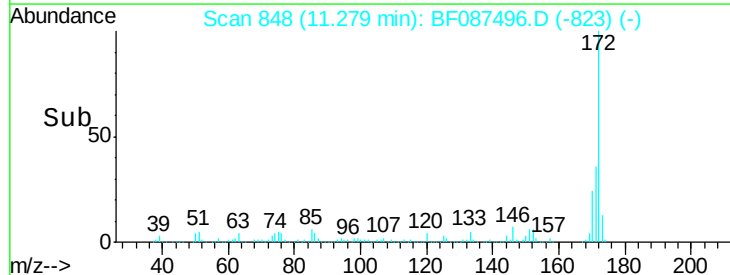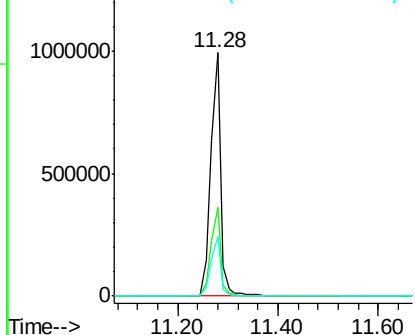







#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 14.72 min Scan# 1149
Delta R.T. -0.01 min
Lab File: BF087496.D
Acq: 29 May 2016 00:37

Instrument :
BNA_F
ClientSampleId :
FIELDBLANK

Tgt Ion:188 Resp: 415228
Ion Ratio Lower Upper
188 100
94 10.8 6.8 10.2#
80 12.5 7.1 10.7#

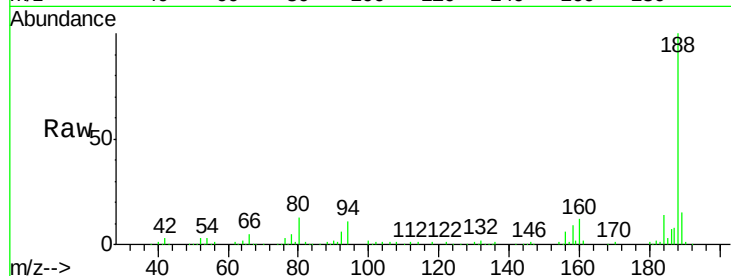


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0


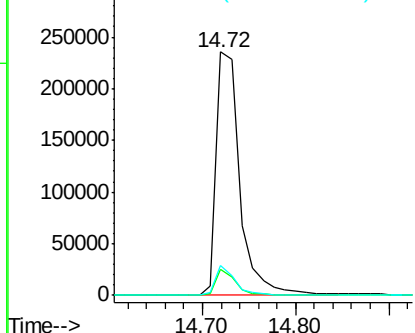



#75
Chrysene-d12
Concen: 20.00 ng
RT: 18.43 min Scan# 1474
Delta R.T. 0.00 min
Lab File: BF087496.D
Acq: 29 May 2016 00:37

Tgt Ion:240 Resp: 324855
Ion Ratio Lower Upper
240 100
120 10.1 11.2 16.8#
236 26.2 21.2 31.8



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

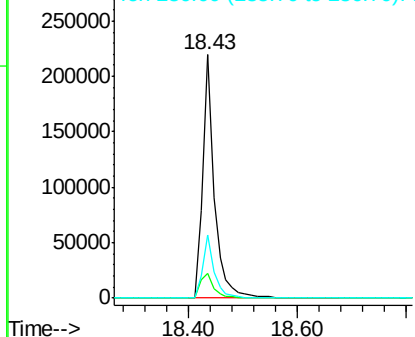

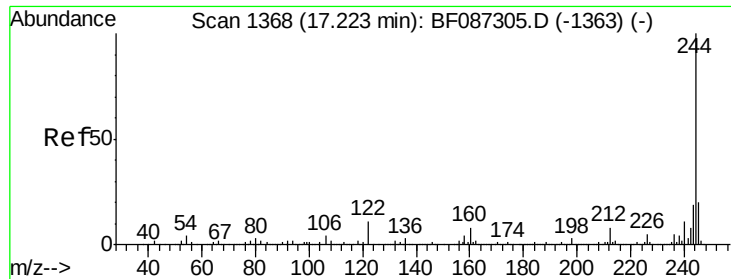

#78

Terphenyl-d14

Concen: 87.56 ng

RT: 17.09 min Scan# 1356

Delta R.T. 0.00 min

Lab File: BF087496.D

Acq: 29 May 2016 00:37

Instrument :

BNA_F

ClientSampled :

FIELDBLANK


Tgt Ion:244 Resp: 1337908

Ion Ratio Lower Upper

244 100

212 8.1 6.2 9.2




122 13.2 12.0 18.0



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

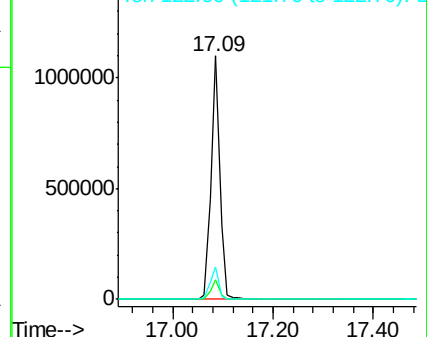

#86

Perylene-d12

Concen: 20.00 ng

RT: 20.10 min Scan# 1620

Delta R.T. 0.00 min

Lab File: BF087496.D

Acq: 29 May 2016 00:37


Tgt Ion:264 Resp: 226523

Ion Ratio Lower Upper

264 100

260 24.3 19.5 29.3

265 20.8 17.3 25.9



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

