


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052816\
 Data File : BF087476.D
 Acq On : 28 May 2016 13:04
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 25 16:26:52 2016

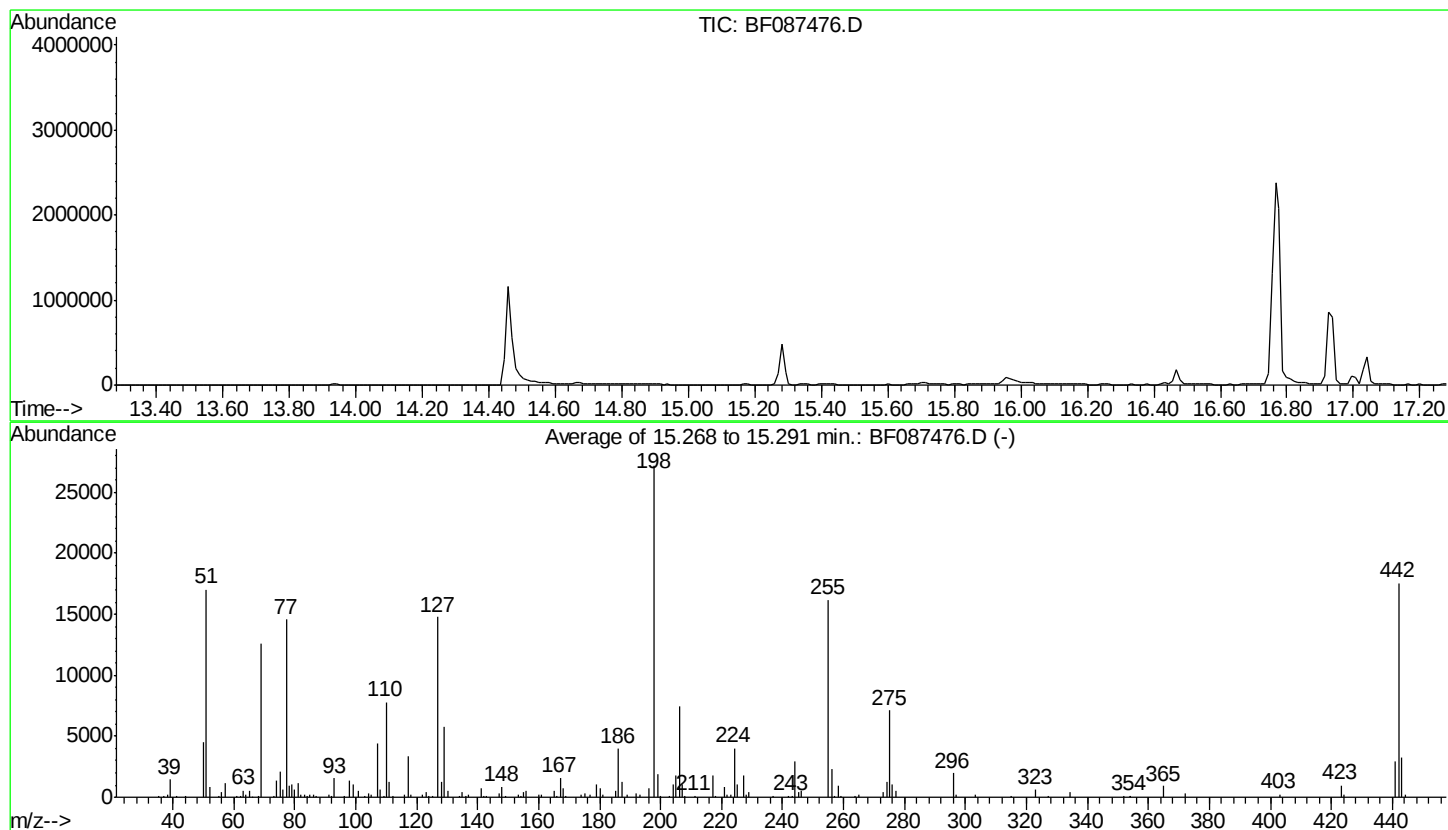

AutoFind: Scans 1197, 1198, 1199; Background Corrected with Scan 1193

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.7	17054	PASS
68	69	0.00	2	1.2	155	PASS
69	198	0.00	100	46.5	12643	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.3	14757	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	27185	PASS
199	198	5	9	6.8	1850	PASS
275	198	10	60	26.2	7110	PASS
365	198	1	100	3.3	899	PASS
441	442	0.01	24	16.6	2917	PASS
442	198	50	100	64.6	17549	PASS
443	442	15	24	18.8	3297	PASS