
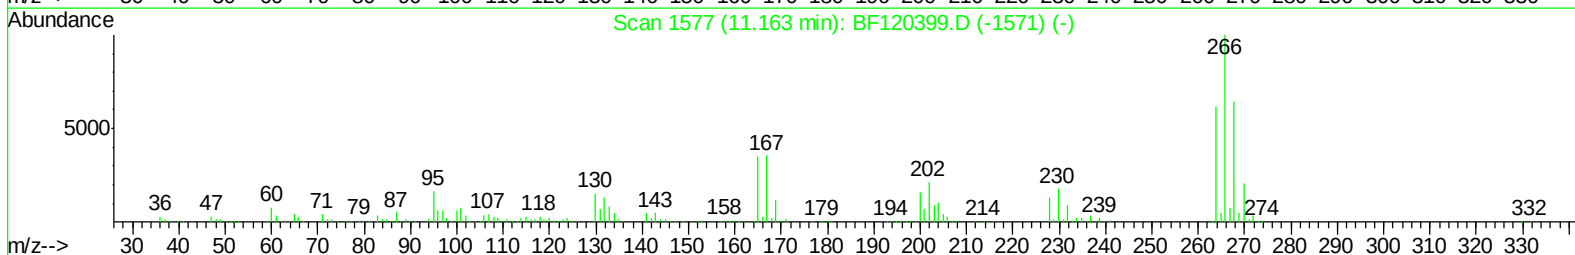
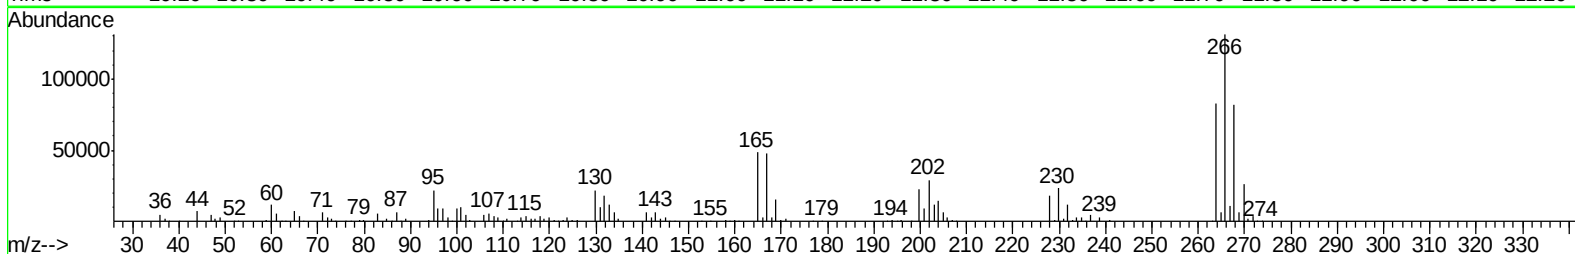


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF052820\
Data File : BF120396.D
Acq On : 28 May 2020 9:32
Operator : MA/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 07:46:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 28 13:47:54 2020
Response via : Initial Calibration

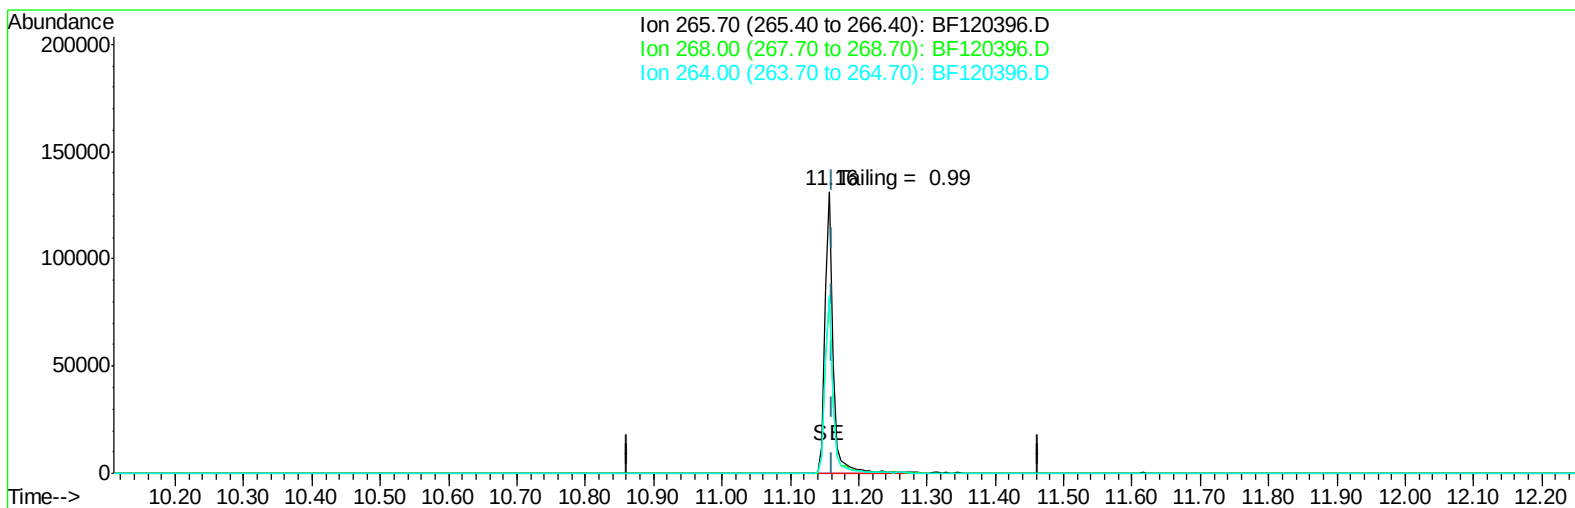

TIC: BF120396.D

(70) Pentachlorophenol (C)




11.157min (-0.006) 31462.18ng

response 112491

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	62.49
264.00	61.40	63.13
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF052820\
Data File : BF120396.D
Acq On : 28 May 2020 9:32
Operator : MA/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 07:46:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 28 13:47:54 2020
Response via : Initial Calibration

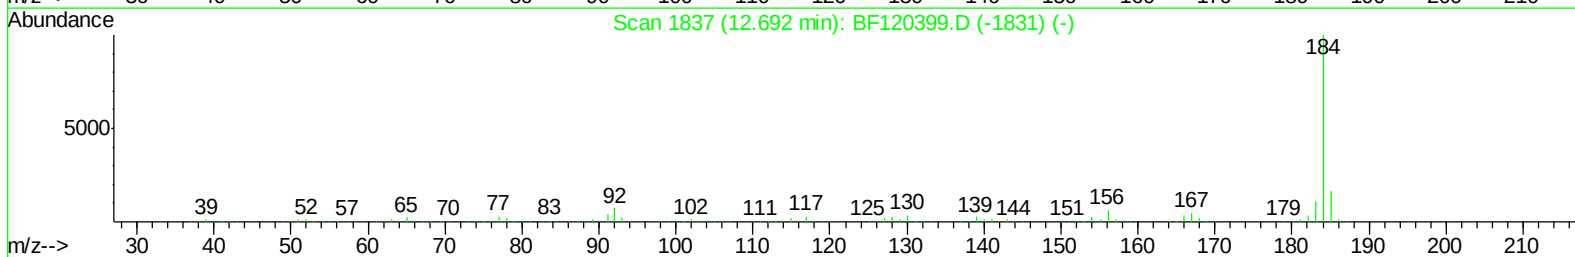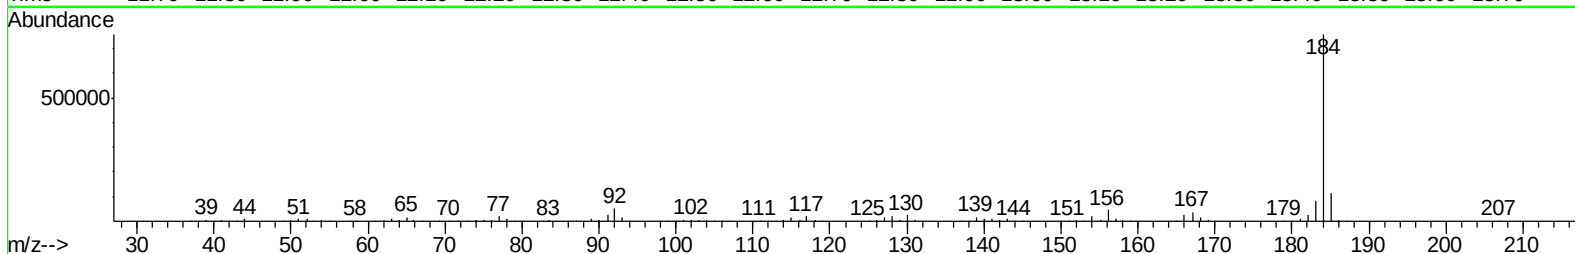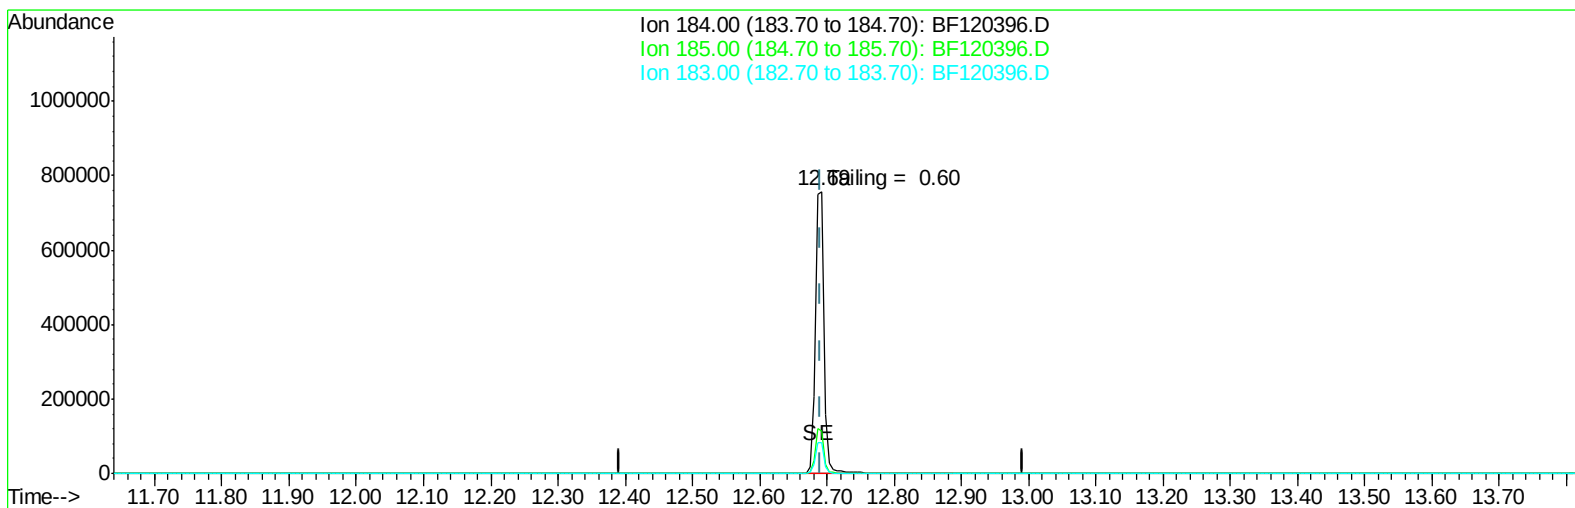

TIC: BF120396.D

(77) Benzidine

12.692min (+0.000) 0.00ng

response 694712

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.82
183.00	10.70	10.95
0.00	0.00	0.00