


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052820\
 Data File : BF120396.D
 Acq On : 28 May 2020 9:32
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 28 13:47:54 2020

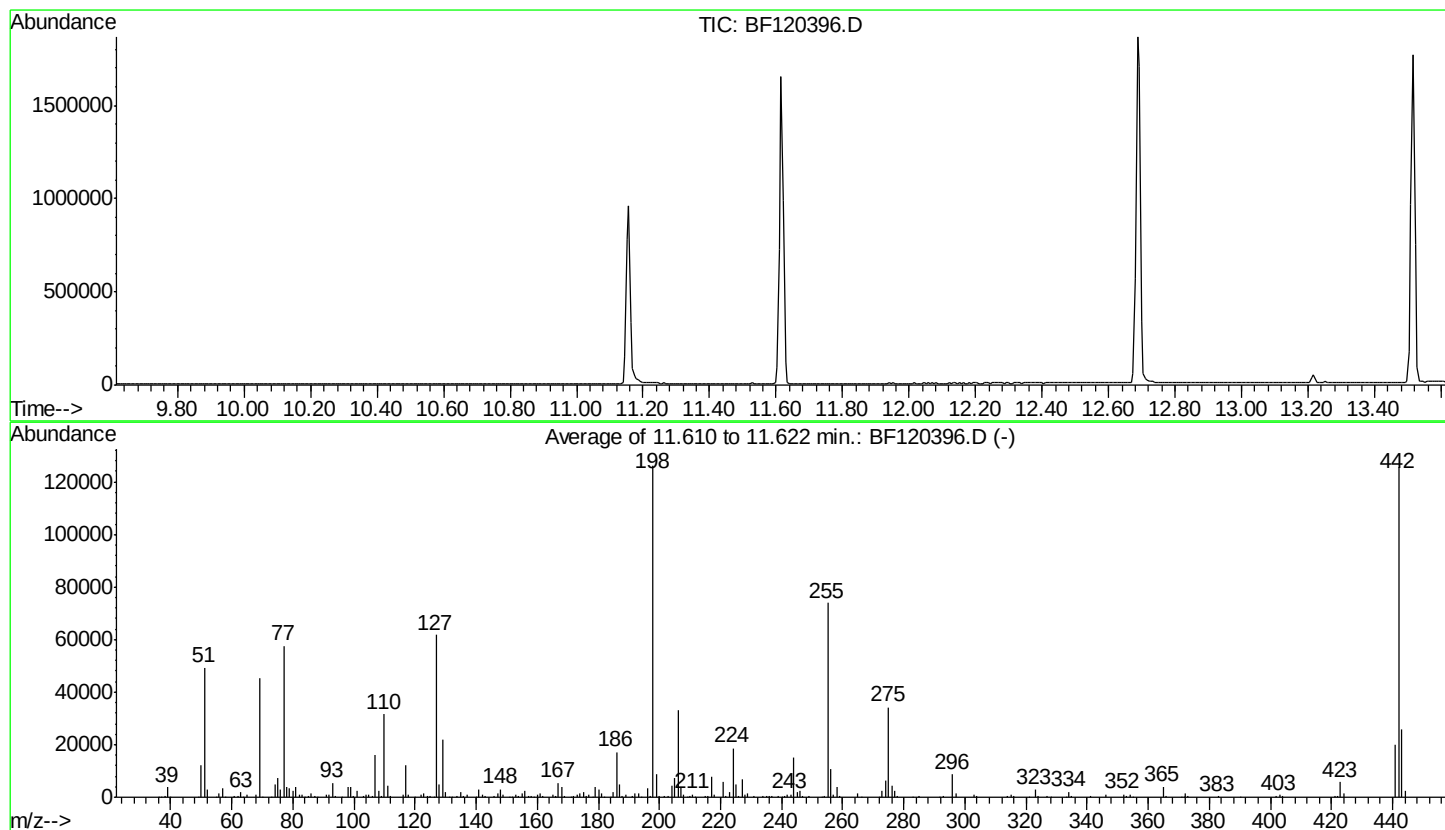

AutoFind: Scans 1653, 1654, 1655; Background Corrected with Scan 1648

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	49421	PASS
68	69	0.00	2	1.8	793	PASS
69	198	0.00	100	35.9	45285	PASS
70	69	0.00	2	0.3	139	PASS
127	198	10	80	48.9	61693	PASS
197	198	0.00	2	0.6	731	PASS
198	198	100	100	100.0	126184	PASS
199	198	5	9	7.1	8902	PASS
275	198	10	60	27.1	34154	PASS
365	198	1	100	3.2	4012	PASS
441	198	0.01	100	15.8	19960	PASS
442	198	50	100	99.5	125597	PASS
443	442	15	24	20.5	25687	PASS