


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF052820\  
 Data File : BF120405.D  
 Acq On : 28 May 2020 13:50  
 Operator : MA/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF052820.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu May 28 13:47:54 2020

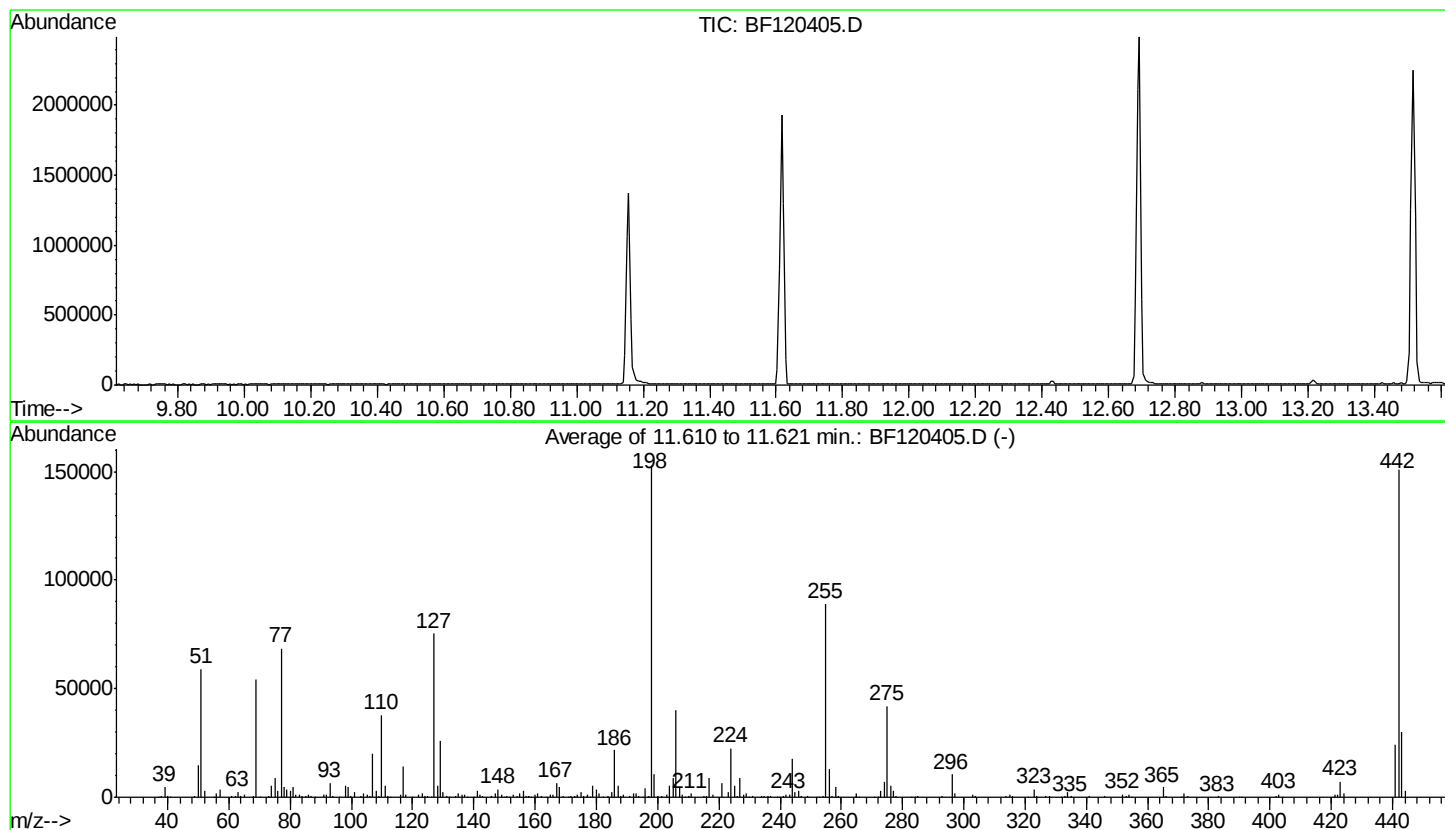

AutoFind: Scans 1653, 1654, 1655; Background Corrected with Scan 1648

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 38.7         | 59101      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 886        | PASS                |
| 69             | 198             | 0.00            | 100             | 35.5         | 54232      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.2          | 110        | PASS                |
| 127            | 198             | 10              | 80              | 49.4         | 75410      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.4          | 670        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 152754     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 10399      | PASS                |
| 275            | 198             | 10              | 60              | 27.5         | 41936      | PASS                |
| 365            | 198             | 1               | 100             | 3.0          | 4649       | PASS                |
| 441            | 198             | 0.01            | 100             | 15.7         | 23914      | PASS                |
| 442            | 198             | 50              | 100             | 98.9         | 151010     | PASS                |
| 443            | 442             | 15              | 24              | 19.9         | 30078      | PASS                |