

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052822\
 Data File : BF128540.D
 Acq On : 28 May 2022 10:48
 Operator : CG\JU
 Sample : PB144997BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB144997BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128540.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.463	534	540	543	rBV	4624438	5516562	79.16%	12.919%
2	6.469	704	711	713	rBV	4367236	5537712	79.47%	12.969%
3	6.834	770	773	777	rBV	1278834	1149251	16.49%	2.691%
4	7.398	863	869	872	rBV	3354583	3843490	55.15%	9.001%
5	8.116	986	991	995	rBV	1581734	1521285	21.83%	3.563%
6	9.198	1169	1175	1178	rBV	6094325	6685149	95.93%	15.656%
7	9.875	1284	1290	1293	rBV	1948185	1756534	25.21%	4.114%
8	10.663	1417	1424	1428	rBV	3768191	4176986	59.94%	9.782%
9	11.363	1537	1543	1546	rBV	2146317	1861894	26.72%	4.360%
10	12.957	1809	1814	1817	rBV	6520951	6968670	100.00%	16.320%
11	14.004	1987	1992	1995	rBV	1859113	1695705	24.33%	3.971%
12	14.098	2002	2008	2019	rBV	343324	406628	5.84%	0.952%
13	15.468	2235	2241	2246	rBV	1183295	1480924	21.25%	3.468%
14	16.927	2480	2489	2490	rBV7	48769	99794	1.43%	0.234%




Sum of corrected areas: 42700584

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052822\
Data File : BF128540.D
Acq On : 28 May 2022 10:48
Operator : CG\JU
Sample : PB144997BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144997BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

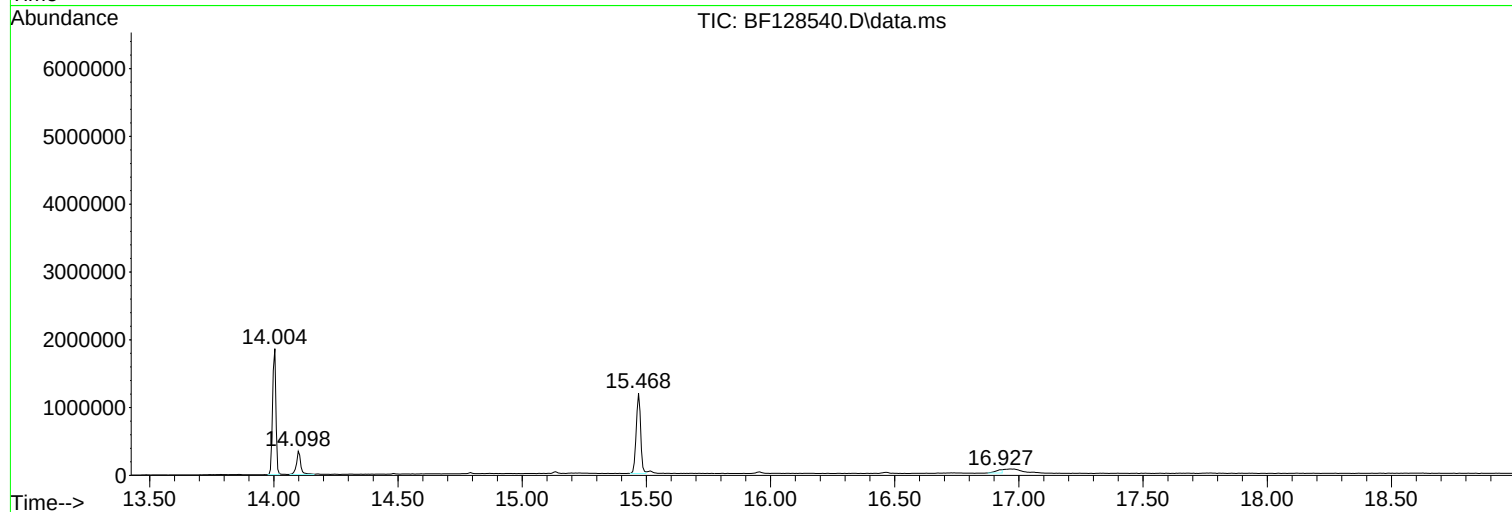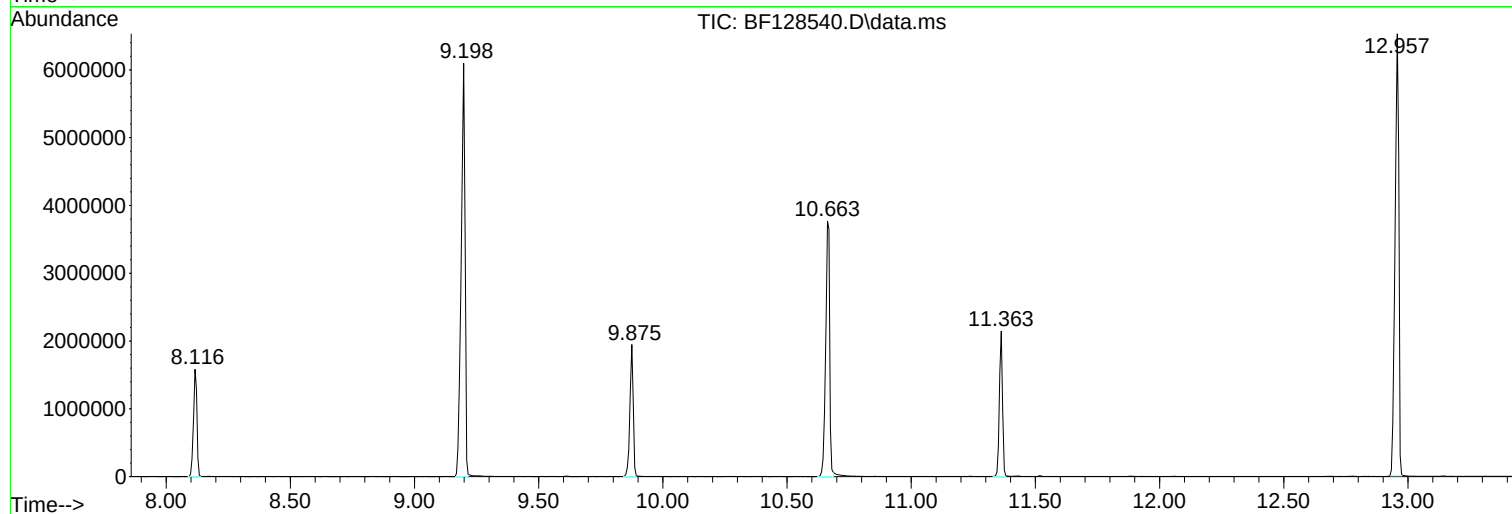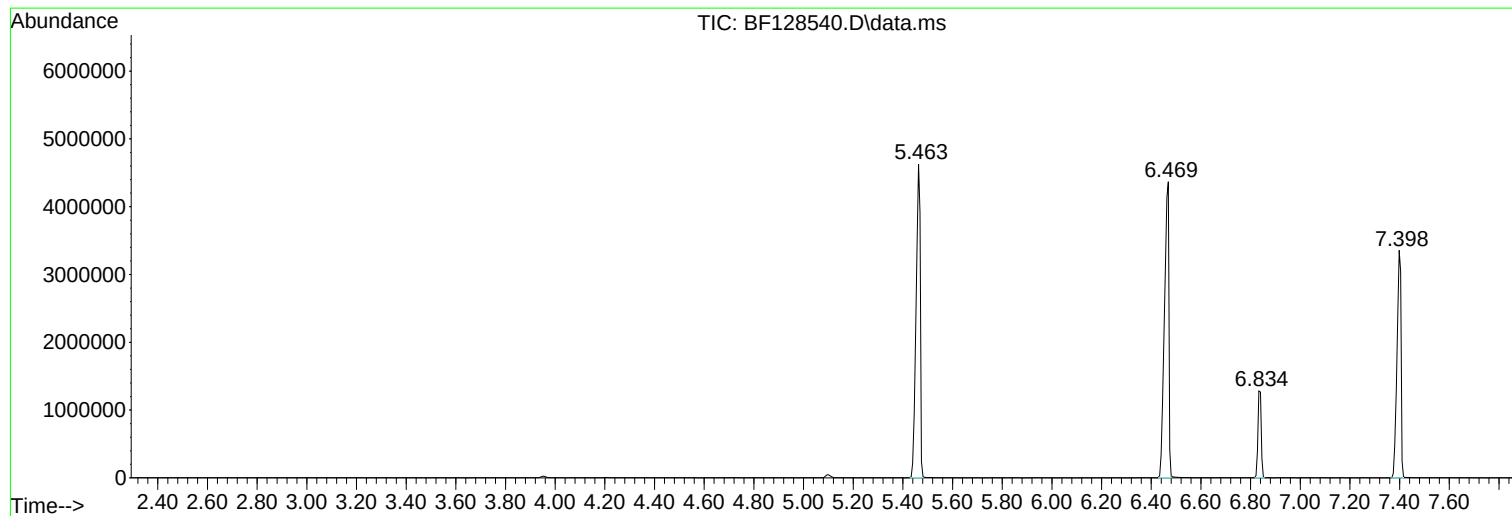

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052822\
Data File : BF128540.D
Acq On : 28 May 2022 10:48
Operator : CG\JU
Sample : PB144997BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144997BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.098	4.80 ng	406628	Chrysene-d12	14.004

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	92
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	64
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	42
4			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	35
5			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	25

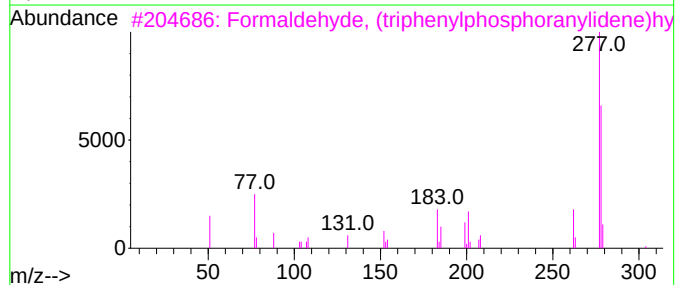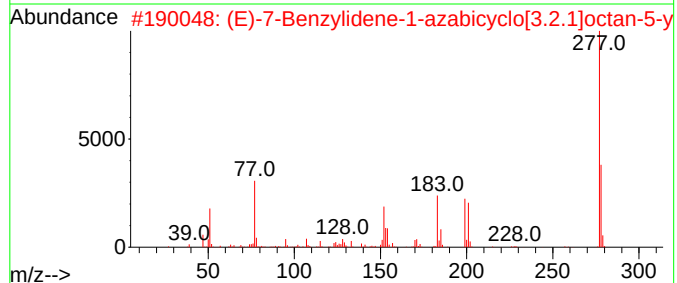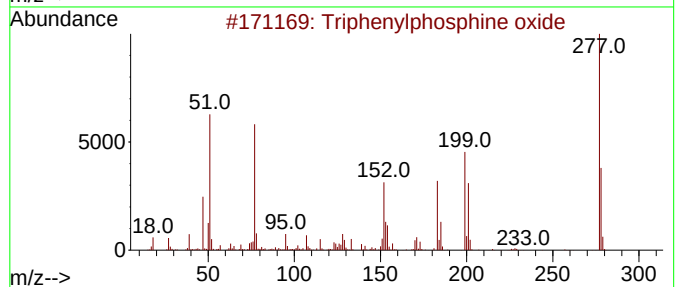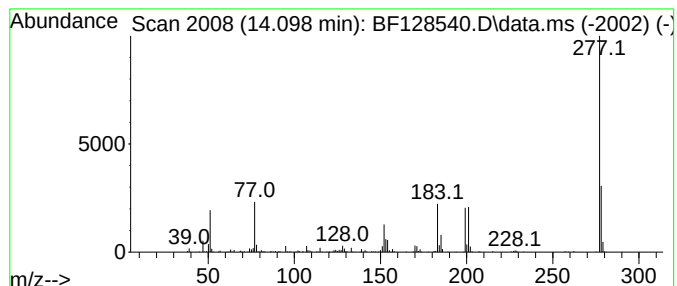

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052822\
Data File : BF128540.D
Acq On : 28 May 2022 10:48
Operator : CG\JU
Sample : PB144997BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB144997BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.098	4.8	ng	406628	5	14.004	1695710	20.0