


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052822\
 Data File : BF128538.D
 Acq On : 28 May 2022 09:45
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 27 01:51:59 2022

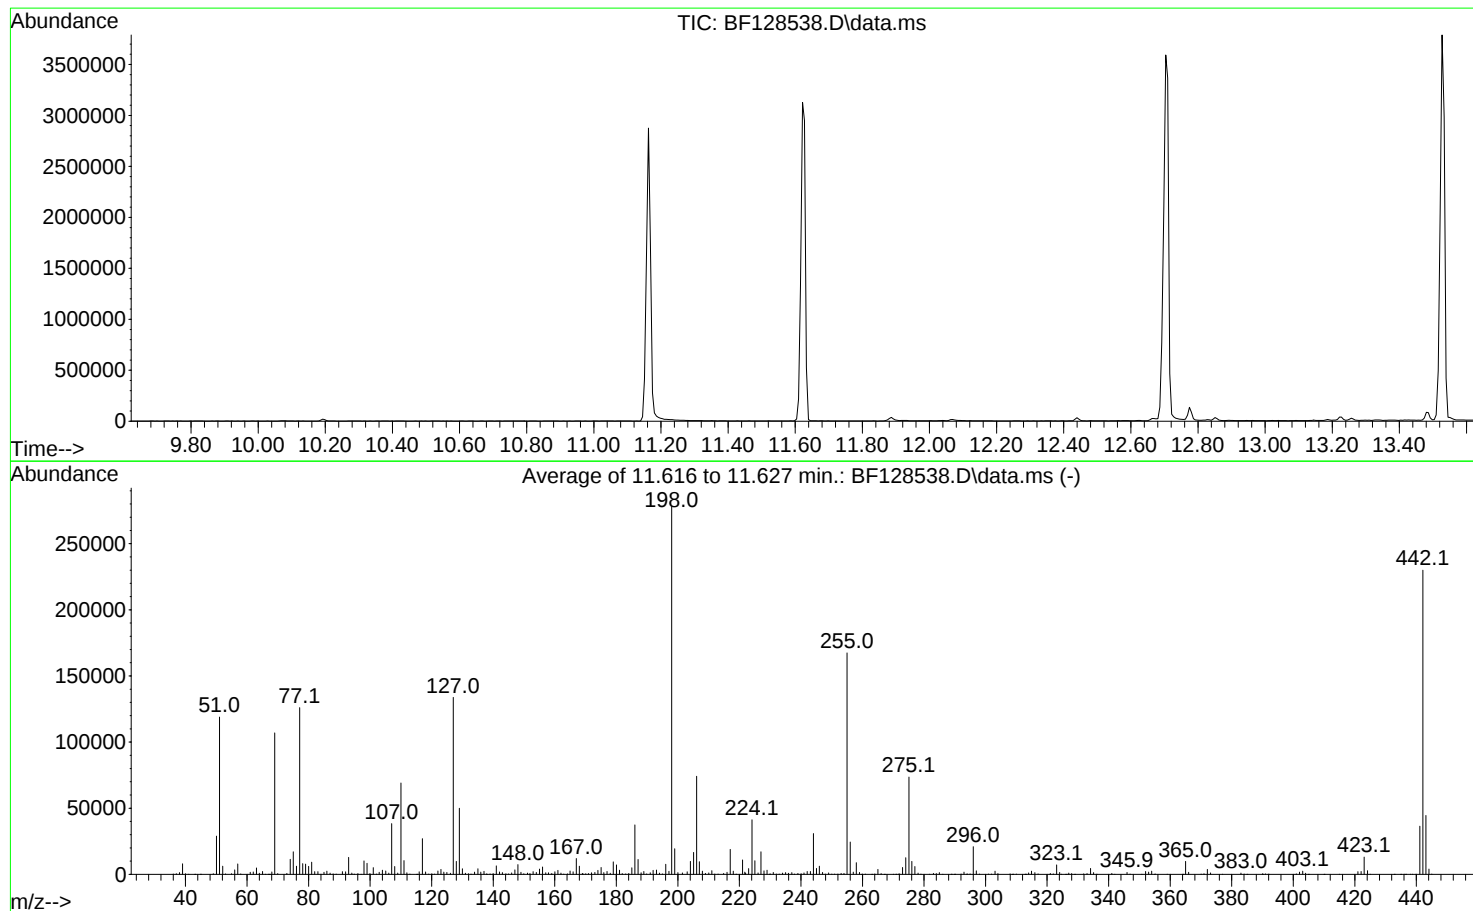

AutoFind: Scans 1586, 1587, 1588; Background Corrected with Scan 1580

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	118925	PASS
68	69	0.00	2	1.7	1790	PASS
69	198	0.00	100	38.4	106883	PASS
70	69	0.00	2	0.5	584	PASS
127	198	10	80	48.1	133728	PASS
197	198	0.00	2	0.8	2345	PASS
198	198	100	100	100.0	278101	PASS
199	198	5	9	7.0	19329	PASS
275	198	10	60	26.5	73597	PASS
365	198	1	100	3.5	9779	PASS
441	198	0.01	100	13.1	36406	PASS
442	442	50	100	100.0	229925	PASS
443	442	15	24	19.4	44518	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/28/2022	BNA_F	<u>BF128538.D</u>
Compound Name	Response	Retention Time
DDT	663576	13.527
DDD	9700	13.221
DDE	357	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10057	673633	1.49

Instrument :
BNA_F
ClientSampleId :
DFTPP

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052822\  
Data File : BF128538.D  
Acq On    : 28 May 2022  09:45  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 28 10:16:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration

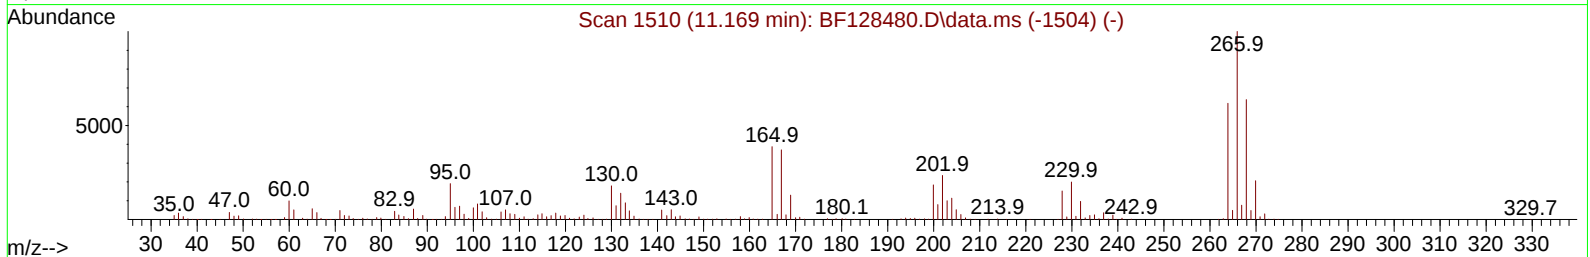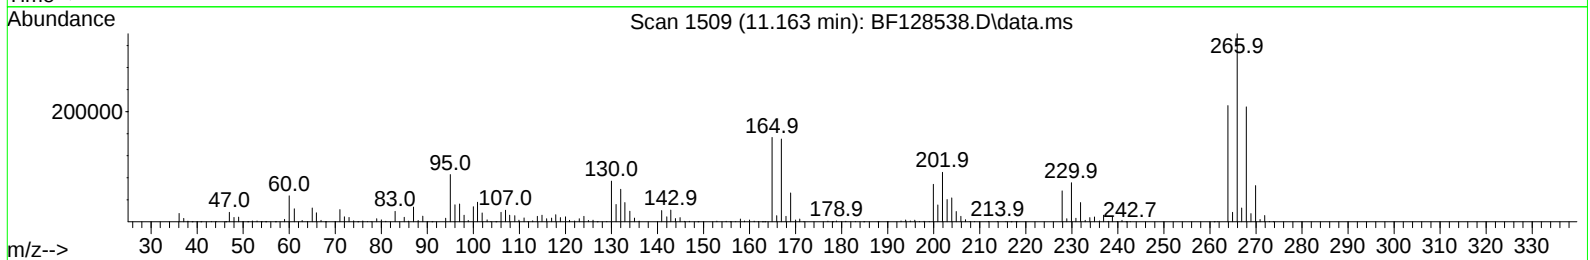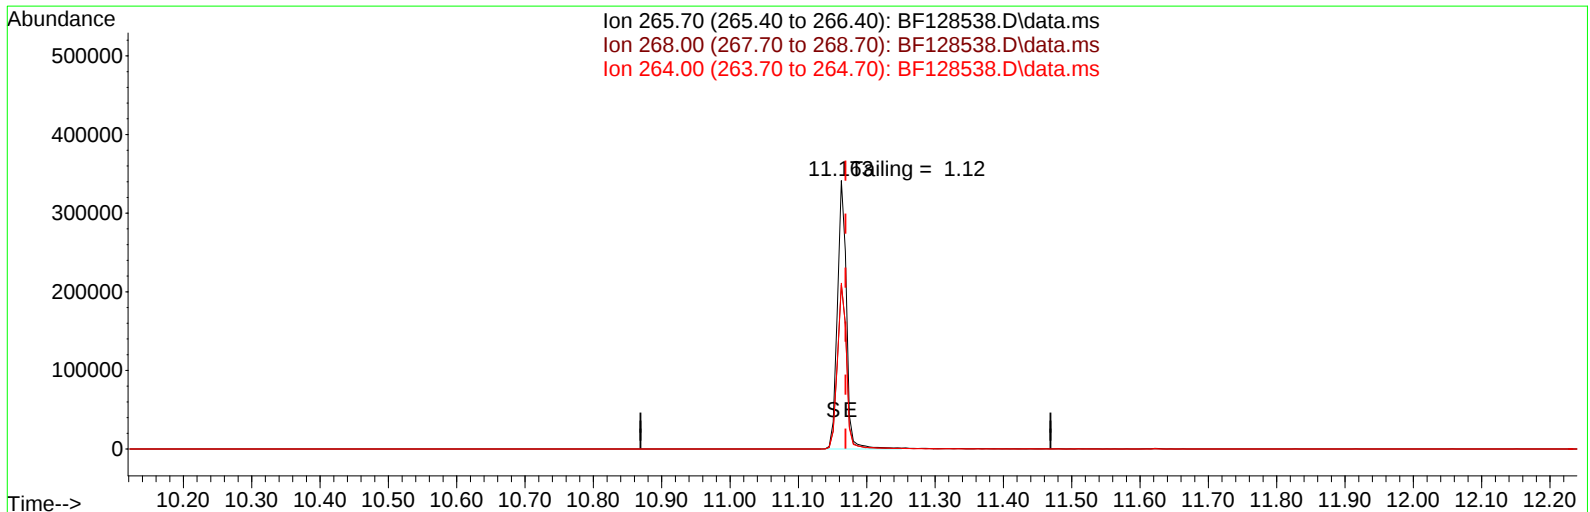

TIC: BF128538.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.006) 159854.80 ng




response 312313

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	61.14
264.00	61.80	61.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052822\
Data File : BF128538.D
Acq On : 28 May 2022 09:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 28 10:16:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration

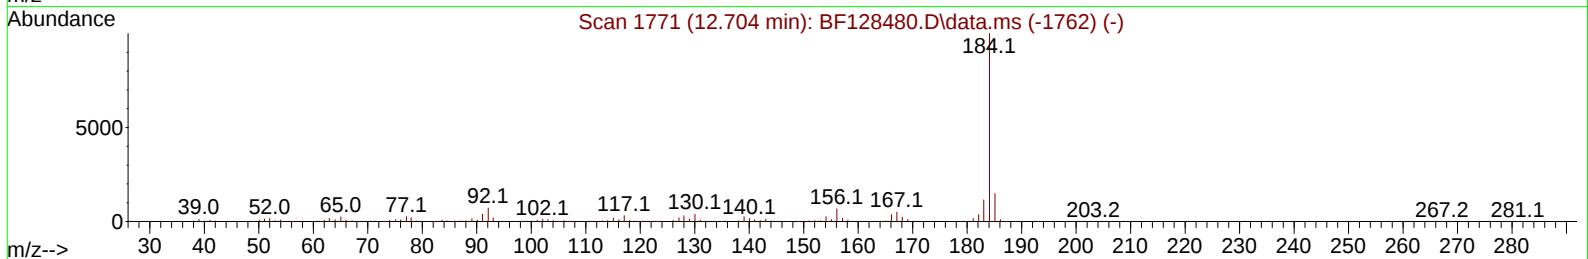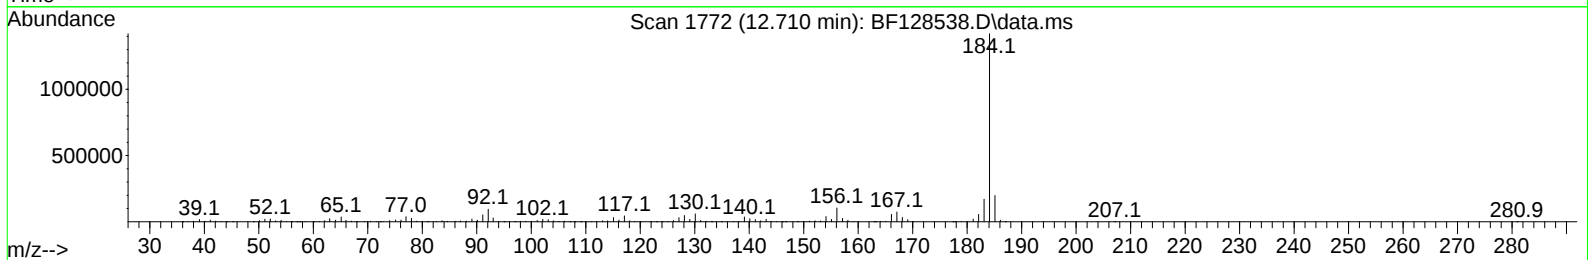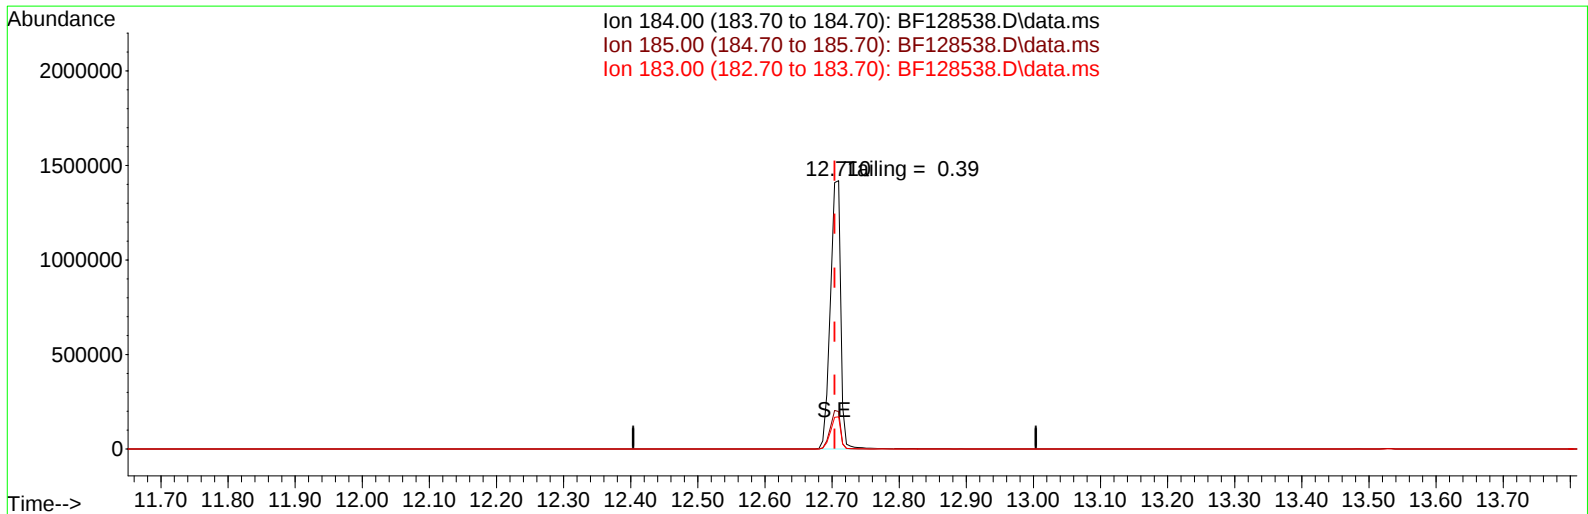

TIC: BF128538.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 183209.51 ng

response 1517075

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.95
183.00	11.60	12.00
0.00	0.00	0.00