
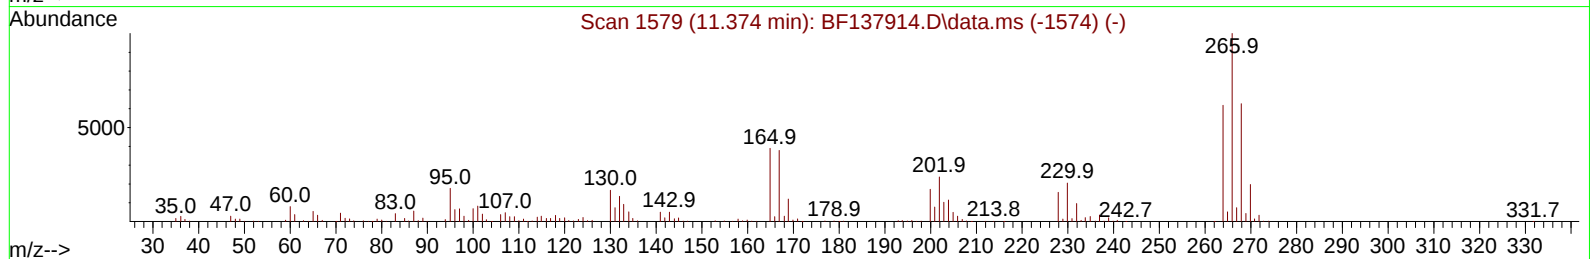
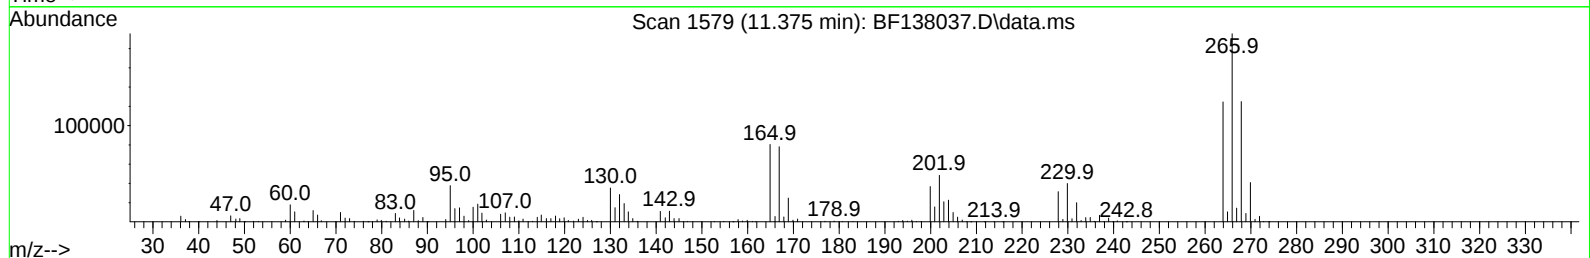


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF052824\  
Data File : BF138037.D  
Acq On : 28 May 2024 10:11  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 02:49:46 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF051424.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 15 04:12:16 2024  
Response via : Initial Calibration

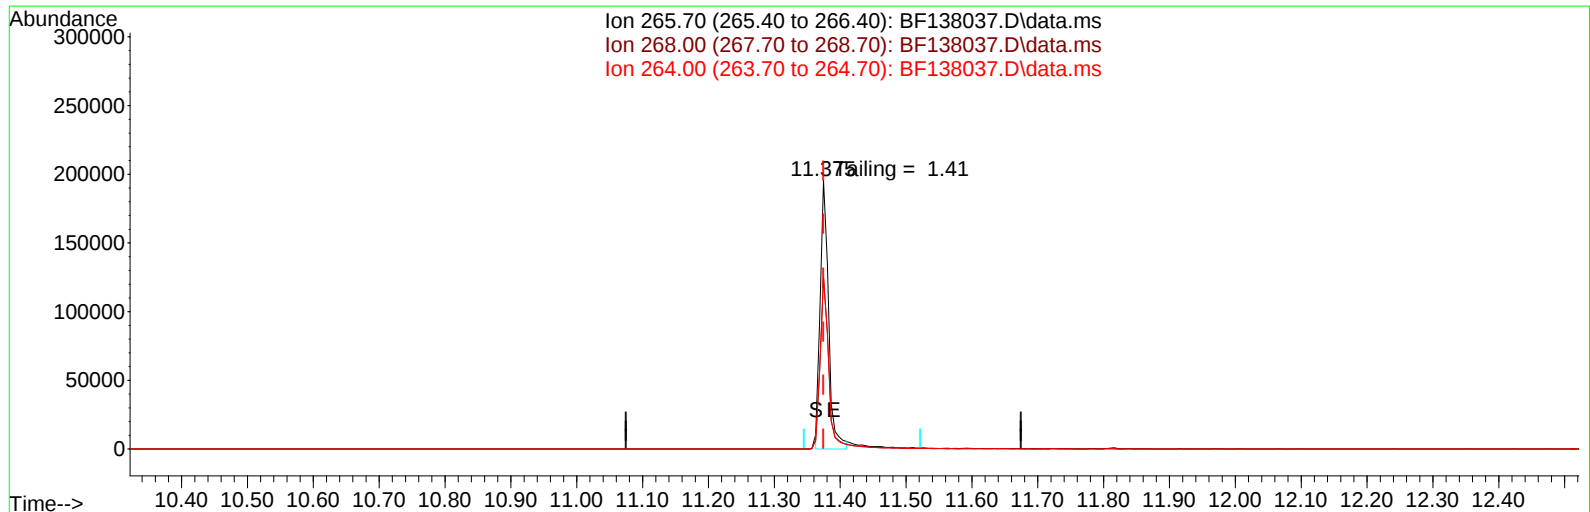

TIC: BF138037.D\data.ms

**(70) Pentachlorophenol (C)**




11.375min (+ 0.000) 29284.18 ng

response 187708

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.60  | 63.93  |
| 264.00 | 61.80  | 63.79  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF052824\  
Data File : BF138037.D  
Acq On : 28 May 2024 10:11  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 29 02:49:46 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF051424.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed May 15 04:12:16 2024  
Response via : Initial Calibration

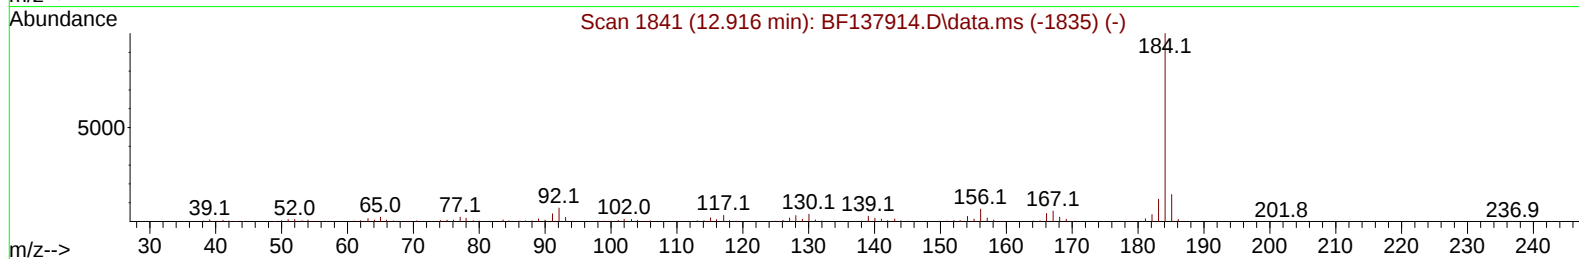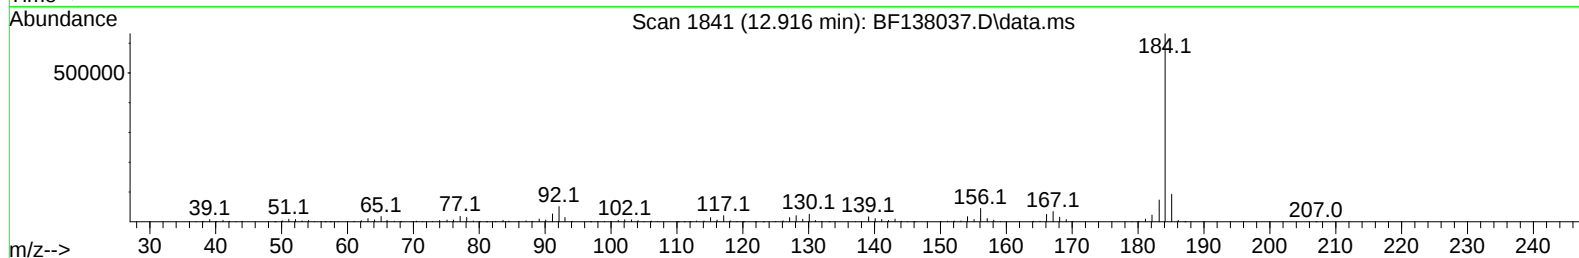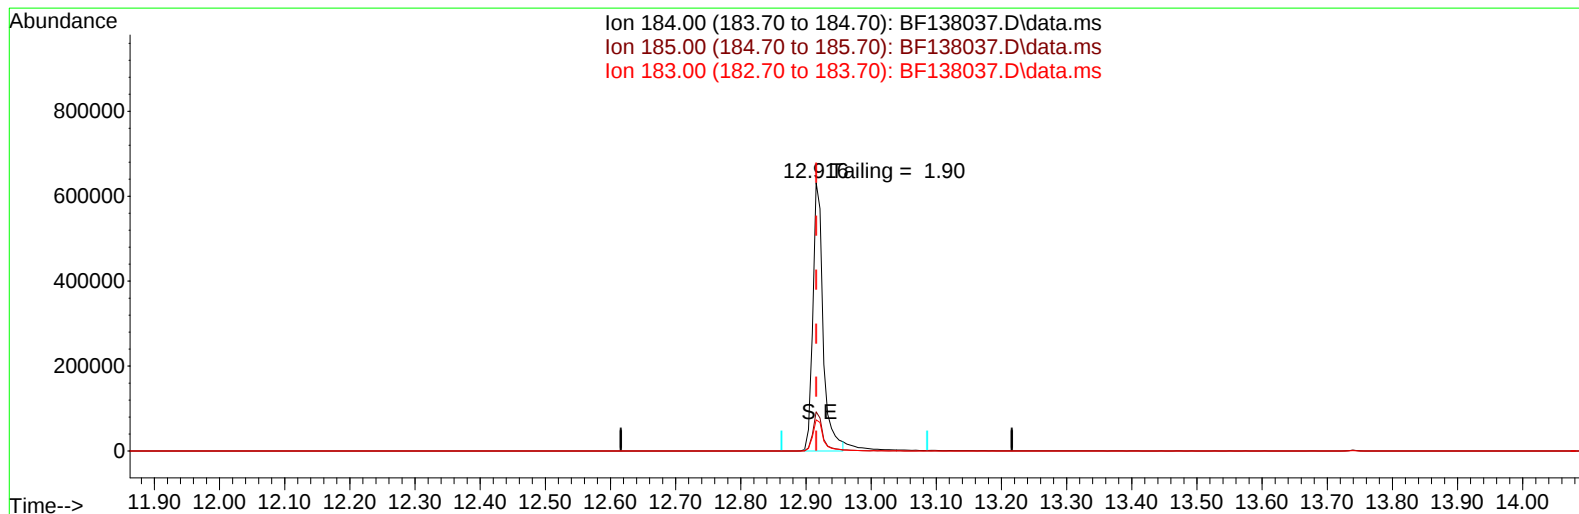

TIC: BF138037.D\data.ms

**(77) Benzidine**

12.916min (-0.000) 0.00 ng

response 730020

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.30  | 14.65  |
| 183.00 | 11.90  | 11.64  |
| 0.00   | 0.00   | 0.00   |