


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052824\
Data File : BF138037.D
Acq On : 28 May 2024 10:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed May 15 04:12:16 2024

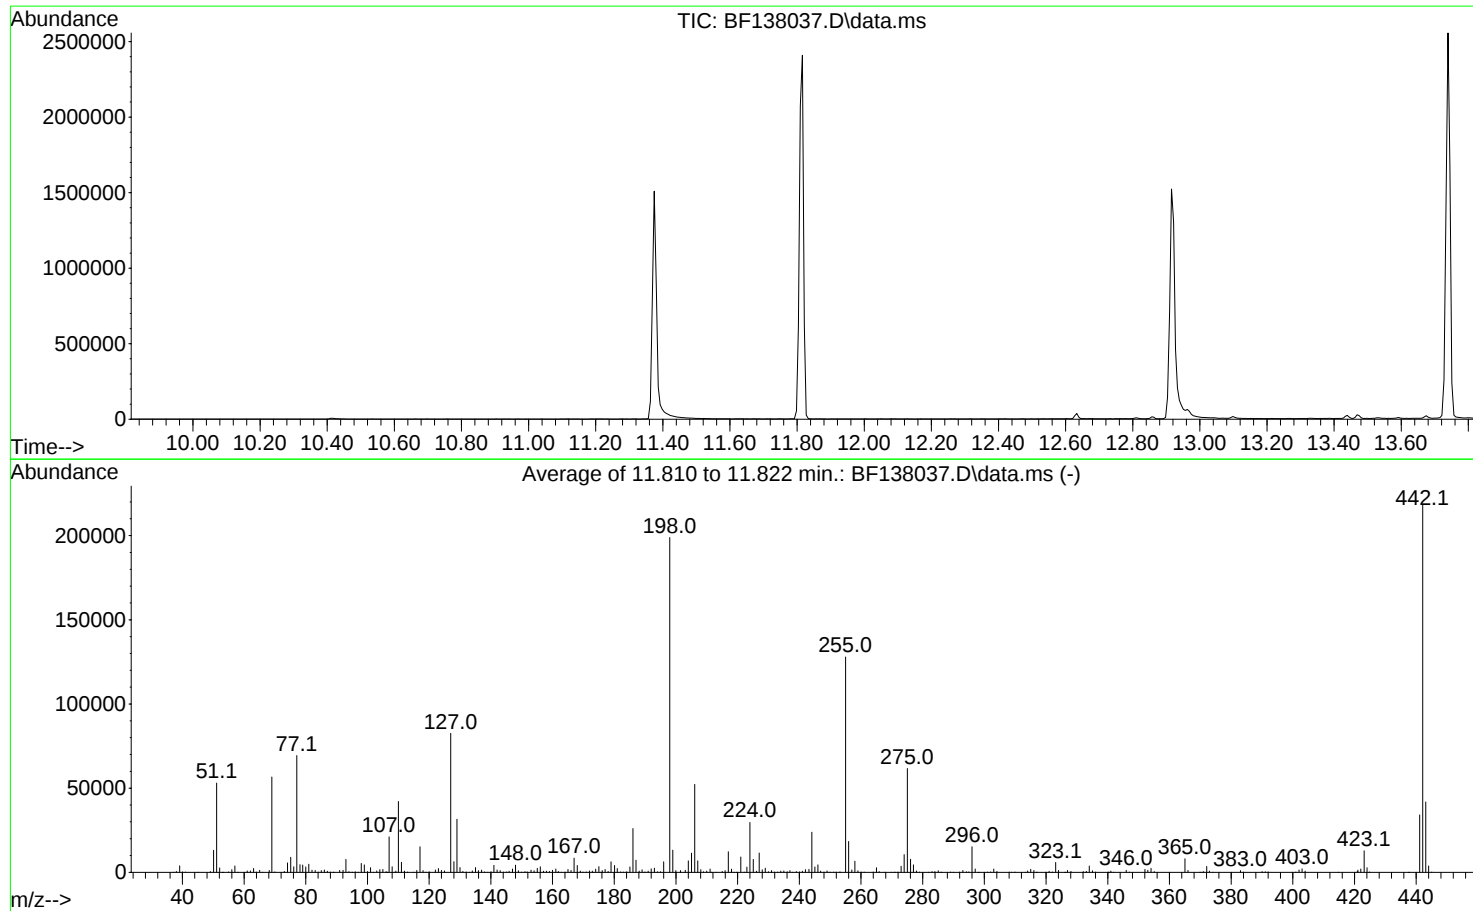

AutoFind: Scans 1653, 1654, 1655; Background Corrected with Scan 1647

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.6	52987	PASS
68	69	0.00	2	2.0	1123	PASS
69	198	0.00	100	28.5	56650	PASS
70	69	0.00	2	0.5	285	PASS
127	198	10	80	41.5	82573	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	198869	PASS
199	198	5	9	6.6	13199	PASS
275	198	10	60	31.0	61667	PASS
365	198	1	100	4.1	8075	PASS
441	198	0.01	100	17.2	34125	PASS
442	442	50	100	100.0	218475	PASS
443	442	15	24	19.1	41813	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/28/2024	BNA_F	<u>BF138037.D</u>
Compound Name	Response	Retention Time
DDT	452307	13.739
DDD	8636	13.439
DDE	2102	13.098
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10738	463045	2.32

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052824\
Data File : BF138037.D
Acq On : 28 May 2024 10:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 29 02:49:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

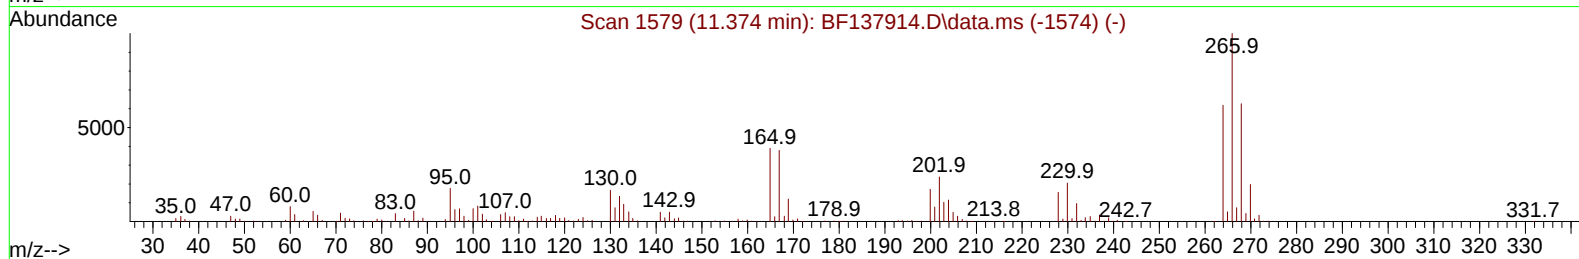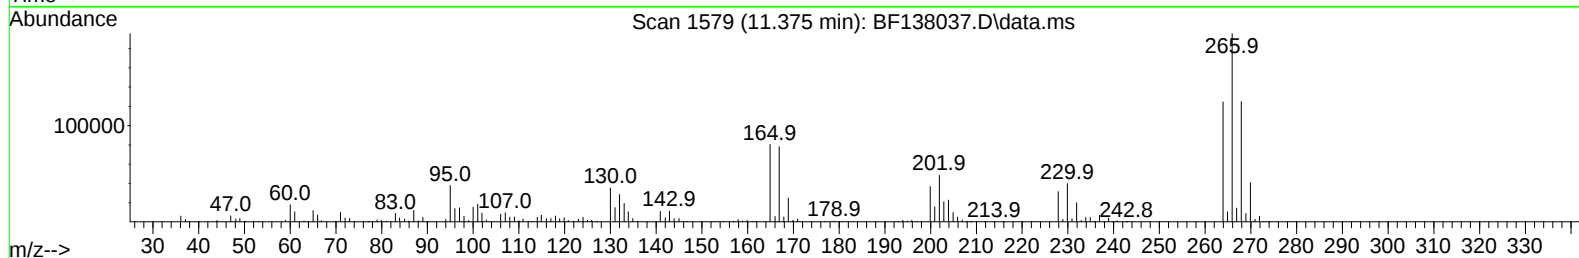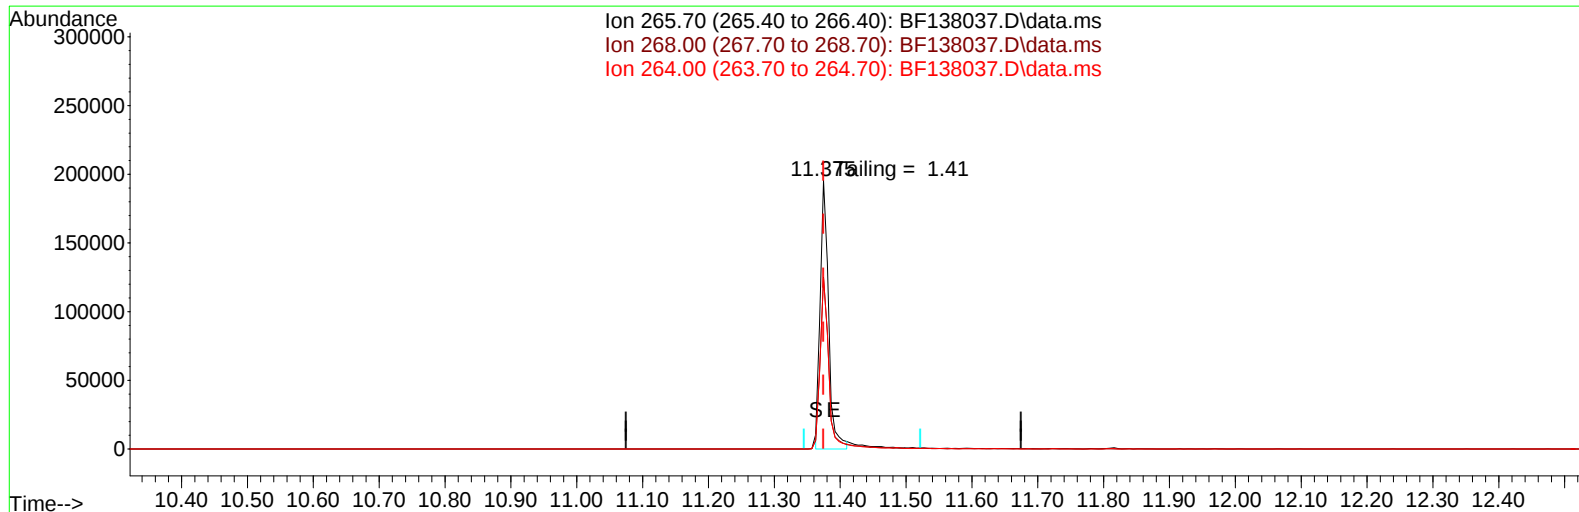

TIC: BF138037.D\data.ms

(70) Pentachlorophenol (C)

11.375min (+ 0.000) 29284.18 ng




response 187708

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.93
264.00	61.80	63.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052824\
Data File : BF138037.D
Acq On : 28 May 2024 10:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 29 02:49:46 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF051424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 15 04:12:16 2024
Response via : Initial Calibration

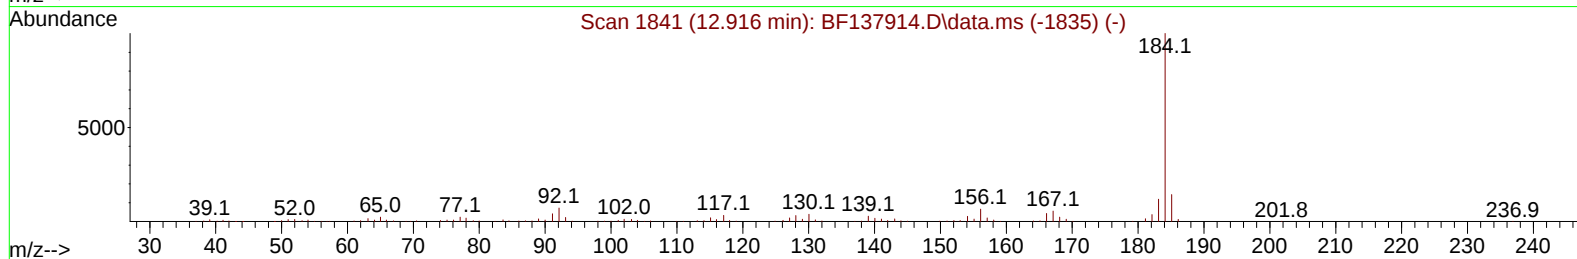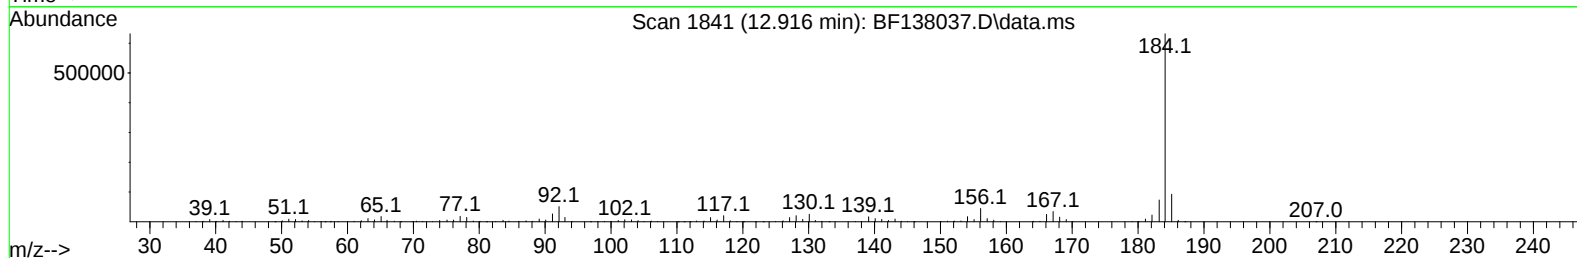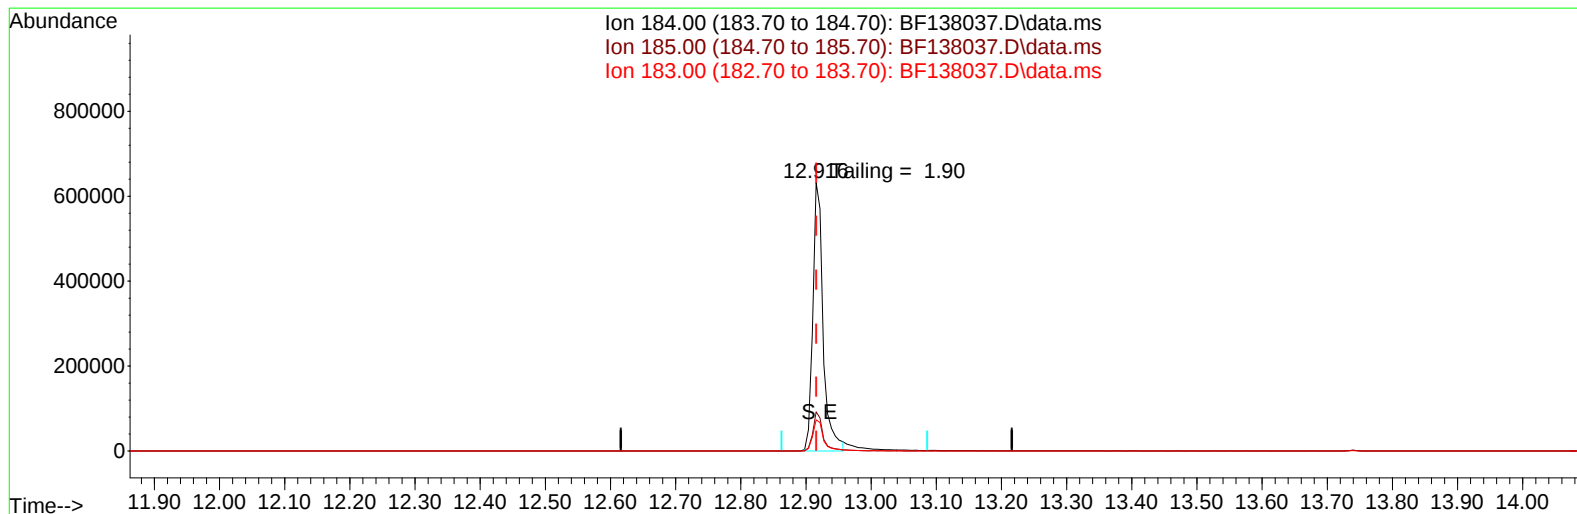

TIC: BF138037.D\data.ms

(77) Benzidine

12.916min (-0.000) 0.00 ng

response 730020

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.65
183.00	11.90	11.64
0.00	0.00	0.00