
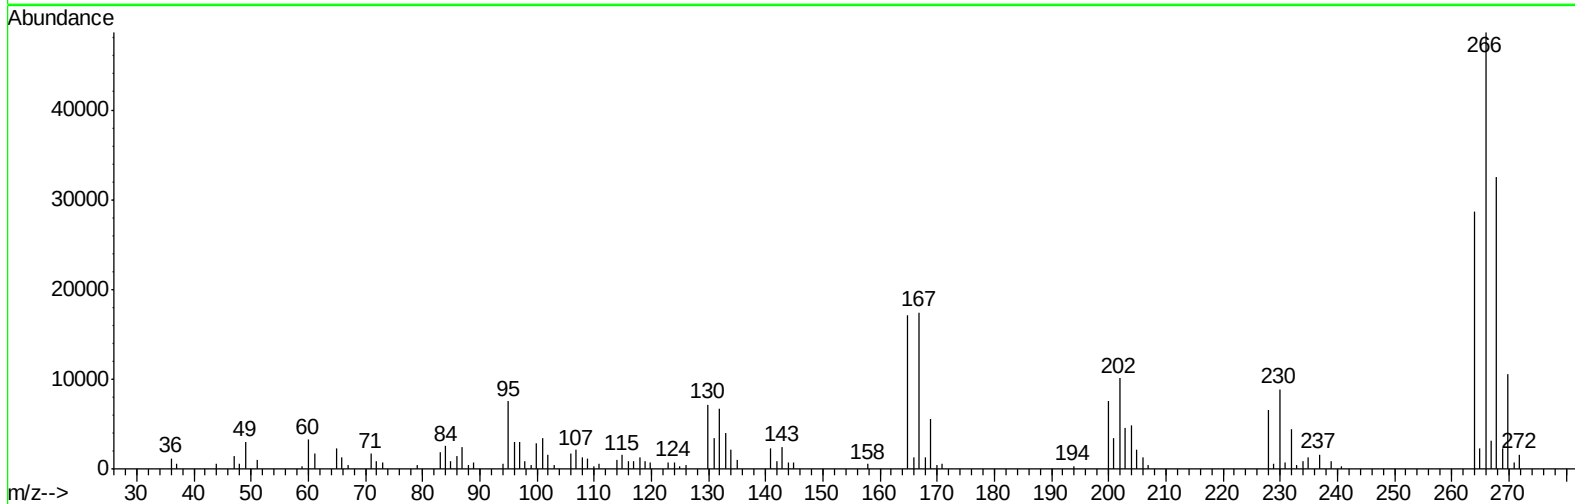


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052915\
Data File : BF079558.D
Acq On : 29 May 2015 13:24
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 05:31:19 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 29 23:13:06 2015
Response via : Initial Calibration

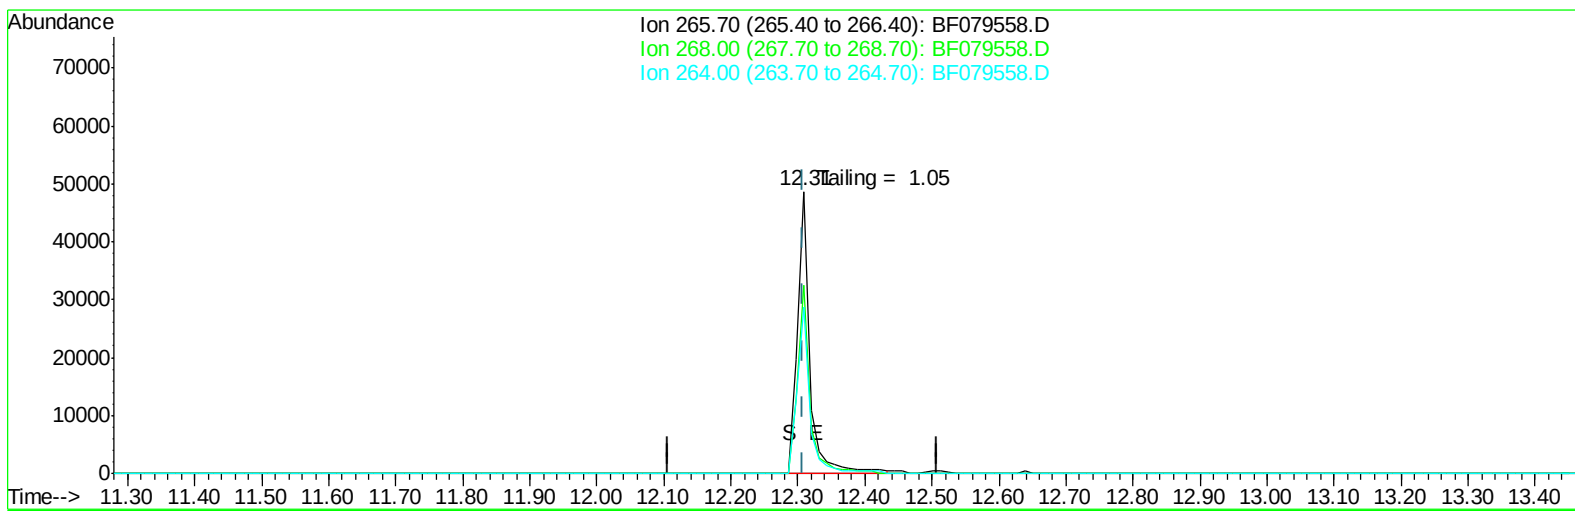

TIC: BF079558.D

(69) Pentachlorophenol (C)



12.308min (-0.000) 3965.16ng

response 63470

Ion	Exp%	Act%
265.70	100	100
268.00	70.10	66.85
264.00	62.50	59.05
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052915\
Data File : BF079558.D
Acq On : 29 May 2015 13:24
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 05:31:19 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 29 23:13:06 2015
Response via : Initial Calibration

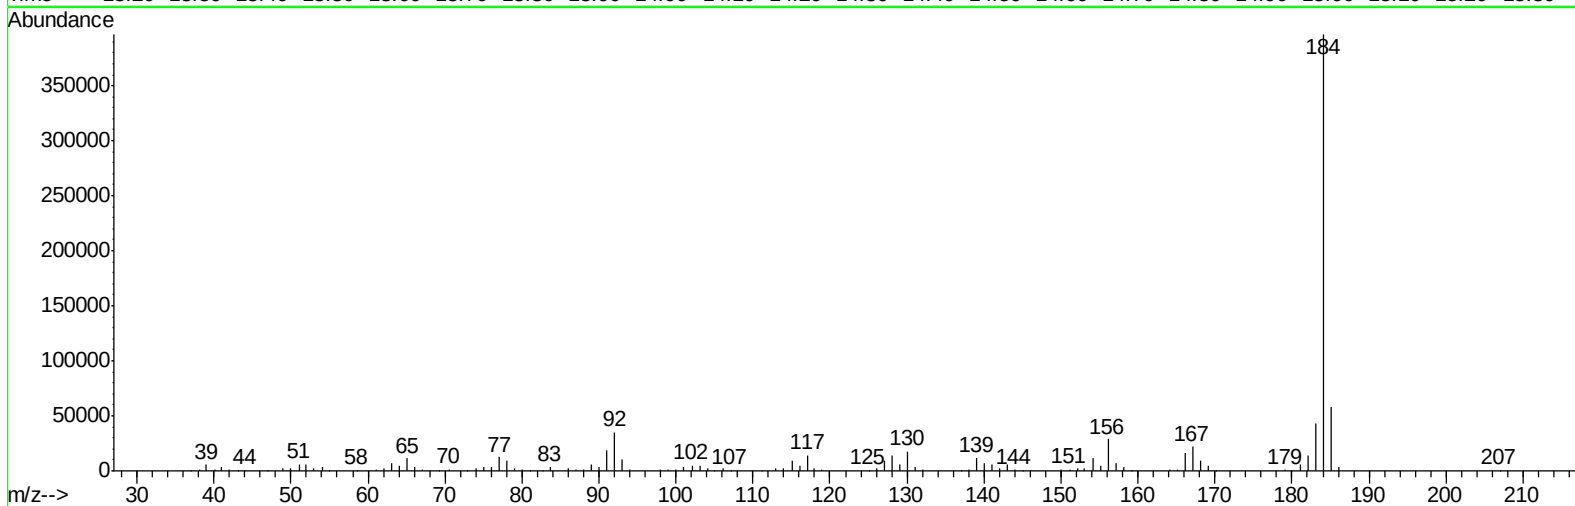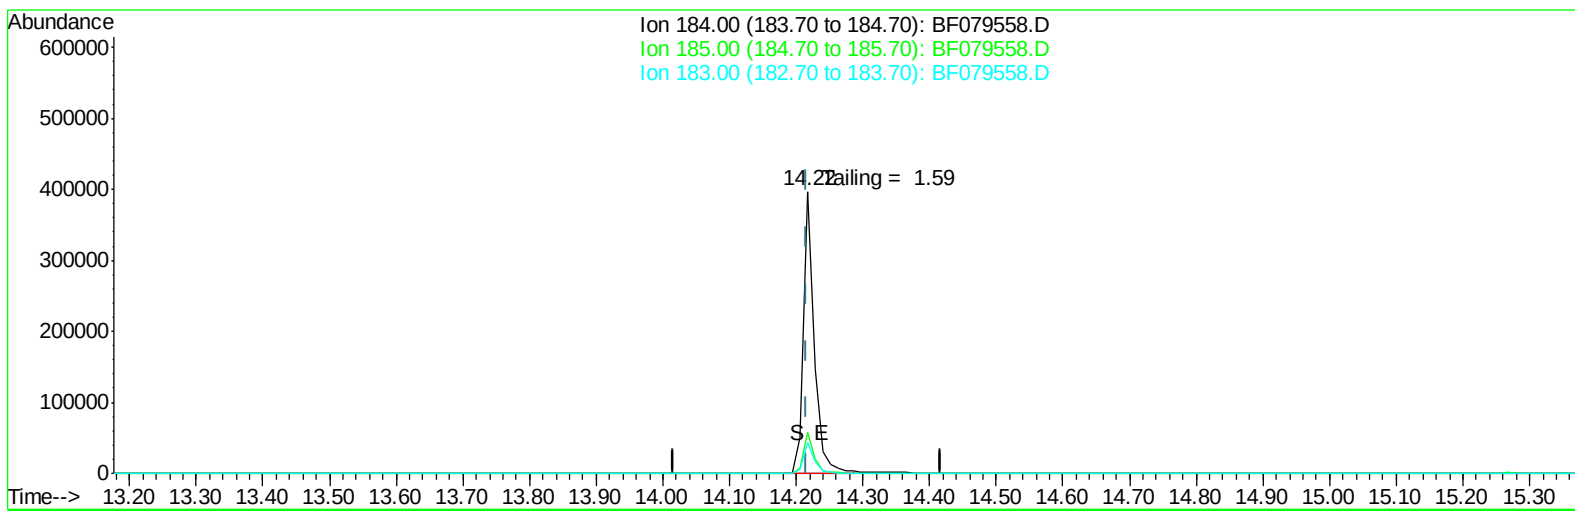

TIC: BF079558.D

(76) Benzidine

14.217min (-0.000) 0.00ng

response 453606

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.64
183.00	10.70	10.84
0.00	0.00	0.00