
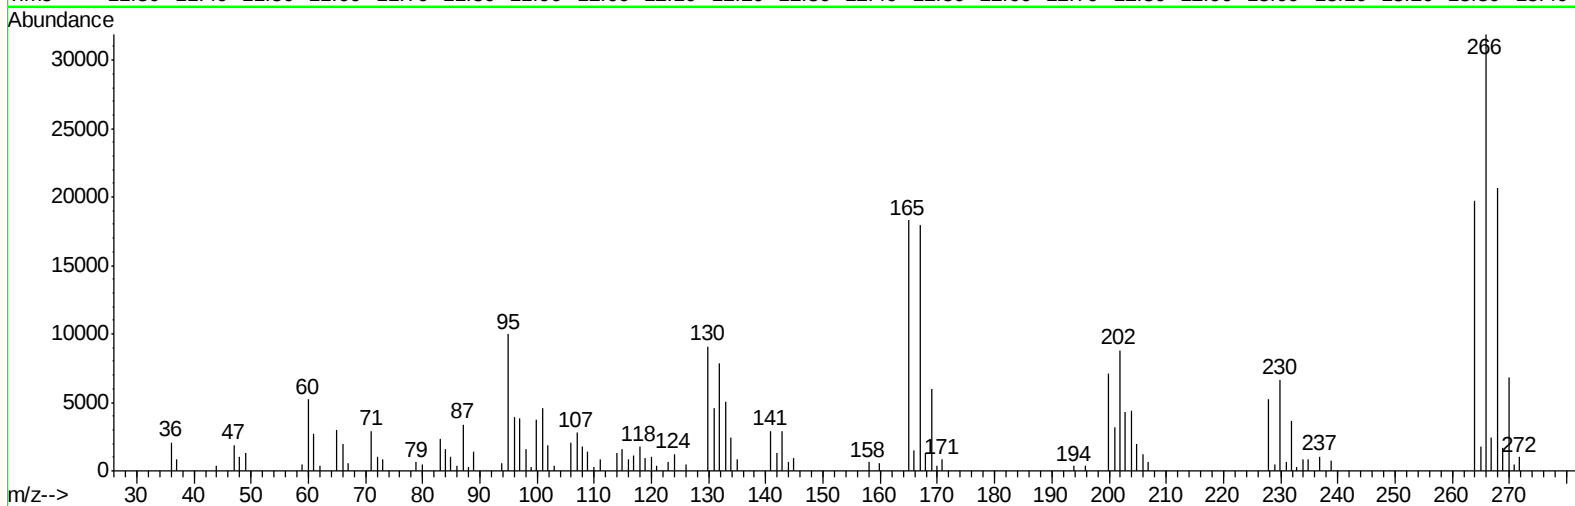


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052915\
Data File : BF079581.D
Acq On : 30 May 2015 2:19
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 05:32:07 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 29 23:13:06 2015
Response via : Initial Calibration

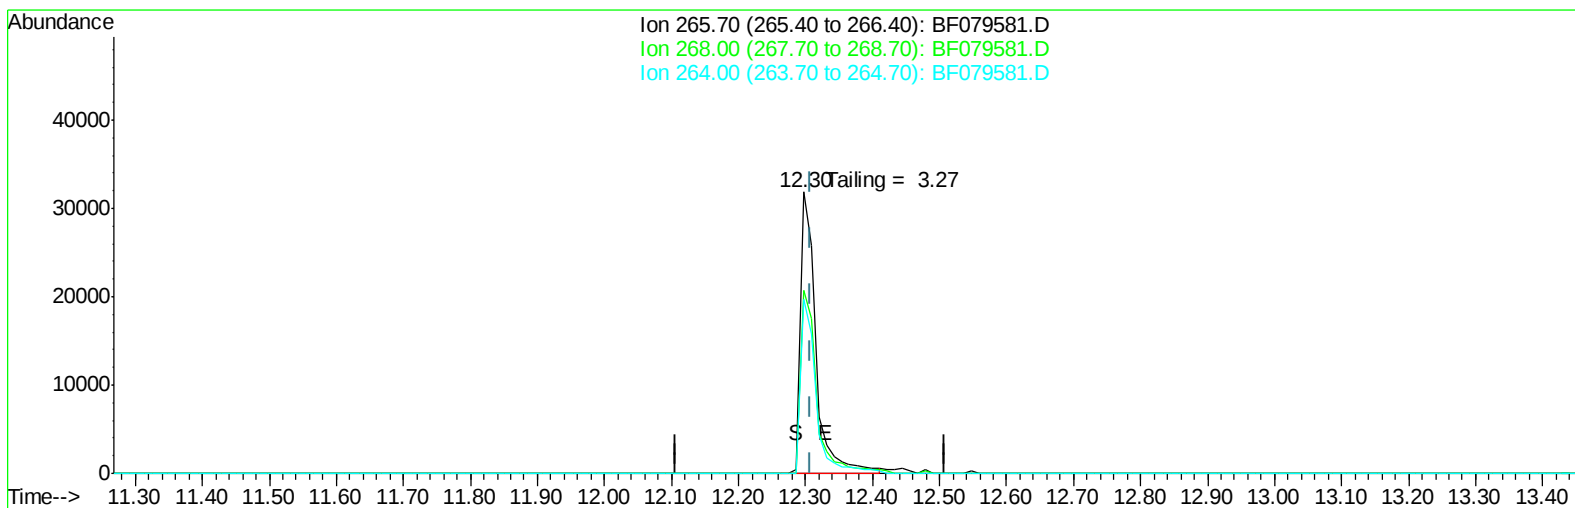

TIC: BF079581.D

(69) Pentachlorophenol (C)




12.297min (-0.011) 54241.93ng

response 52451

Ion	Exp%	Act%
265.70	100	100
268.00	70.10	64.89
264.00	62.50	61.81
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052915\
Data File : BF079581.D
Acq On : 30 May 2015 2:19
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 05:32:07 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 29 23:13:06 2015
Response via : Initial Calibration

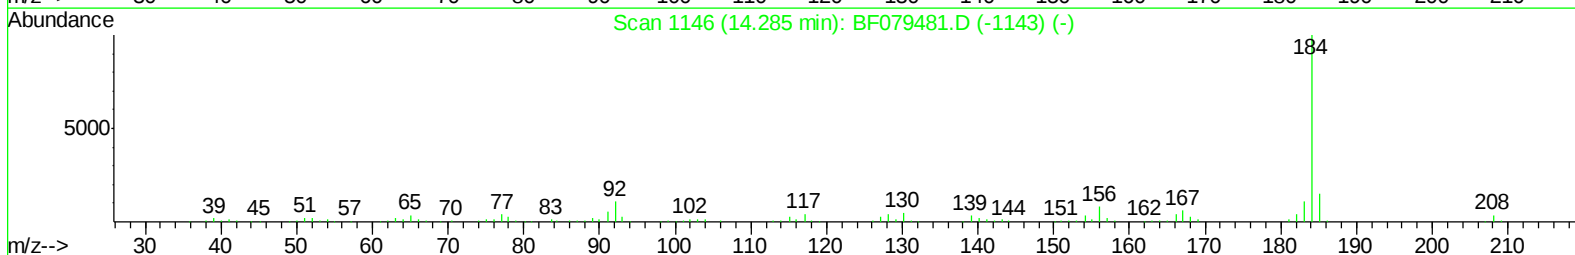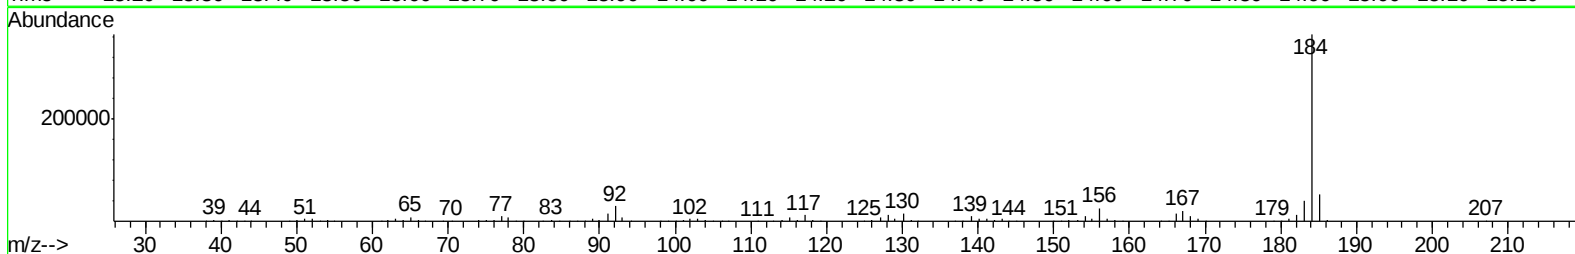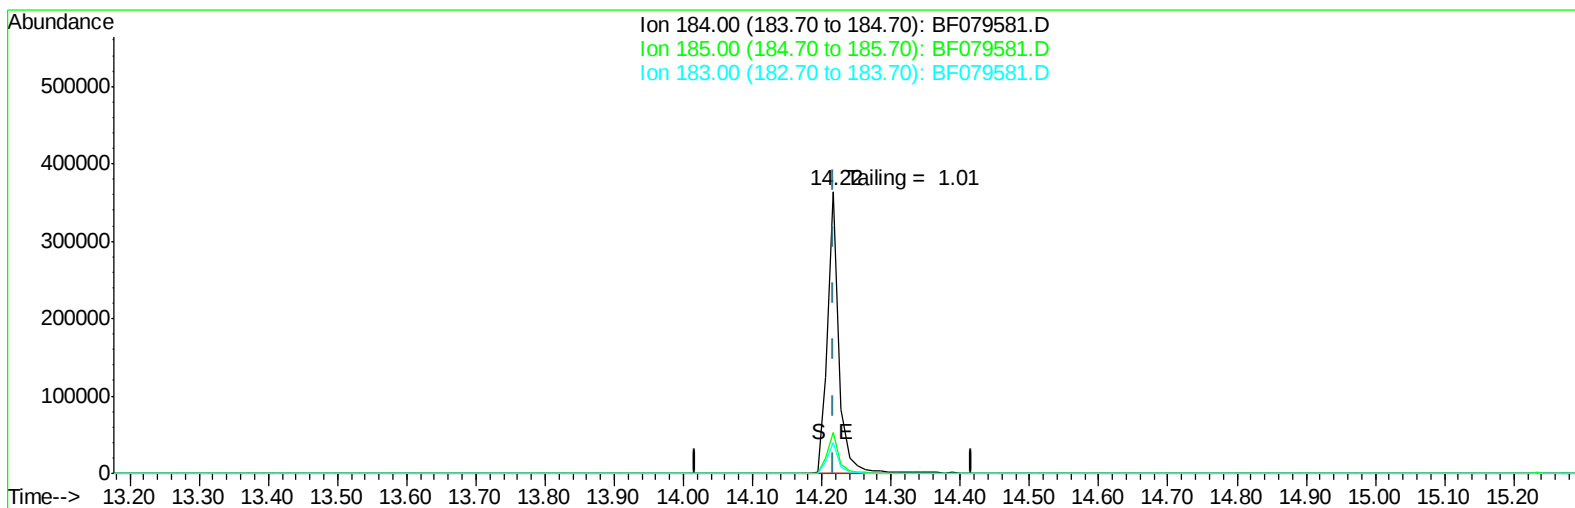

TIC: BF079581.D

(76) Benzidine

14.217min (+0.000) 79478.12ng

response 422177

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.65
183.00	10.70	11.03
0.00	0.00	0.00