

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052915\
 Data File : BF079573.D
 Acq On : 29 May 2015 21:33
 Operator : TP/IZ
 Sample : G2420-35
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FB-5-27-15

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.553	31	32	40	rVV	480986	787926	9.27%	2.899%
2	1.655	40	41	82	rVB	3573787	8501696	100.00%	31.276%
3	4.661	303	304	314	rBV	50179	89306	1.05%	0.329%
4	5.233	351	354	365	rBV	579002	929081	10.93%	3.418%
5	6.547	467	469	477	rBV	553040	595284	7.00%	2.190%
6	6.662	477	479	482	rBV	1640019	1811824	21.31%	6.665%
7	6.947	502	504	507	rBV	400170	398806	4.69%	1.467%
8	7.130	518	520	523	rBV	1554061	1783991	20.98%	6.563%
9	7.656	563	566	568	rBV	1275115	1455148	17.12%	5.353%
10	8.525	640	642	645	rBV	551586	546369	6.43%	2.010%
11	9.873	758	760	763	rBV	2673655	2893241	34.03%	10.643%
12	10.696	829	832	834	rBV	513283	621471	7.31%	2.286%
13	11.668	915	917	920	rBV2	1508682	1895897	22.30%	6.975%
14	12.525	989	992	995	rBV	655830	635204	7.47%	2.337%
15	14.525	1164	1167	1169	rBV	2219925	3038296	35.74%	11.177%
16	15.817	1278	1280	1283	rBV	491097	563090	6.62%	2.071%
17	15.885	1284	1286	1289	rBV	76058	90656	1.07%	0.333%
18	17.646	1437	1440	1447	rBV	413552	545952	6.42%	2.008%


Sum of corrected areas: 27183238

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052915\
Data File : BF079573.D
Acq On : 29 May 2015 21:33
Operator : TP/IZ
Sample : G2420-35
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-5-27-15

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

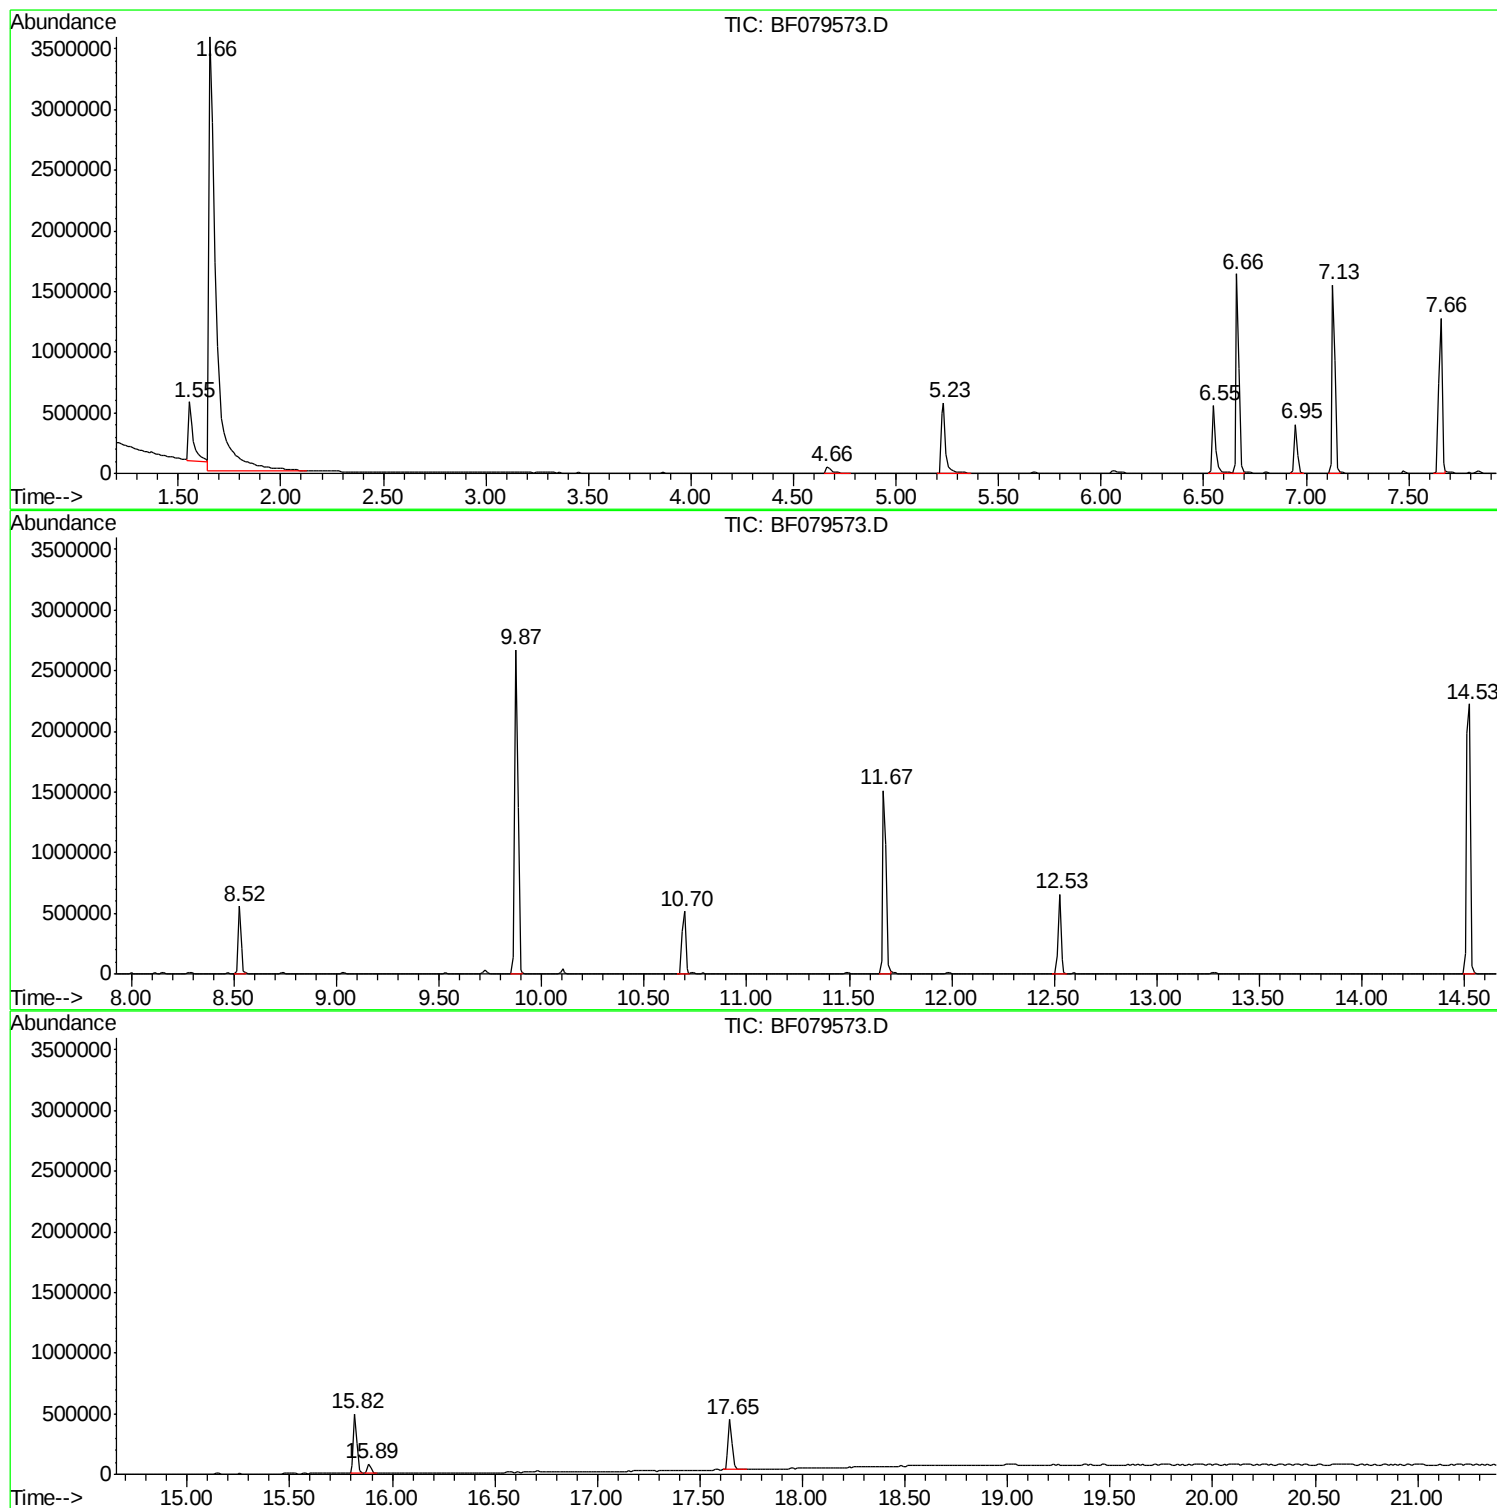

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052915\
Data File : BF079573.D
Acq On : 29 May 2015 21:33
Operator : TP/IZ
Sample : G2420-35
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-5-27-15










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.66	4.48 ng	89306	1,4-Dichlorobenzene-d4	6.95

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56	
2	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39	
3	3-Hexanol	102	C6H14O	000623-37-0	33	
4	3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	25	
5	Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	25	

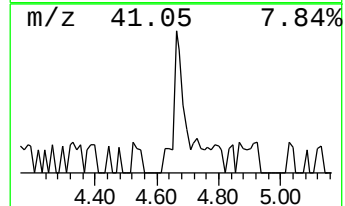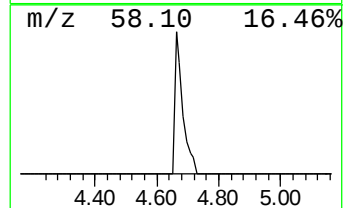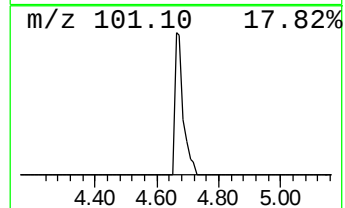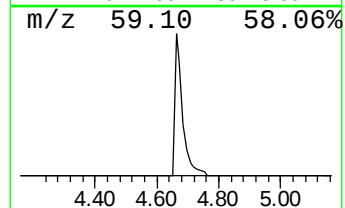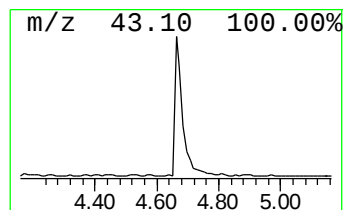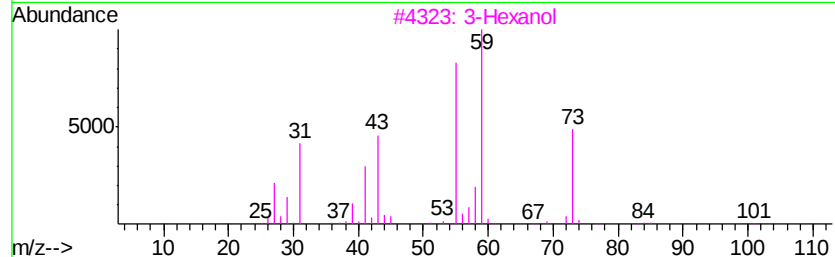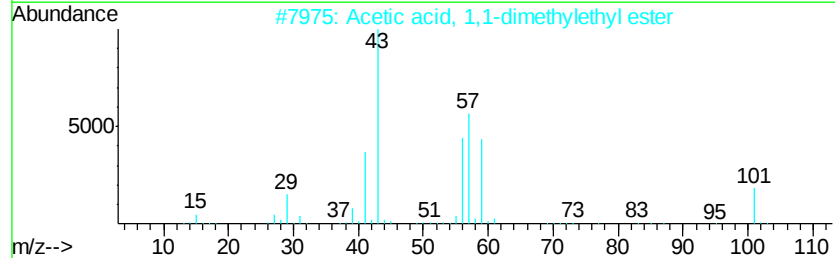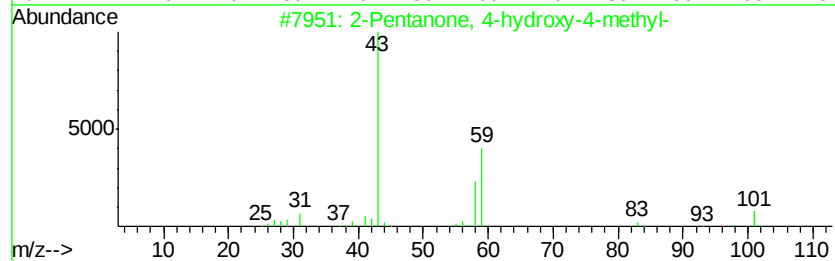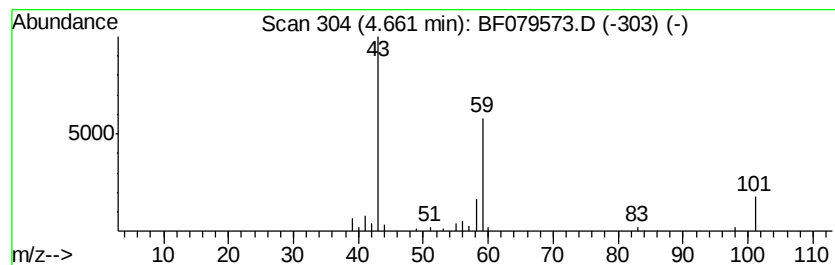

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052915\
Data File : BF079573.D
Acq On : 29 May 2015 21:33
Operator : TP/IZ
Sample : G2420-35
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-5-27-15










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown6.66 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.66	90.86 ng	1811820	1,4-Dichlorobenzene-d4	6.95

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		5-Aminoindole	132	C8H8N2	005192-03-0	10
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

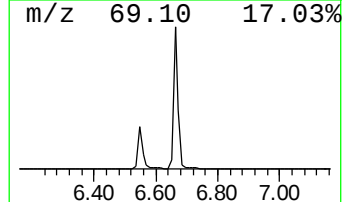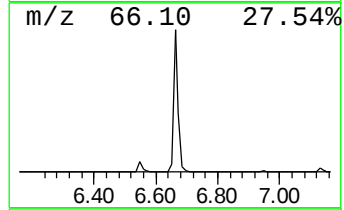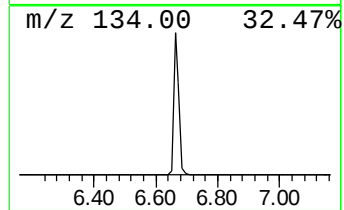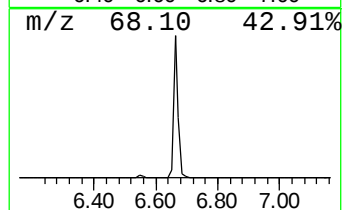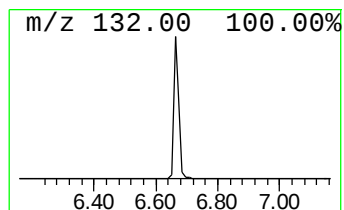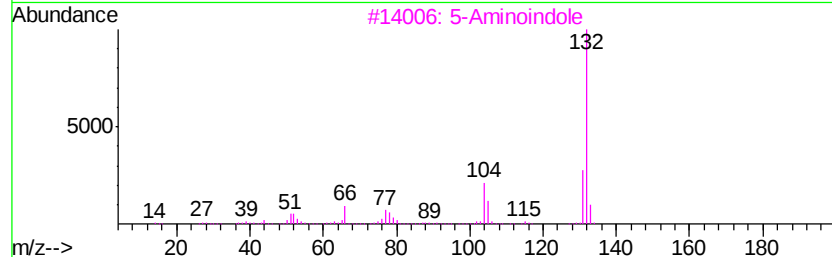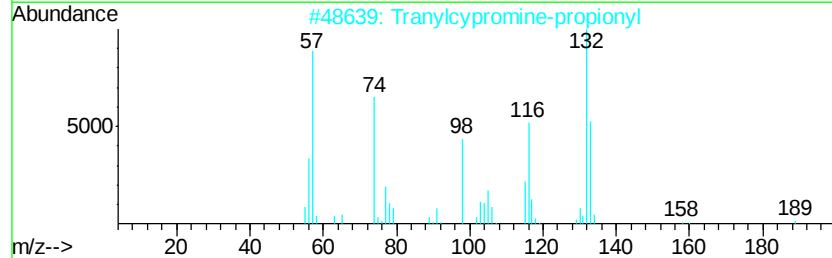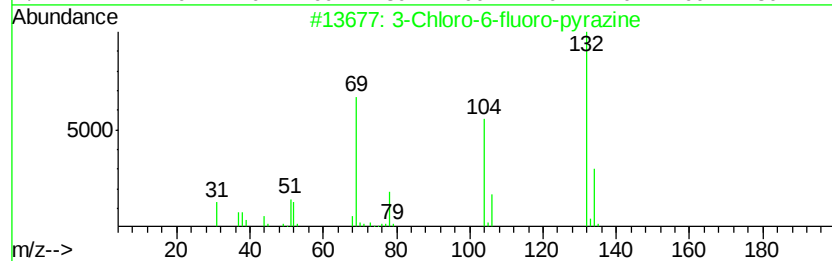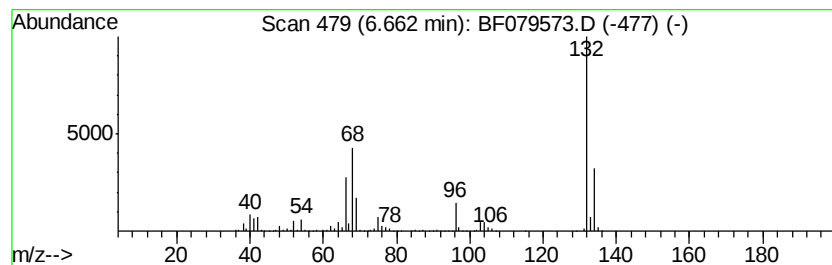

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052915\
Data File : BF079573.D
Acq On : 29 May 2015 21:33
Operator : TP/IZ
Sample : G2420-35
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-5-27-15

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.66	4.5	ng	89306	1	6.95	398806	20.0
unknown6.66	6.66	90.9	ng	1811820	1	6.95	398806	20.0