


Data Path : Z:\HPCHEM1\BNA_F\Data\BF052915\
 Data File : BF079558.D
 Acq On : 29 May 2015 13:24
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 29 17:35:14 2015

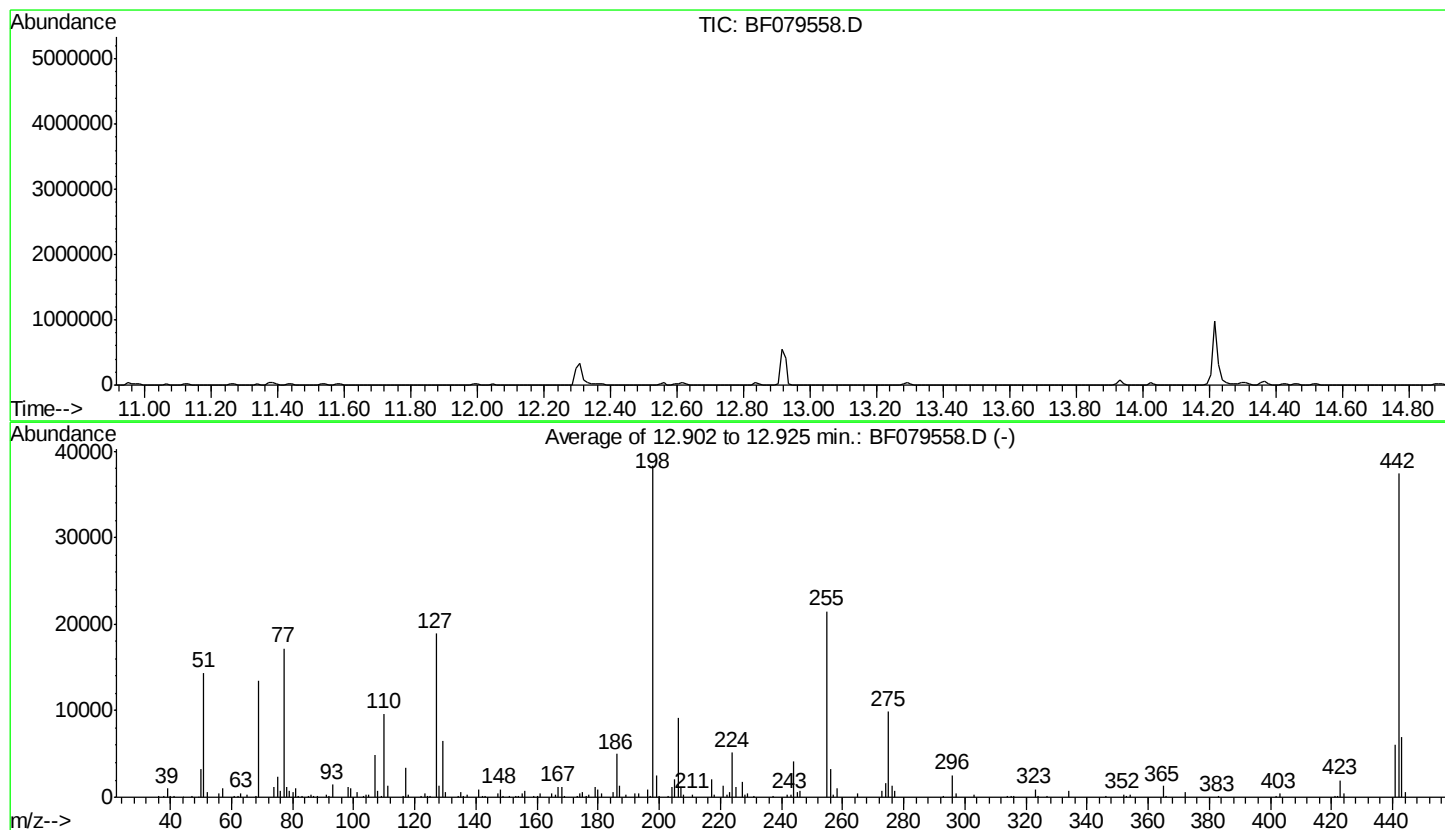

AutoFind: Scans 1025, 1026, 1027; Background Corrected with Scan 1022

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	14367	PASS
68	69	0.00	2	1.4	193	PASS
69	198	0.00	100	35.1	13440	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.3	18901	PASS
197	198	0.00	2	0.3	122	PASS
198	198	100	100	100.0	38331	PASS
199	198	5	9	6.7	2573	PASS
275	198	10	60	25.9	9914	PASS
365	198	1	100	3.3	1281	PASS
441	442	0.01	24	16.2	6055	PASS
442	198	50	100	97.6	37392	PASS
443	442	15	24	18.5	6915	PASS