


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052915\
 Data File : BF079581.D
 Acq On : 30 May 2015 2:19
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 29 23:13:06 2015

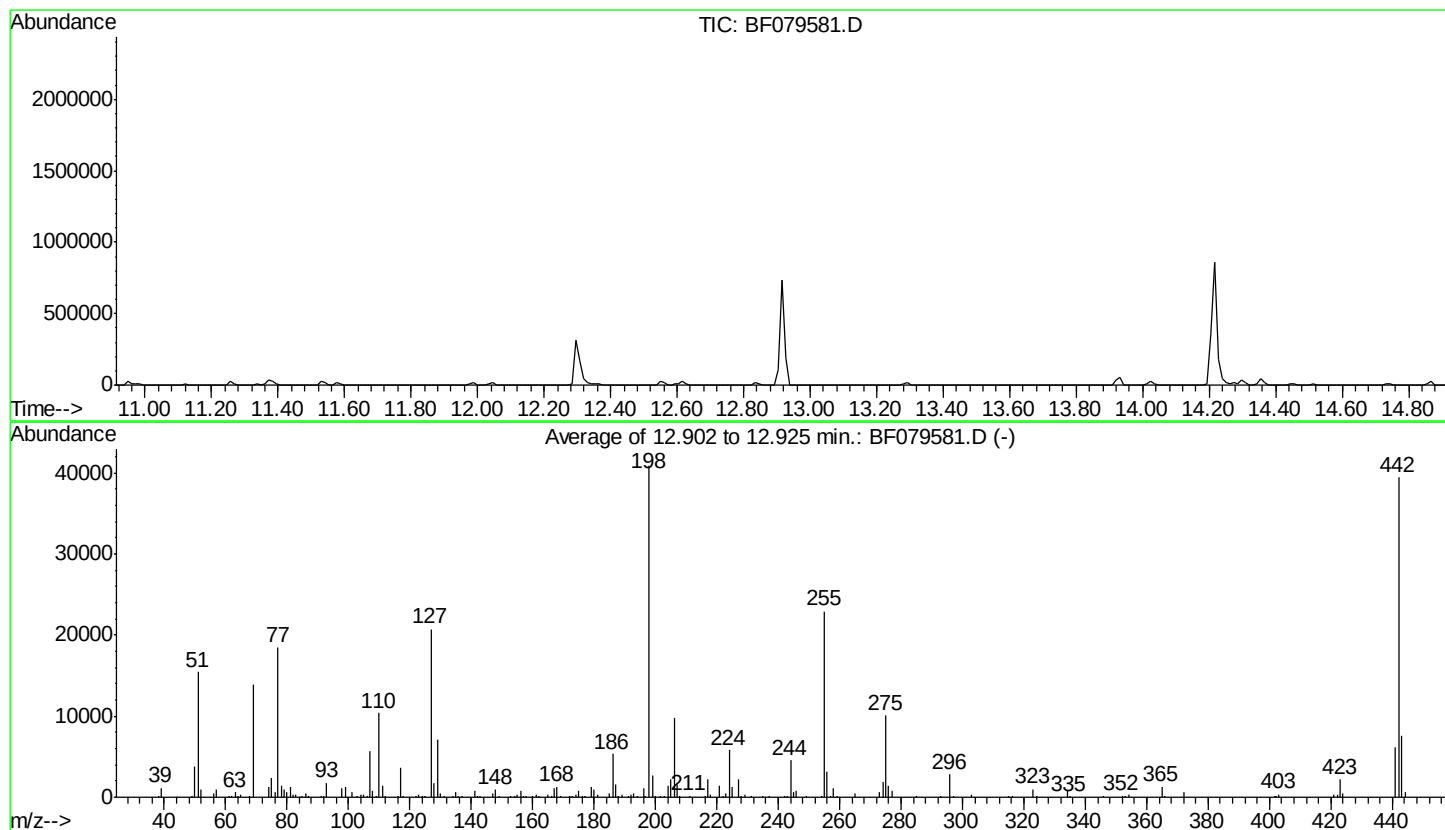

AutoFind: Scans 1025, 1026, 1027; Background Corrected with Scan 1022

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	15435	PASS
68	69	0.00	2	1.2	171	PASS
69	198	0.00	100	34.1	13949	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.7	20741	PASS
197	198	0.00	2	0.4	152	PASS
198	198	100	100	100.0	40889	PASS
199	198	5	9	6.7	2742	PASS
275	198	10	60	24.7	10087	PASS
365	198	1	100	3.2	1296	PASS
441	442	0.01	24	15.6	6147	PASS
442	198	50	100	96.5	39458	PASS
443	442	15	24	19.4	7655	PASS