

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052916\
 Data File : BF087560.D
 Acq On : 30 May 2016 20:30
 Operator : UM/SJ
 Sample : H3317-15
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 GMW-02

Quant Time: May 31 00:42:38 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 25 16:26:52 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	104420	20.00	ng	-0.05
21) Naphthalene-d8	9.51	136	416746	20.00	ng	-0.05
38) Acenaphthene-d10	12.33	164	191606	20.00	ng	-0.06
63) Phenanthrene-d10	14.74	188	356304	20.00	ng	-0.03
75) Chrysene-d12	18.47	240	232726	20.00	ng	-0.01
86) Perylene-d12	20.15	264	212742	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.39	112	343430	57.79	ng	-0.02
7) Phenol-d6	7.06	99	272283	33.91	ng	-0.01
23) Nitrobenzene-d5	8.39	82	737190	89.15	ng	-0.06
41) 2,4,6-Tribromophenol	13.63	330	234957	127.60	ng	-0.05
44) 2-Fluorobiphenyl	11.28	172	1243764	91.51	ng	-0.06
78) Terphenyl-d14	17.09	244	1007805	92.07	ng	-0.05
Target Compounds						
15) Benzyl Alcohol	7.70	79	13843	2.36	ng	# 43
19) n-Nitroso-di-n-propylamine	8.39	70	92806	15.50	ng	# 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052916\
Data File : BF087560.D
Acq On : 30 May 2016 20:30
Operator : UM/SJ
Sample : H3317-15
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GMW-02

Quant Time: May 31 00:42:38 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 25 16:26:52 2016
Response via : Initial Calibration

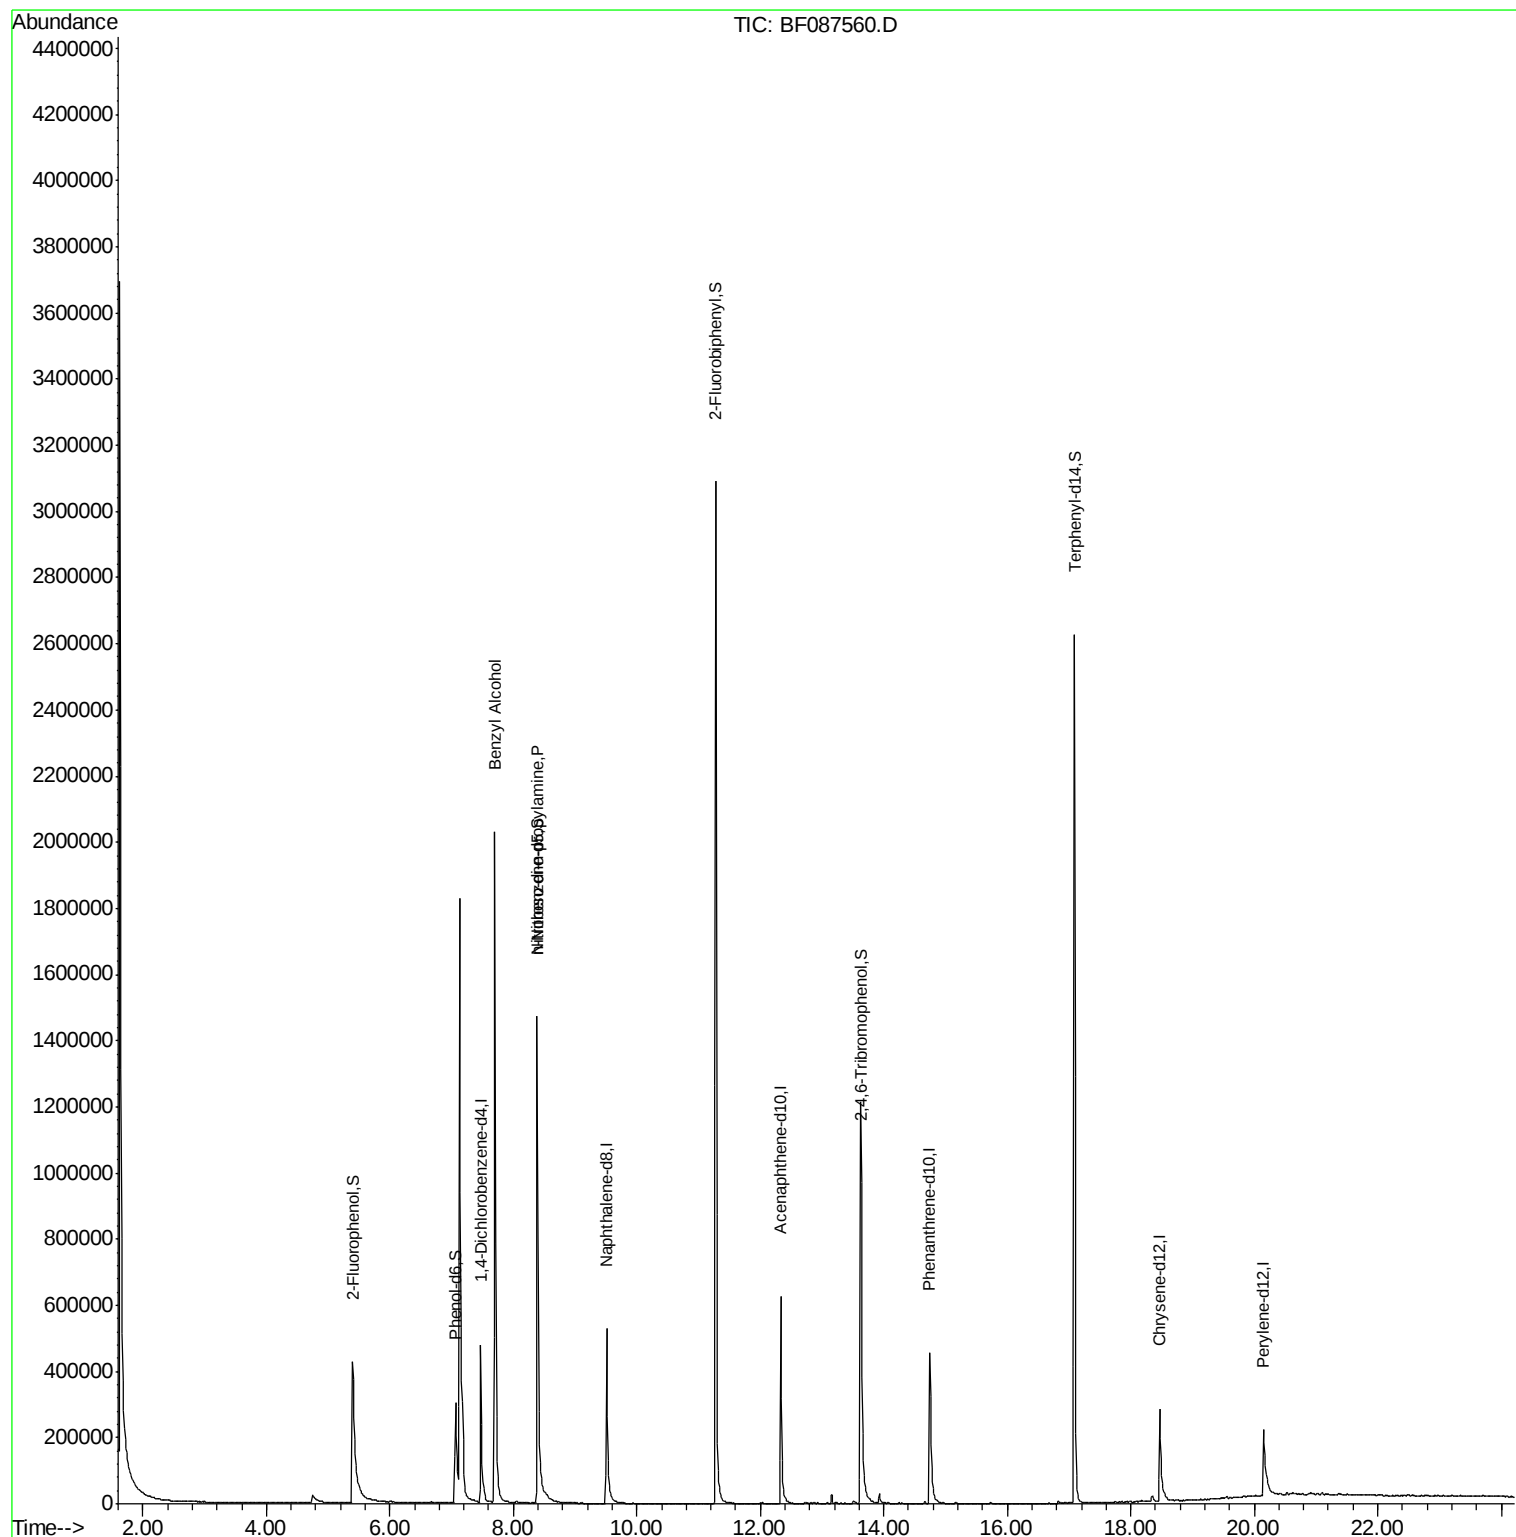

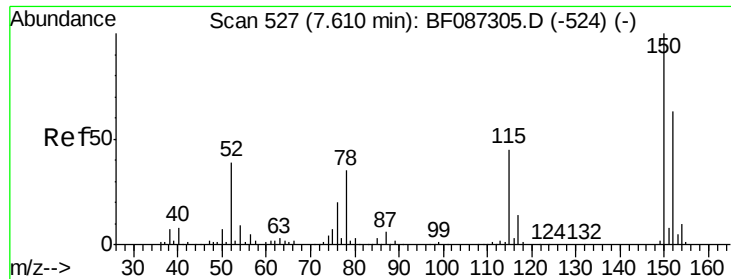

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.47 min Scan# 515

Delta R.T. -0.05 min

Lab File: BF087560.D

Acq: 30 May 2016 20:30

Instrument :

BNA_F

ClientSampleId :

GMW-02


Tgt Ion:152 Resp: 104420

Ion Ratio Lower Upper

152 100

150 156.7 125.8 188.6




115 65.6 51.5 77.3

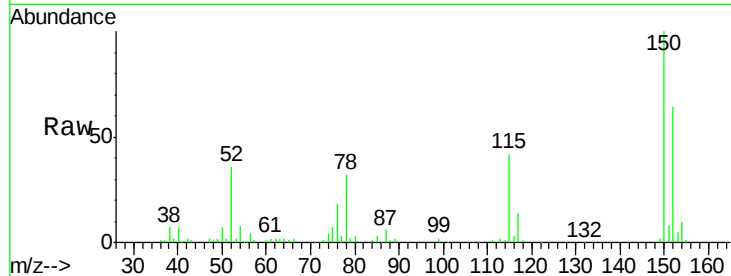

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

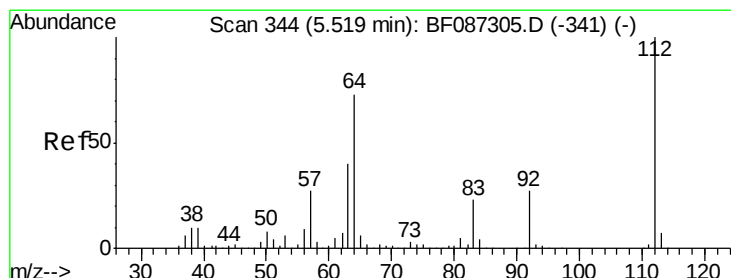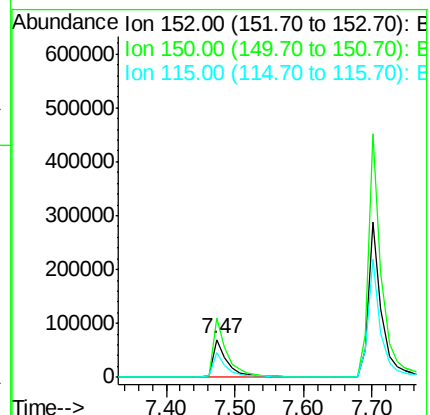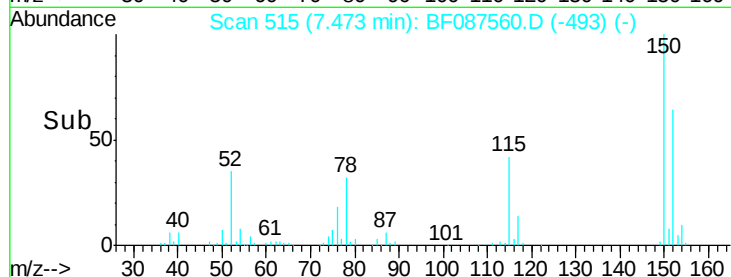

#5

2-Fluorophenol

Concen: 57.79 ng

RT: 5.39 min Scan# 333

Delta R.T. -0.02 min

Lab File: BF087560.D

Acq: 30 May 2016 20:30


Tgt Ion:112 Resp: 343430

Ion Ratio Lower Upper

112 100

64 77.4 52.1 78.1



63 44.0 25.7 38.5

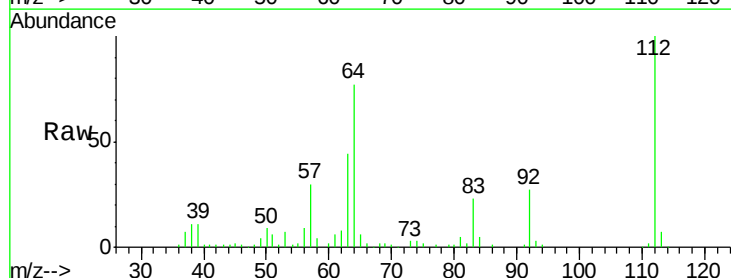

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

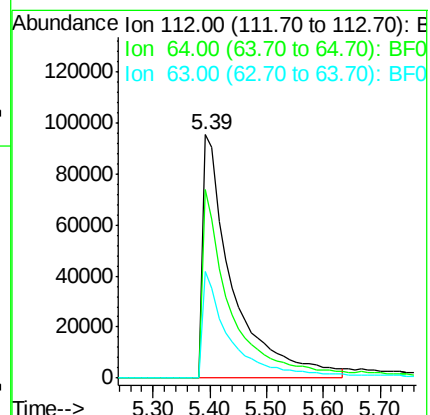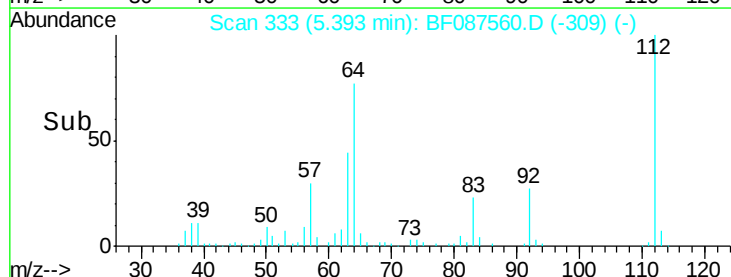



#7

Phenol-d6

Concen: 33.91 ng

RT: 7.06 min Scan# 479

Delta R.T. -0.01 min

Lab File: BF087560.D

Acq: 30 May 2016 20:30

Instrument :

BNA_F

ClientSampleId :

GMW-02





Tgt Ion: 99 Resp: 272283

Ion Ratio Lower Upper

99 100

42 29.0 13.6 20.4#

71 39.3 24.6 36.8#

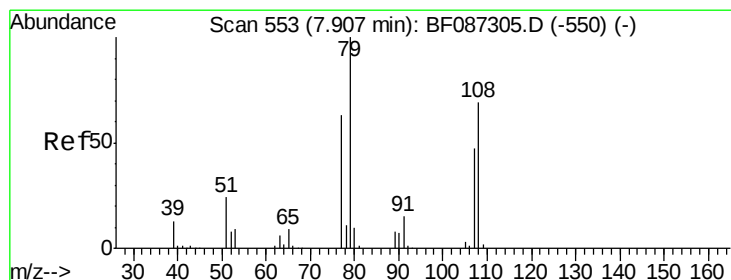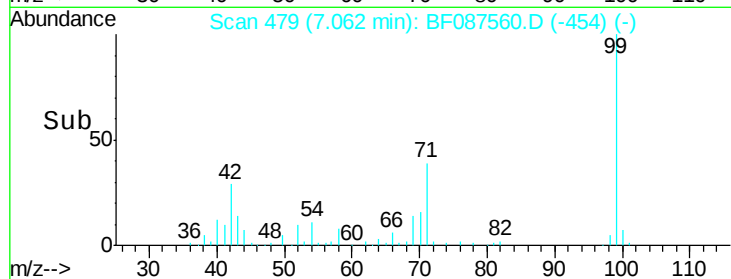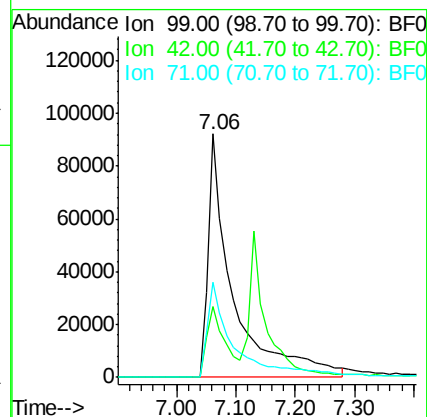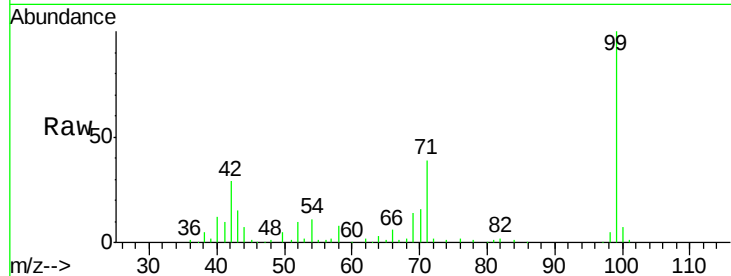

#15

Benzyl Alcohol

Concen: 2.36 ng

RT: 7.70 min Scan# 535

Delta R.T. -0.11 min

Lab File: BF087560.D

Acq: 30 May 2016 20:30




Tgt Ion: 79 Resp: 13843


Ion Ratio Lower Upper

79 100

108 28.4 68.4 102.6#

77 101.5 50.6 76.0#


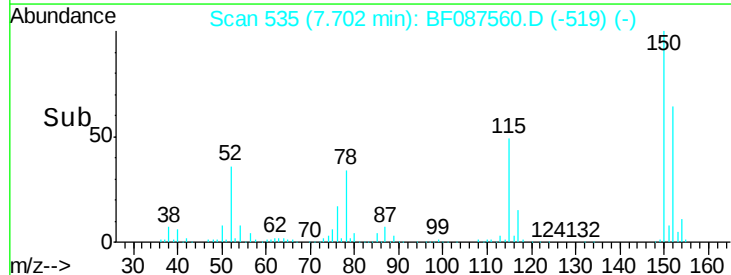
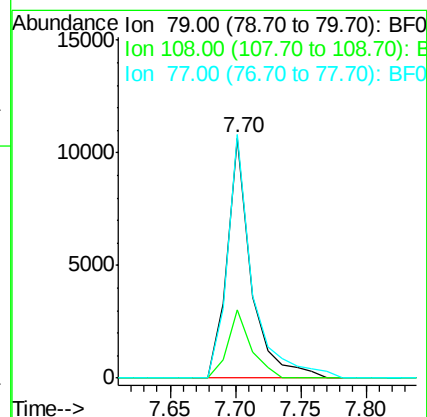
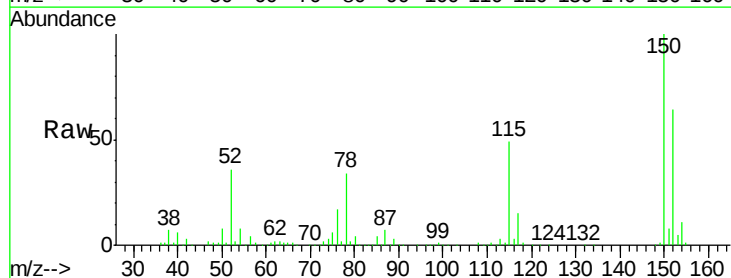


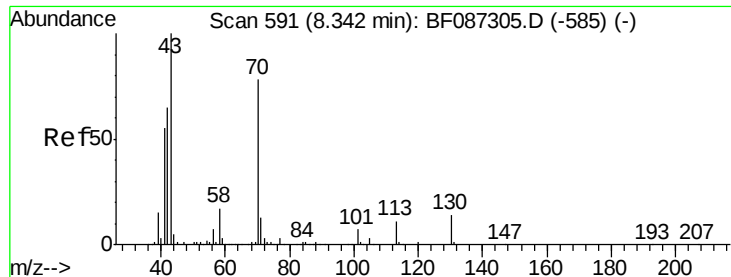

#19
n-Nitroso-di-n-propylamine
Concen: 15.50 ng
RT: 8.39 min Scan# 595
Delta R.T. 0.14 min
Lab File: BF087560.D
Acq: 30 May 2016 20:30




Instrument :
BNA_F
ClientSampleId :
GMW-02


Tgt Ion: 70 Resp: 92806
Ion Ratio Lower Upper
70 100
42 68.5 43.1 64.7#
101 0.0 8.1 12.1#
130 1.4 18.6 28.0#

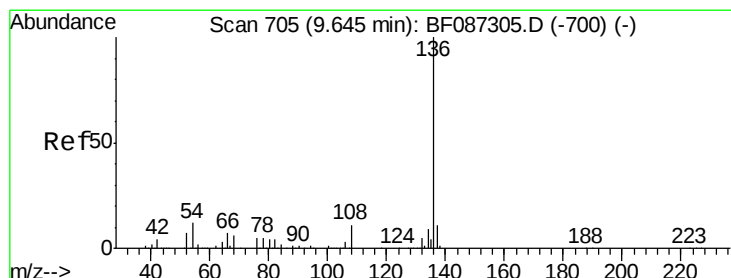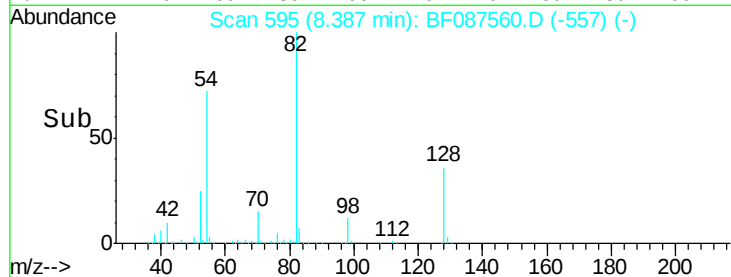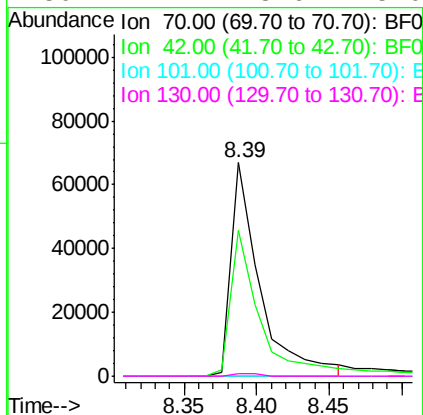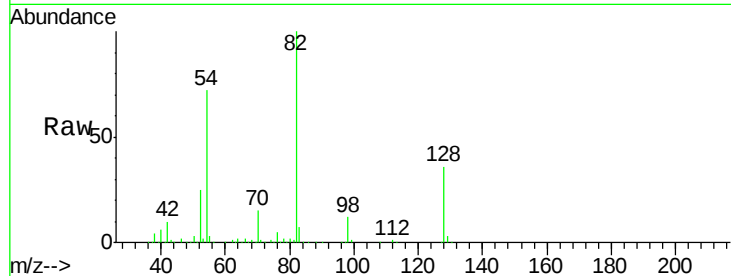

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 9.51 min Scan# 693
Delta R.T. -0.05 min
Lab File: BF087560.D
Acq: 30 May 2016 20:30

Tgt Ion: 136 Resp: 416746
Ion Ratio Lower Upper
136 100
137 10.8 8.8 13.2
54 10.9 5.0 7.4#
68 5.3 4.4 6.6

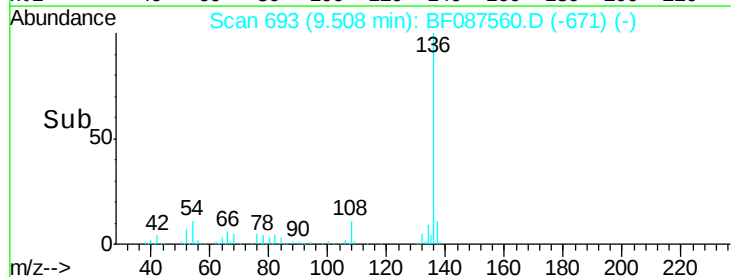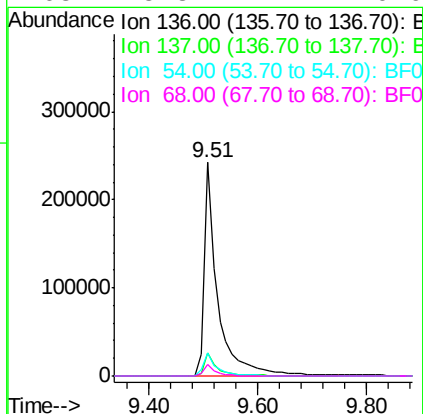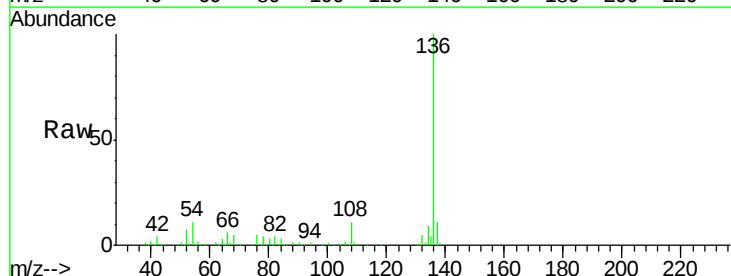


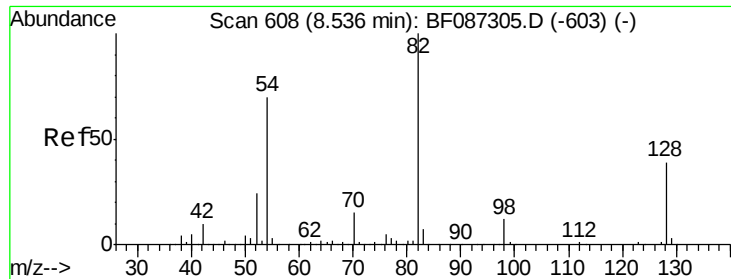




#23
 Nitrobenzene-d5
 Concen: 89.15 ng
 RT: 8.39 min Scan# 595
 Delta R.T. -0.06 min
 Lab File: BF087560.D
 Acq: 30 May 2016 20:30

Instrument :
 BNA_F
 ClientSampleId :
 GMW-02

Tgt Ion: 82 Resp: 737190
 Ion Ratio Lower Upper
 82 100
 128 35.7 40.6 61.0#
 54 71.8 38.1 57.1#

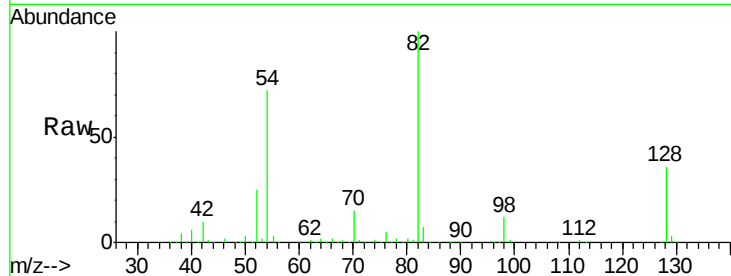


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

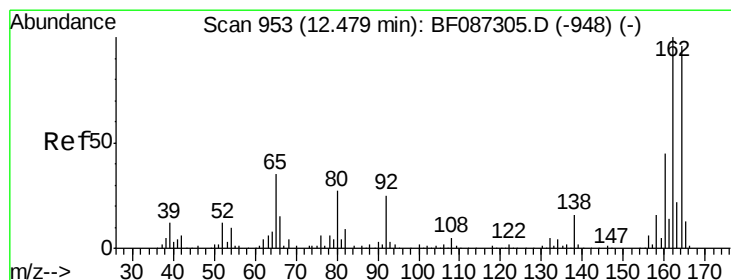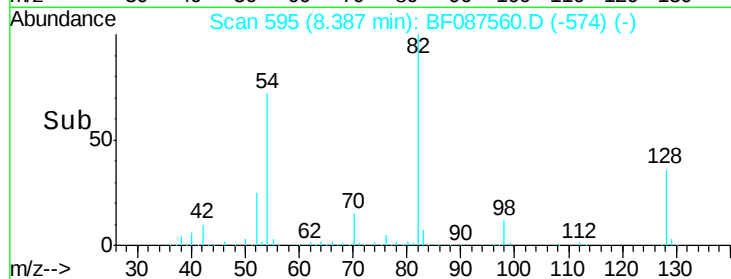
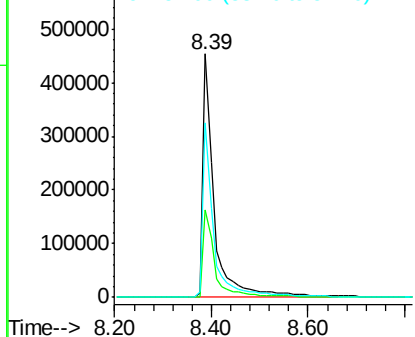



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 12.33 min Scan# 940
 Delta R.T. -0.06 min
 Lab File: BF087560.D
 Acq: 30 May 2016 20:30

Tgt Ion: 164 Resp: 191606
 Ion Ratio Lower Upper
 164 100
 162 103.2 82.8 124.2
 160 48.0 36.9 55.3

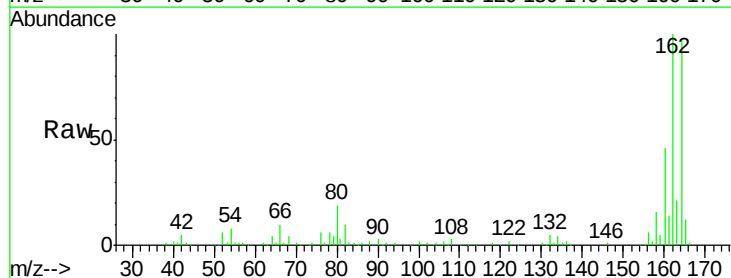

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

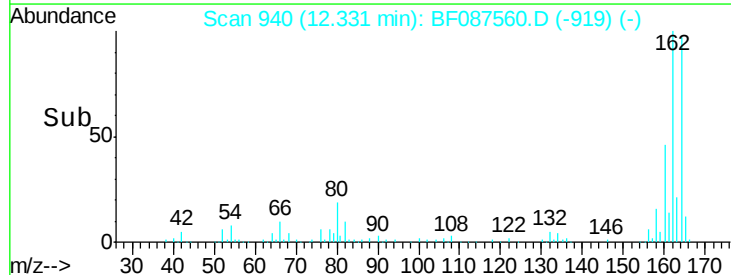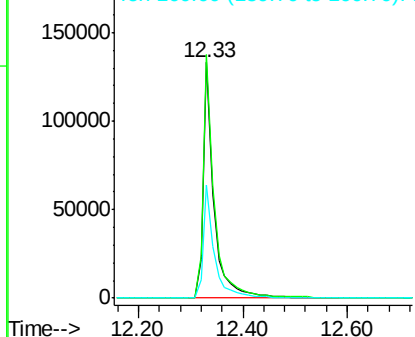


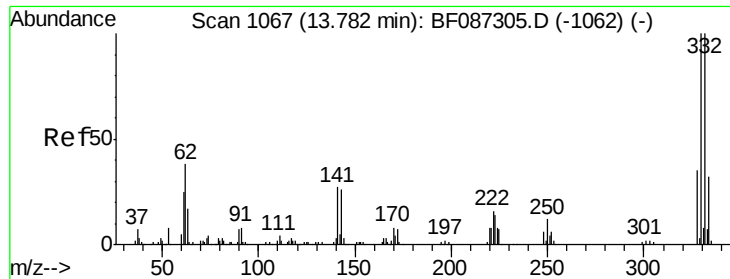




#41
 2,4,6-Tribromophenol
 Concen: 127.60 ng
 RT: 13.63 min Scan# 1054
 Delta R.T. -0.05 min
 Lab File: BF087560.D
 Acq: 30 May 2016 20:30

Instrument :
 BNA_F
 ClientSampleId :
 GMW-02

Tgt Ion:330 Resp: 234957
 Ion Ratio Lower Upper
 330 100
 332 97.8 79.0 118.4
 141 45.0 31.2 46.8

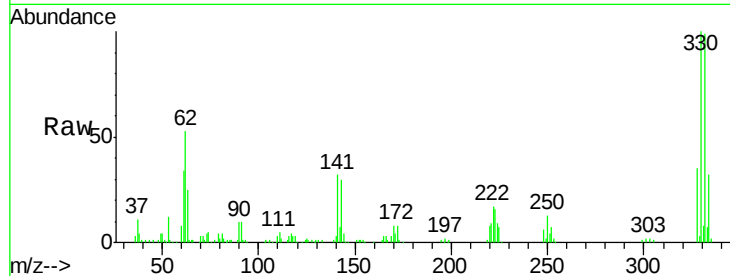


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

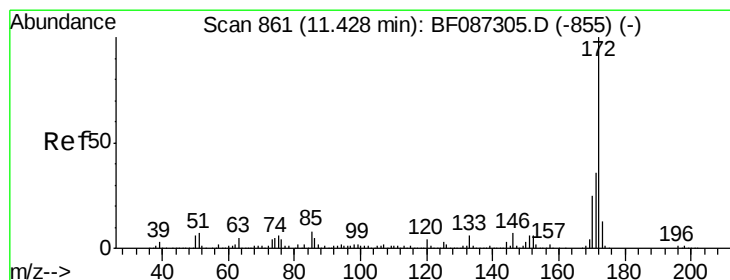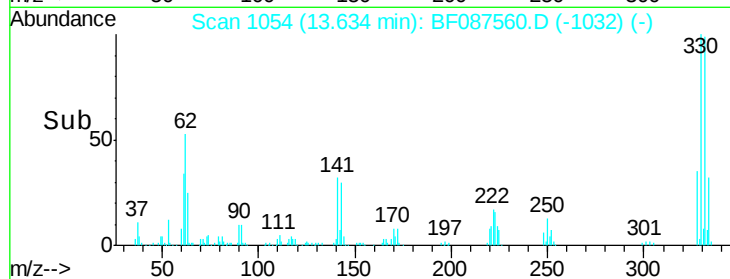
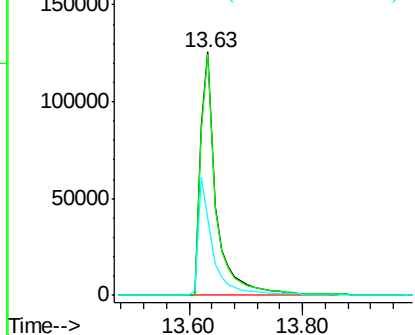



#44
 2-Fluorobiphenyl
 Concen: 91.51 ng
 RT: 11.28 min Scan# 848
 Delta R.T. -0.06 min
 Lab File: BF087560.D
 Acq: 30 May 2016 20:30

Tgt Ion:172 Resp: 1243764
 Ion Ratio Lower Upper
 172 100
 171 36.3 29.0 43.6
 170 24.2 19.8 29.8

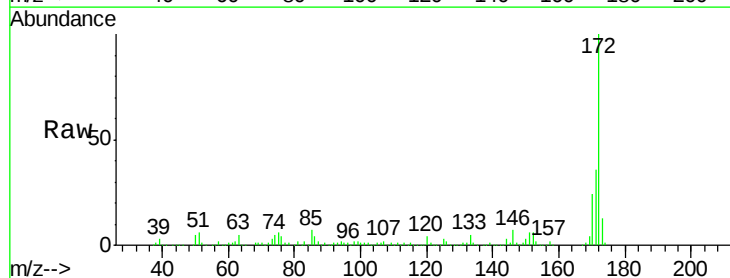

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

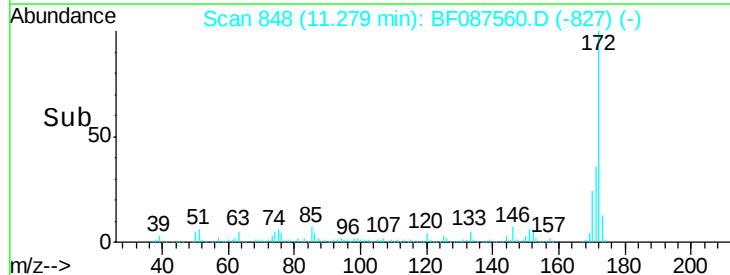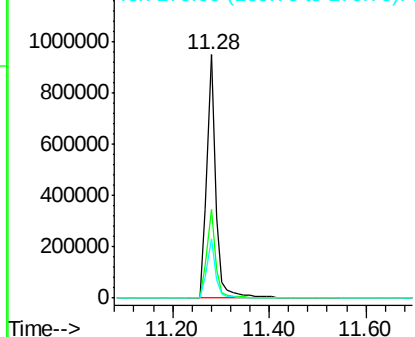


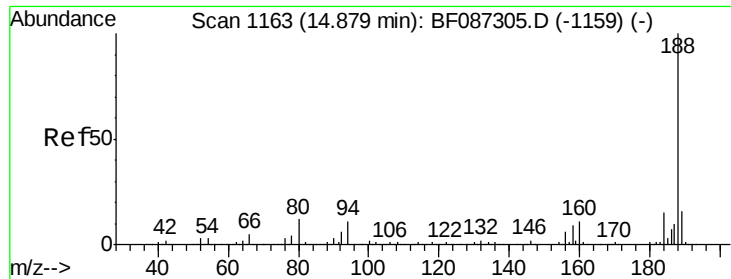




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 14.74 min Scan# 1151
Delta R.T. -0.03 min
Lab File: BF087560.D
Acq: 30 May 2016 20:30

Instrument :
BNA_F
ClientSampleId :
GMW-02

Tgt Ion:188 Resp: 356304
Ion Ratio Lower Upper
188 100
94 9.5 6.8 10.2
80 10.7 7.1 10.7#

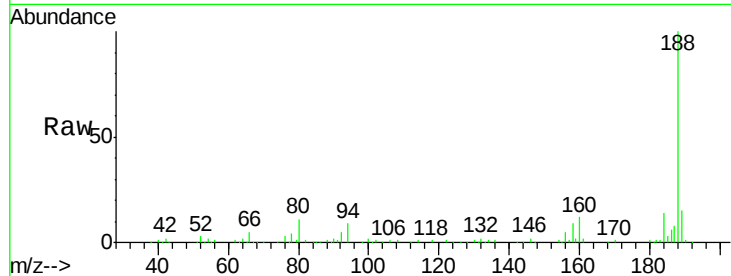


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

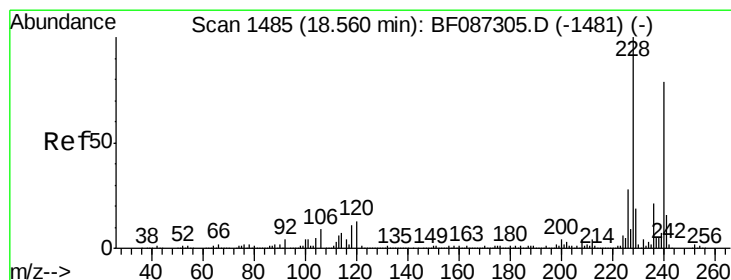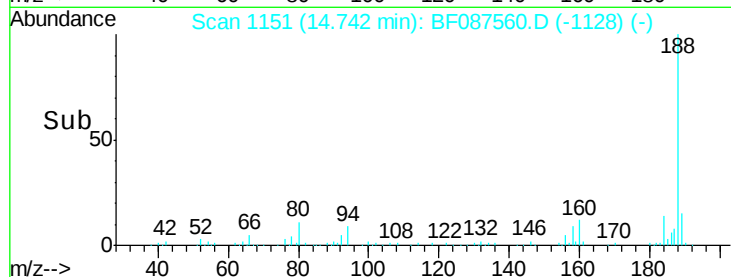
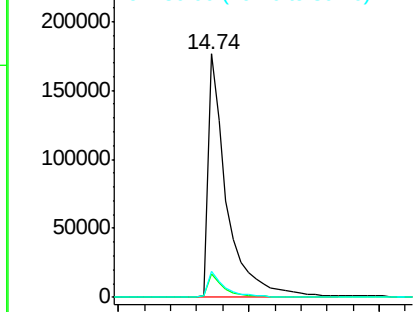



#75
Chrysene-d12
Concen: 20.00 ng
RT: 18.47 min Scan# 1477
Delta R.T. -0.01 min
Lab File: BF087560.D
Acq: 30 May 2016 20:30

Tgt Ion:240 Resp: 232726
Ion Ratio Lower Upper
240 100
120 10.3 11.2 16.8#
236 25.6 21.2 31.8

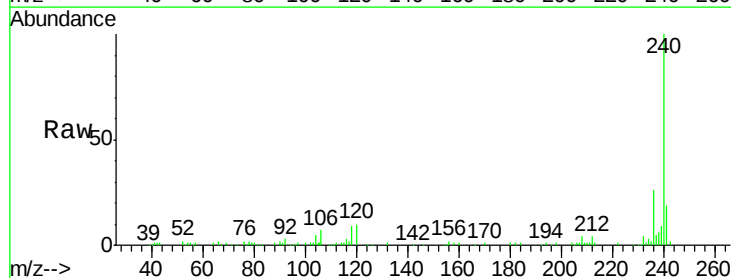

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

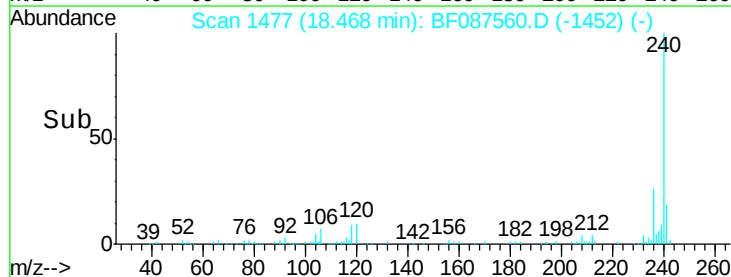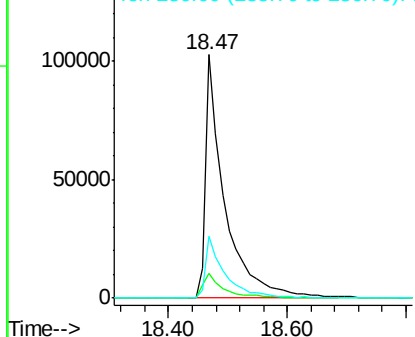

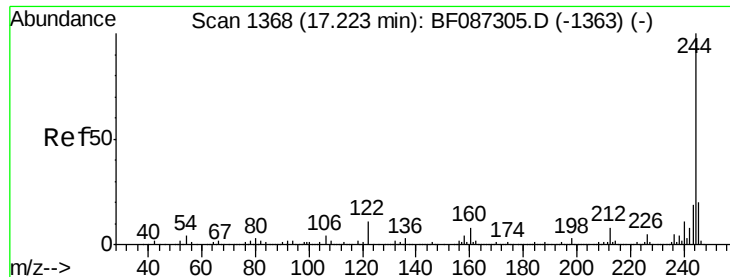

#78

Terphenyl-d14

Concen: 92.07 ng

RT: 17.09 min Scan# 1356

Delta R.T. -0.05 min

Lab File: BF087560.D

Acq: 30 May 2016 20:30

Instrument :

BNA_F

ClientSampleId :

GMW-02


Tgt Ion:244 Resp: 1007805

Ion Ratio Lower Upper

244 100

212 8.2 6.2 9.2




122 13.9 12.0 18.0

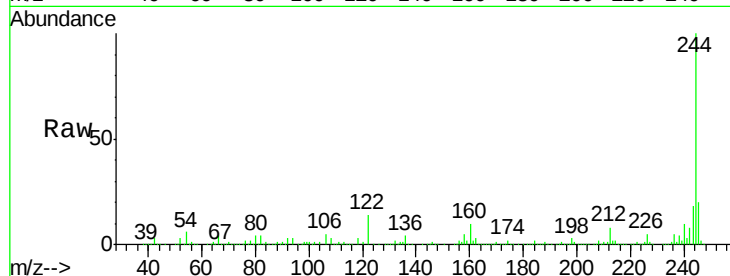

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

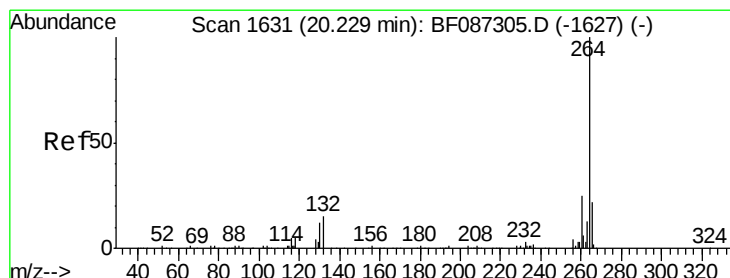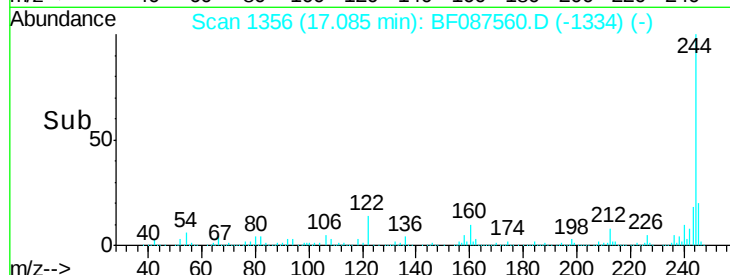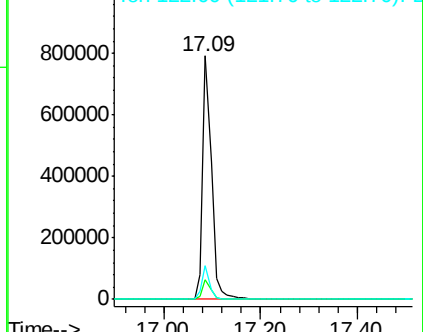

#86

Perylene-d12

Concen: 20.00 ng

RT: 20.15 min Scan# 1624

Delta R.T. 0.01 min

Lab File: BF087560.D

Acq: 30 May 2016 20:30


Tgt Ion:264 Resp: 212742

Ion Ratio Lower Upper

264 100

260 23.6 19.5 29.3

265 22.2 17.3 25.9

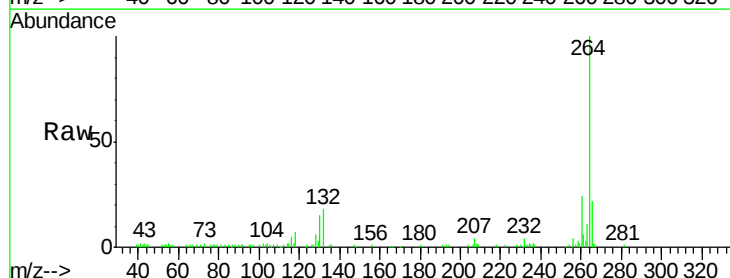

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

