

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052916\
 Data File : BF087569.D
 Acq On : 31 May 2016 2:11
 Operator : UM/SJ
 Sample : H3249-06
 Misc :
 ALS Vial : 87 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-25

Quant Time: May 31 03:10:05 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 31 00:45:12 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	105252	20.00	ng	0.01
21) Naphthalene-d8	9.52	136	424743	20.00	ng	0.01
38) Acenaphthene-d10	12.34	164	199830	20.00	ng	0.01
63) Phenanthrene-d10	14.77	188	344964	20.00	ng	0.02
75) Chrysene-d12	18.49	240	251564	20.00	ng	0.05
86) Perylene-d12	20.19	264	191846	20.00	ng	0.07
System Monitoring Compounds						
5) 2-Fluorophenol	5.40	112	348736	58.22	ng	0.03
7) Phenol-d6	7.06	99	257594	31.83	ng	0.02
23) Nitrobenzene-d5	8.40	82	803269	95.31	ng	-0.01
41) 2,4,6-Tribromophenol	13.63	330	221449	115.32	ng	0.00
44) 2-Fluorobiphenyl	11.28	172	1305986	92.14	ng	-0.01
78) Terphenyl-d14	17.10	244	1117892	94.47	ng	0.00
Target Compounds						
15) Benzyl Alcohol	7.70	79	13971	2.37	ng	# 46
19) n-Nitroso-di-n-propylamine	8.40	70	97997	16.24	ng	# 79
50) 2,6-Dinitrotoluene	12.34	165	19789	6.14	ng	# 18

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052916\
Data File : BF087569.D
Acq On : 31 May 2016 2:11
Operator : UM/SJ
Sample : H3249-06
Misc :
ALS Vial : 87 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-25

Quant Time: May 31 03:10:05 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 31 00:45:12 2016
Response via : Initial Calibration




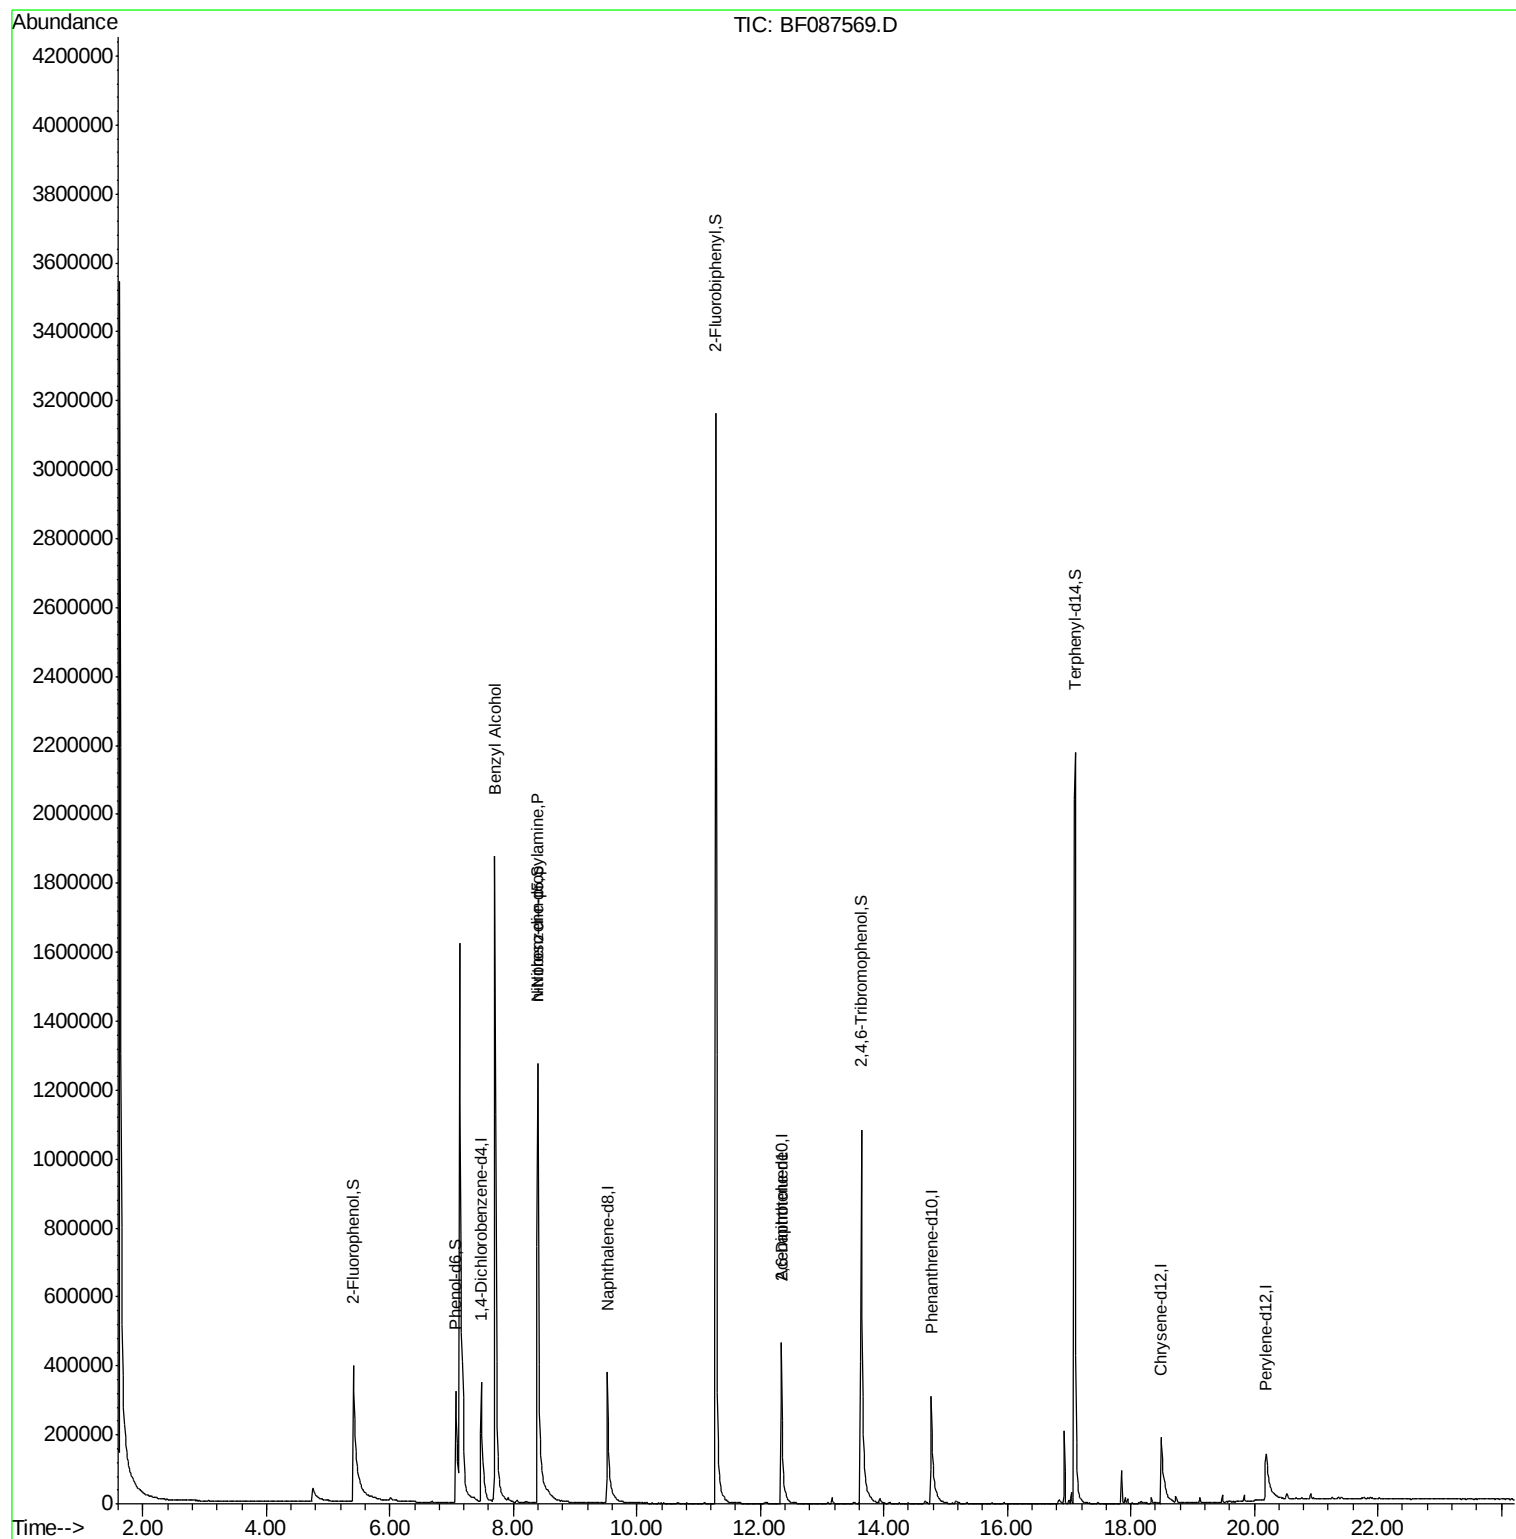




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.48 min Scan# 516
 Delta R.T. 0.01 min
 Lab File: BF087569.D
 Acq: 31 May 2016 2:11




Instrument :
 BNA_F
 ClientSampled :
 MW-25

Tgt Ion:152 Resp: 105252
 Ion Ratio Lower Upper
 152 100
 150 160.6 125.8 188.6
 115 65.1 51.5 77.3

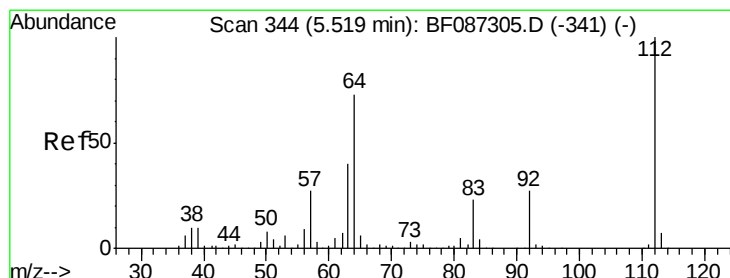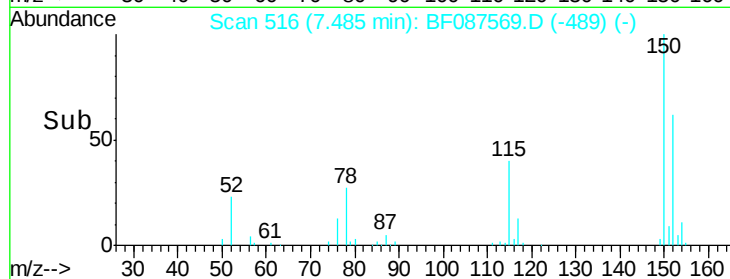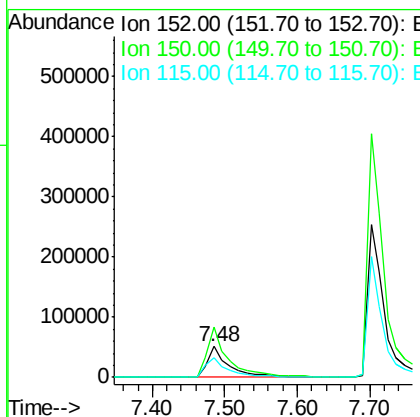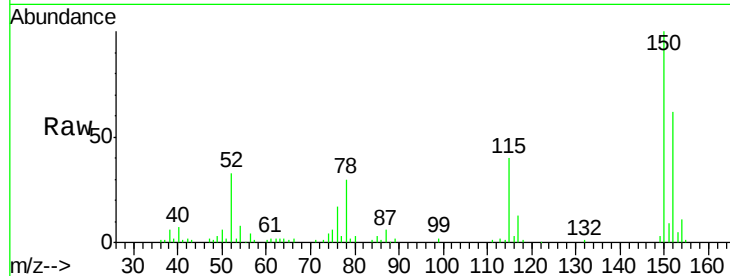

#5
 2-Fluorophenol
 Concen: 58.22 ng
 RT: 5.40 min Scan# 334
 Delta R.T. 0.03 min
 Lab File: BF087569.D
 Acq: 31 May 2016 2:11

Tgt Ion:112 Resp: 348736
 Ion Ratio Lower Upper
 112 100
 64 71.7 52.1 78.1
 63 41.1 25.7 38.5#

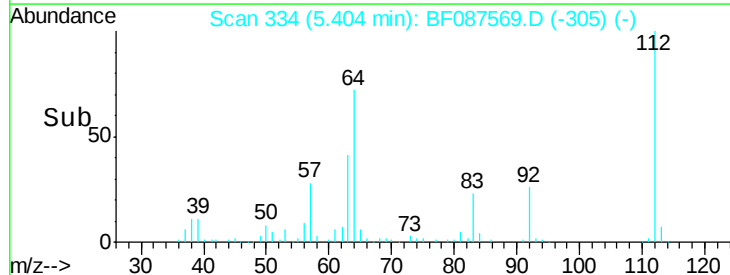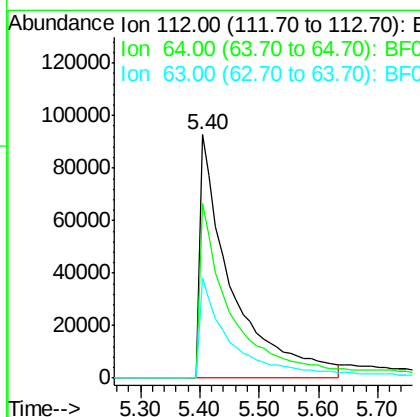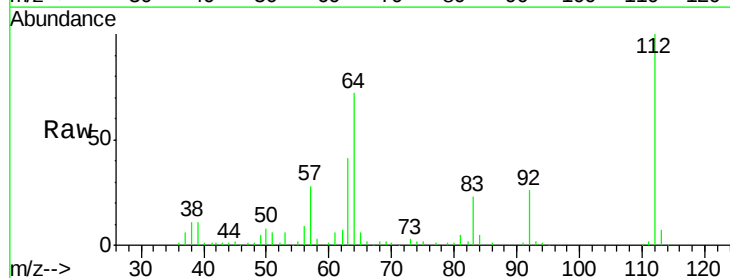



#7

Phenol-d6

Concen: 31.83 ng

RT: 7.06 min Scan# 479

Delta R.T. 0.02 min

Lab File: BF087569.D

Acq: 31 May 2016 2:11

Instrument :

BNA_F

ClientSampleId :

MW-25


Tgt Ion: 99 Resp: 257594

Ion Ratio Lower Upper

99 100

42 30.4 13.6 20.4#




71 41.8 24.6 36.8#

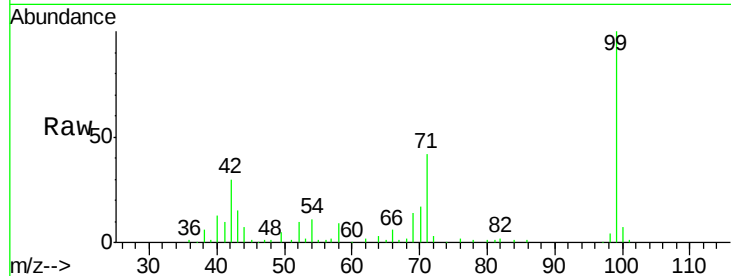

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

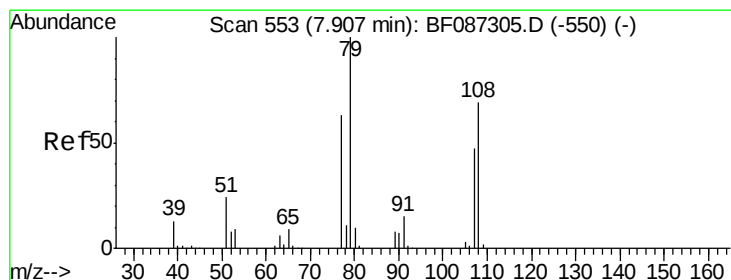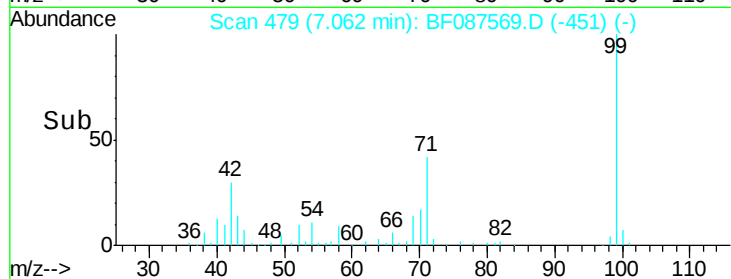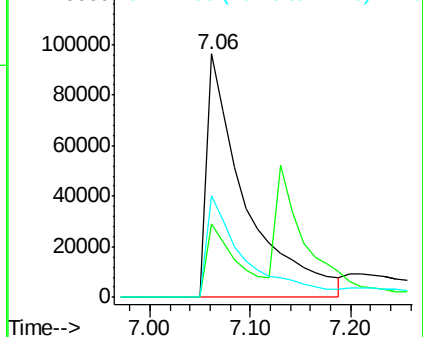

#15

Benzyl Alcohol

Concen: 2.37 ng

RT: 7.70 min Scan# 535

Delta R.T. -0.08 min

Lab File: BF087569.D

Acq: 31 May 2016 2:11


Tgt Ion: 79 Resp: 13971

Ion Ratio Lower Upper

79 100

108 29.9 68.4 102.6#



77 98.7 50.6 76.0#

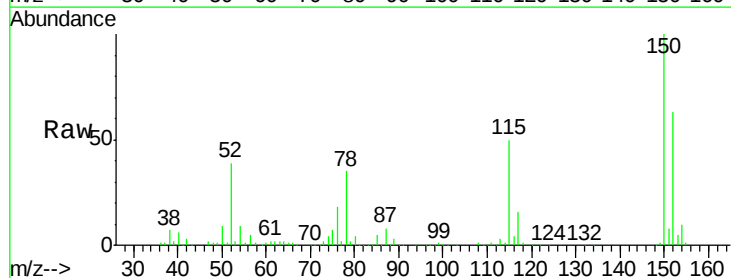


Abundance Ion 79.00 (78.70 to 79.70): BF0

Ion 108.00 (107.70 to 108.70): BF0

Ion 77.00 (76.70 to 77.70): BF0

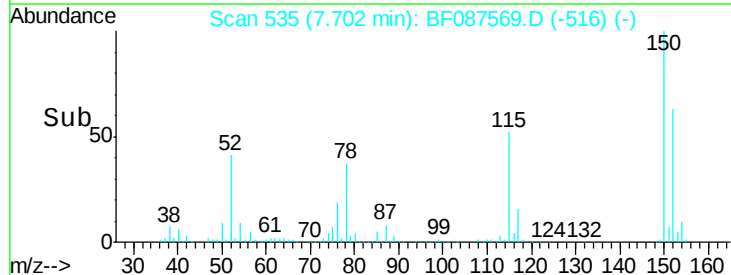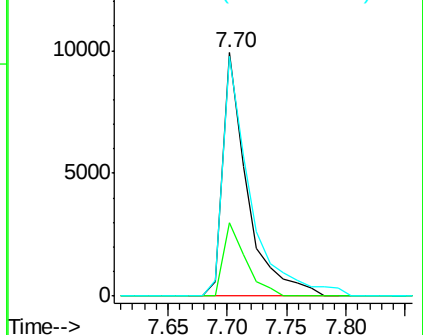

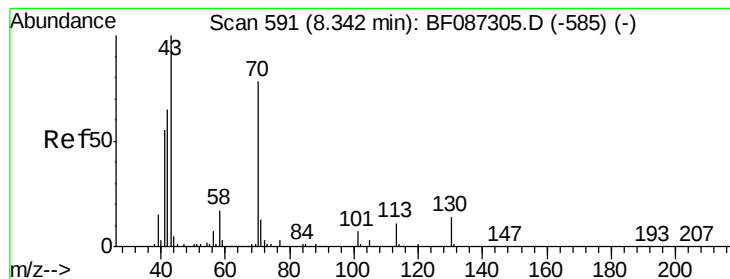

#19

n-Nitroso-di-n-propylamine

Concen: 16.24 ng

RT: 8.40 min Scan# 596

Delta R.T. 0.18 min

Lab File: BF087569.D

Acq: 31 May 2016 2:11

Instrument :

BNA_F

ClientSampleId :

MW-25

Tgt Ion: 70 Resp: 97997





Ion Ratio Lower Upper

70 100

42 61.4 43.1 64.7

101 0.0 8.1 12.1#

130 1.9 18.6 28.0#

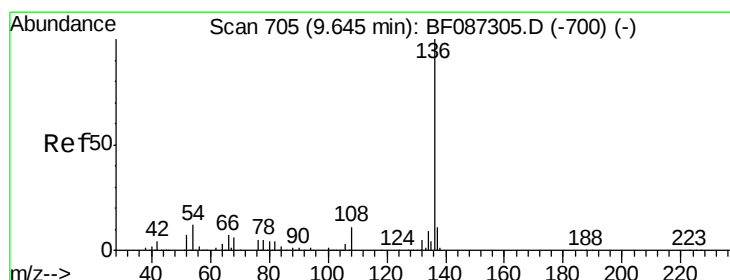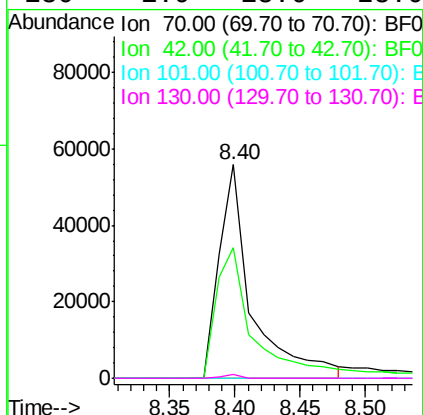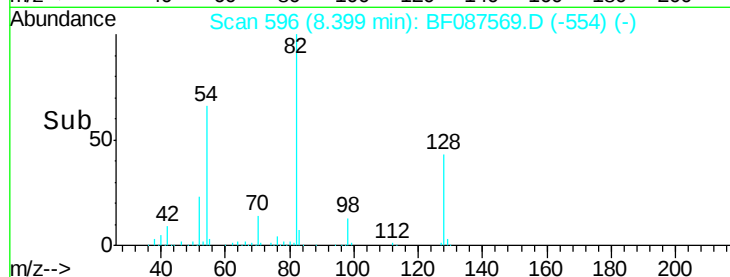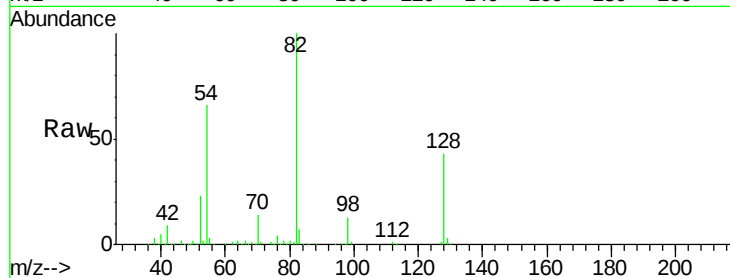

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.52 min Scan# 694

Delta R.T. 0.01 min

Lab File: BF087569.D

Acq: 31 May 2016 2:11

Tgt Ion: 136 Resp: 424743




Ion Ratio Lower Upper


136 100

137 10.6 8.8 13.2

54 10.3 5.0 7.4#

68 5.1 4.4 6.6

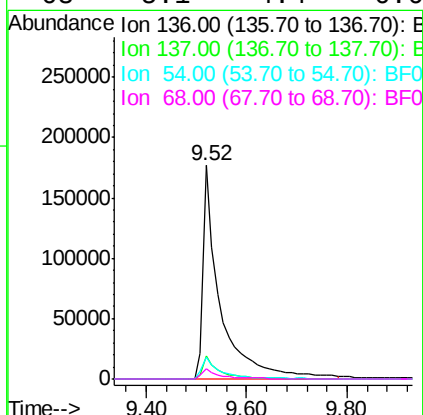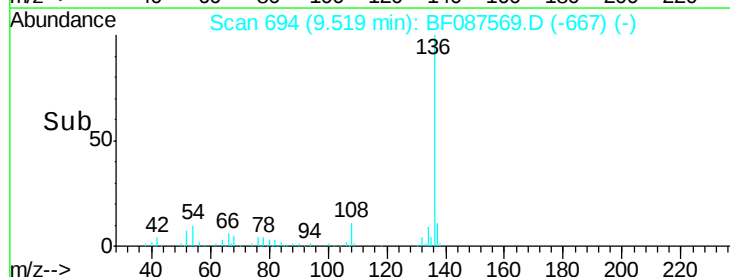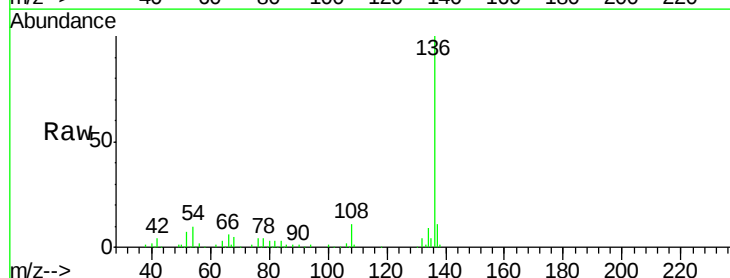

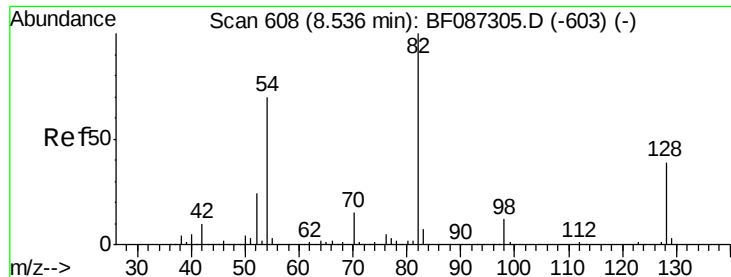

#23

Nitrobenzene-d5

Concen: 95.31 ng

RT: 8.40 min Scan# 596

Delta R.T. -0.01 min

Lab File: BF087569.D

Acq: 31 May 2016 2:11

Instrument :

BNA_F

ClientSampleId :

MW-25


Tgt Ion: 82 Resp: 803269

Ion Ratio Lower Upper




82 100

128 42.7 40.6 61.0

54 66.4 38.1 57.1#

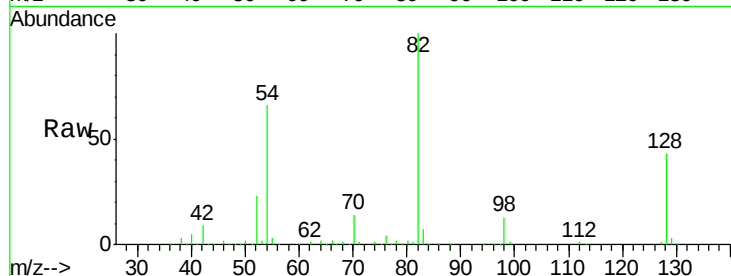

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): B
Ion 54.00 (53.70 to 54.70): BF0

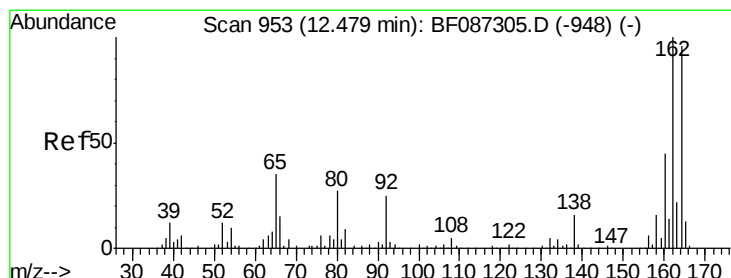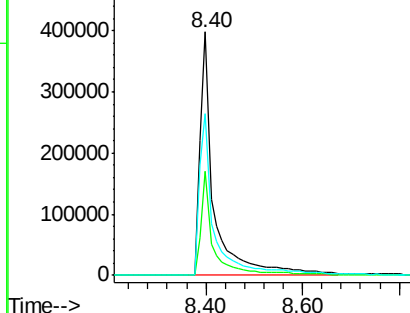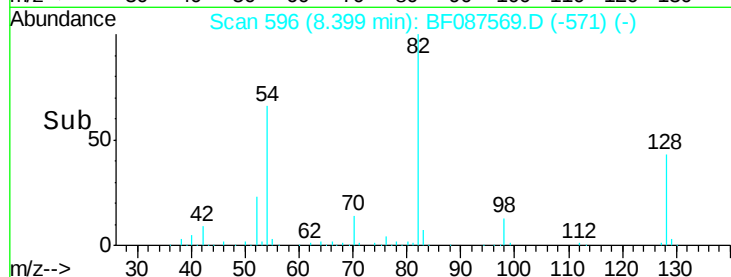

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 12.34 min Scan# 941

Delta R.T. 0.01 min

Lab File: BF087569.D

Acq: 31 May 2016 2:11


Tgt Ion: 164 Resp: 199830

Ion Ratio Lower Upper



164 100


162 103.0 82.8 124.2

160 46.6 36.9 55.3

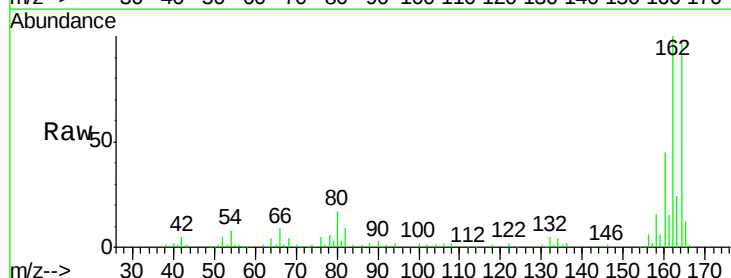

Abundance Ion 164.00 (163.70 to 164.70): B
Ion 162.00 (161.70 to 162.70): B
Ion 160.00 (159.70 to 160.70): B



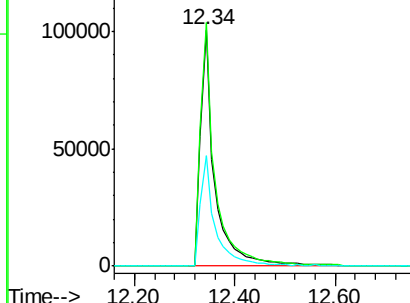
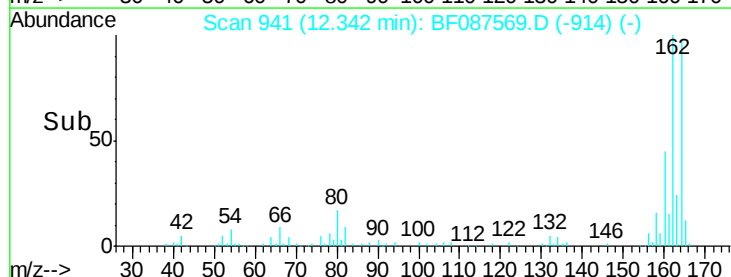


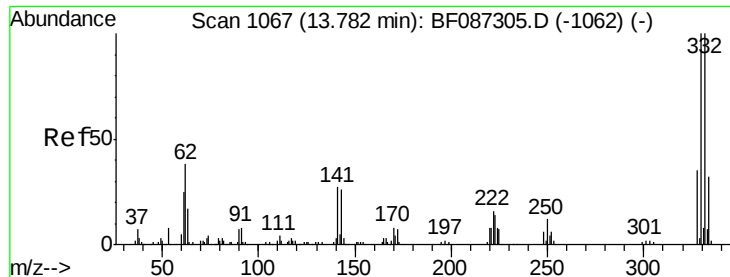

#41
 2,4,6-Tribromophenol
 Concen: 115.32 ng
 RT: 13.63 min Scan# 1054
 Delta R.T. -0.00 min
 Lab File: BF087569.D
 Acq: 31 May 2016 2:11




Instrument :
 BNA_F
 ClientSampleId :
 MW-25


Tgt Ion:330 Resp: 221449
 Ion Ratio Lower Upper
 330 100
 332 97.2 79.0 118.4
 141 46.1 31.2 46.8

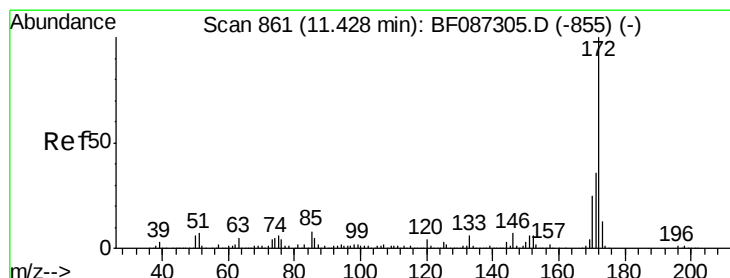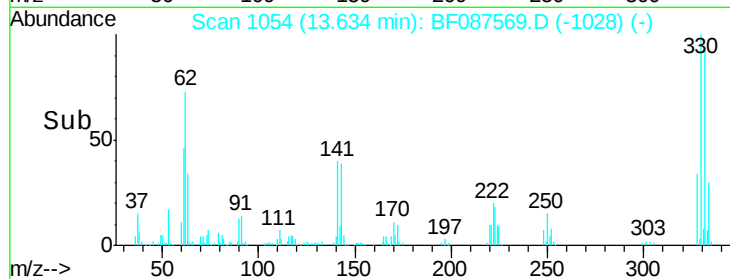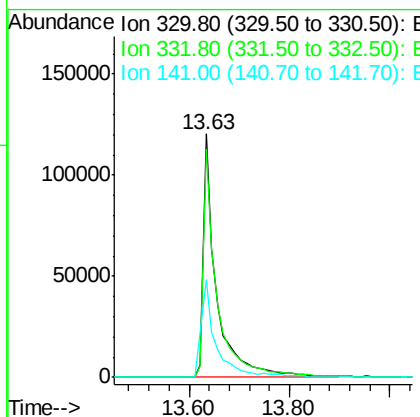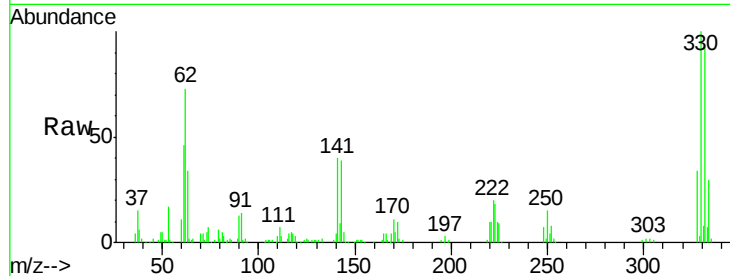

#44
 2-Fluorobiphenyl
 Concen: 92.14 ng
 RT: 11.28 min Scan# 848
 Delta R.T. -0.01 min
 Lab File: BF087569.D
 Acq: 31 May 2016 2:11

Tgt Ion:172 Resp: 1305986
 Ion Ratio Lower Upper
 172 100
 171 36.2 29.0 43.6
 170 24.3 19.8 29.8

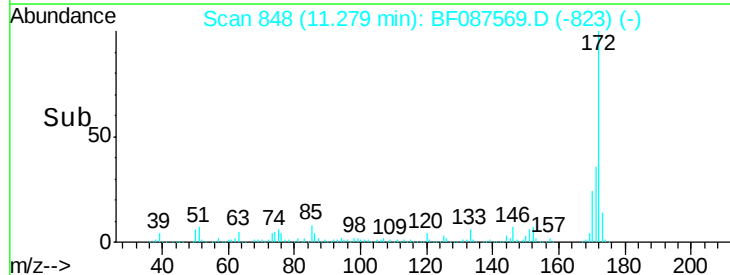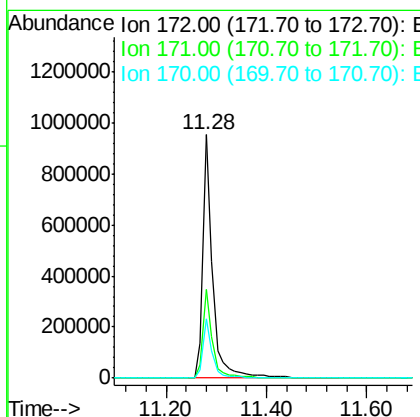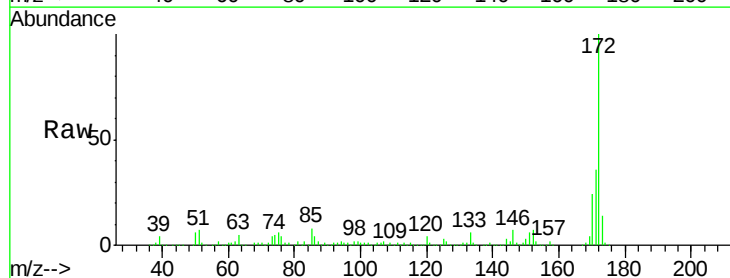


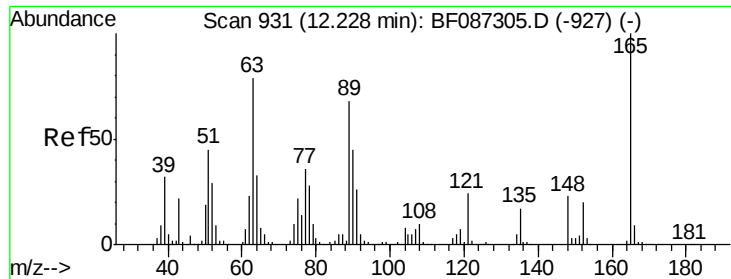




#50
 2,6-Dinitrotoluene
 Concen: 6.14 ng
 RT: 12.34 min Scan# 941
 Delta R.T. 0.24 min
 Lab File: BF087569.D
 Acq: 31 May 2016 2:11

Instrument :
 BNA_F
 ClientSampleId :
 MW-25

Tgt Ion:165 Resp: 19789
 Ion Ratio Lower Upper
 165 100
 63 0.0 51.8 77.8#
 89 0.0 50.7 76.1#

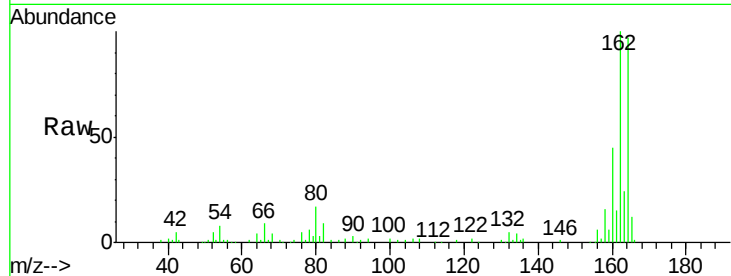


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF0
 Ion 89.00 (88.70 to 89.70): BF0

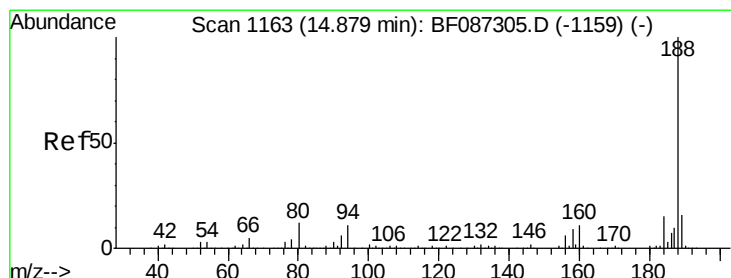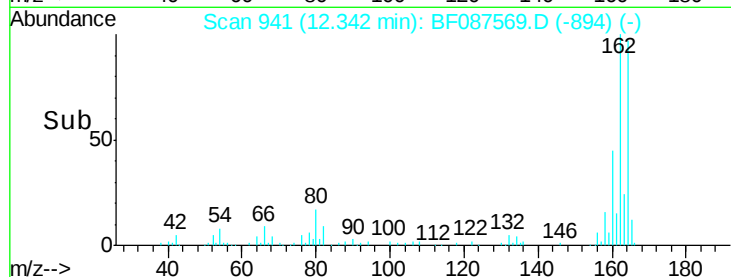
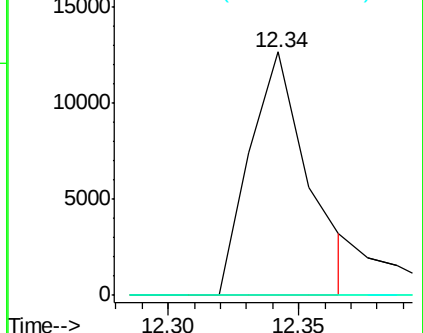


#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 14.77 min Scan# 1153
 Delta R.T. 0.02 min
 Lab File: BF087569.D
 Acq: 31 May 2016 2:11

Tgt Ion:188 Resp: 344964
 Ion Ratio Lower Upper
 188 100
 94 8.5 6.8 10.2
 80 9.6 7.1 10.7

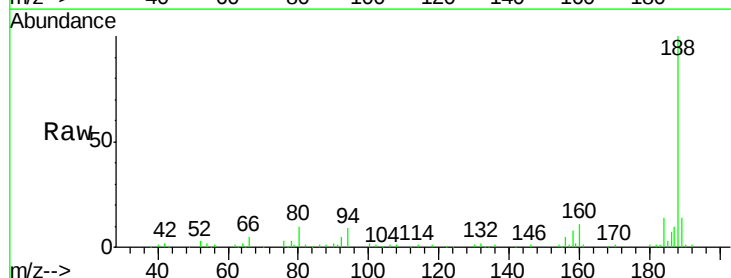

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

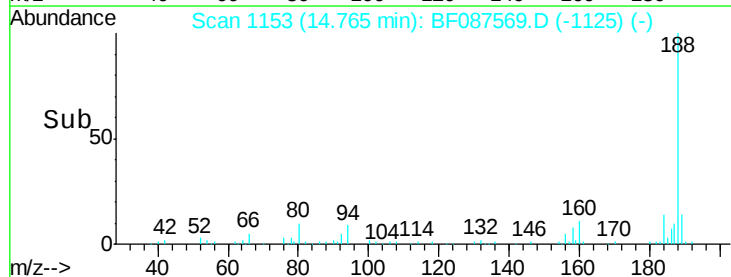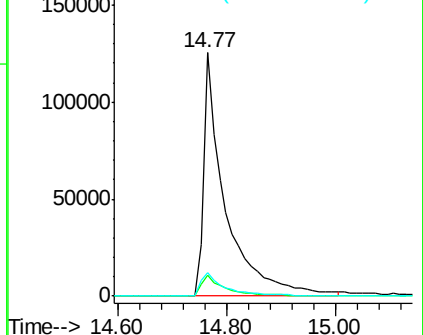



#75

Chrysene-d12

Concen: 20.00 ng

RT: 18.49 min Scan# 1479

Delta R.T. 0.05 min

Lab File: BF087569.D

Acq: 31 May 2016 2:11

Instrument :

BNA_F

ClientSampleId :

MW-25


Tgt Ion:240 Resp: 251564

Ion Ratio Lower Upper

240 100

120 11.4 11.2 16.8




236 25.0 21.2 31.8

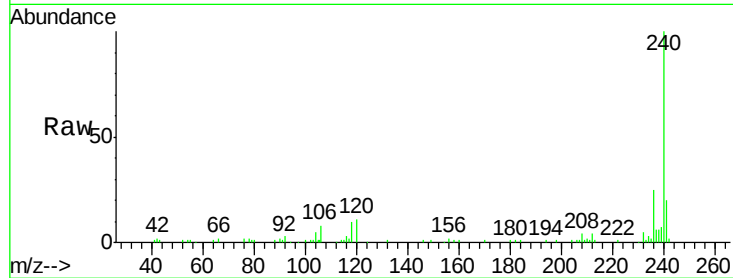

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

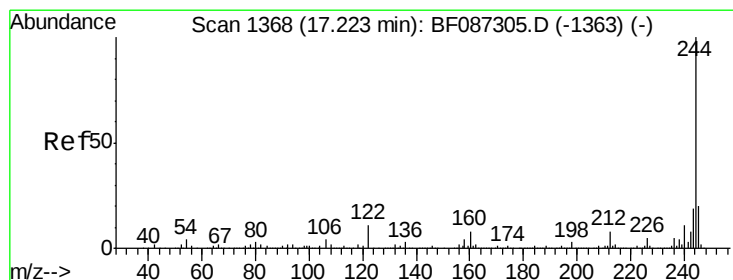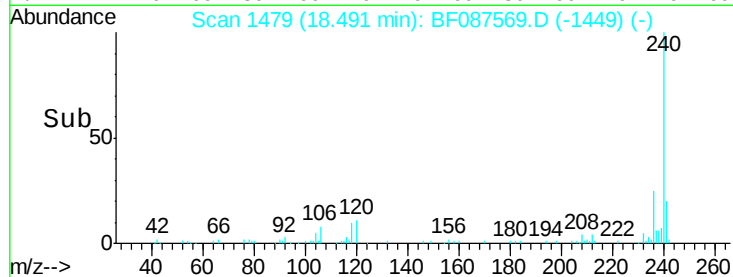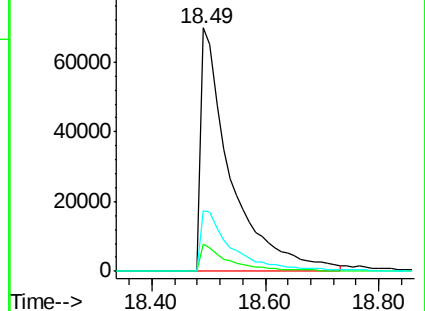

#78

Terphenyl-d14

Concen: 94.47 ng

RT: 17.10 min Scan# 1357

Delta R.T. -0.00 min

Lab File: BF087569.D

Acq: 31 May 2016 2:11


Tgt Ion:244 Resp: 1117892

Ion Ratio Lower Upper

244 100

212 7.6 6.2 9.2



122 8.5 12.0 18.0#

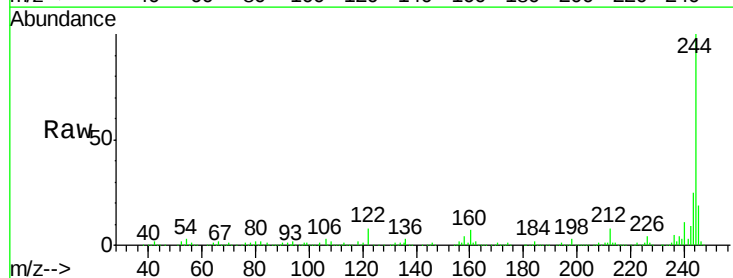


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

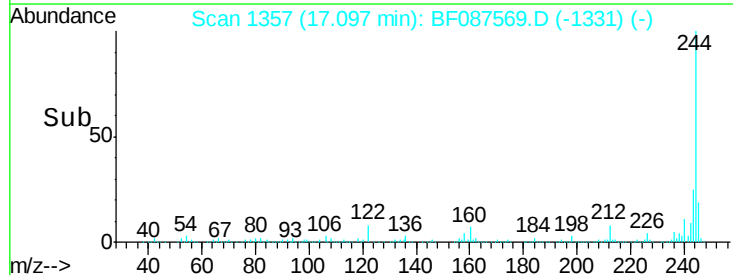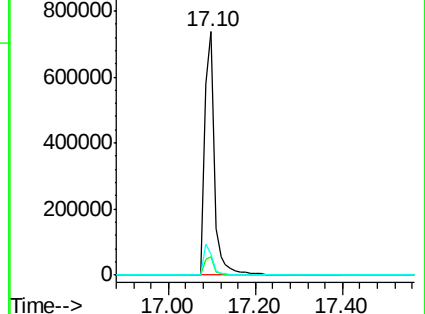

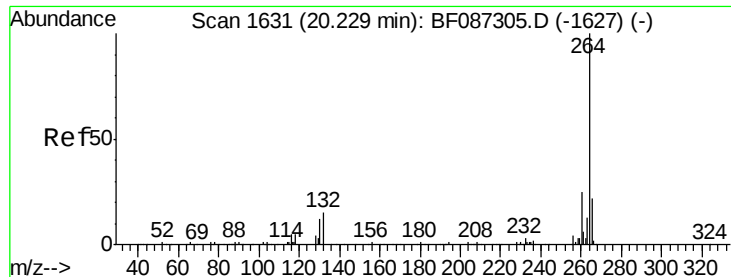

#86
Perylene-d12
Concen: 20.00 ng
RT: 20.19 min Scan# 1628
Delta R.T. 0.07 min
Lab File: BF087569.D
Acq: 31 May 2016 2:11

Instrument :
BNA_F
ClientSampleId :
MW-25

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.6	19.5	29.3
265	21.1	17.3	25.9

