

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052916\
 Data File : BF087573.D
 Acq On : 31 May 2016 4:28
 Operator : UM/SJ
 Sample : H3316-02
 Misc :
 ALS Vial : 91 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-01-COMP

Quant Time: May 31 06:00:10 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\BFDDTBREAKDOWN.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 01 16:14:27 2010
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ng	-10.26
2) Naphthalene-d8	0.00	136	0	0.00	ng	-11.72
3) Acenaphthene-d10	0.00	164	0	0.00	ng	-14.91
4) Phenanthrene-d10	14.77	188	312279	40.00	ng	-0.33
8) Chrysene-d12	0.00	240	0	0.00	ng	-30.93
9) Perylene-d12	0.00	264	0	0.00	ng	-34.56


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) DDE	0.00	246	0	N.D.		
6) DDD	0.00	235	0	N.D.		
7) DDT	0.00	235	0	N.D.		


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052916\
Data File : BF087573.D
Acq On : 31 May 2016 4:28
Operator : UM/SJ
Sample : H3316-02
Misc :
ALS Vial : 91 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-01-COMP

Quant Time: May 31 06:00:10 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\BFDDTBREAKDOWN.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 01 16:14:27 2010
Response via : Initial Calibration

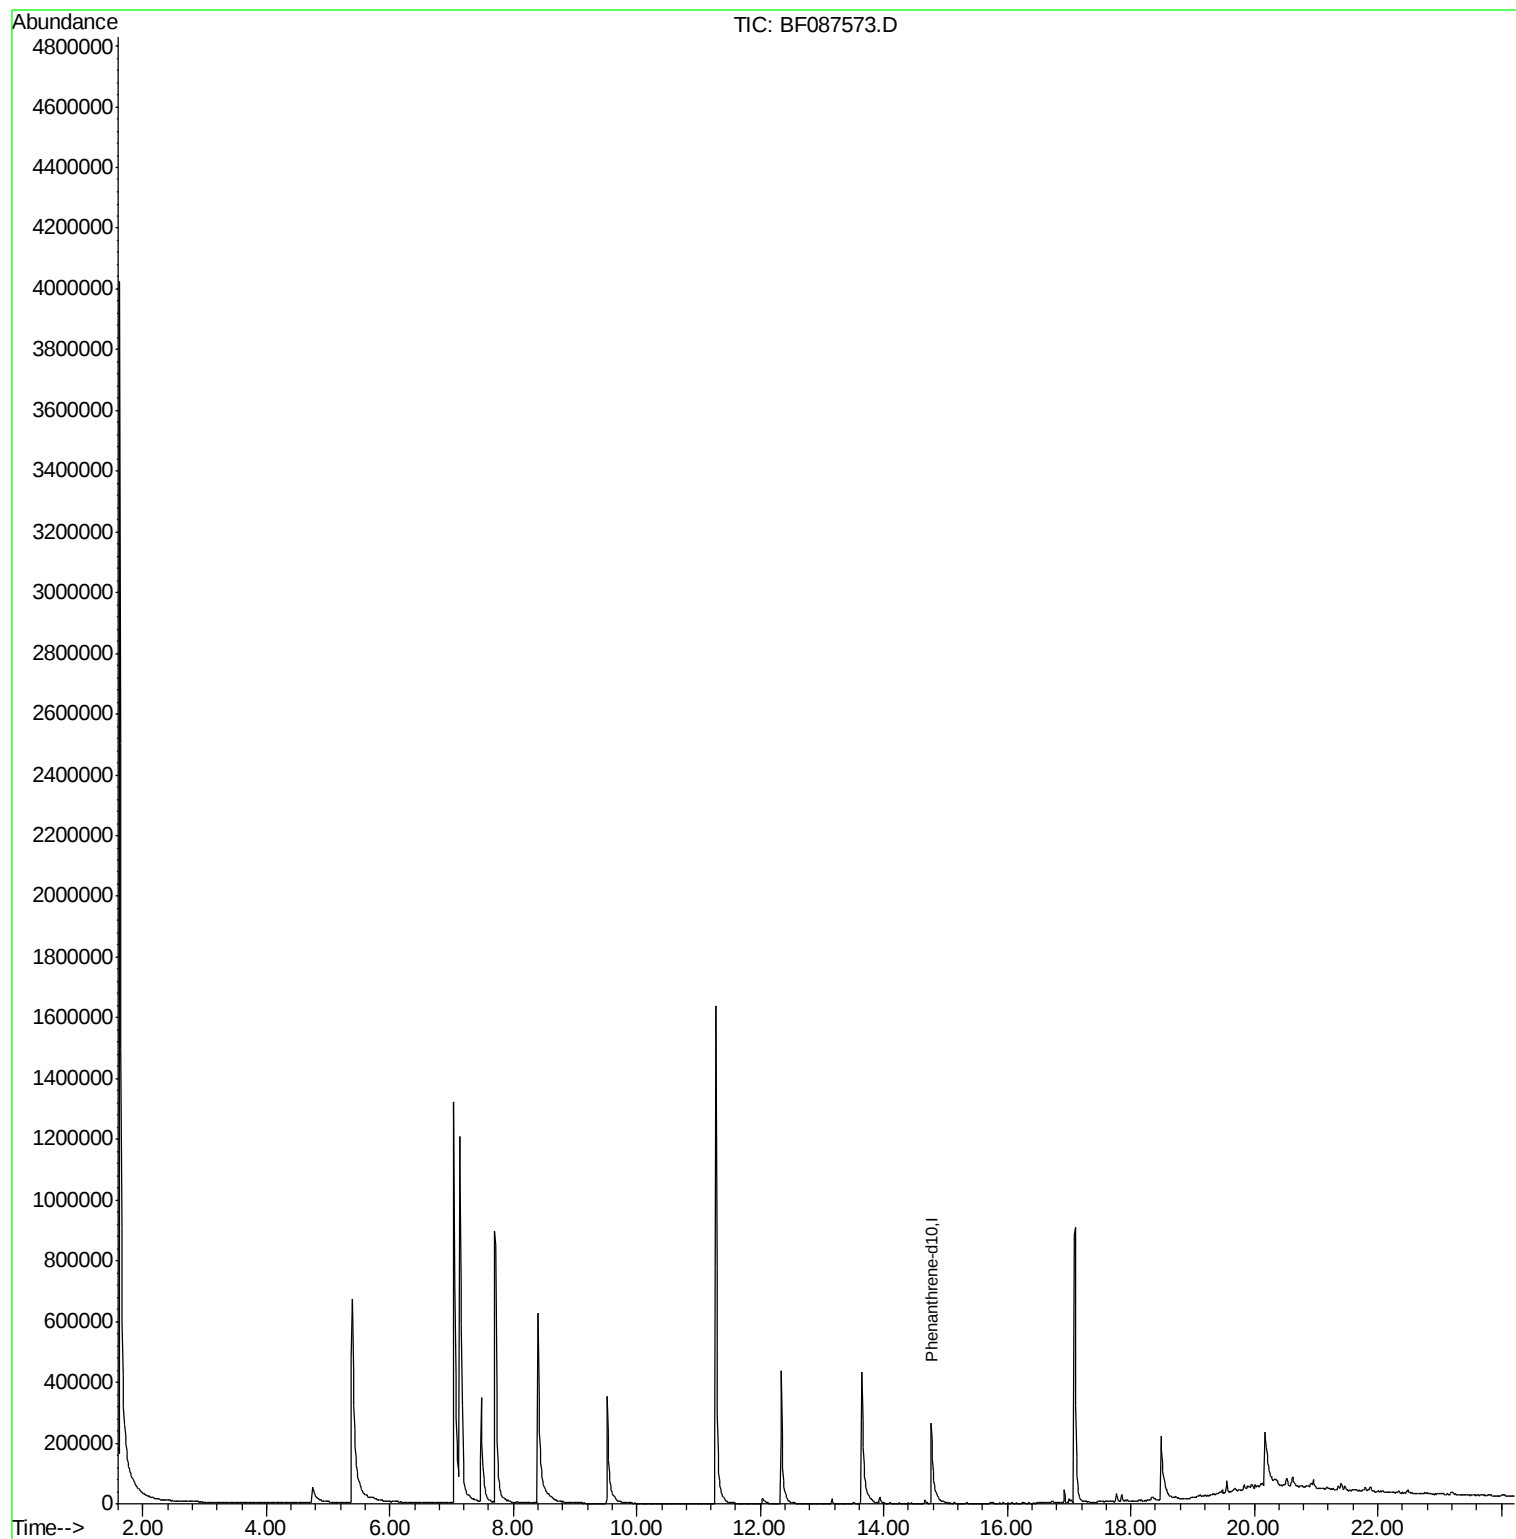

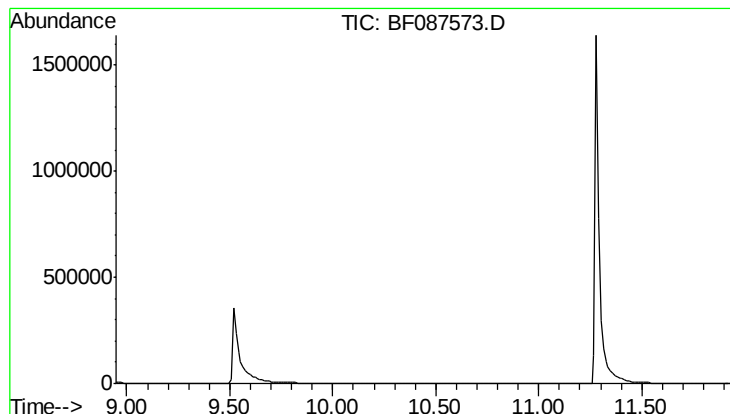



#5
DDE
Concen: N.D.
Expected RT: 10.44 min

Lab File: BF087573.D
Acq: 31 May 2016 4:28

Instrument :
BNA_F
ClientSampleId :
SB-01-COMP

Tgt Ion: 246

Sig	Exp Ratio
246	100
248	1793.6
318	201.9
176	4805.3

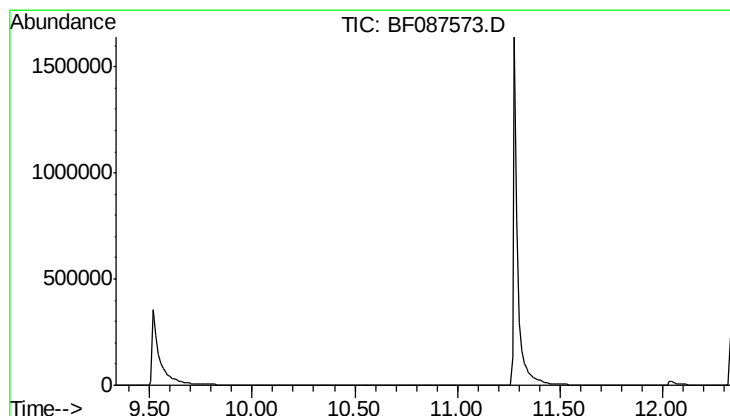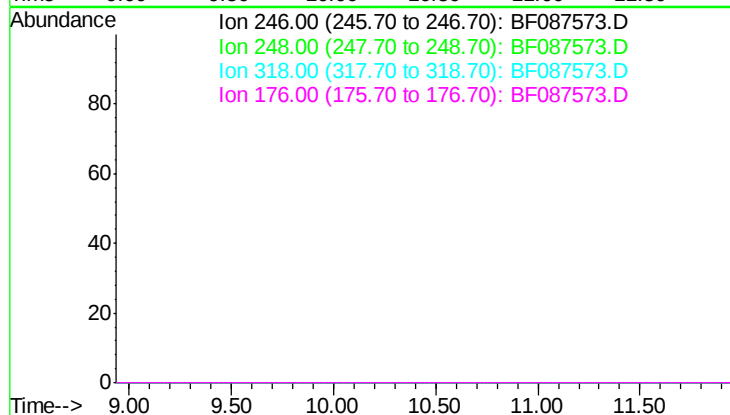



#6
DDD
Concen: N.D.
Expected RT: 10.83 min

Lab File: BF087573.D
Acq: 31 May 2016 4:28

Tgt Ion: 235

Sig	Exp Ratio
235	100
237	6000.0
165	6000.0

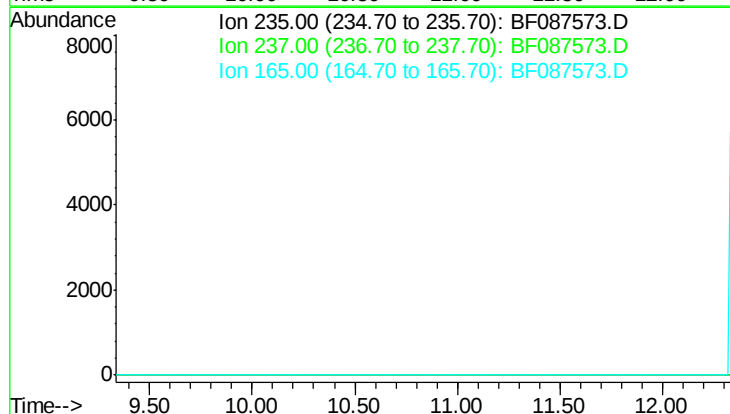

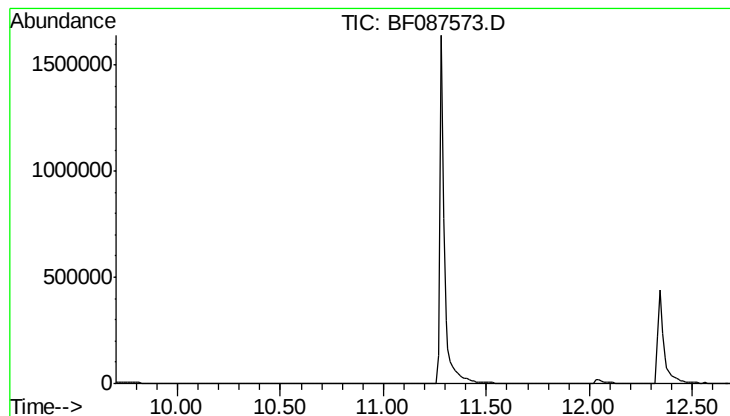

#7
DDT
Concen: N.D.
Expected RT: 11.19 min
Lab File: BF087573.D
Acq: 31 May 2016 4:28

Instrument :
BNA_F
ClientSampleId :
SB-01-COMP

Tgt Ion: 235
Sig Exp Ratio
235 100
237 0.0
165 0.2

