
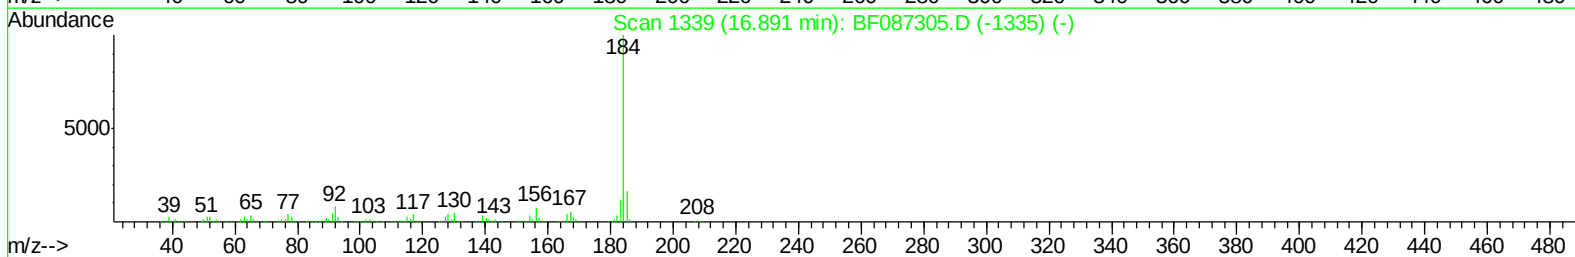
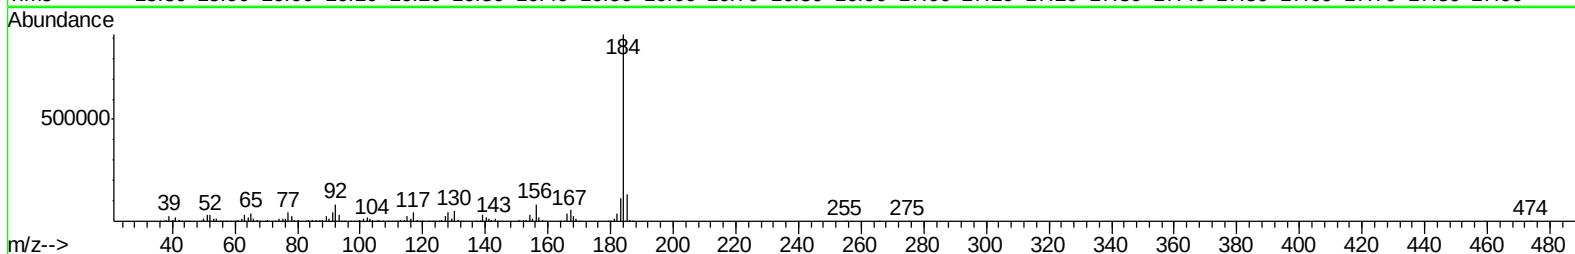


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052916\
Data File : BF087521.D
Acq On : 29 May 2016 19:59
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 08:02:41 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 30 07:00:04 2016
Response via : Initial Calibration

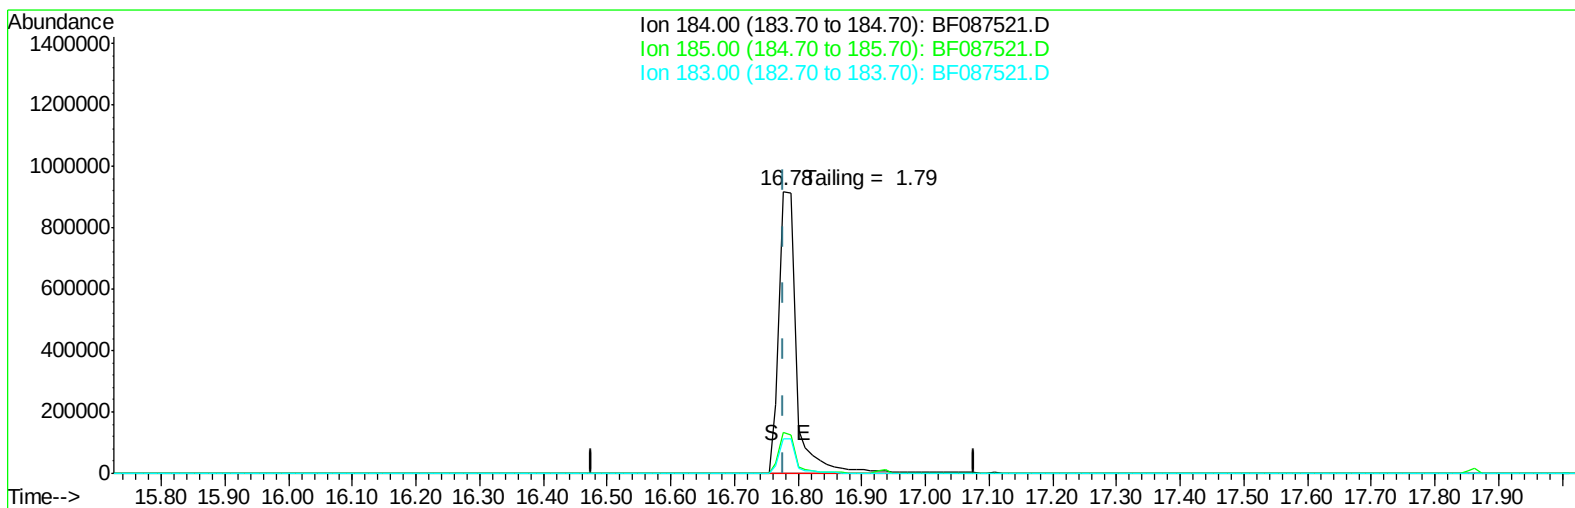

TIC: BF087521.D

(76) Benzidine




16.777min (-0.000) 0.00ng

response 1746508

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.55
183.00	12.20	12.48
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052916\
Data File : BF087521.D
Acq On : 29 May 2016 19:59
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 08:02:41 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 30 07:00:04 2016
Response via : Initial Calibration

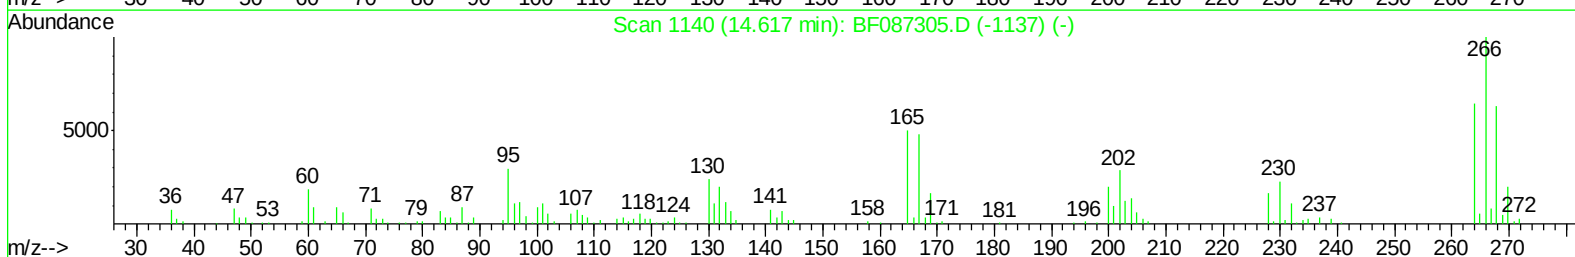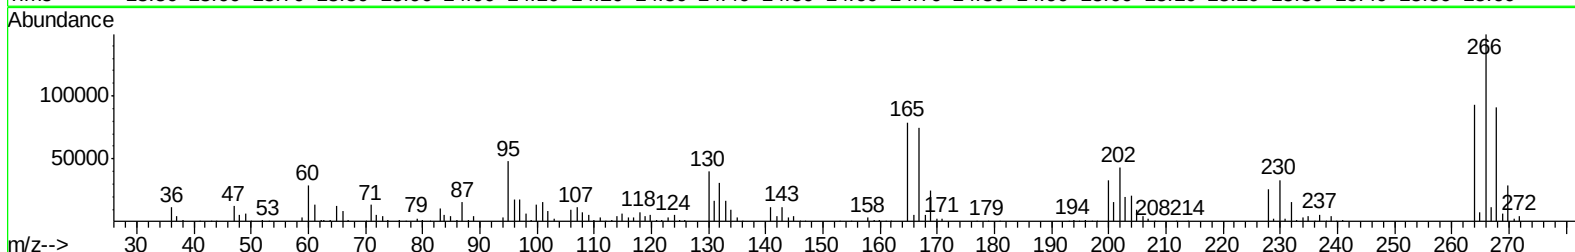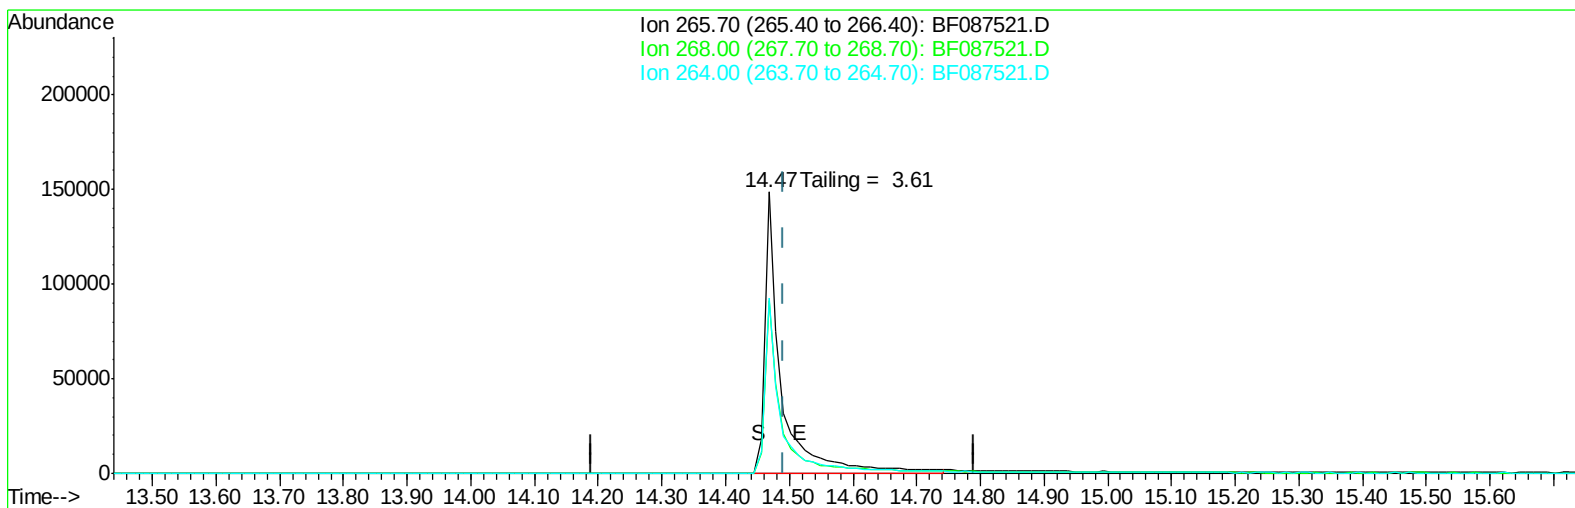

TIC: BF087521.D

(69) Pentachlorophenol (C)

14.468min (-0.023) 0.00ng

response 272883

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	61.16
264.00	66.10	62.42
0.00	0.00	0.00