
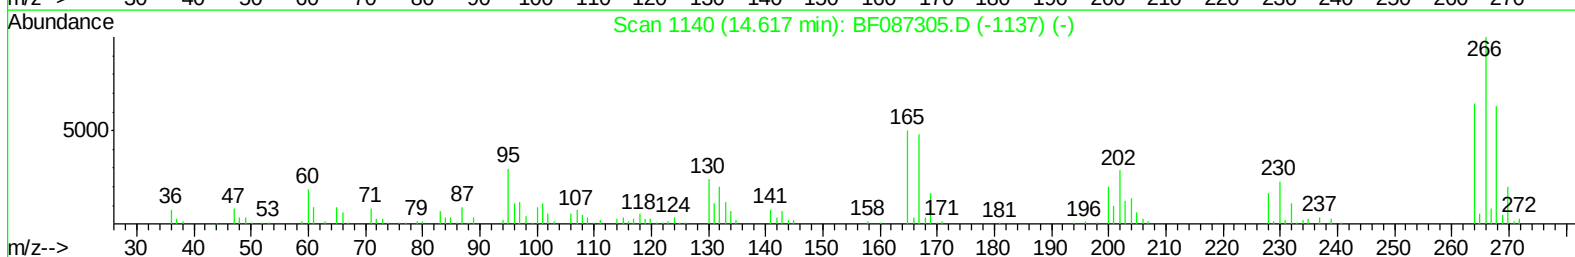
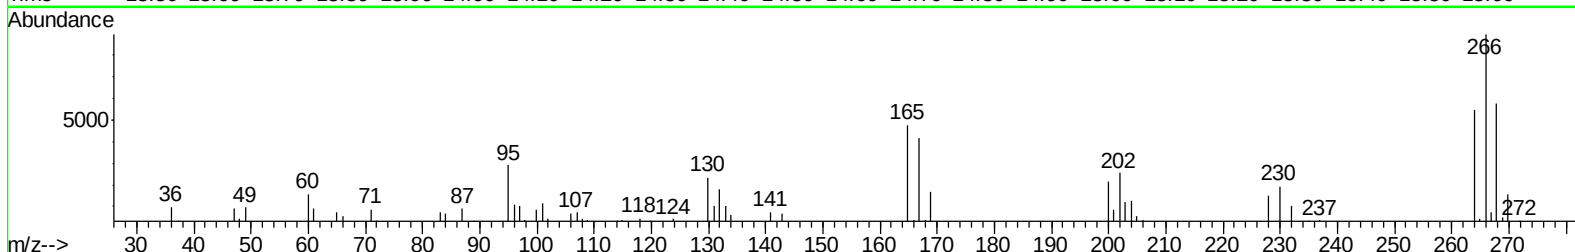


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052916\
Data File : BF087542.D
Acq On : 30 May 2016 10:12
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: May 31 04:14:25 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 31 00:45:12 2016
Response via : Initial Calibration

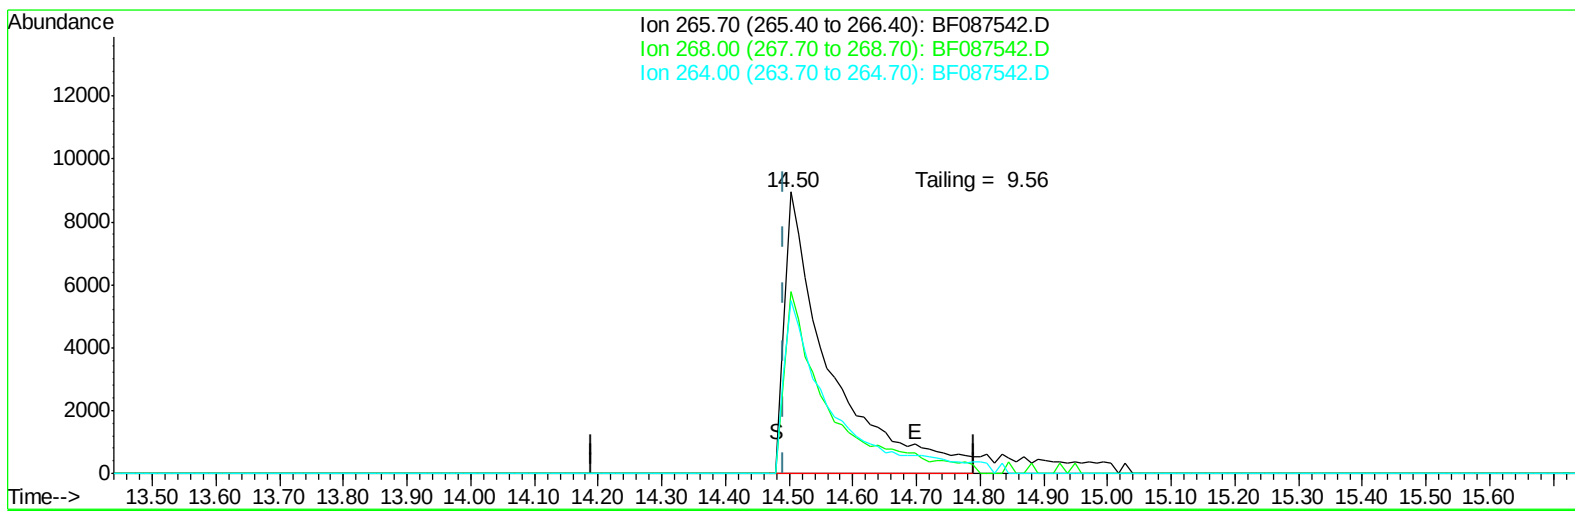

TIC: BF087542.D

(69) Pentachlorophenol (C)




14.502min (+0.011) 0.00ng

response 42648

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	64.44
264.00	66.10	61.26
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052916\
Data File : BF087542.D
Acq On : 30 May 2016 10:12
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: May 31 04:14:25 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 31 00:45:12 2016
Response via : Initial Calibration

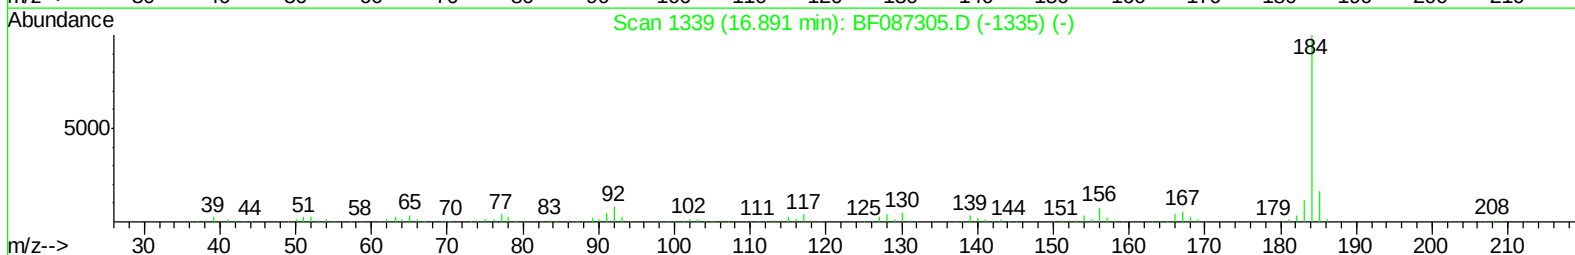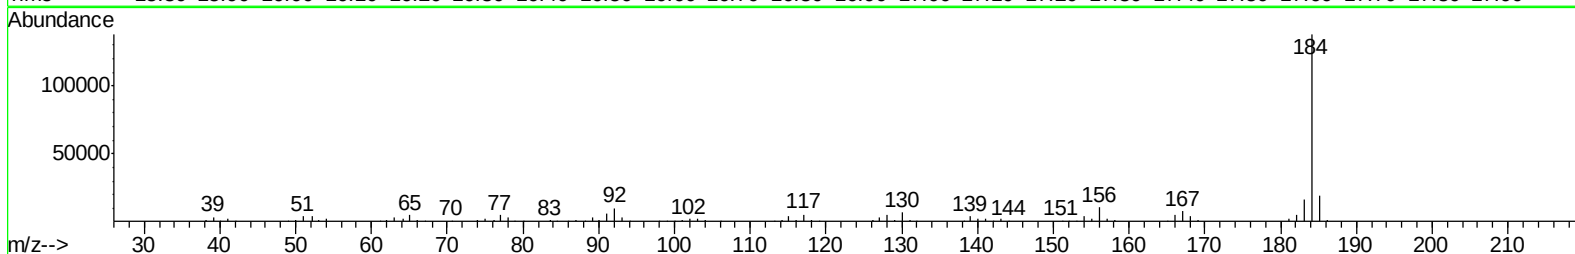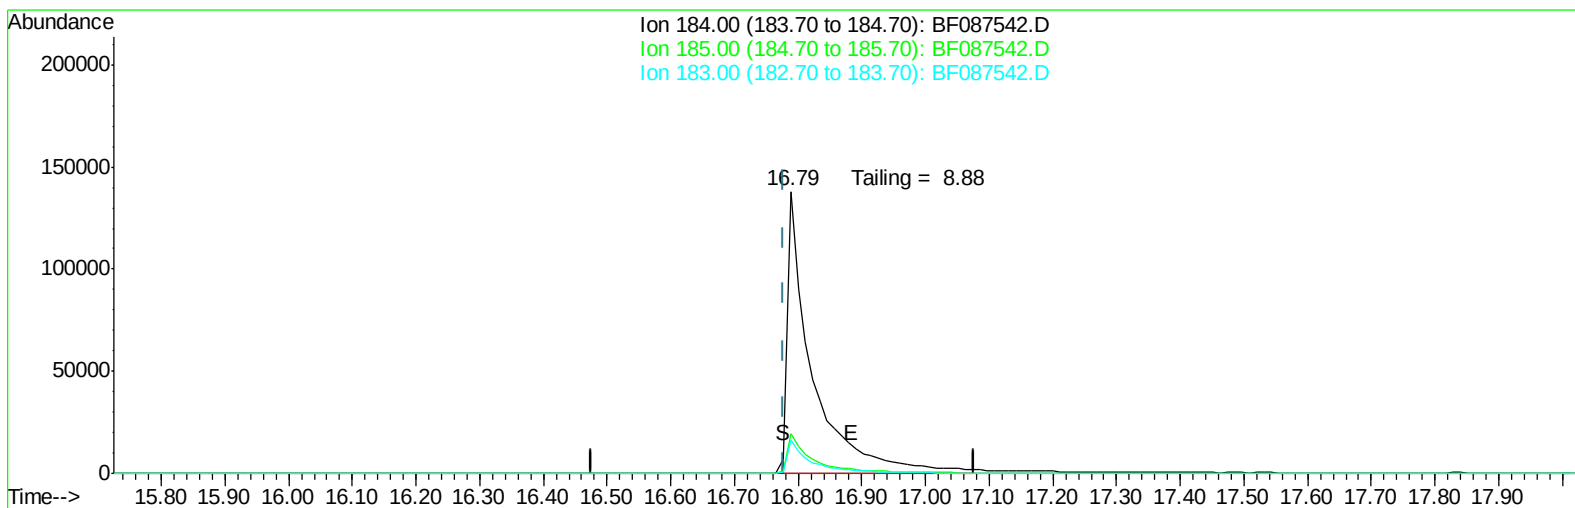

TIC: BF087542.D

(76) Benzidine

16.788min (+0.011) 0.00ng

response 368154

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	14.20
183.00	12.20	11.94
0.00	0.00	0.00