
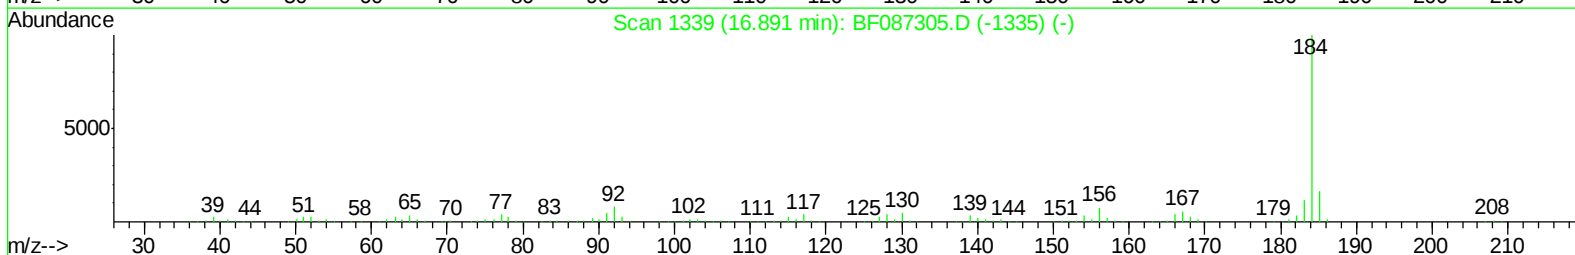
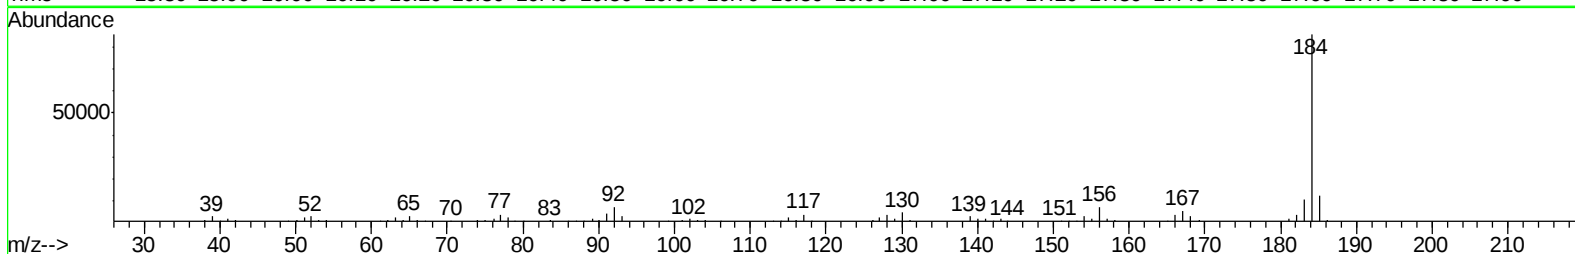


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052916\
Data File : BF087562.D
Acq On : 30 May 2016 22:10
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: May 31 04:15:11 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 31 00:45:12 2016
Response via : Initial Calibration

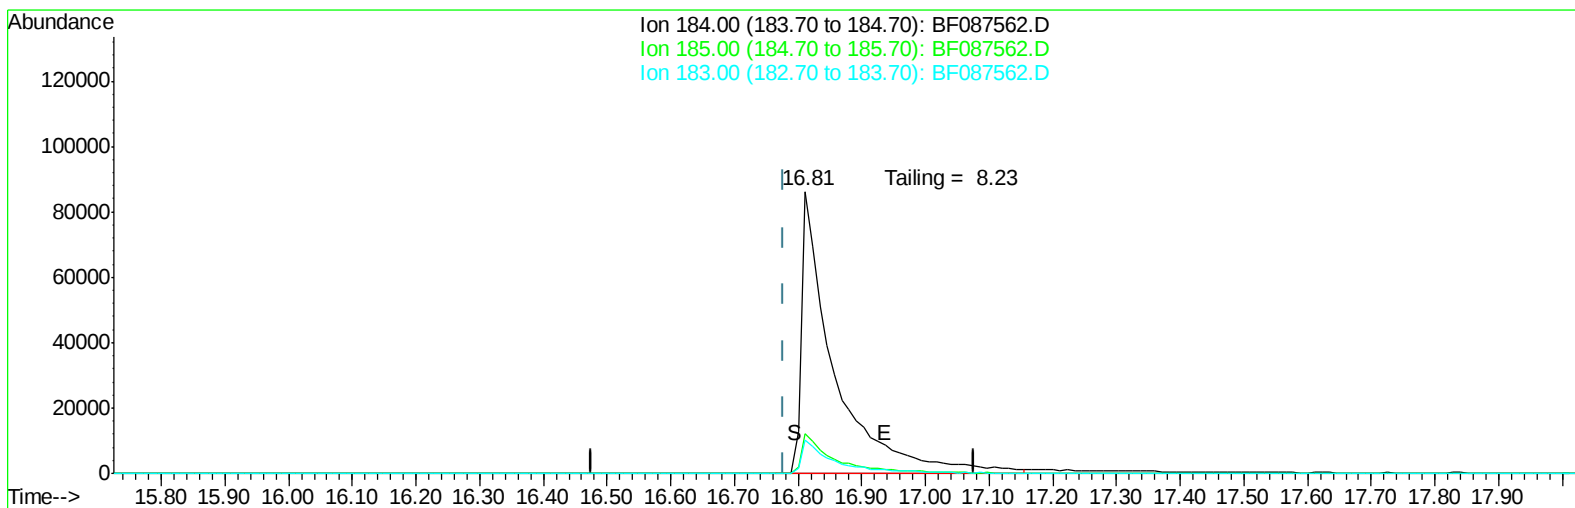

TIC: BF087562.D

(76) Benzidine




16.811min (+0.034) 0.00ng

response 293533

Ion	Exp%	Act%
184.00	100	100
185.00	17.00	13.92
183.00	12.20	11.74
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052916\
Data File : BF087562.D
Acq On : 30 May 2016 22:10
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: May 31 04:15:11 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 31 00:45:12 2016
Response via : Initial Calibration

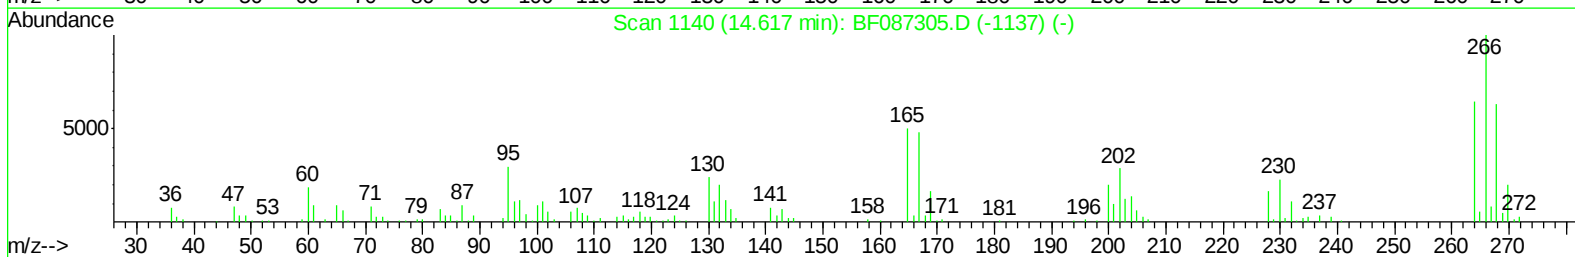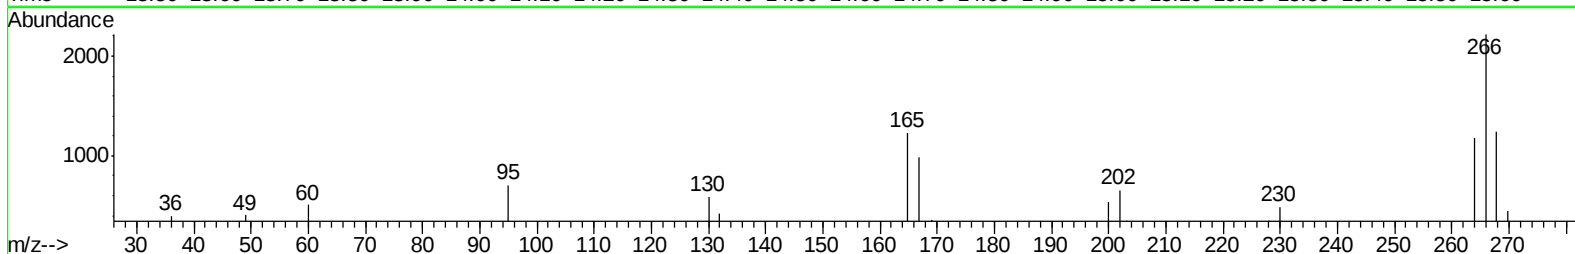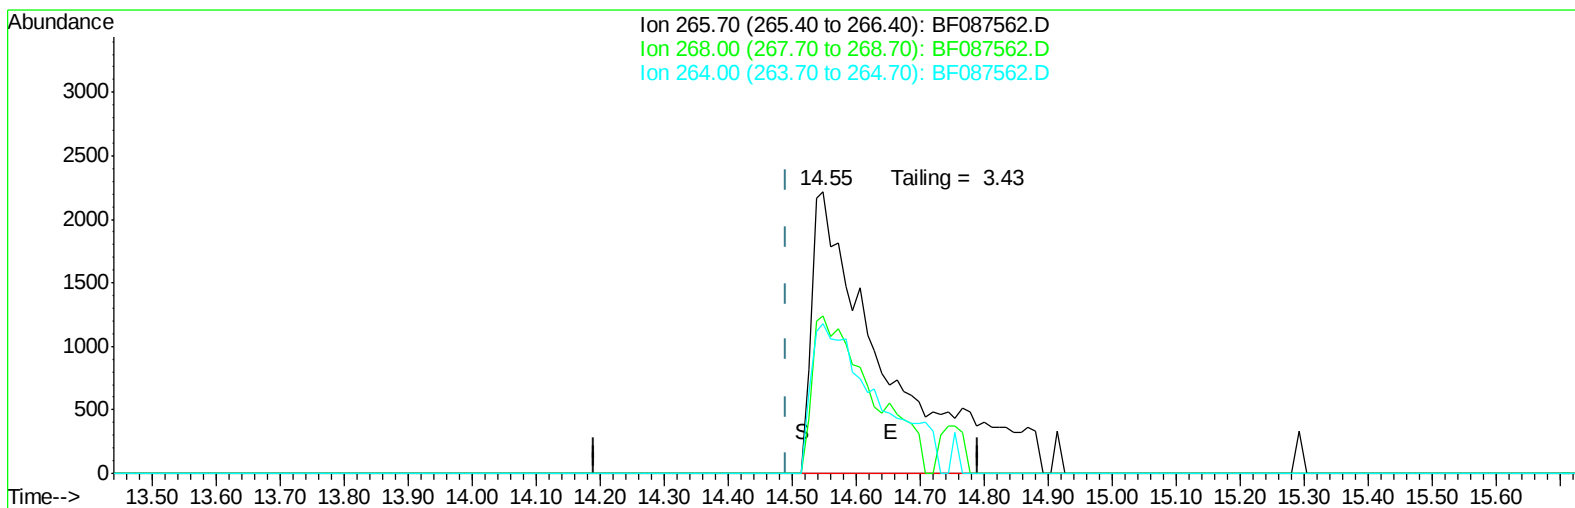

TIC: BF087562.D

(69) Pentachlorophenol (C)

14.548min (+0.057) 0.00ng m

response 17820

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	56.11
264.00	66.10	53.41
0.00	0.00	0.00