

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052916\
 Data File : BF087526.D
 Acq On : 29 May 2016 23:23
 Operator : UM/SJ
 Sample : H3222-11
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-13

Quant Time: May 30 07:07:21 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF052316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 30 07:00:04 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	115903	20.00	ng	0.00
21) Naphthalene-d8	9.51	136	443060	20.00	ng	0.00
38) Acenaphthene-d10	12.33	164	206566	20.00	ng	0.00
63) Phenanthrene-d10	14.74	188	380985	20.00	ng	0.00
75) Chrysene-d12	18.46	240	269964	20.00	ng	0.01
86) Perylene-d12	20.15	264	200859	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.38	112	307453	46.61	ng	0.01
7) Phenol-d6	7.04	99	235487	26.42	ng	0.00
23) Nitrobenzene-d5	8.39	82	697004	79.29	ng	-0.02
41) 2,4,6-Tribromophenol	13.62	330	216726	109.18	ng	-0.01
44) 2-Fluorobiphenyl	11.28	172	1198906	81.82	ng	-0.01
78) Terphenyl-d14	17.09	244	935958	73.71	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052916\
Data File : BF087526.D
Acq On : 29 May 2016 23:23
Operator : UM/SJ
Sample : H3222-11
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-13

Quant Time: May 30 07:07:21 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 30 07:00:04 2016
Response via : Initial Calibration

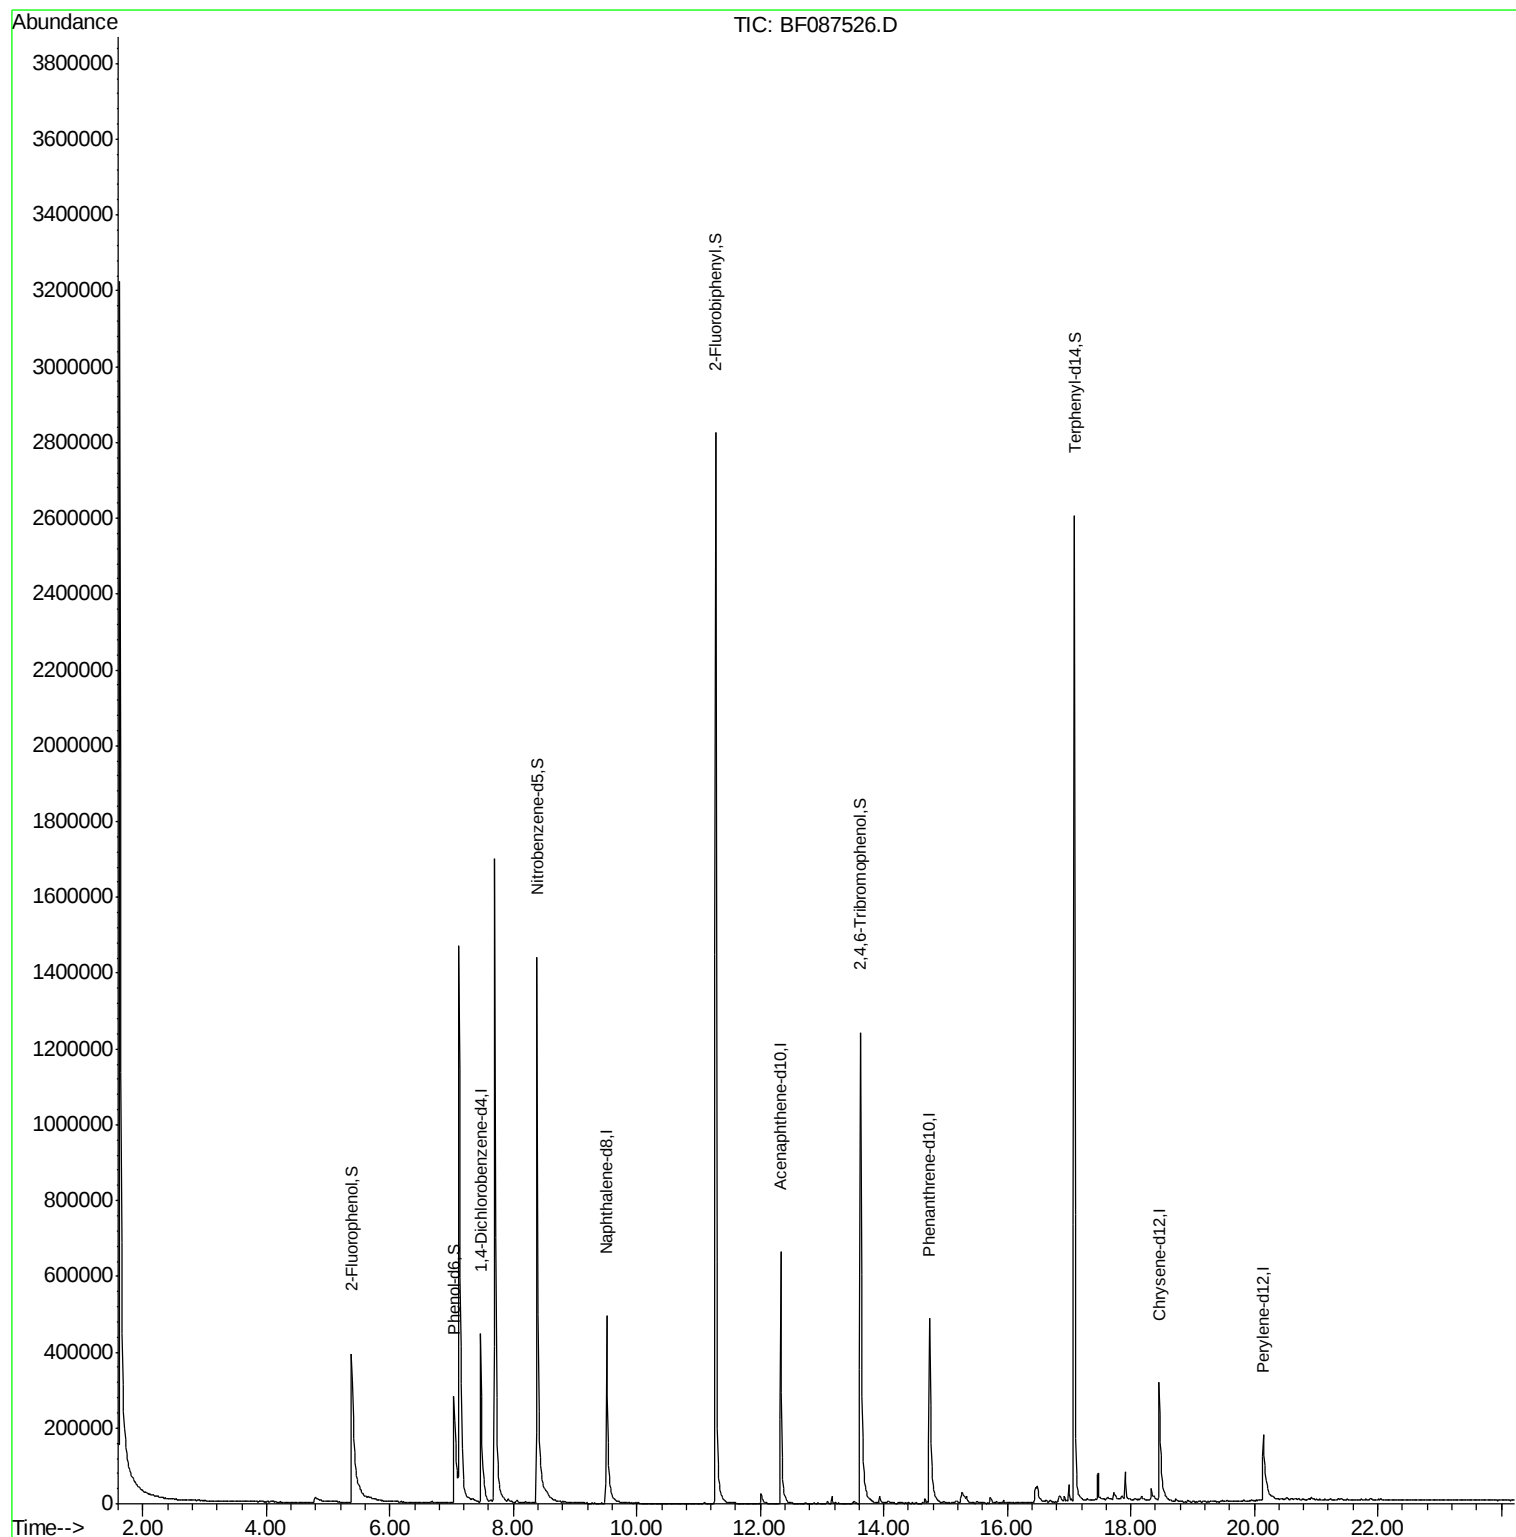

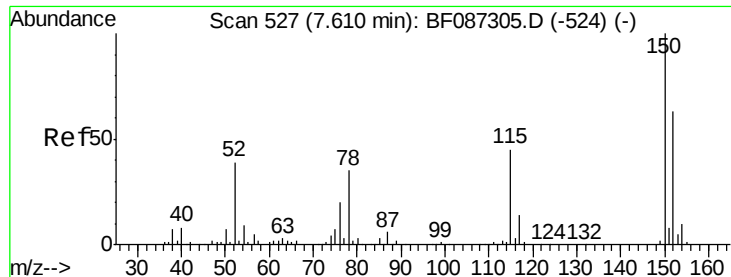


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.47 min Scan# 515
Delta R.T. 0.00 min
Lab File: BF087526.D
Acq: 29 May 2016 23:23

Instrument :
BNA_F
ClientSampled :
MW-13

Tot Ion:152 Resp: 115903
Ion Ratio Lower Upper
152 100
150 156.9 125.8 188.6
115 69.5 51.5 77.3

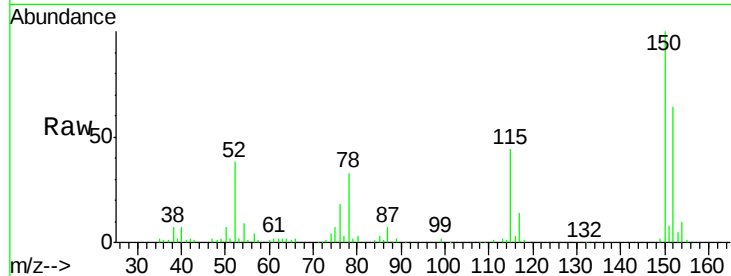


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

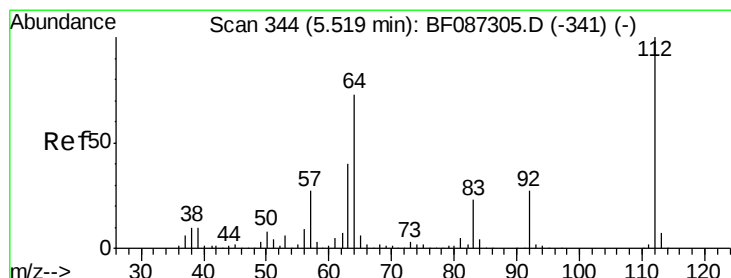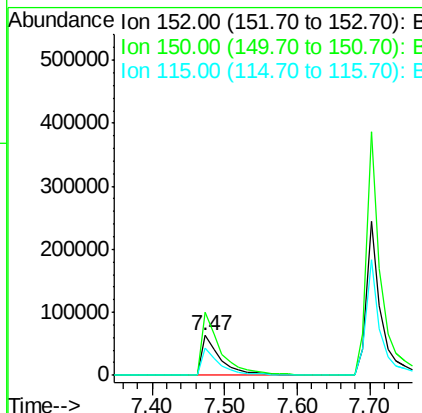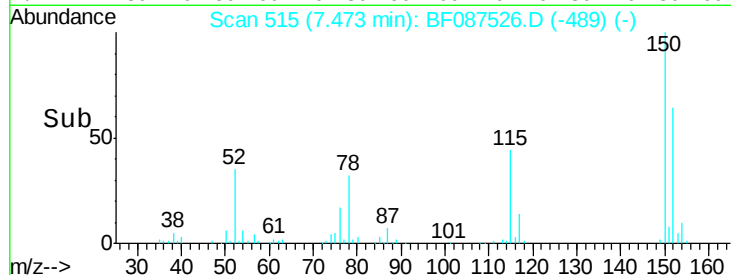



#5

2-Fluorophenol
Concen: 46.61 ng
RT: 5.38 min Scan# 332
Delta R.T. 0.01 min
Lab File: BF087526.D
Acq: 29 May 2016 23:23

Tgt Ion:112 Resp: 307453
Ion Ratio Lower Upper
112 100
64 73.3 52.1 78.1
63 40.1 25.7 38.5#

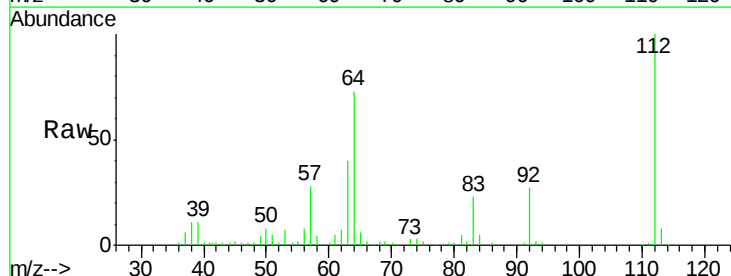

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

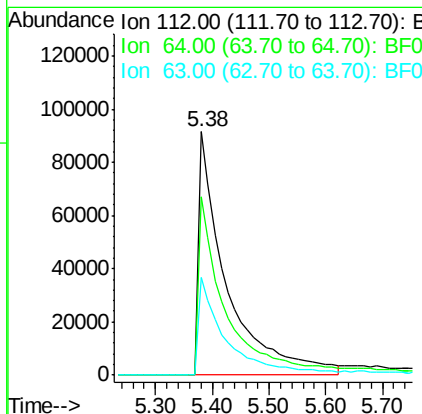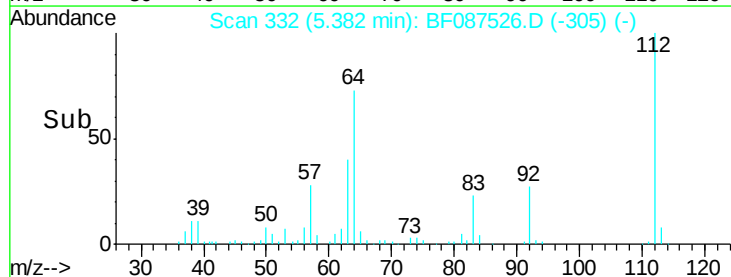



#7

Phenol-d6

Concen: 26.42 ng

RT: 7.04 min Scan# 477

Delta R.T. 0.00 min

Lab File: BF087526.D

Acq: 29 May 2016 23:23

Instrument :

BNA_F

ClientSampleId :

MW-13


Tot Ion: 99 Resp: 235487

Ion Ratio Lower Upper

99 100

42 28.7 13.6 20.4#




71 39.9 24.6 36.8#

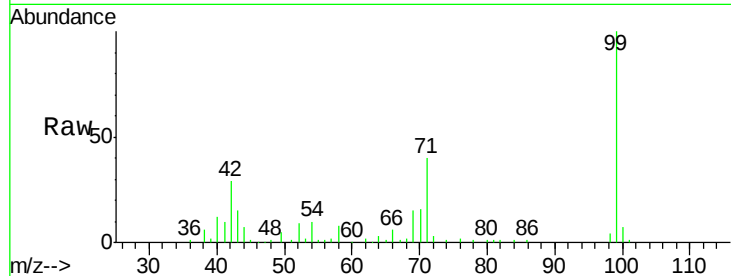

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

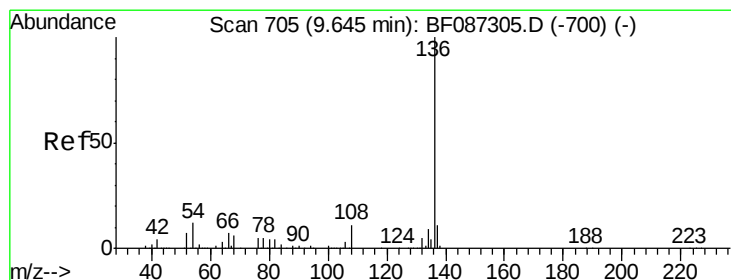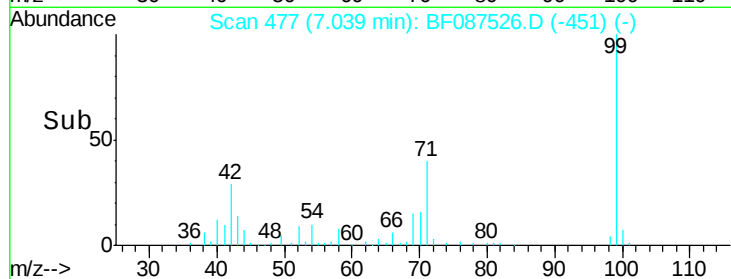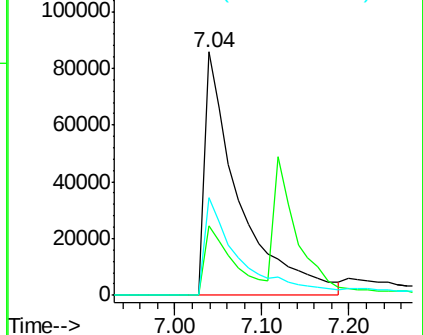

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.51 min Scan# 693

Delta R.T. 0.00 min

Lab File: BF087526.D

Acq: 29 May 2016 23:23

Tgt Ion: 136 Resp: 443060


Ion Ratio Lower Upper

136 100

137 11.1 8.8 13.2

54 11.0 5.0 7.4#

68 5.1 4.4 6.6


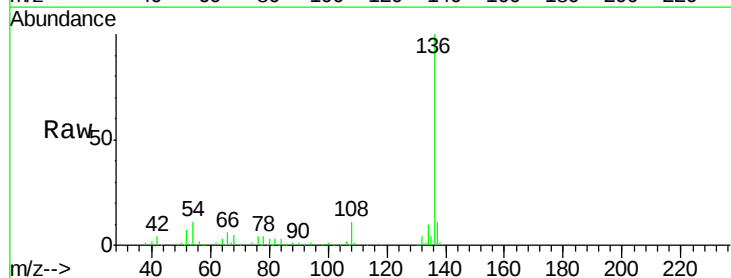


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0


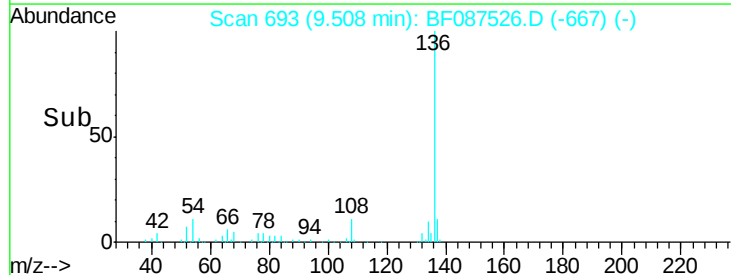
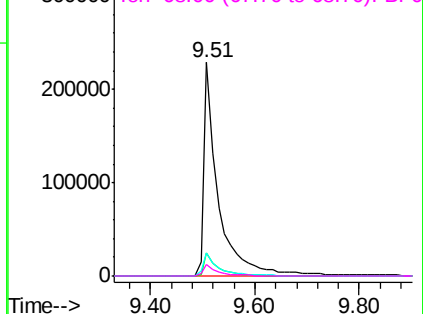




#23
 Nitrobenzene-d5
 Concen: 79.29 ng
 RT: 8.39 min Scan# 595
 Delta R.T. -0.02 min
 Lab File: BF087526.D
 Acq: 29 May 2016 23:23




Instrument :
 BNA_F
 ClientSampleId :
 MW-13

Tot Ion: 82 Resp: 697004
 Ion Ratio Lower Upper
 82 100
 128 38.1 40.6 61.0#
 54 69.6 38.1 57.1#

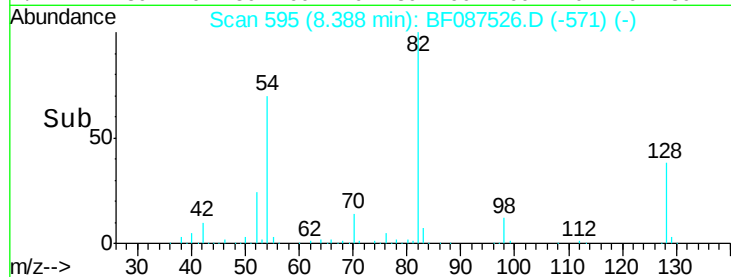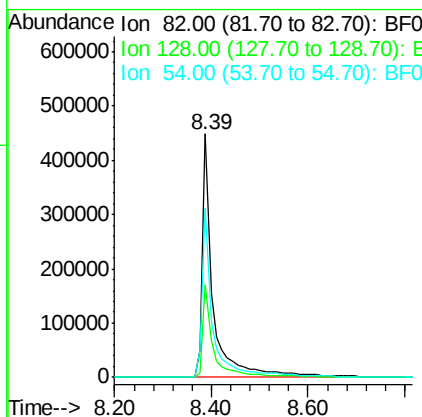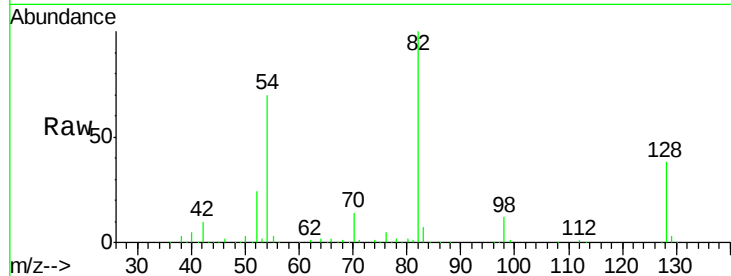

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 12.33 min Scan# 940
 Delta R.T. 0.00 min
 Lab File: BF087526.D
 Acq: 29 May 2016 23:23

Tgt Ion: 164 Resp: 206566
 Ion Ratio Lower Upper
 164 100
 162 103.4 82.8 124.2
 160 46.8 36.9 55.3


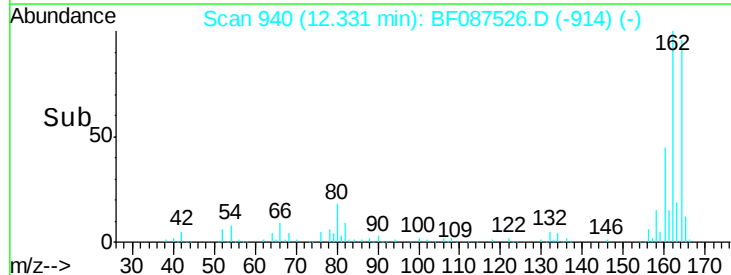
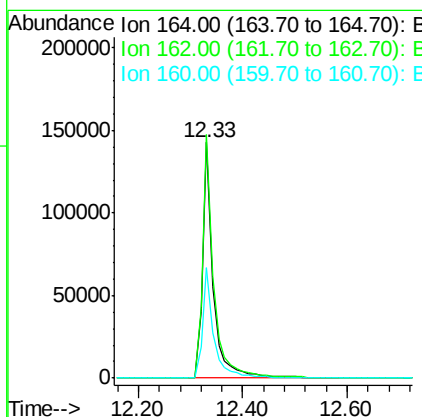
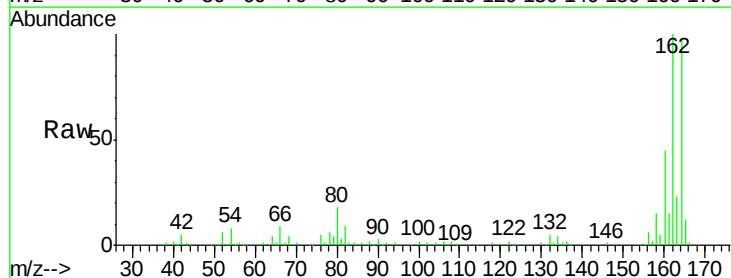




#41
 2,4,6-Tribromophenol
 Concen: 109.18 ng
 RT: 13.62 min Scan# 1053
 Delta R.T. -0.01 min
 Lab File: BF087526.D
 Acq: 29 May 2016 23:23




Instrument :
 BNA_F
 ClientSampleId :
 MW-13


Tot Ion	Ratio	Lower	Upper
330	100		
332	97.4	79.0	118.4
141	46.3	31.2	46.8

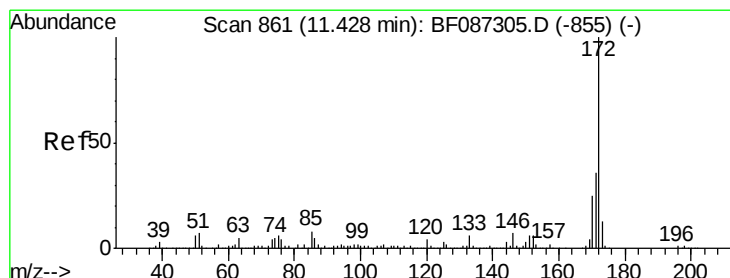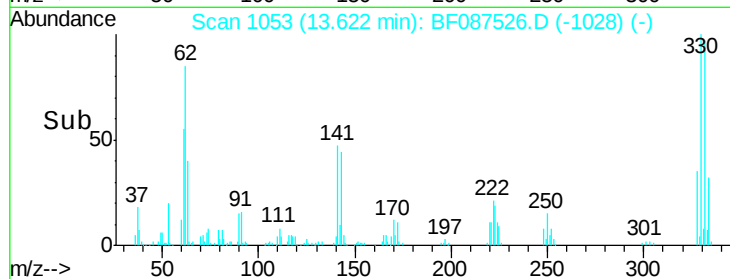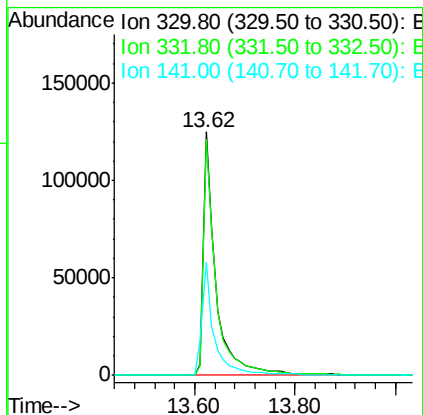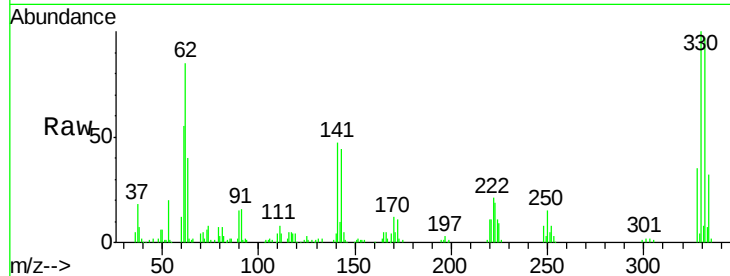

#44
 2-Fluorobiphenyl
 Concen: 81.82 ng
 RT: 11.28 min Scan# 848
 Delta R.T. -0.01 min
 Lab File: BF087526.D
 Acq: 29 May 2016 23:23

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.3	29.0	43.6
170	24.1	19.8	29.8

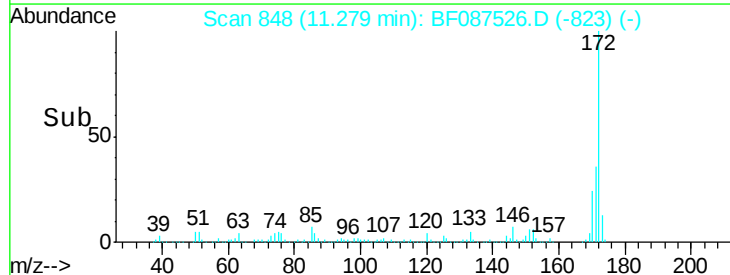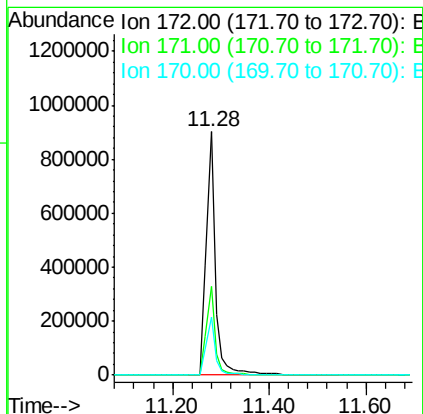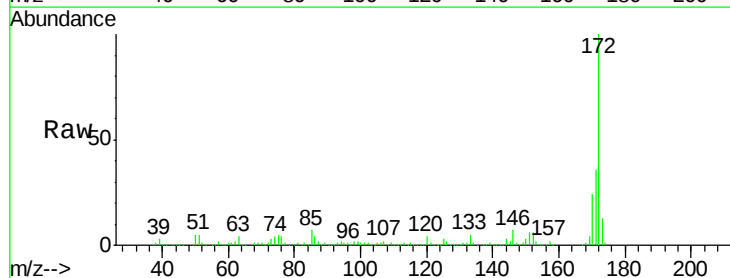


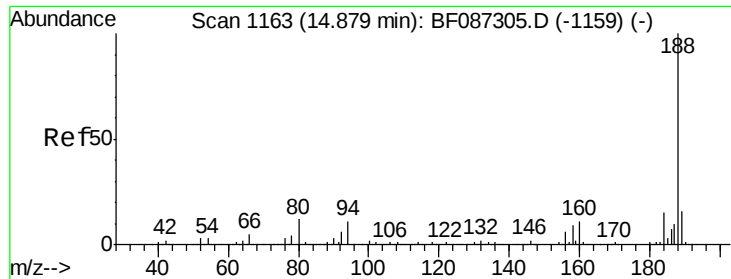




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 14.74 min Scan# 1151
Delta R.T. 0.00 min
Lab File: BF087526.D
Acq: 29 May 2016 23:23

Instrument :
BNA_F
ClientSampleId :
MW-13

Tot Ion	Ratio	Lower	Upper
188	100		
94	8.6	6.8	10.2
80	9.2	7.1	10.7

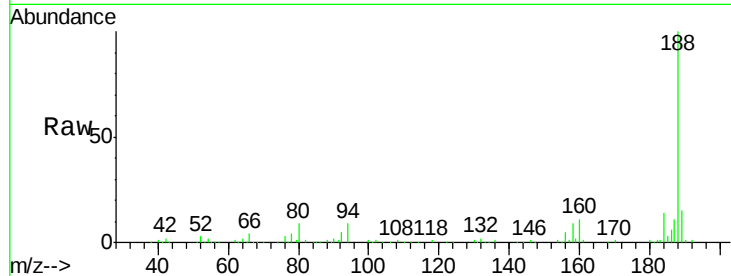


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

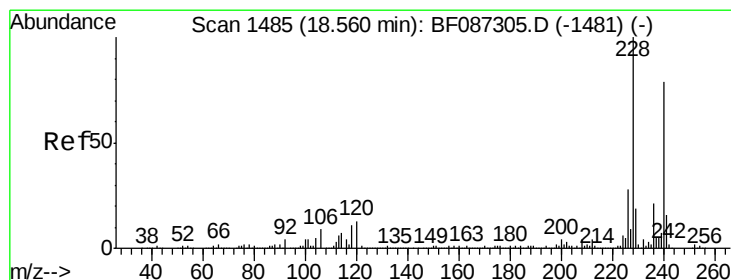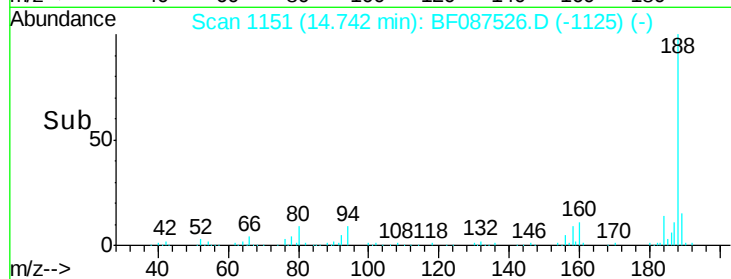
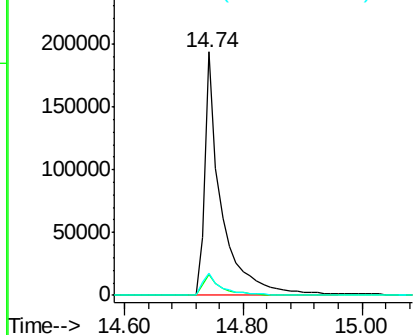



#75
Chrysene-d12
Concen: 20.00 ng
RT: 18.46 min Scan# 1476
Delta R.T. 0.01 min
Lab File: BF087526.D
Acq: 29 May 2016 23:23

Tgt Ion	Ratio	Lower	Upper
240	100		
120	11.3	11.2	16.8
236	26.4	21.2	31.8

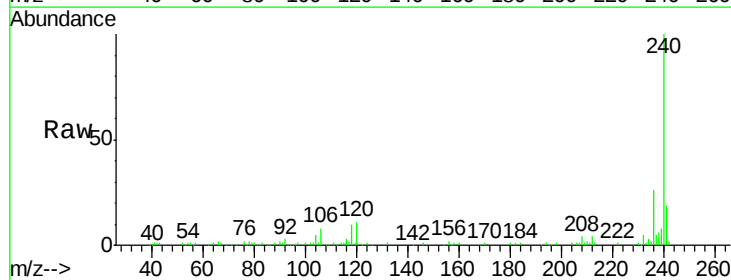

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

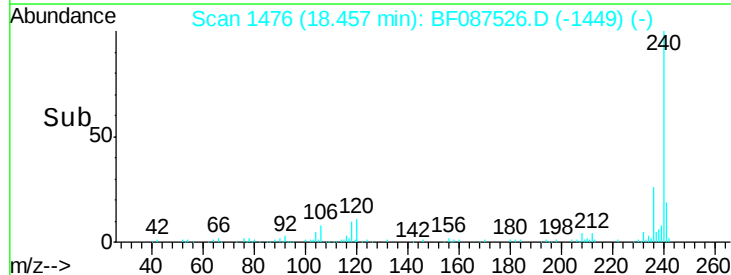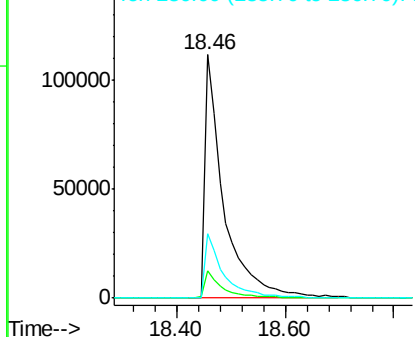

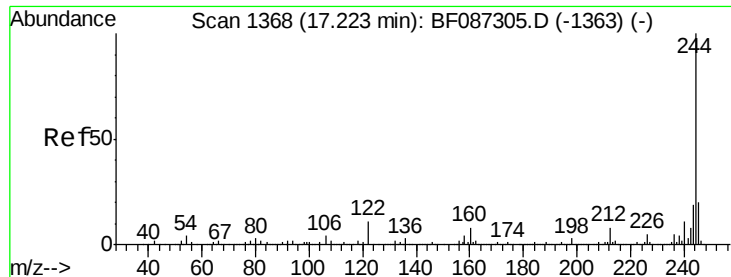

#78

Terphenyl-d14

Concen: 73.71 ng

RT: 17.09 min Scan# 1356

Delta R.T. -0.01 min

Lab File: BF087526.D

Acq: 29 May 2016 23:23

Instrument :

BNA_F

ClientSampleId :

MW-13


Tot Ion:244 Resp: 935958

Ion Ratio Lower Upper

244 100

212 8.0 6.2 9.2




122 12.3 12.0 18.0

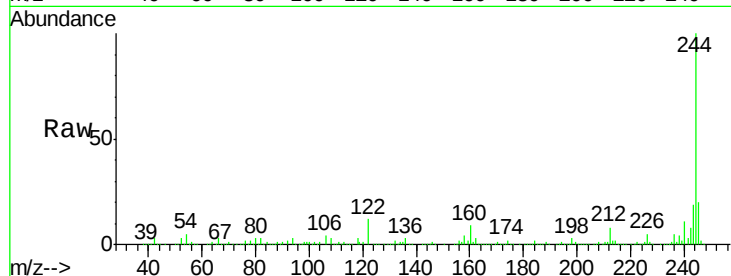

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

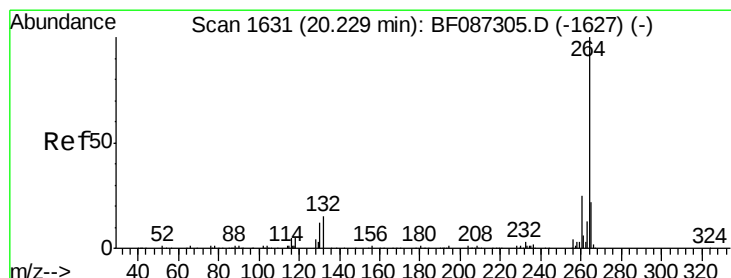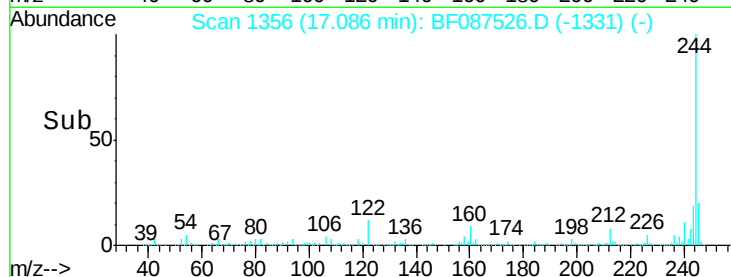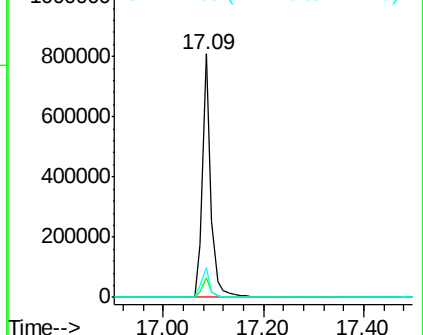

#86

Perylene-d12

Concen: 20.00 ng

RT: 20.15 min Scan# 1624

Delta R.T. 0.02 min

Lab File: BF087526.D

Acq: 29 May 2016 23:23


Tgt Ion:264 Resp: 200859

Ion Ratio Lower Upper

264 100

260 24.0 19.5 29.3

265 21.7 17.3 25.9

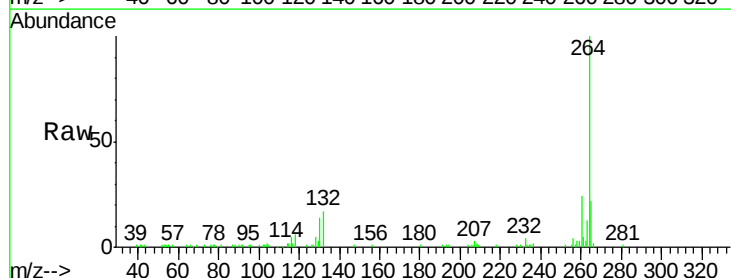

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

