

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052916\
 Data File : BF087530.D
 Acq On : 30 May 2016 1:41
 Operator : UM/SJ
 Sample : H3222-15
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-28

Quant Time: May 30 07:17:17 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF052316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon May 30 07:00:04 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.47	152	115482	20.00	ng	0.00
21) Naphthalene-d8	9.51	136	446670	20.00	ng	0.00
38) Acenaphthene-d10	12.33	164	209118	20.00	ng	0.00
63) Phenanthrene-d10	14.74	188	381703	20.00	ng	0.00
75) Chrysene-d12	18.46	240	268939	20.00	ng	0.01
86) Perylene-d12	20.15	264	205642	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	465030	70.76	ng	0.00
7) Phenol-d6	7.03	99	486218	54.75	ng	-0.01
23) Nitrobenzene-d5	8.39	82	754198	85.10	ng	-0.02
41) 2,4,6-Tribromophenol	13.62	330	247443	123.13	ng	-0.01
44) 2-Fluorobiphenyl	11.28	172	1298864	87.56	ng	-0.01
78) Terphenyl-d14	17.09	244	1134004	89.64	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052916\
Data File : BF087530.D
Acq On : 30 May 2016 1:41
Operator : UM/SJ
Sample : H3222-15
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-28

Quant Time: May 30 07:17:17 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon May 30 07:00:04 2016
Response via : Initial Calibration

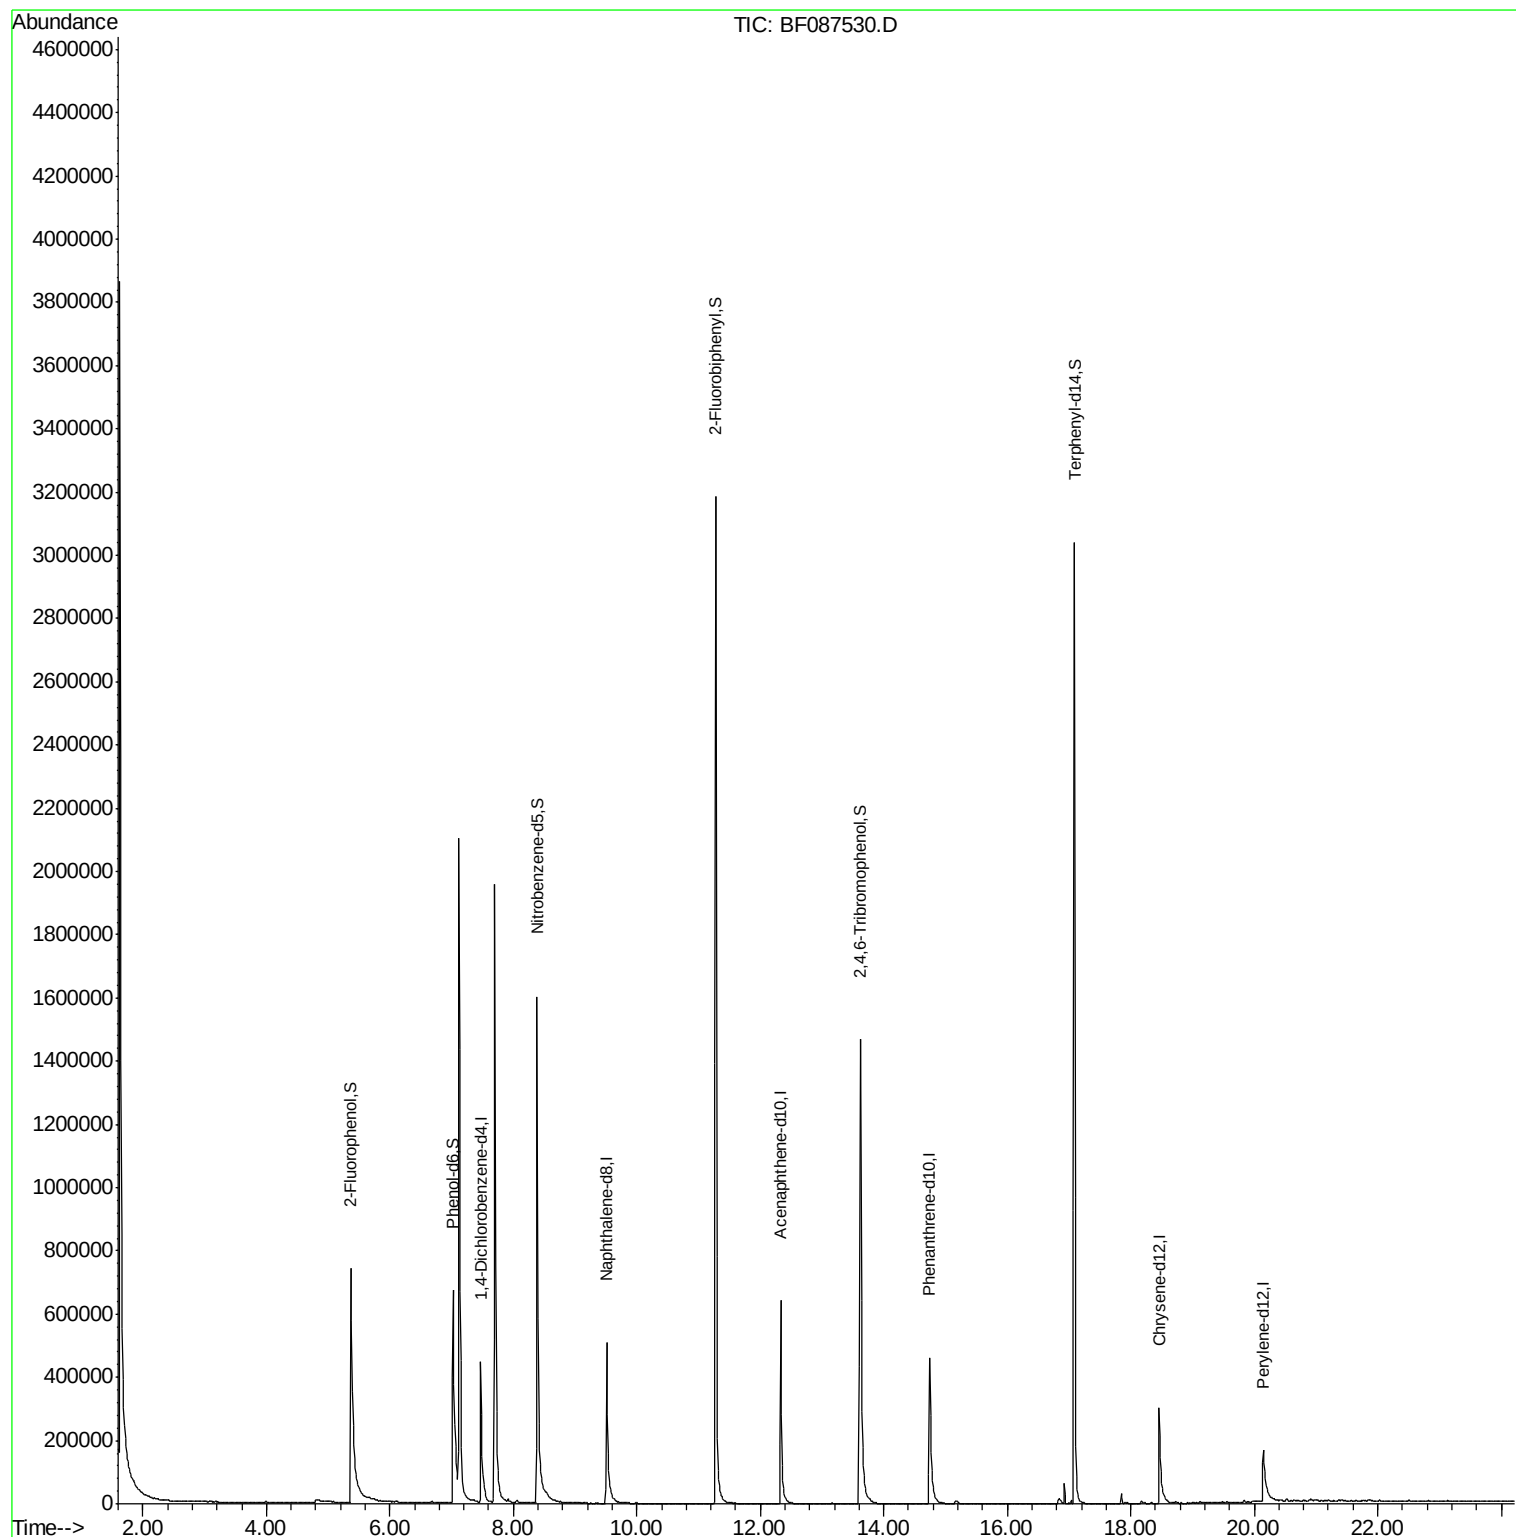

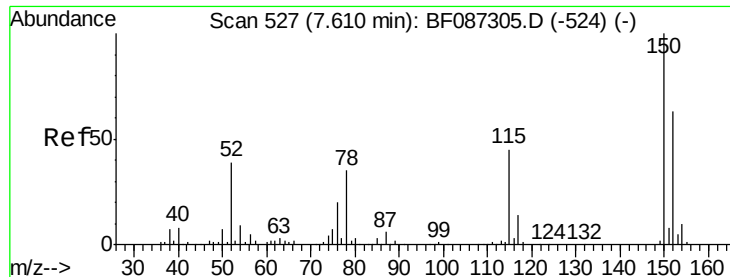


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.47 min Scan# 515
Delta R.T. -0.00 min
Lab File: BF087530.D
Acq: 30 May 2016 1:41

Instrument :
BNA_F
ClientSampled :
MW-28

Tot Ion:152 Resp: 115482
Ion Ratio Lower Upper
152 100
150 158.2 125.8 188.6
115 69.1 51.5 77.3

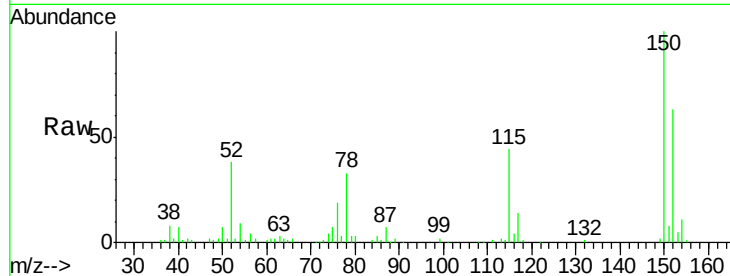


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

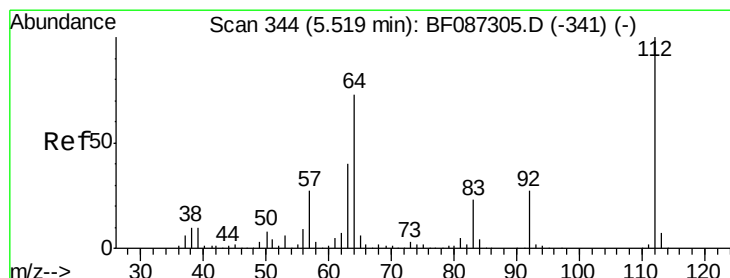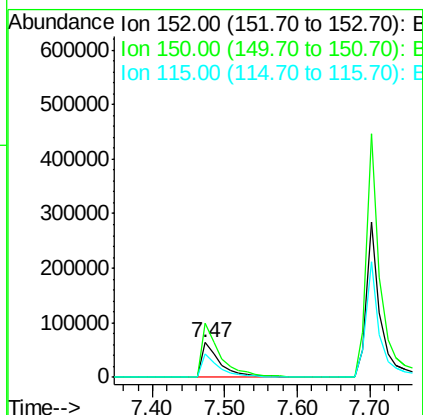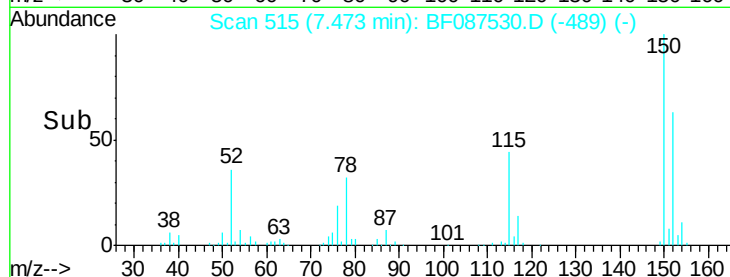



#5


2-Fluorophenol
Concen: 70.76 ng
RT: 5.37 min Scan# 331
Delta R.T. -0.00 min
Lab File: BF087530.D
Acq: 30 May 2016 1:41

Tgt Ion:112 Resp: 465030
Ion Ratio Lower Upper
112 100
64 75.1 52.1 78.1
63 42.2 25.7 38.5#

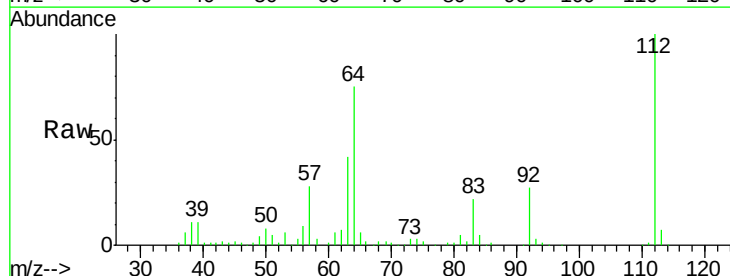

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

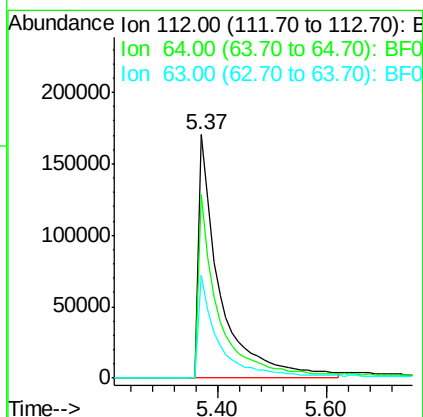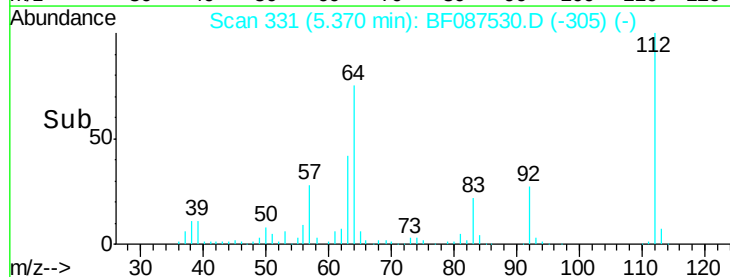

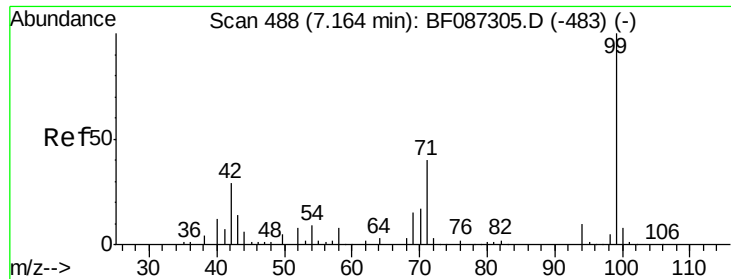

#7

Phenol-d6

Concen: 54.75 ng

RT: 7.03 min Scan# 476

Delta R.T. -0.01 min

Lab File: BF087530.D

Acq: 30 May 2016 1:41

Instrument :

BNA_F

ClientSampled :

MW-28


Tot Ion: 99 Resp: 486218

Ion Ratio Lower Upper

99 100

42 27.7 13.6 20.4#


71 38.6 24.6 36.8#

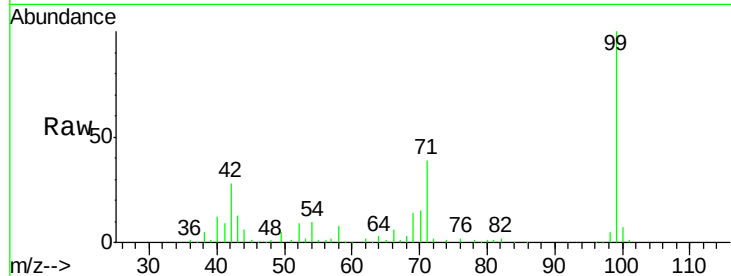



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

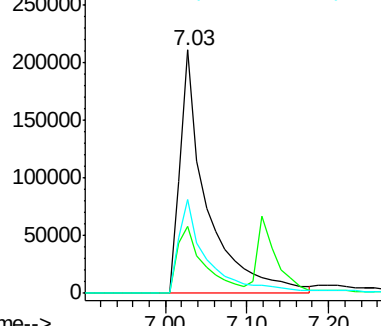

Time-->

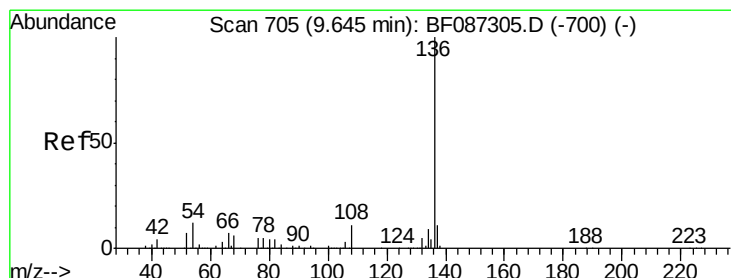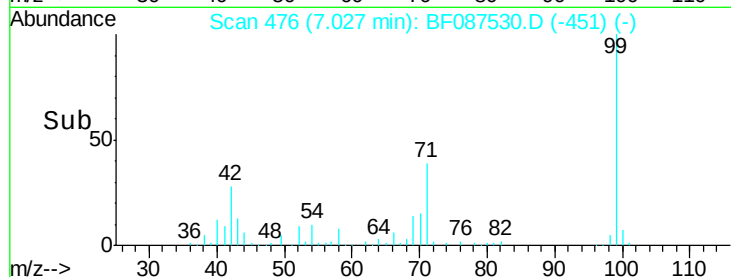

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.51 min Scan# 693

Delta R.T. -0.00 min

Lab File: BF087530.D

Acq: 30 May 2016 1:41

Tgt Ion: 136 Resp: 446670


Ion Ratio Lower Upper

136 100

137 11.0 8.8 13.2

54 10.9 5.0 7.4#

68 5.2 4.4 6.6

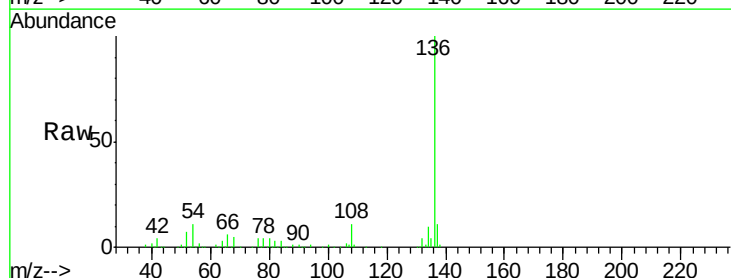


Abundance Ion 136.00 (135.70 to 136.70): E


Ion 137.00 (136.70 to 137.70): E


Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

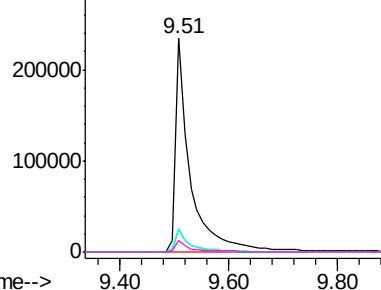

Time-->




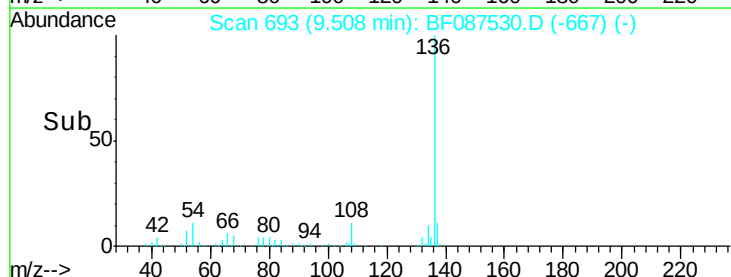


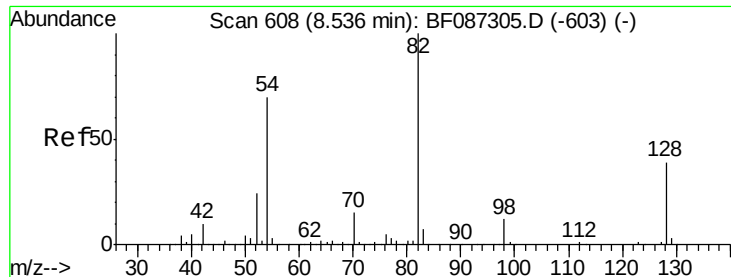

#23
Nitrobenzene-d5
Concen: 85.10 ng
RT: 8.39 min Scan# 595
Delta R.T. -0.02 min
Lab File: BF087530.D
Acq: 30 May 2016 1:41




Instrument :
BNA_F
ClientSampleId :
MW-28


Tot Ion: 82 Resp: 754198
Ion Ratio Lower Upper
82 100
128 38.3 40.6 61.0#
54 70.8 38.1 57.1#

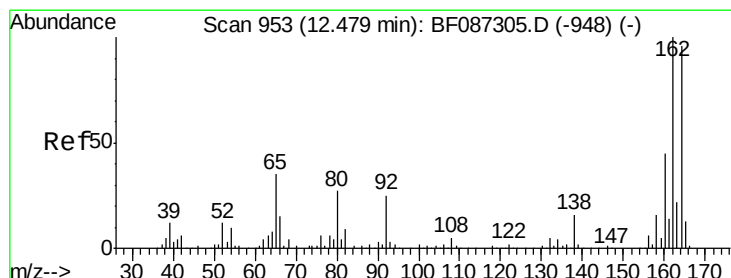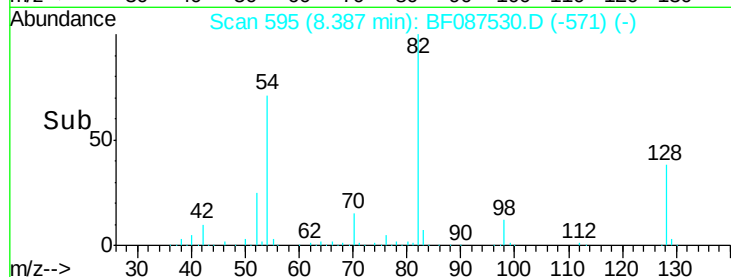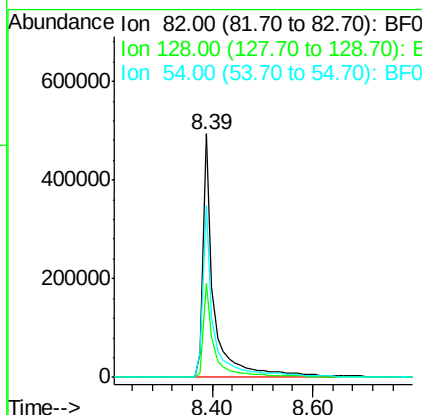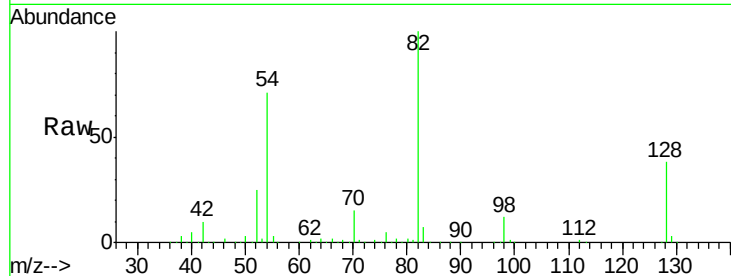

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 12.33 min Scan# 940
Delta R.T. -0.00 min
Lab File: BF087530.D
Acq: 30 May 2016 1:41

Tgt Ion:164 Resp: 209118
Ion Ratio Lower Upper
164 100
162 103.7 82.8 124.2
160 47.3 36.9 55.3

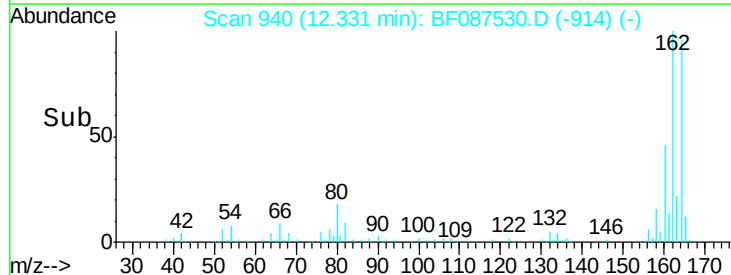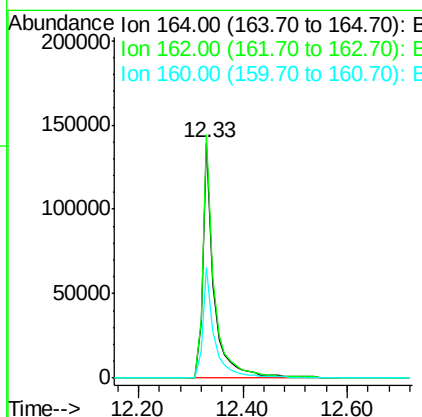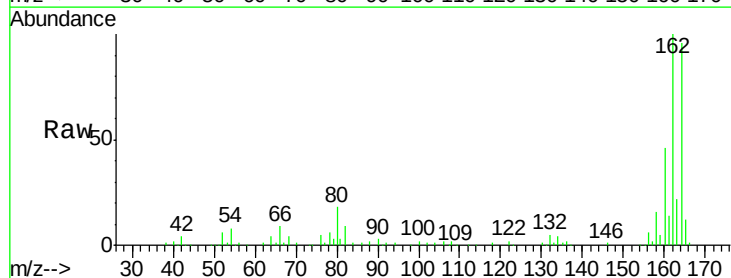


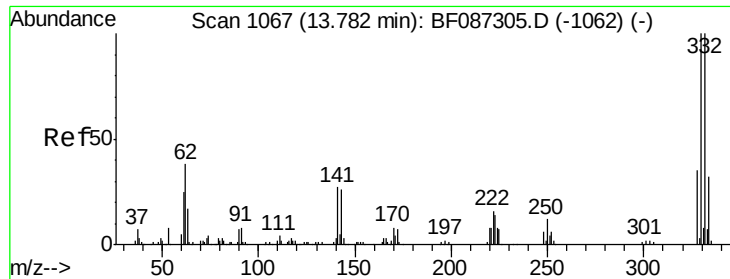




#41
 2,4,6-Tribromophenol
 Concen: 123.13 ng
 RT: 13.62 min Scan# 1053
 Delta R.T. -0.01 min
 Lab File: BF087530.D
 Acq: 30 May 2016 1:41

Instrument :
 BNA_F
 ClientSampled :
 MW-28

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.0	79.0	118.4
141	45.3	31.2	46.8

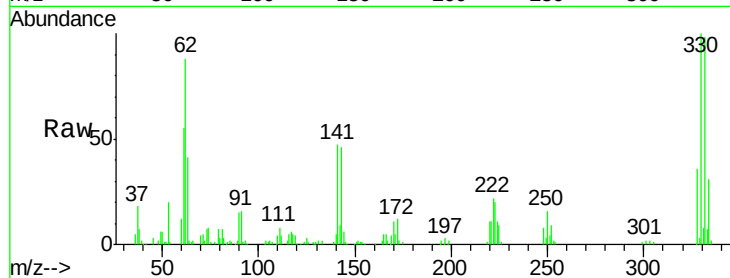


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

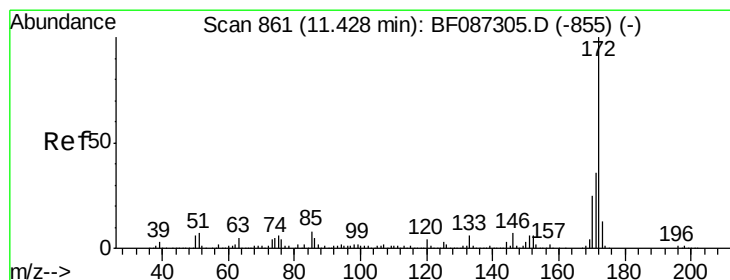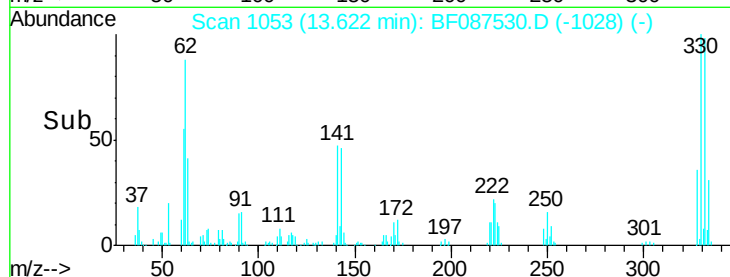
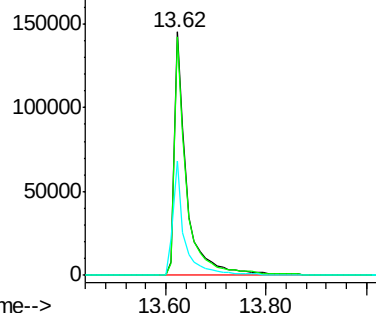



#44
 2-Fluorobiphenyl
 Concen: 87.56 ng
 RT: 11.28 min Scan# 848
 Delta R.T. -0.01 min
 Lab File: BF087530.D
 Acq: 30 May 2016 1:41

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.0	29.0	43.6
170	24.4	19.8	29.8

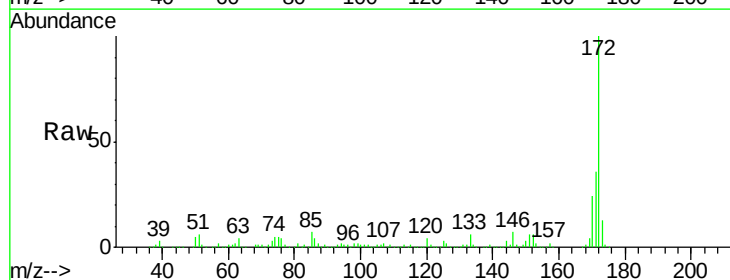

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

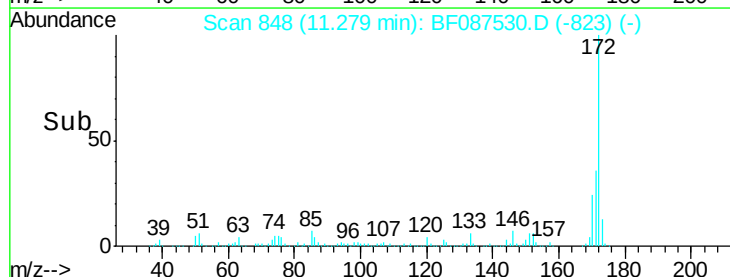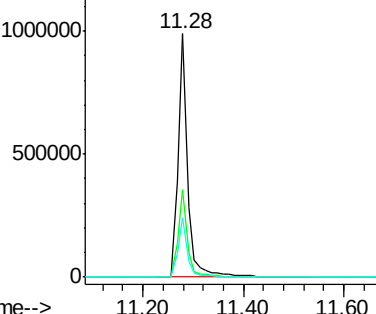


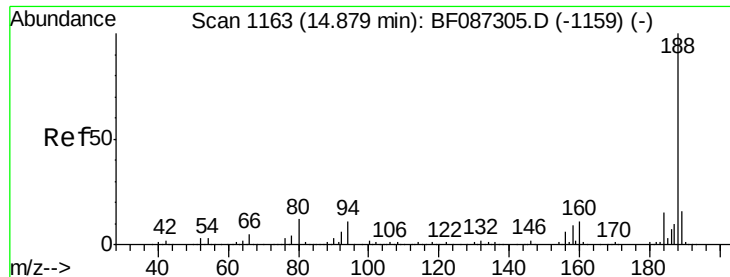




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 14.74 min Scan# 1151
Delta R.T. -0.00 min
Lab File: BF087530.D
Acq: 30 May 2016 1:41

Instrument :
BNA_F
ClientSampleId :
MW-28

Tot Ion:188 Resp: 381703
Ion Ratio Lower Upper
188 100
94 9.1 6.8 10.2
80 10.0 7.1 10.7

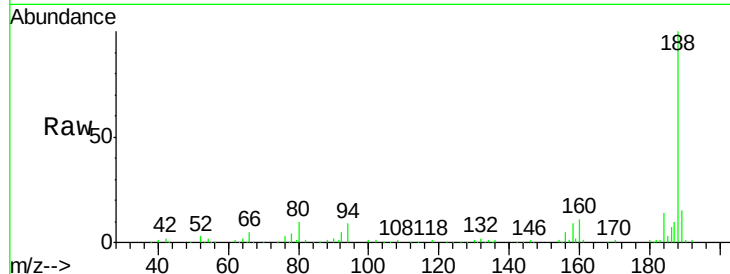


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

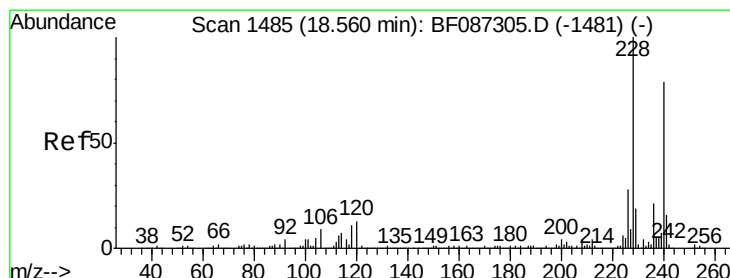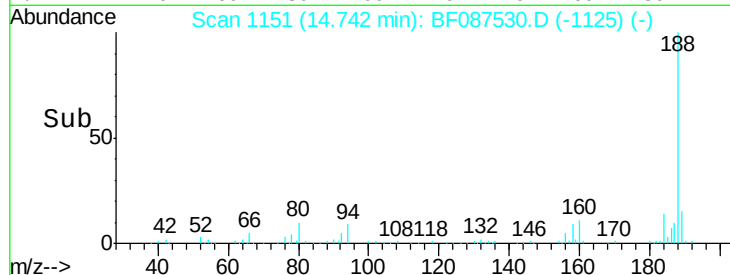
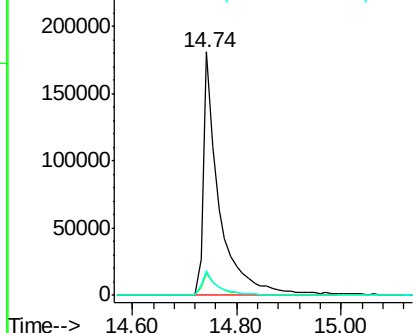



#75
Chrysene-d12
Concen: 20.00 ng
RT: 18.46 min Scan# 1476
Delta R.T. 0.01 min
Lab File: BF087530.D
Acq: 30 May 2016 1:41

Tgt Ion:240 Resp: 268939
Ion Ratio Lower Upper
240 100
120 11.1 11.2 16.8#
236 25.6 21.2 31.8

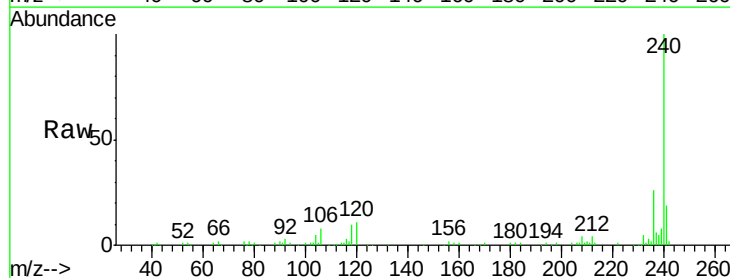

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



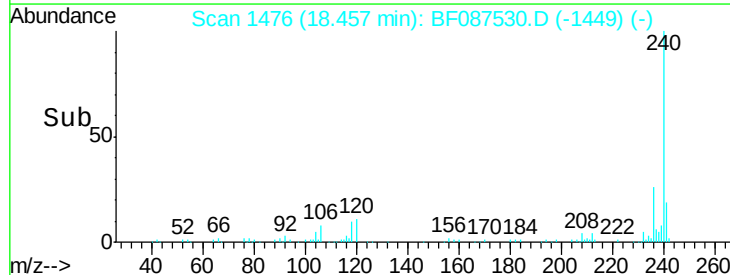
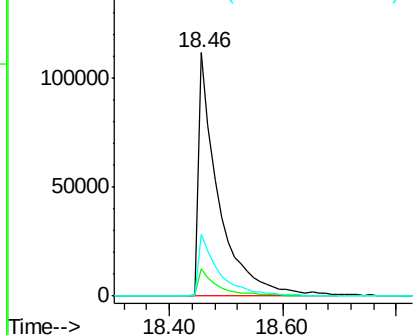


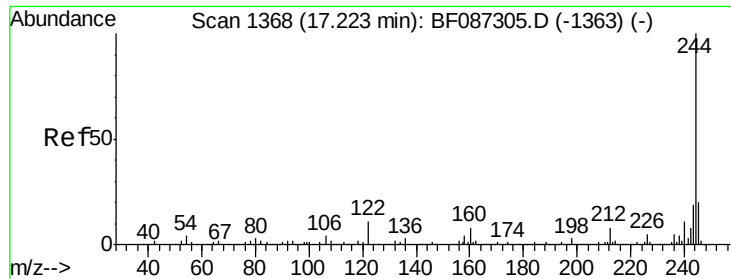

#78
 Terphenyl-d14
 Concen: 89.64 ng
 RT: 17.09 min Scan# 1356
 Delta R.T. -0.01 min
 Lab File: BF087530.D
 Acq: 30 May 2016 1:41

Instrument :
 BNA_F
 ClientSampleId :
 MW-28

Tot Ion:244 Resp: 1134004
 Ion Ratio Lower Upper
 244 100
 212 8.0 6.2 9.2
 122 12.6 12.0 18.0

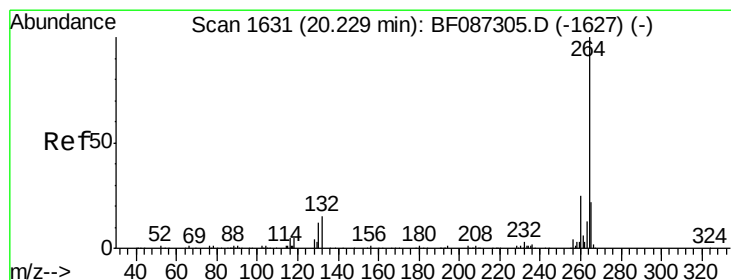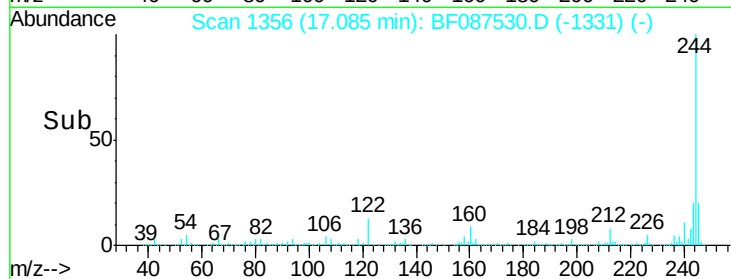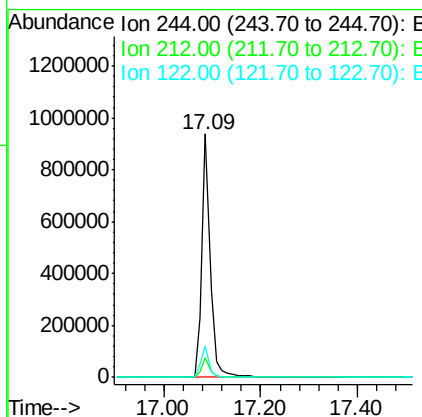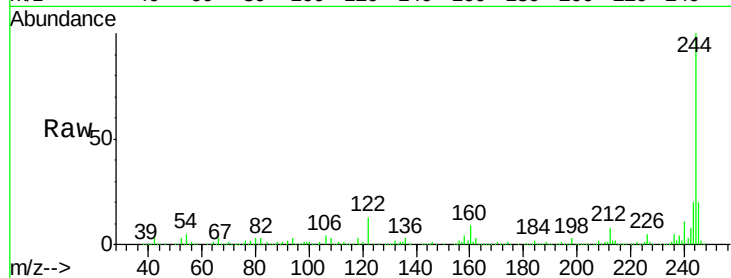

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 20.15 min Scan# 1624
 Delta R.T. 0.02 min
 Lab File: BF087530.D
 Acq: 30 May 2016 1:41

Tgt Ion:264 Resp: 205642
 Ion Ratio Lower Upper
 264 100
 260 23.5 19.5 29.3
 265 20.1 17.3 25.9

