

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052916\
 Data File : BF087569.D
 Acq On : 31 May 2016 2:11
 Operator : UM/SJ
 Sample : H3249-06
 Misc :
 ALS Vial : 87 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-25

Quant Time: May 31 03:10:53 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF052316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue May 31 00:45:12 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.48	152	105252	20.00	ng	0.01
21) Naphthalene-d8	9.52	136	424743	20.00	ng	0.01
38) Acenaphthene-d10	12.34	164	199830	20.00	ng	0.01
63) Phenanthrene-d10	14.77	188	344964	20.00	ng	0.02
75) Chrysene-d12	18.49	240	251564	20.00	ng	0.05
86) Perylene-d12	20.19	264	191846	20.00	ng	0.07
System Monitoring Compounds						
5) 2-Fluorophenol	5.40	112	348736	58.22	ng	0.03
7) Phenol-d6	7.06	99	257594	31.83	ng	0.02
23) Nitrobenzene-d5	8.40	82	803269	95.31	ng	-0.01
41) 2,4,6-Tribromophenol	13.63	330	221449	115.32	ng	0.00
44) 2-Fluorobiphenyl	11.28	172	1305986	92.14	ng	-0.01
78) Terphenyl-d14	17.10	244	1117892	94.47	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052916\
Data File : BF087569.D
Acq On : 31 May 2016 2:11
Operator : UM/SJ
Sample : H3249-06
Misc :
ALS Vial : 87 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-25

Quant Time: May 31 03:10:53 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue May 31 00:45:12 2016
Response via : Initial Calibration

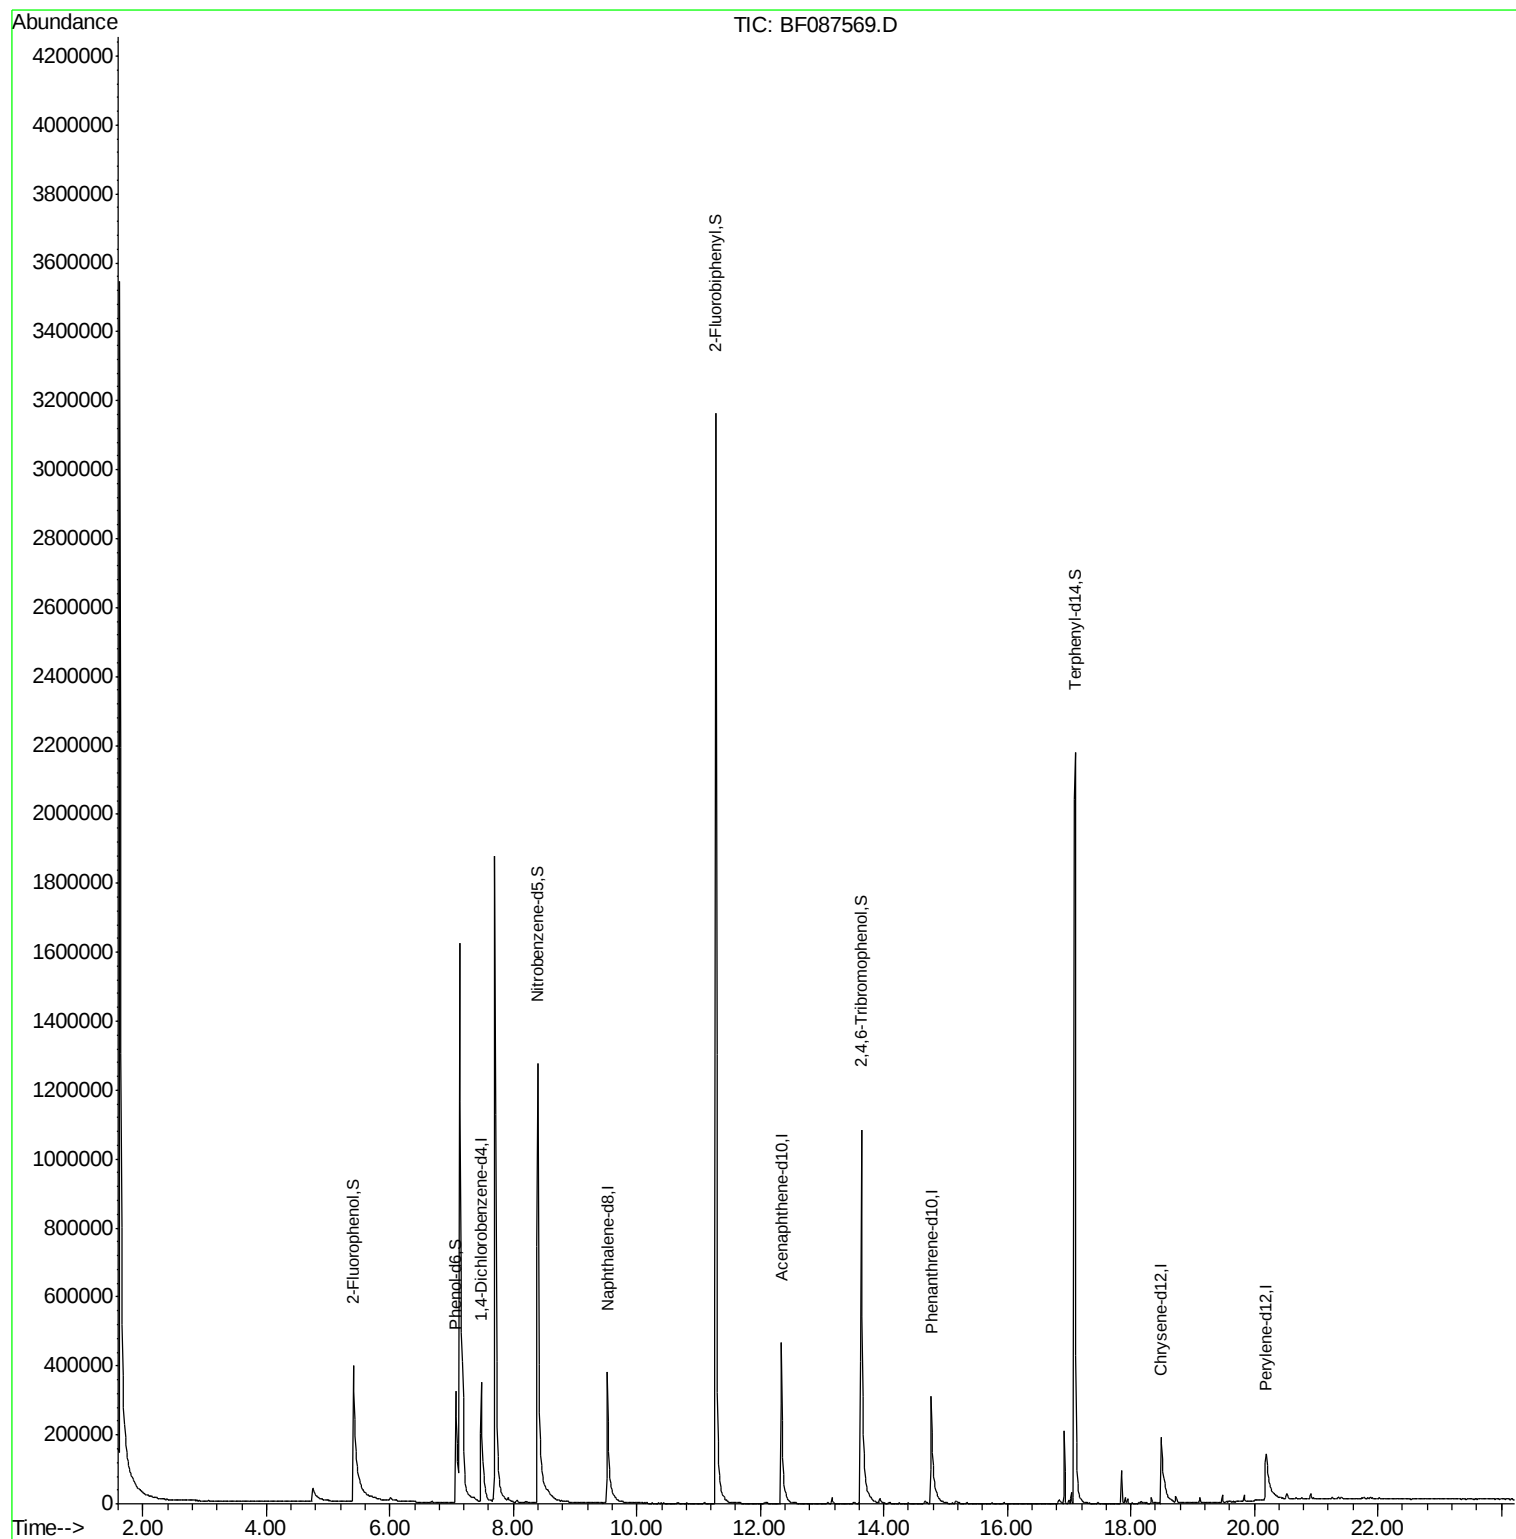

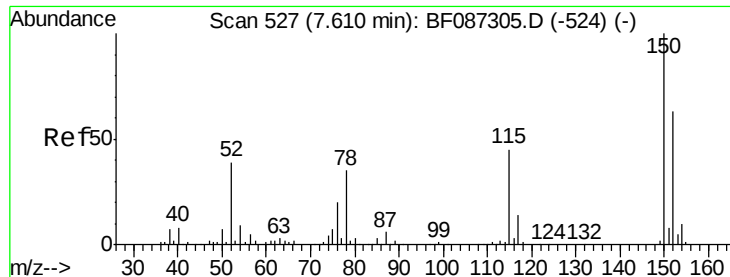

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 7.48 min Scan# 516

Delta R.T. 0.01 min

Lab File: BF087569.D

Acq: 31 May 2016 2:11

Instrument :

BNA_F

ClientSampled :

MW-25


Tot Ion:152 Resp: 105252

Ion Ratio Lower Upper

152 100

150 160.6 125.8 188.6




115 65.1 51.5 77.3

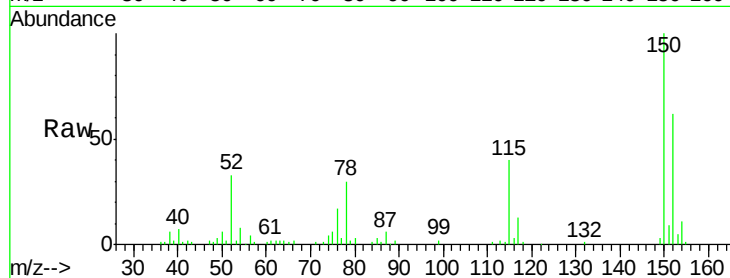

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

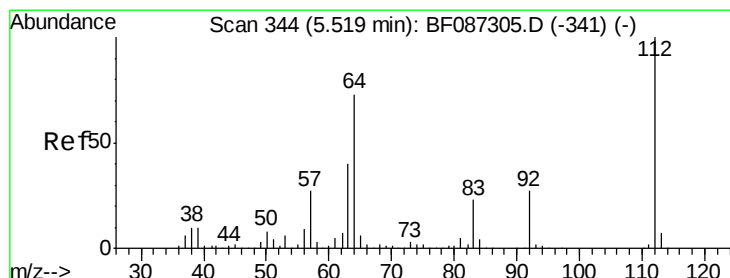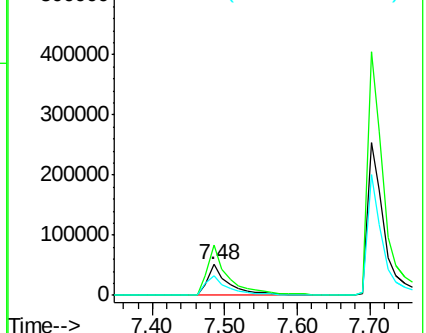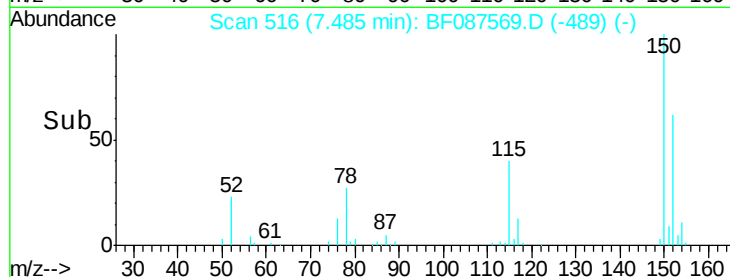

#5

2-Fluorophenol

Concen: 58.22 ng

RT: 5.40 min Scan# 334

Delta R.T. 0.03 min

Lab File: BF087569.D

Acq: 31 May 2016 2:11


Tgt Ion:112 Resp: 348736

Ion Ratio Lower Upper

112 100

64 71.7 52.1 78.1



63 41.1 25.7 38.5#

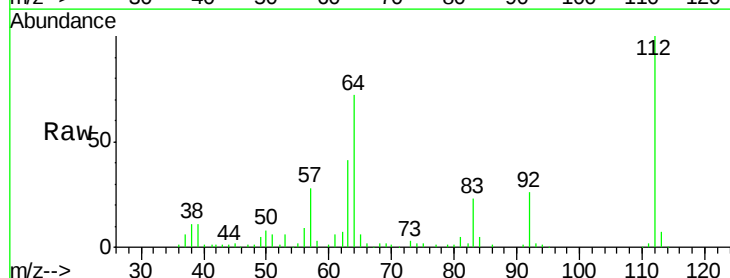


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

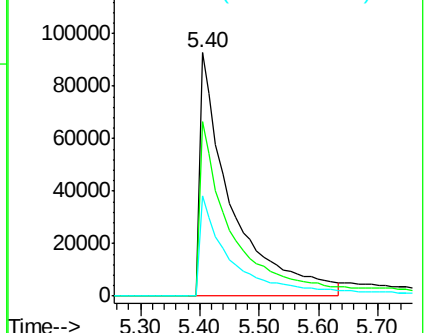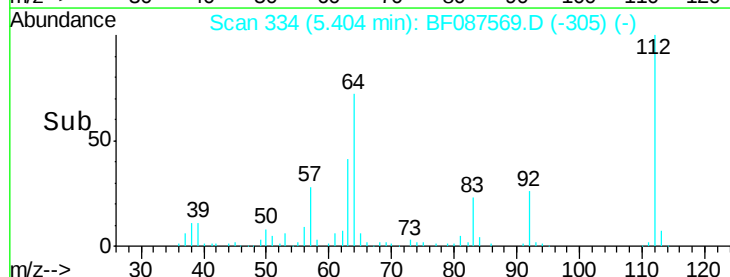

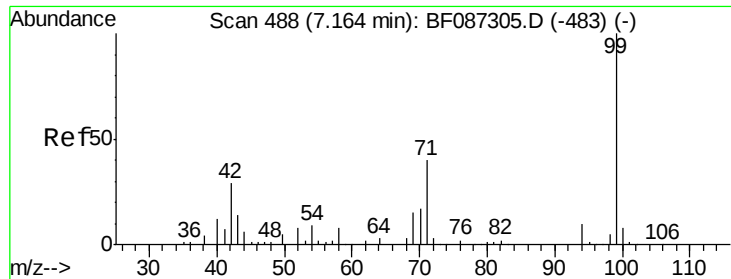

#7

Phenol-d6

Concen: 31.83 ng

RT: 7.06 min Scan# 479

Delta R.T. 0.02 min

Lab File: BF087569.D

Acq: 31 May 2016 2:11

Instrument :

BNA_F

ClientSampleId :

MW-25


Tot Ion: 99 Resp: 257594

Ion Ratio Lower Upper

99 100

42 30.4 13.6 20.4#




71 41.8 24.6 36.8#

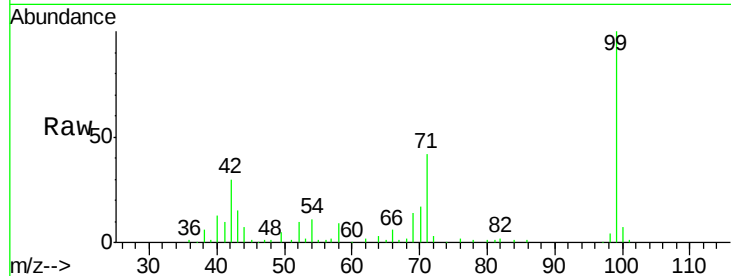

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

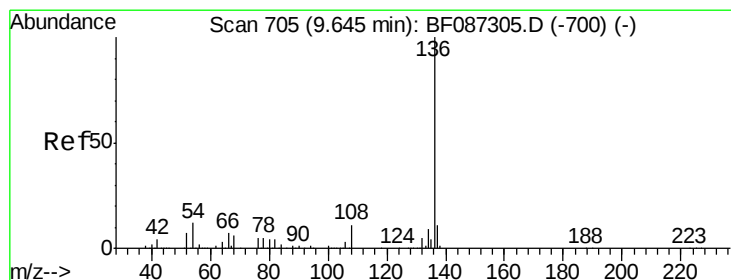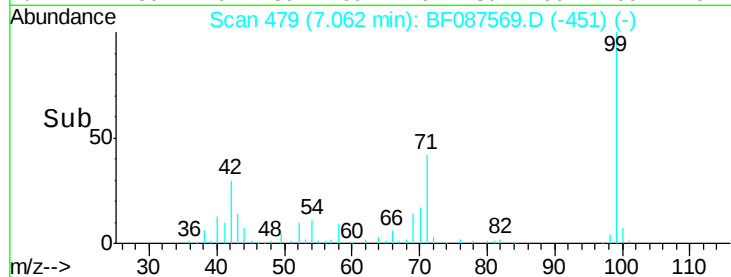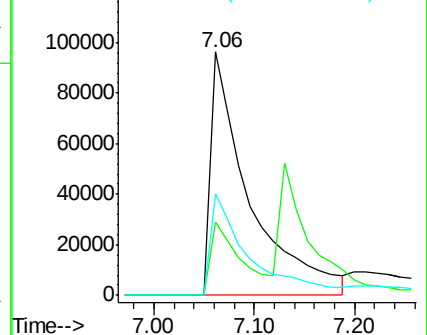

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 9.52 min Scan# 694

Delta R.T. 0.01 min

Lab File: BF087569.D

Acq: 31 May 2016 2:11

Tgt Ion: 136 Resp: 424743


Ion Ratio Lower Upper

136 100

137 10.6 8.8 13.2

54 10.3 5.0 7.4#

68 5.1 4.4 6.6


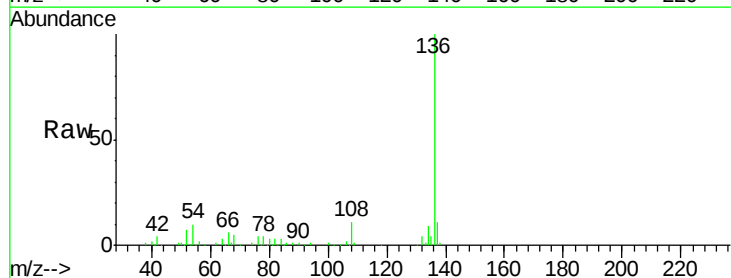



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



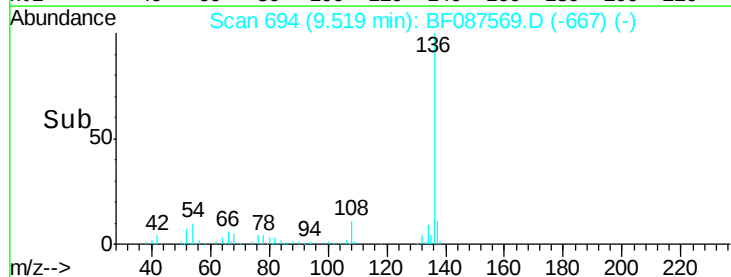
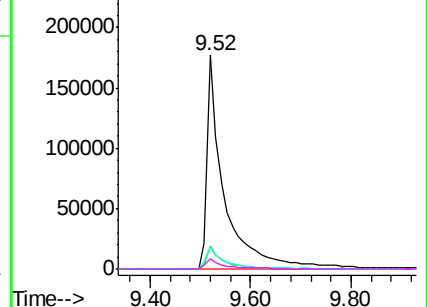


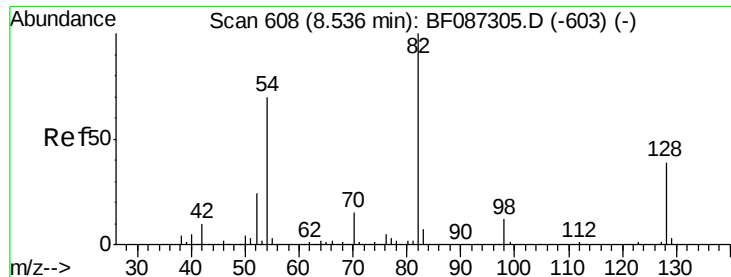

#23
Nitrobenzene-d5
Concen: 95.31 ng
RT: 8.40 min Scan# 596
Delta R.T. -0.01 min
Lab File: BF087569.D
Acq: 31 May 2016 2:11




Instrument :
BNA_F
ClientSampleId :
MW-25


Tot Ion: 82 Resp: 803269
Ion Ratio Lower Upper
82 100
128 42.7 40.6 61.0
54 66.4 38.1 57.1#

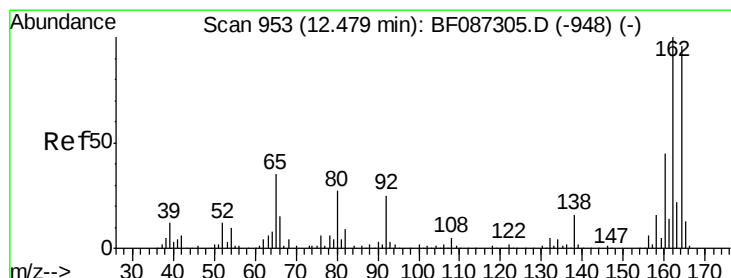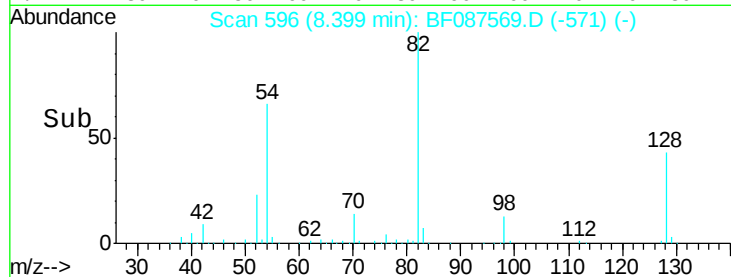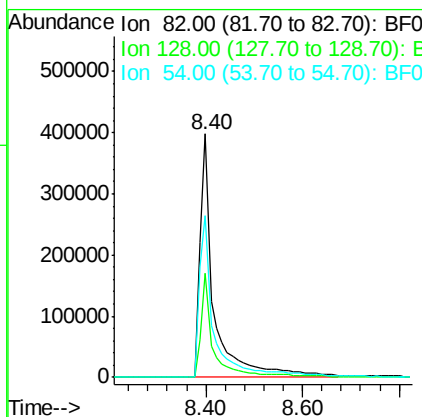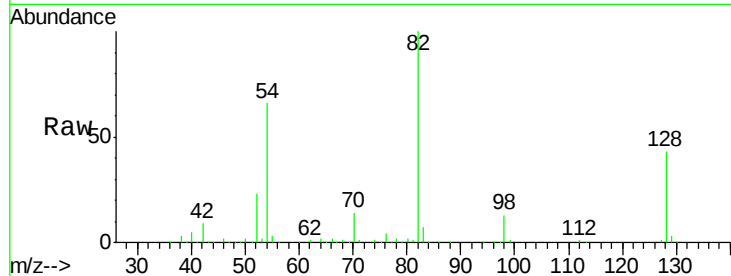

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 12.34 min Scan# 941
Delta R.T. 0.01 min
Lab File: BF087569.D
Acq: 31 May 2016 2:11

Tgt Ion: 164 Resp: 199830
Ion Ratio Lower Upper
164 100
162 103.0 82.8 124.2
160 46.6 36.9 55.3


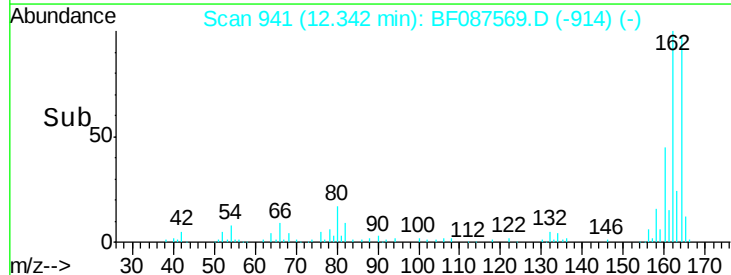
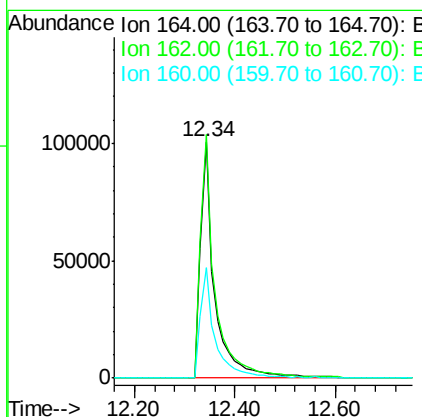
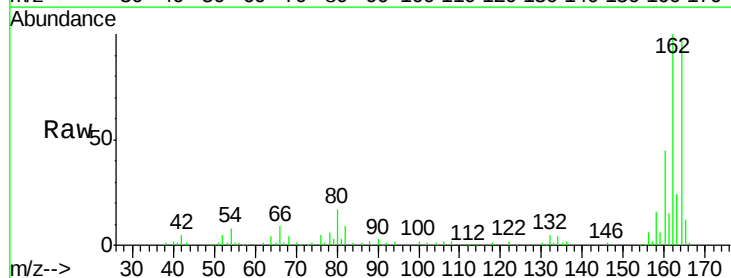


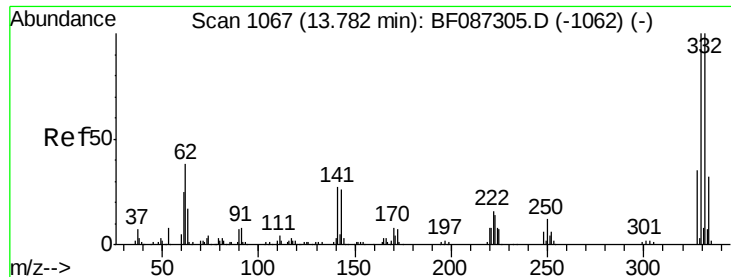

#41
 2,4,6-Tribromophenol
 Concen: 115.32 ng
 RT: 13.63 min Scan# 1054
 Delta R.T. -0.00 min
 Lab File: BF087569.D
 Acq: 31 May 2016 2:11




Instrument :
 BNA_F
 ClientSampleId :
 MW-25


Tot Ion	Ratio	Lower	Upper
330	100		
332	97.2	79.0	118.4
141	46.1	31.2	46.8

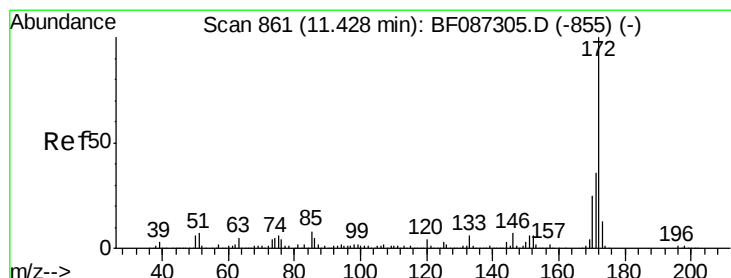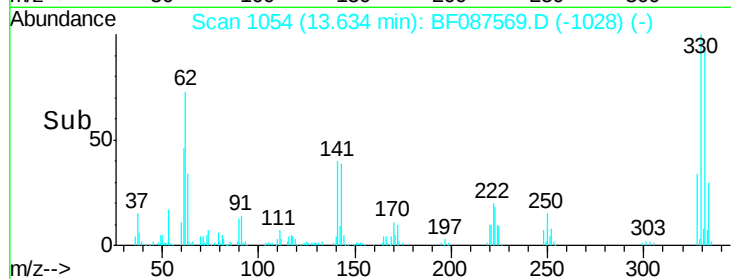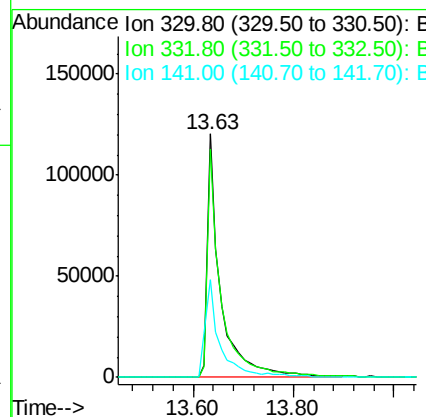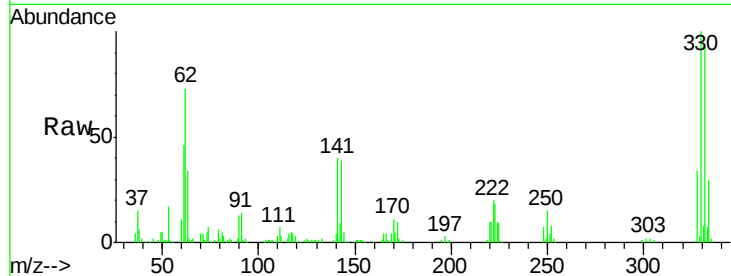

#44
 2-Fluorobiphenyl
 Concen: 92.14 ng
 RT: 11.28 min Scan# 848
 Delta R.T. -0.01 min
 Lab File: BF087569.D
 Acq: 31 May 2016 2:11

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.2	29.0	43.6
170	24.3	19.8	29.8


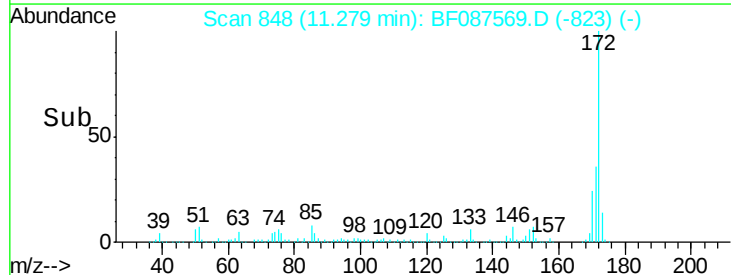
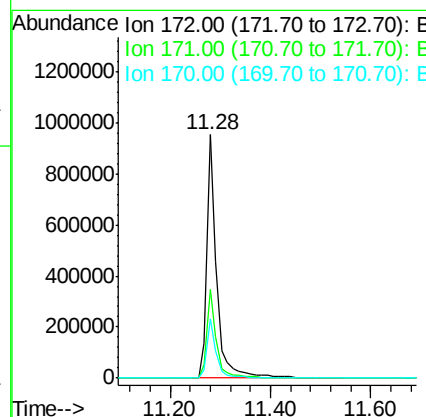
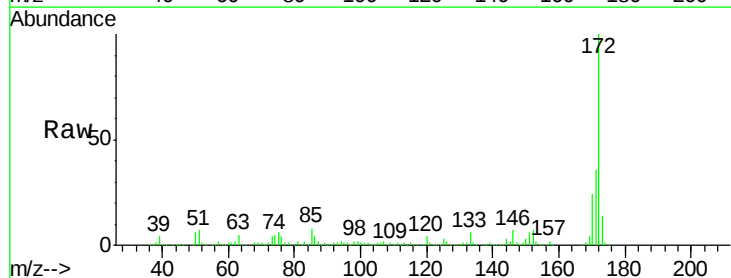


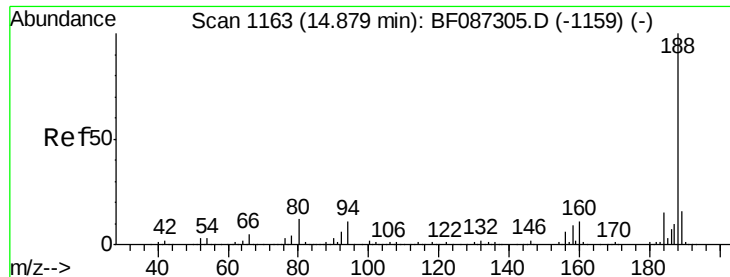

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 14.77 min Scan# 1153
 Delta R.T. 0.02 min
 Lab File: BF087569.D
 Acq: 31 May 2016 2:11




Instrument :
 BNA_F
 ClientSampleId :
 MW-25


Tot Ion:188 Resp: 344964
 Ion Ratio Lower Upper
 188 100
 94 8.5 6.8 10.2
 80 9.6 7.1 10.7

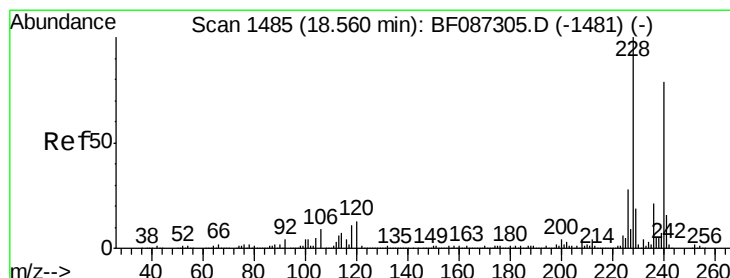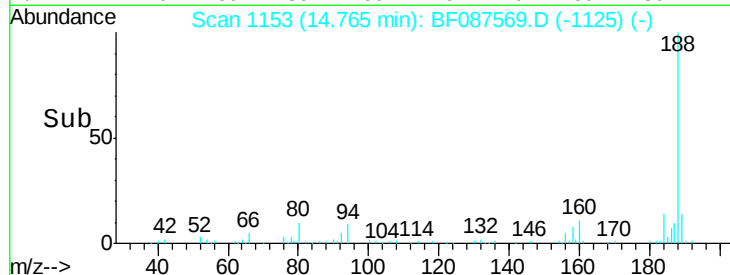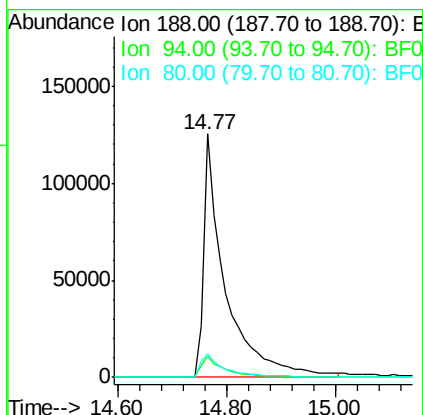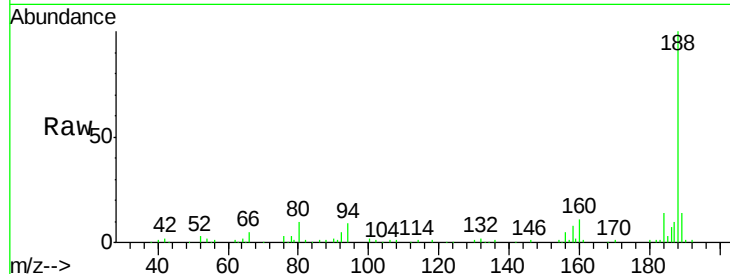

#75
 Chrysene-d12
 Concen: 20.00 ng
 RT: 18.49 min Scan# 1479
 Delta R.T. 0.05 min
 Lab File: BF087569.D
 Acq: 31 May 2016 2:11

Tgt Ion:240 Resp: 251564
 Ion Ratio Lower Upper
 240 100
 120 11.4 11.2 16.8
 236 25.0 21.2 31.8

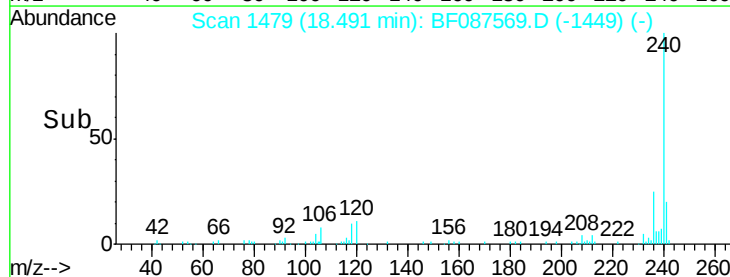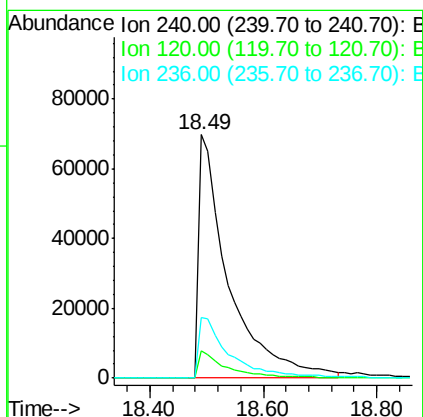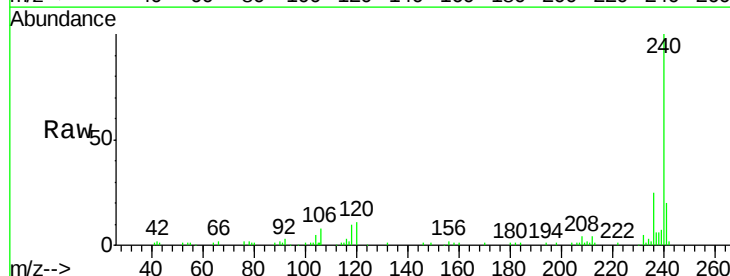

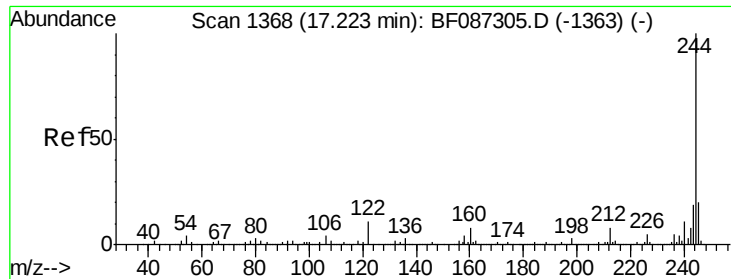

#78

Terphenyl-d14

Concen: 94.47 ng

RT: 17.10 min Scan# 1357

Delta R.T. -0.00 min

Lab File: BF087569.D

Acq: 31 May 2016 2:11

Instrument :

BNA_F

ClientSampleId :

MW-25


Tot Ion:244 Resp: 1117892

Ion Ratio Lower Upper

244 100

212 7.6 6.2 9.2




122 8.5 12.0 18.0#

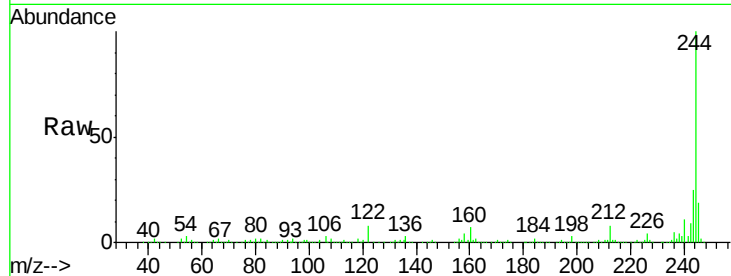

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

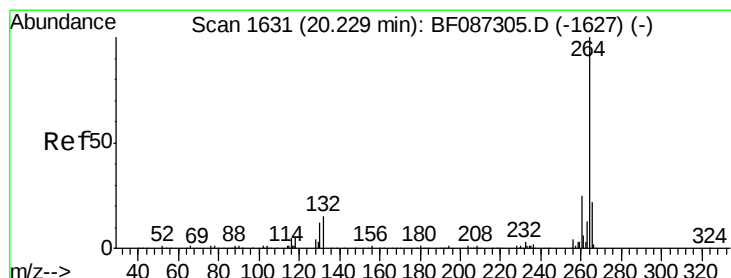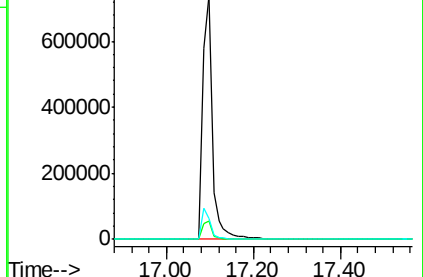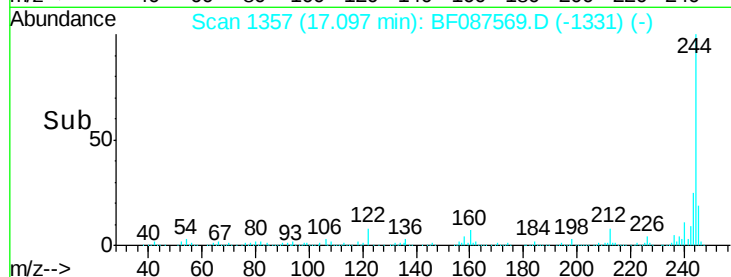

#86

Perylene-d12

Concen: 20.00 ng

RT: 20.19 min Scan# 1628

Delta R.T. 0.07 min

Lab File: BF087569.D

Acq: 31 May 2016 2:11


Tgt Ion:264 Resp: 191846

Ion Ratio Lower Upper

264 100

260 23.6 19.5 29.3

265 21.1 17.3 25.9

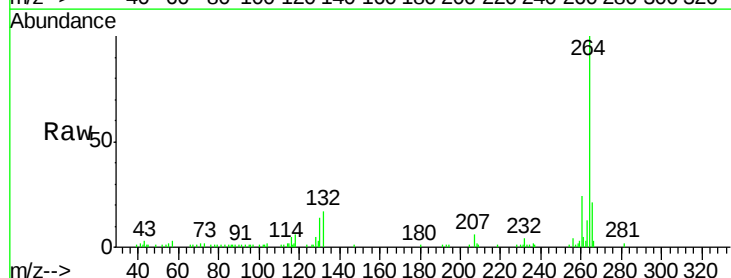

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

