

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052916\
Data File : BF087529.D
Acq On : 30 May 2016 1:06
Operator : UM/SJ
Sample : H3222-14
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-32

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.370	329	331	368	rBV7	698805	2044287	54.39%	7.949%
2	7.027	474	476	482	rBV	540499	1083879	28.84%	4.214%
3	7.119	482	484	501	rVB	1949655	3412115	90.79%	13.267%
4	7.473	514	515	527	rBV	411970	756070	20.12%	2.940%
5	7.702	532	535	552	rVV	1685901	2431439	64.69%	9.454%
6	8.388	593	595	622	rBV	1424031	2241400	59.64%	8.715%
7	9.039	649	652	657	rBV4	11559	43001	1.14%	0.167%
8	9.508	691	693	715	rVB	503324	930599	24.76%	3.618%
9	11.279	845	848	868	rBV	2866893	3758395	100.00%	14.613%
10	12.331	937	940	960	rBV	628252	997361	26.54%	3.878%
11	13.622	1050	1053	1073	rBV	1336037	2287863	60.87%	8.896%
12	14.742	1149	1151	1169	rBV	480095	938513	24.97%	3.649%
13	17.086	1354	1356	1373	rBV	2970312	3515670	93.54%	13.670%
14	18.457	1474	1476	1492	rBV	315878	712233	18.95%	2.769%
15	20.137	1621	1623	1637	rBV	179827	566087	15.06%	2.201%


Sum of corrected areas: 25718912

Data Path : Z:\HPCHEM1\BNA F\DATA\BF052916\
Data File : BF087529.D
Acq On : 30 May 2016 1:06
Operator : UM/SJ
Sample : H3222-14
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-32

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

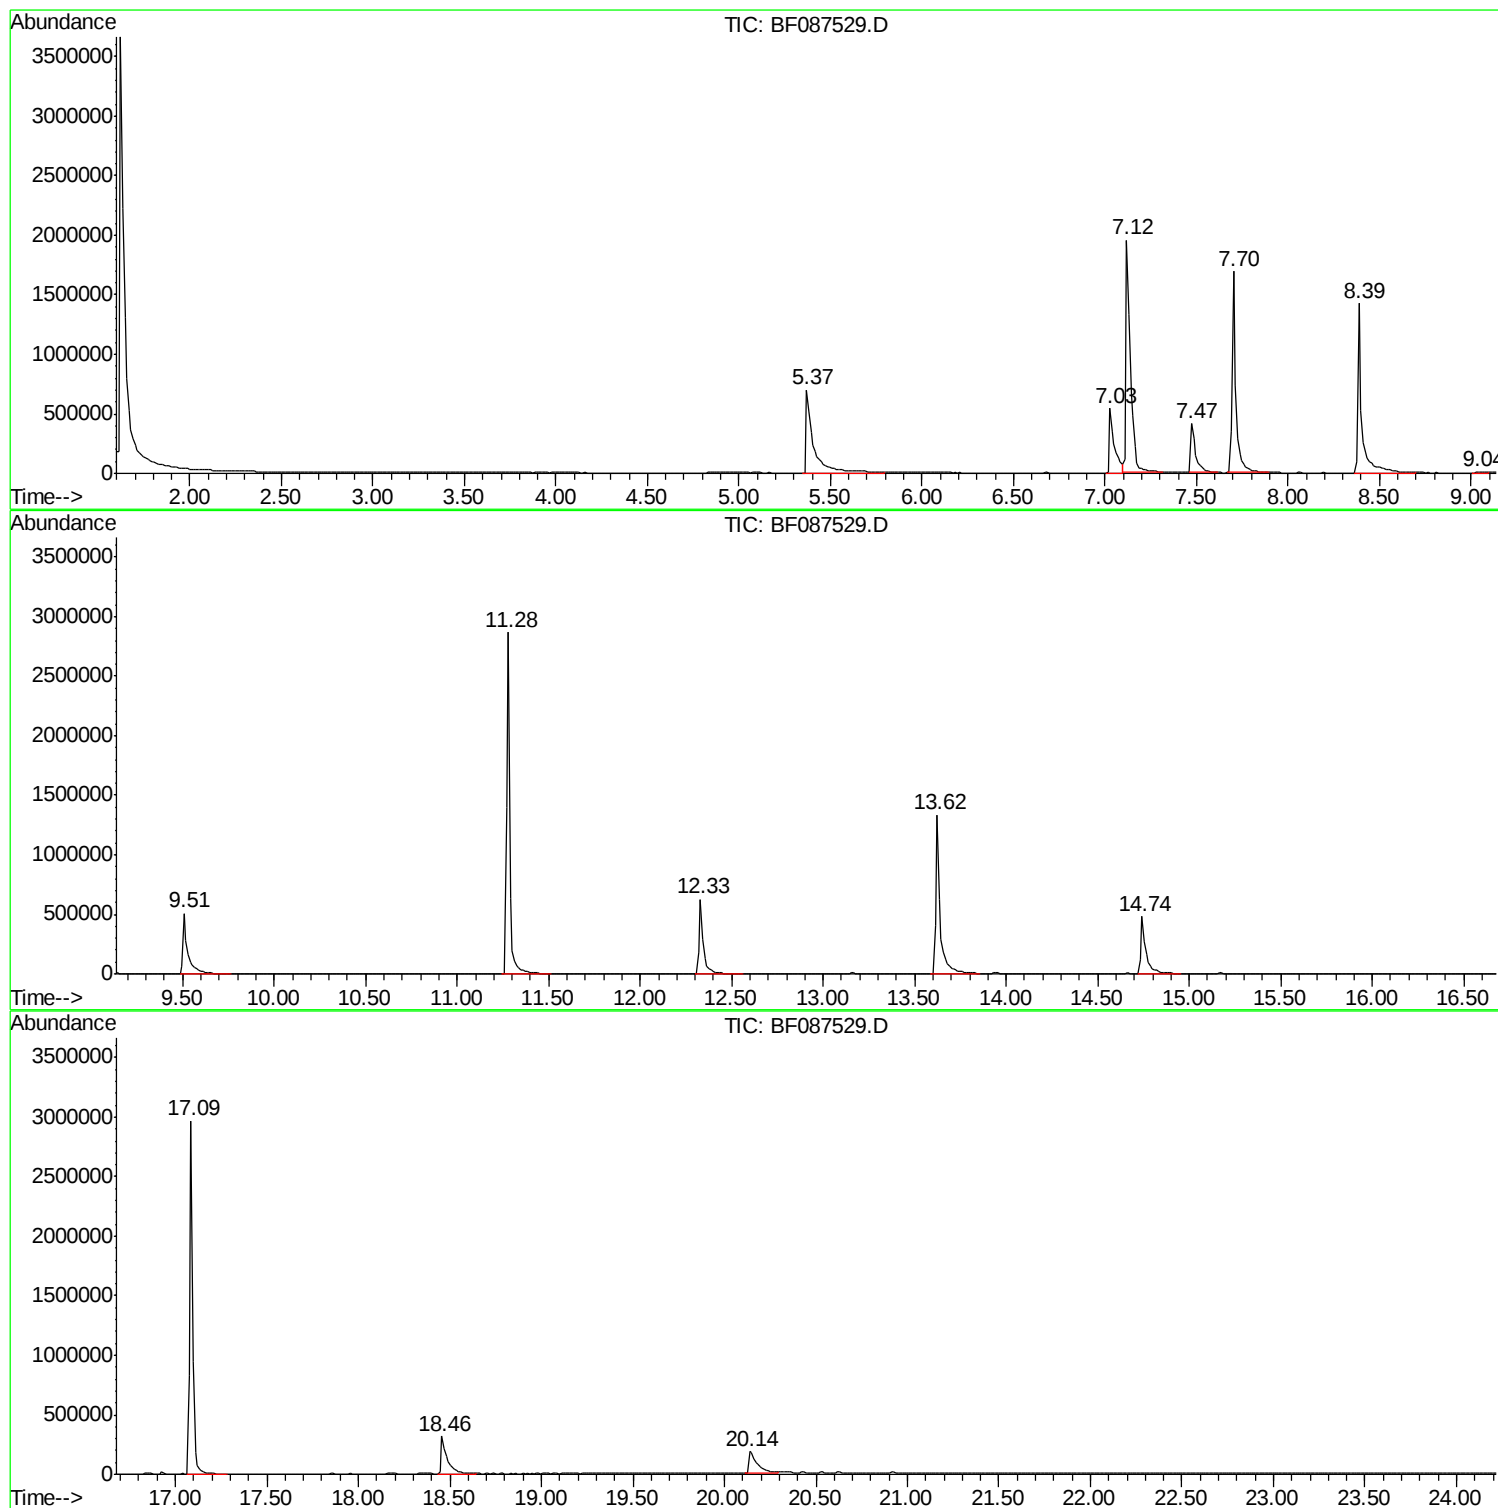

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052916\
Data File : BF087529.D
Acq On : 30 May 2016 1:06
Operator : UM/SJ
Sample : H3222-14
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-32










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.12 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.12	90.26 ng	3412120	1,4-Dichlorobenzene-d4	7.47

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2			4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	27
3			1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	22
4			Pyrazolo(2,3-a)pyridine, 7-methyl-	132	C8H8N2	034760-58-2	22
5			Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	22

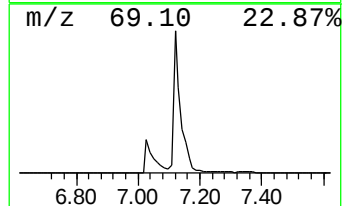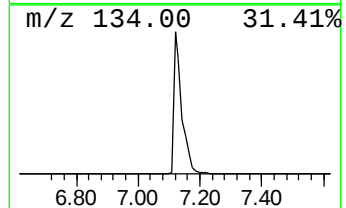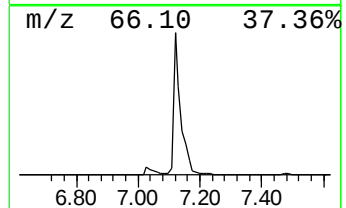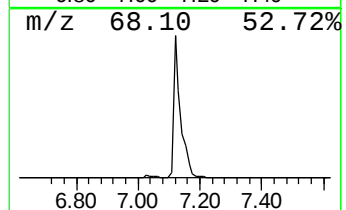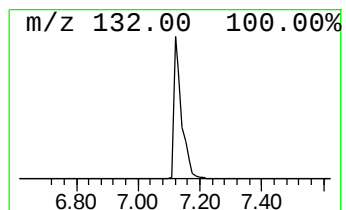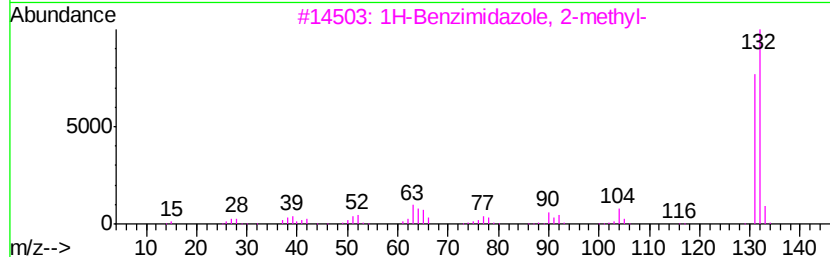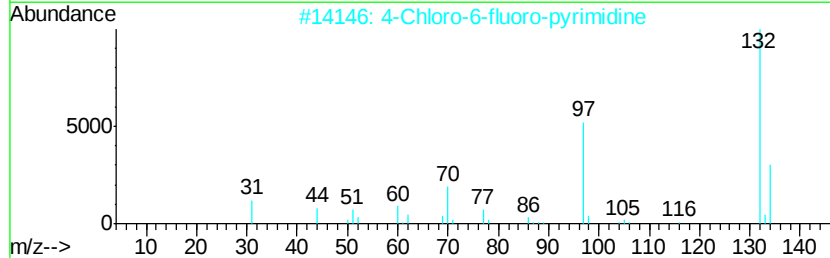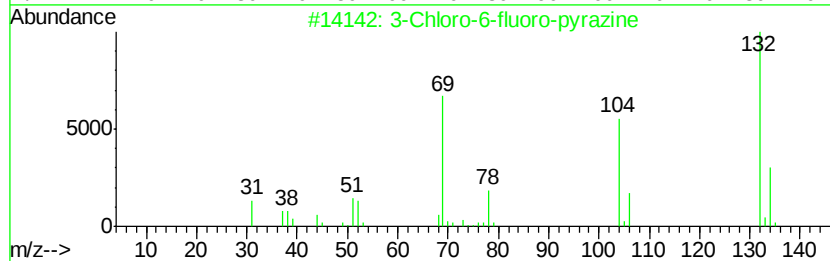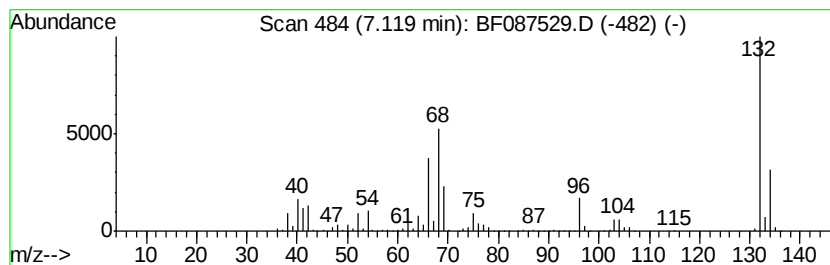

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052916\
Data File : BF087529.D
Acq On : 30 May 2016 1:06
Operator : UM/SJ
Sample : H3222-14
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-32

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.12	7.12	90.3	ng	3412120	1	7.47	756070	20.0