


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF052916\
 Data File : BF087542.D
 Acq On : 30 May 2016 10:12
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 25 16:26:52 2016

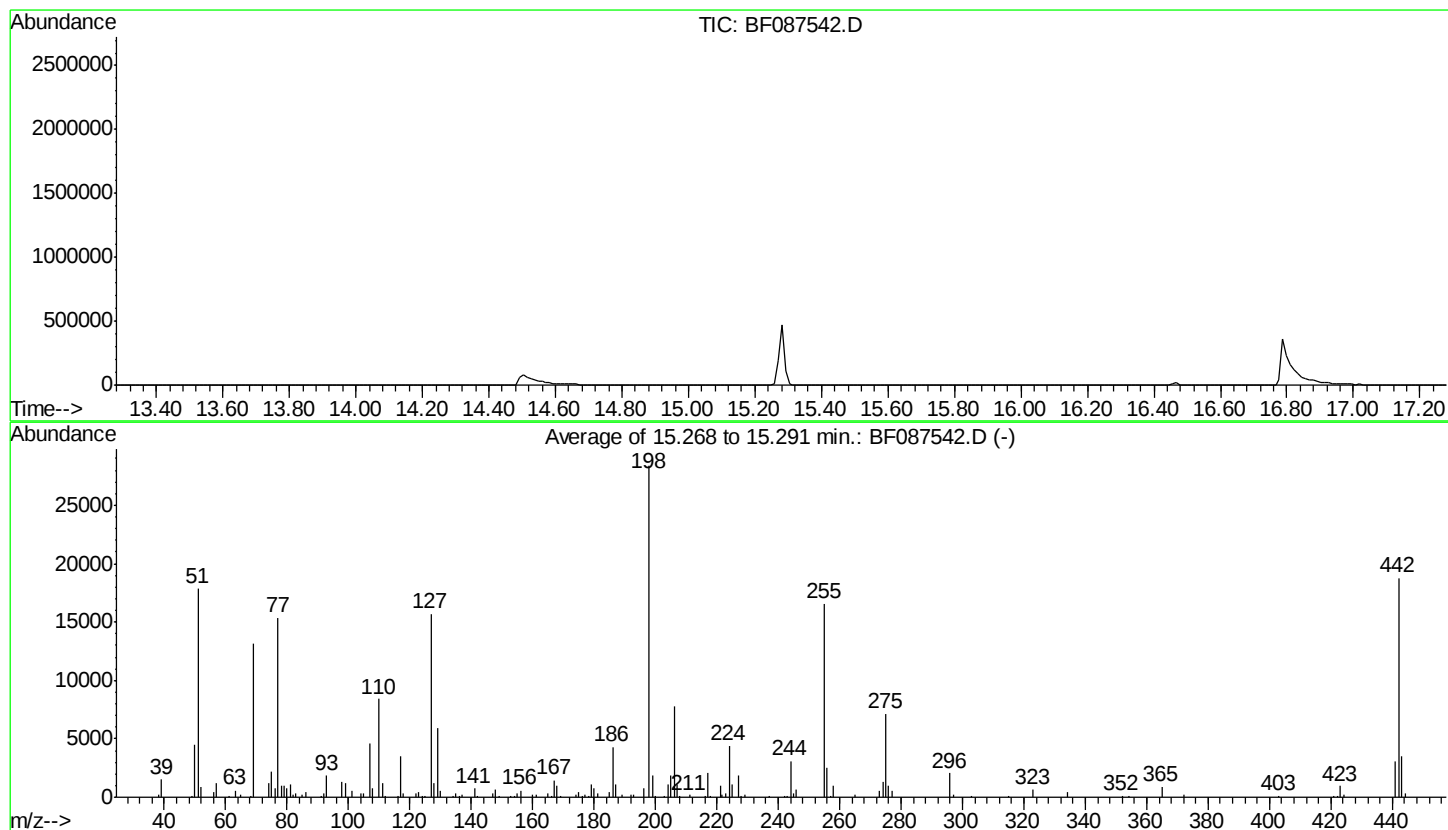

AutoFind: Scans 1197, 1198, 1199; Background Corrected with Scan 1193

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.9	17855	PASS
68	69	0.00	2	1.2	159	PASS
69	198	0.00	100	46.3	13151	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.4	15732	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28396	PASS
199	198	5	9	6.5	1849	PASS
275	198	10	60	25.3	7183	PASS
365	198	1	100	3.2	909	PASS
441	442	0.01	24	16.6	3110	PASS
442	198	50	100	66.1	18777	PASS
443	442	15	24	18.6	3499	PASS