


Data Path : Z:\HPCHEM1\BNA F\DATA\BF052916\
 Data File : BF087562.D
 Acq On : 30 May 2016 22:10
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF052316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed May 25 16:26:52 2016

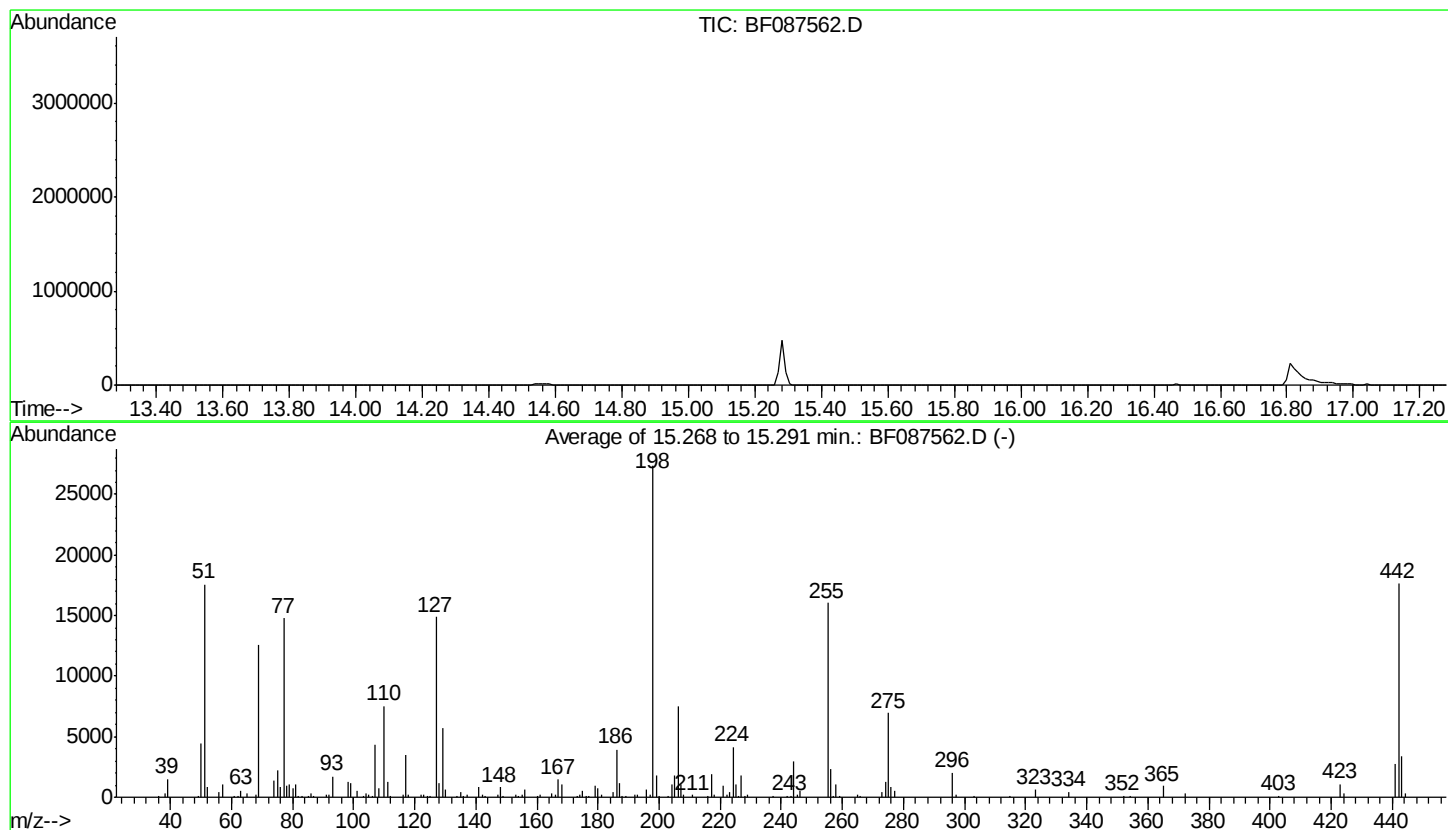

AutoFind: Scans 1197, 1198, 1199; Background Corrected with Scan 1194

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	64.2	17562	PASS
68	69	0.00	2	1.4	177	PASS
69	198	0.00	100	45.9	12555	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.3	14858	PASS
197	198	0.00	2	0.6	170	PASS
198	198	100	100	100.0	27376	PASS
199	198	5	9	6.7	1839	PASS
275	198	10	60	25.4	6942	PASS
365	198	1	100	3.3	912	PASS
441	442	0.01	24	15.7	2770	PASS
442	198	50	100	64.4	17623	PASS
443	442	15	24	18.9	3339	PASS