

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052920\
 Data File : BF120444.D
 Acq On : 29 May 2020 17:33
 Operator : MA/SJ
 Sample : PB129165BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB129165BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.922	3	6	10	rVB	269541	321551	4.13%	0.570%
2	1.963	10	13	33	rVV	1771683	2794440	35.86%	4.955%
3	2.099	33	36	53	rVB	191195	344143	4.42%	0.610%
4	5.457	601	607	610	rBV	5767545	6513648	83.58%	11.549%
5	6.469	772	779	782	rBV	5491866	6714023	86.15%	11.904%
6	6.839	838	842	845	rBV	1763426	1552688	19.92%	2.753%
7	6.998	864	869	872	rBV	5664409	5666405	72.71%	10.047%
8	7.404	931	938	941	rBV	4162146	4603133	59.07%	8.161%
9	8.116	1055	1059	1063	rBV	2308555	1973029	25.32%	3.498%
10	9.198	1237	1243	1246	rBV	7568202	7793232	100.00%	13.818%
11	9.874	1353	1358	1361	rBV	2408188	2155654	27.66%	3.822%
12	10.663	1486	1492	1495	rBV	4564490	4543031	58.29%	8.055%
13	11.357	1606	1610	1613	rBV	2236810	1939984	24.89%	3.440%
14	12.945	1875	1880	1883	rBV	6327509	6503380	83.45%	11.531%
15	13.862	2033	2036	2041	rVB	85194	78238	1.00%	0.139%
16	13.992	2054	2058	2061	rBV	1673011	1418131	18.20%	2.514%
17	15.445	2299	2305	2309	rBV	1266057	1486417	19.07%	2.635%


Sum of corrected areas: 56401127

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF052920\
Data File : BF120444.D
Acq On : 29 May 2020 17:33
Operator : MA/SJ
Sample : PB129165BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB129165BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

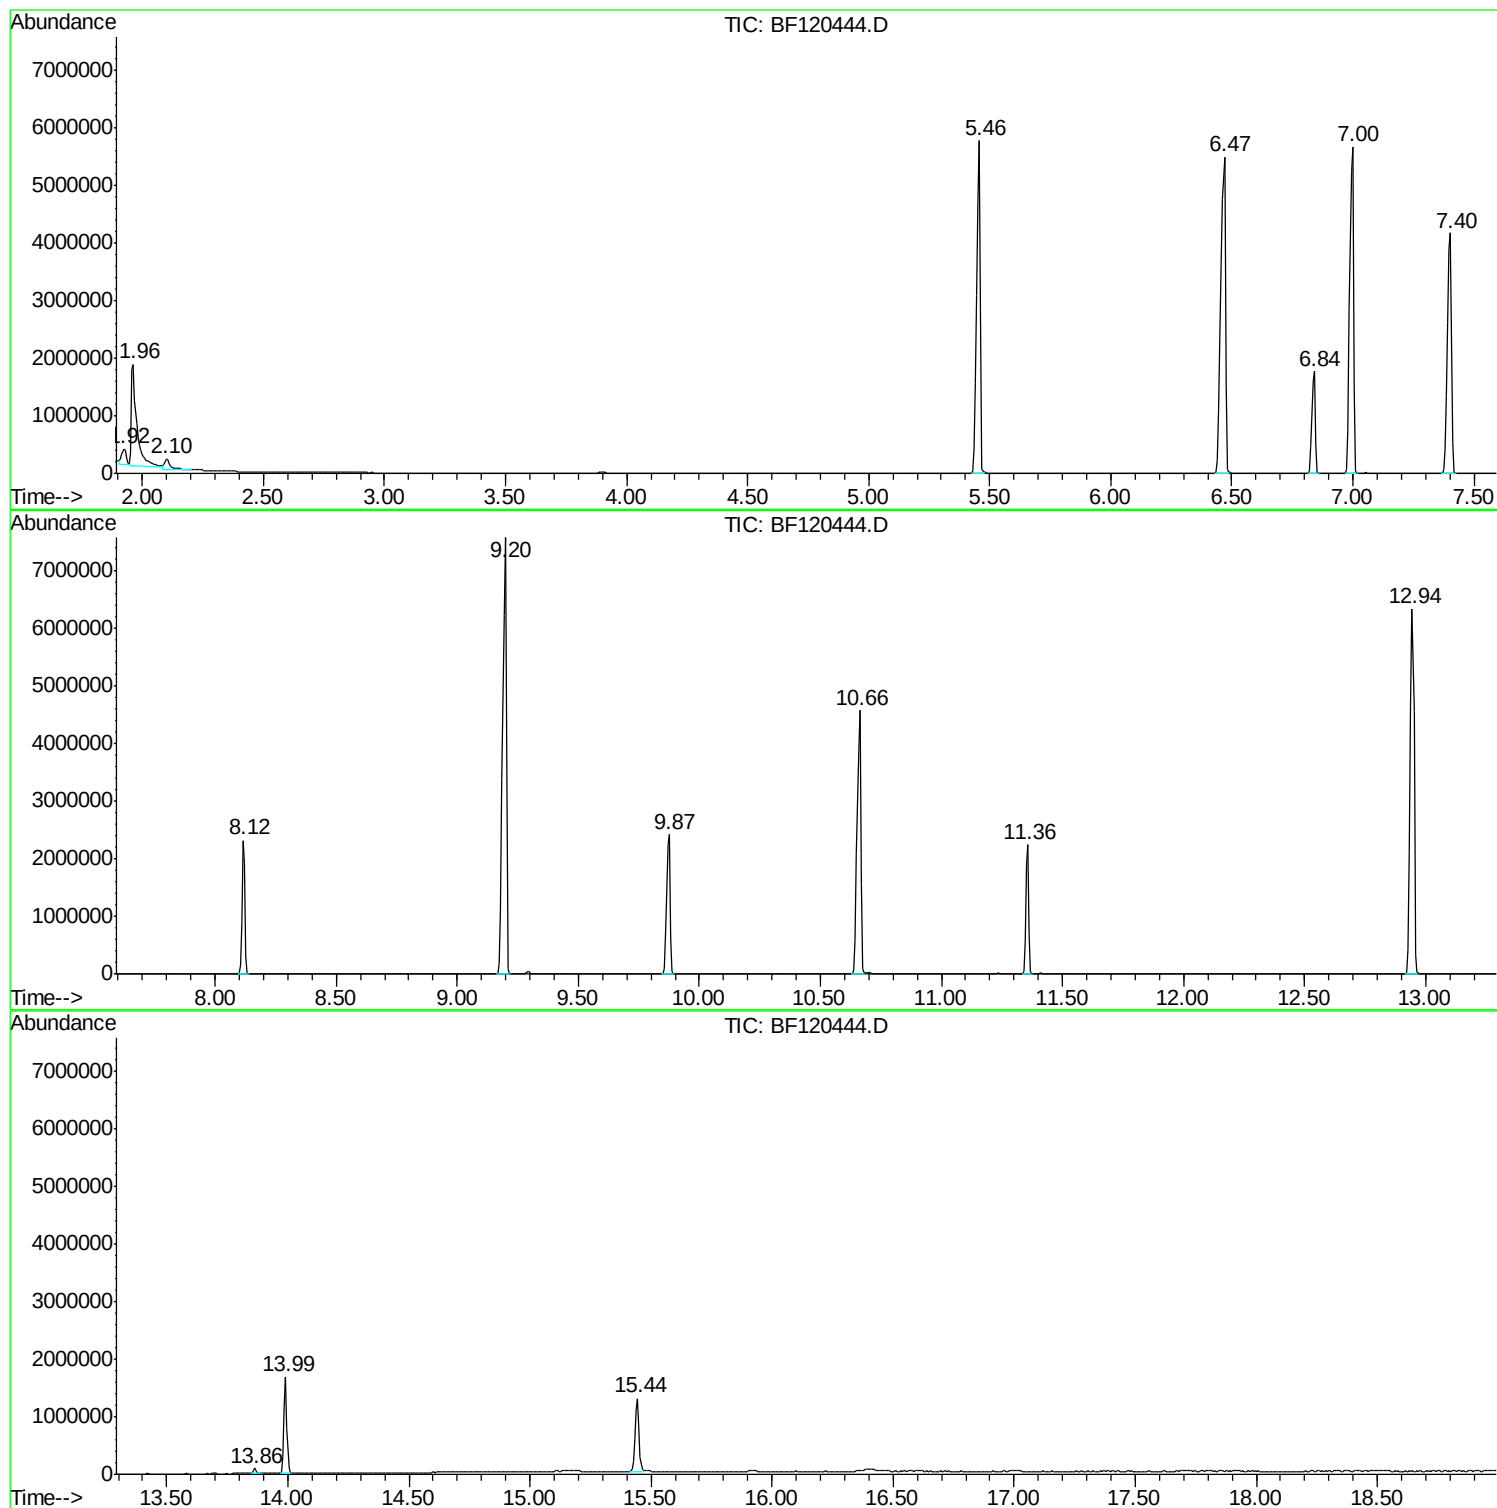

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF052920\
Data File : BF120444.D
Acq On : 29 May 2020 17:33
Operator : MA/SJ
Sample : PB129165BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB129165BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF052820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Butane, 2-methoxy-2-methyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.10	4.43 ng	344143	1,4-Dichlorobenzene-d4	6.84

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3		3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	25
4		2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	25
5		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12

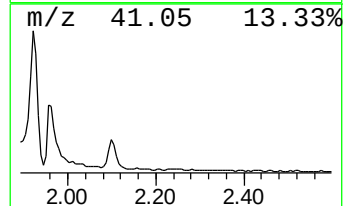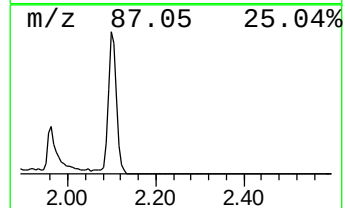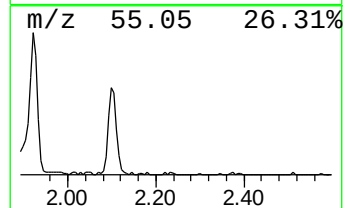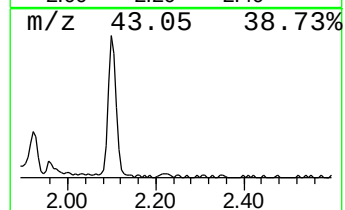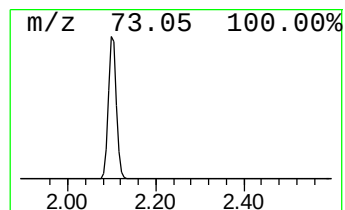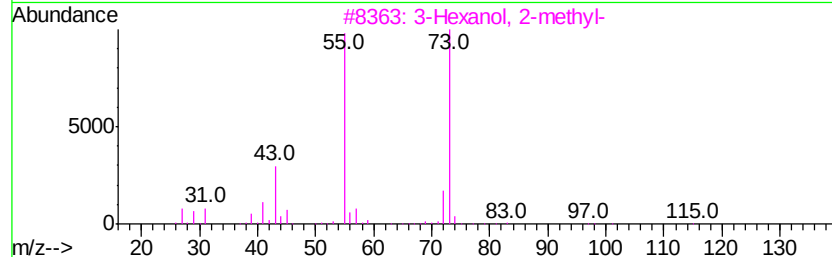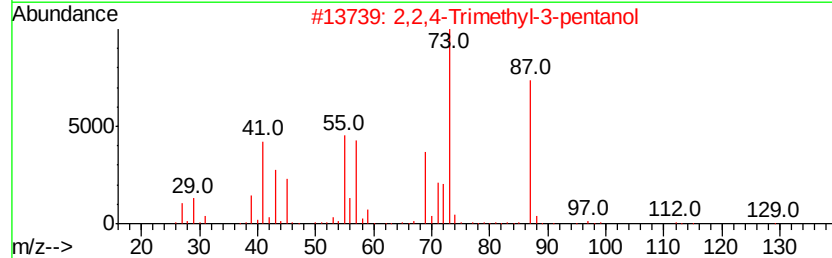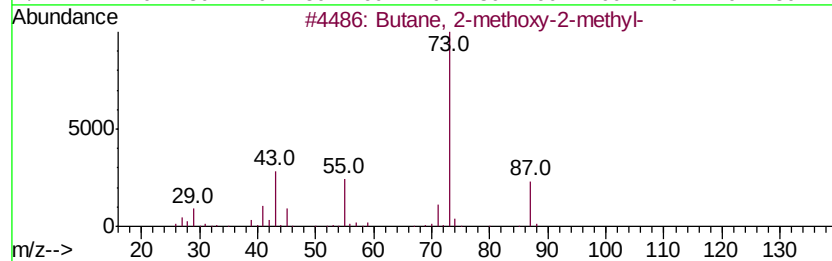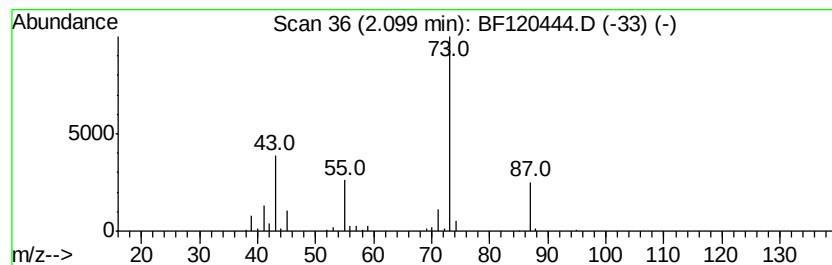

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF052920\
Data File : BF120444.D
Acq On : 29 May 2020 17:33
Operator : MA/SJ
Sample : PB129165BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB129165BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
Butane, 2-methoxy...	2.10	4.4	ng	344143	1	6.84	1552690	20.0