


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052920\
 Data File : BF120431.D
 Acq On : 29 May 2020 11:39
 Operator : MA/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF052820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 29 12:39:43 2020

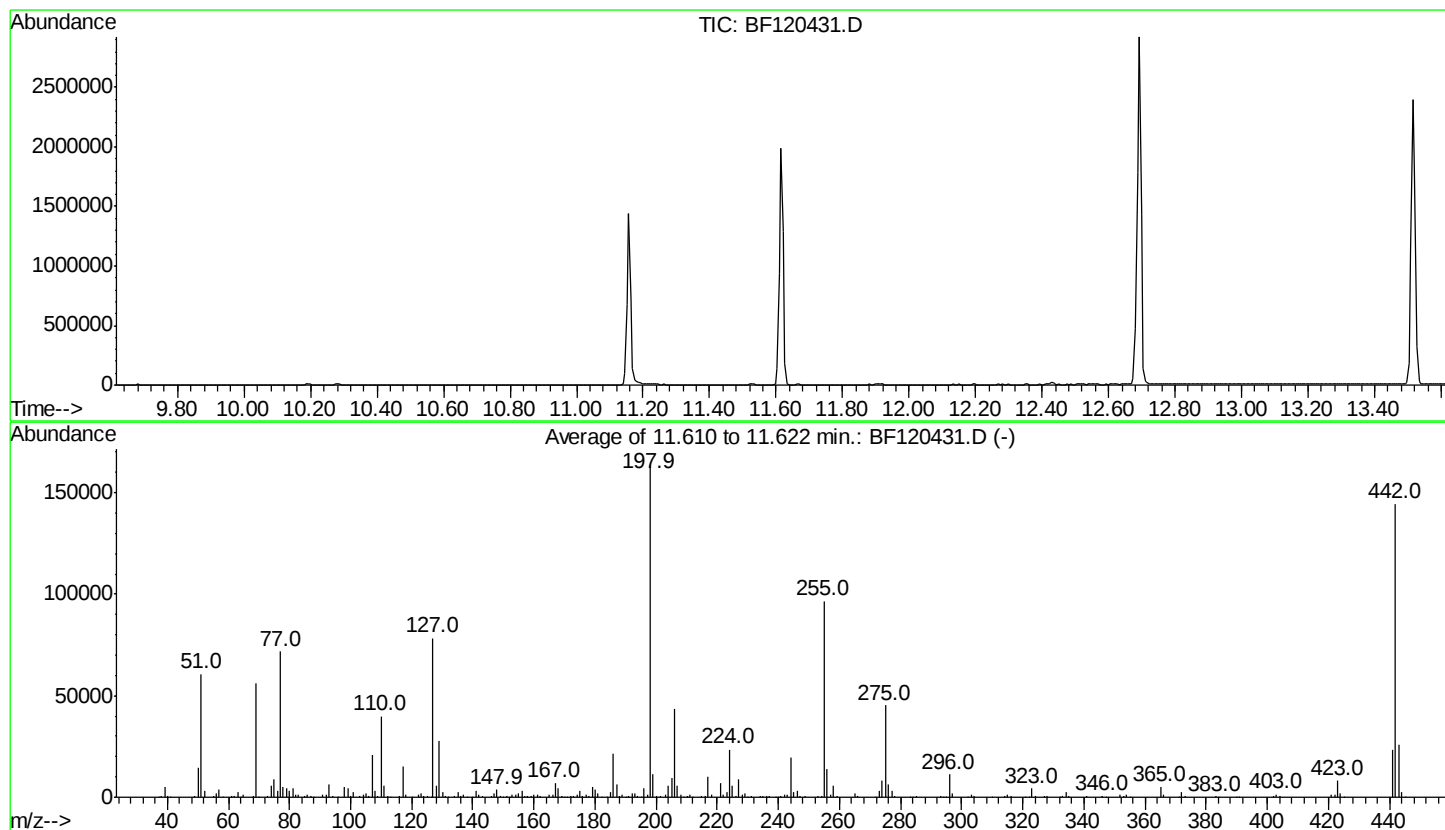

AutoFind: Scans 1653, 1654, 1655; Background Corrected with Scan 1648

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	60810	PASS
68	69	0.00	2	1.6	869	PASS
69	198	0.00	100	34.2	55861	PASS
70	69	0.00	2	0.5	295	PASS
127	198	10	80	48.0	78333	PASS
197	198	0.00	2	0.7	1071	PASS
198	198	100	100	100.0	163328	PASS
199	198	5	9	6.9	11200	PASS
275	198	10	60	27.7	45224	PASS
365	198	1	100	3.2	5193	PASS
441	198	0.01	100	14.2	23122	PASS
442	198	50	100	88.5	144514	PASS
443	442	15	24	18.1	26120	PASS