
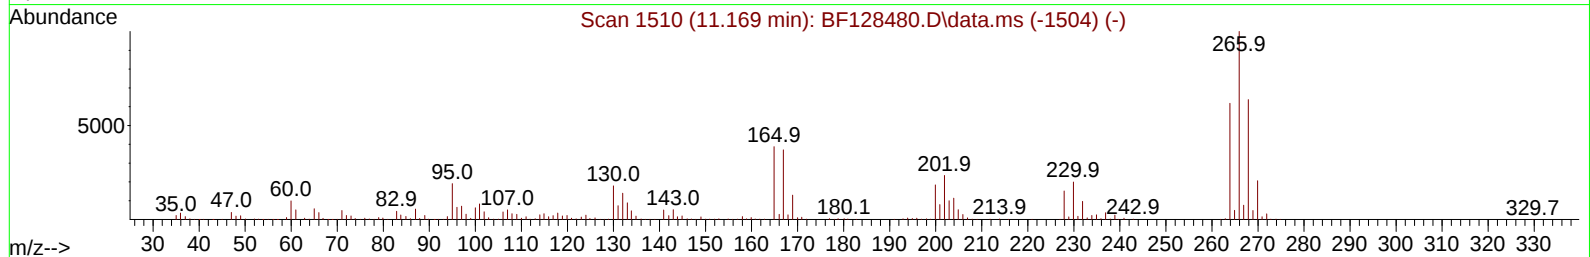
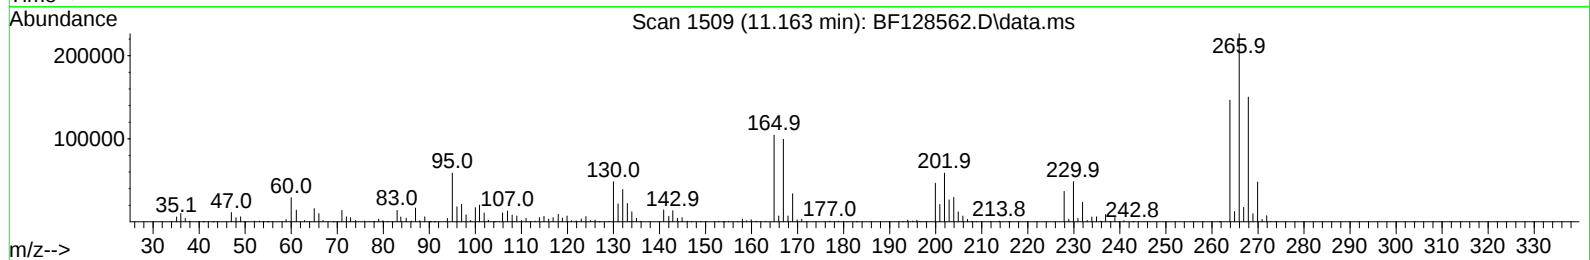


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
Data File : BF128562.D
Acq On : 29 May 2022 10:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 01:54:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration

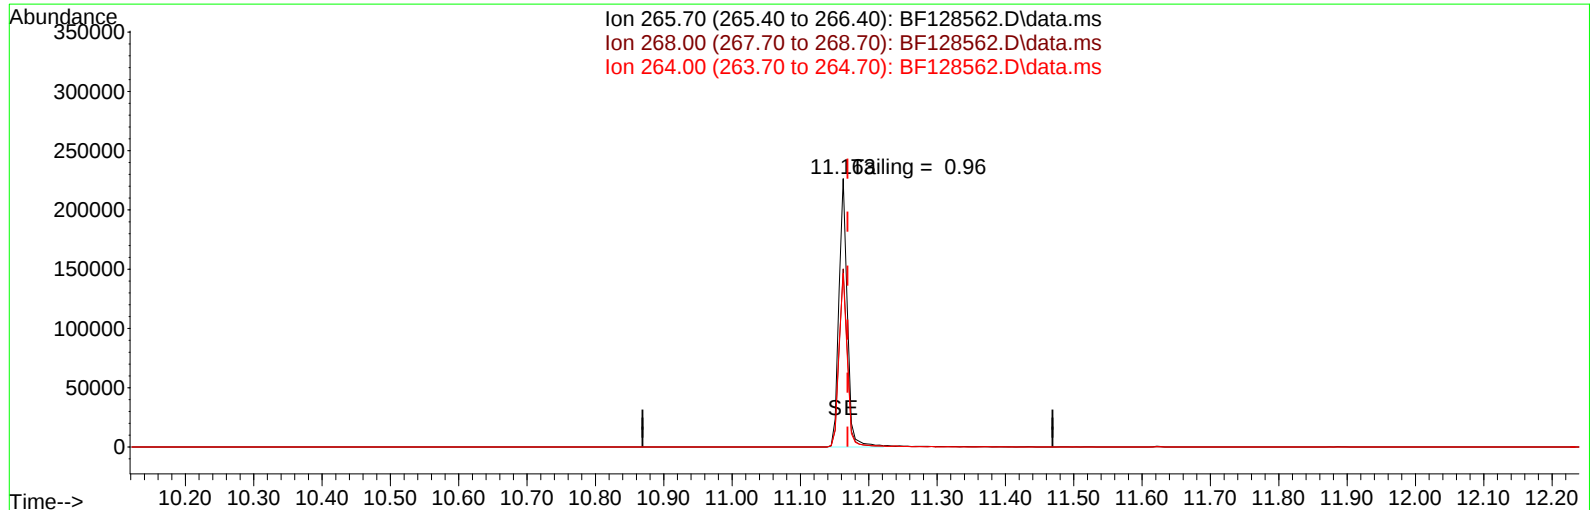

TIC: BF128562.D\data.ms

(70) Pentachlorophenol (C)




11.163min (-0.006) 37714.22 ng

response 193255

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	66.37
264.00	61.80	64.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
Data File : BF128562.D
Acq On : 29 May 2022 10:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 30 01:54:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration

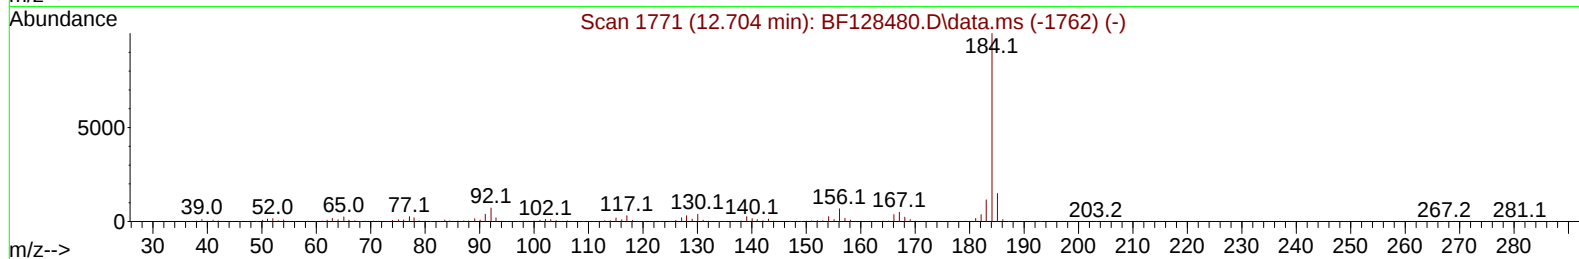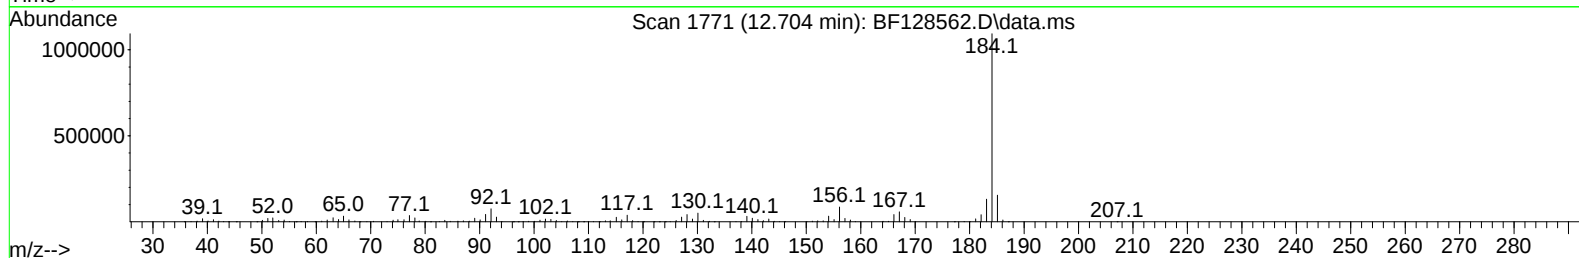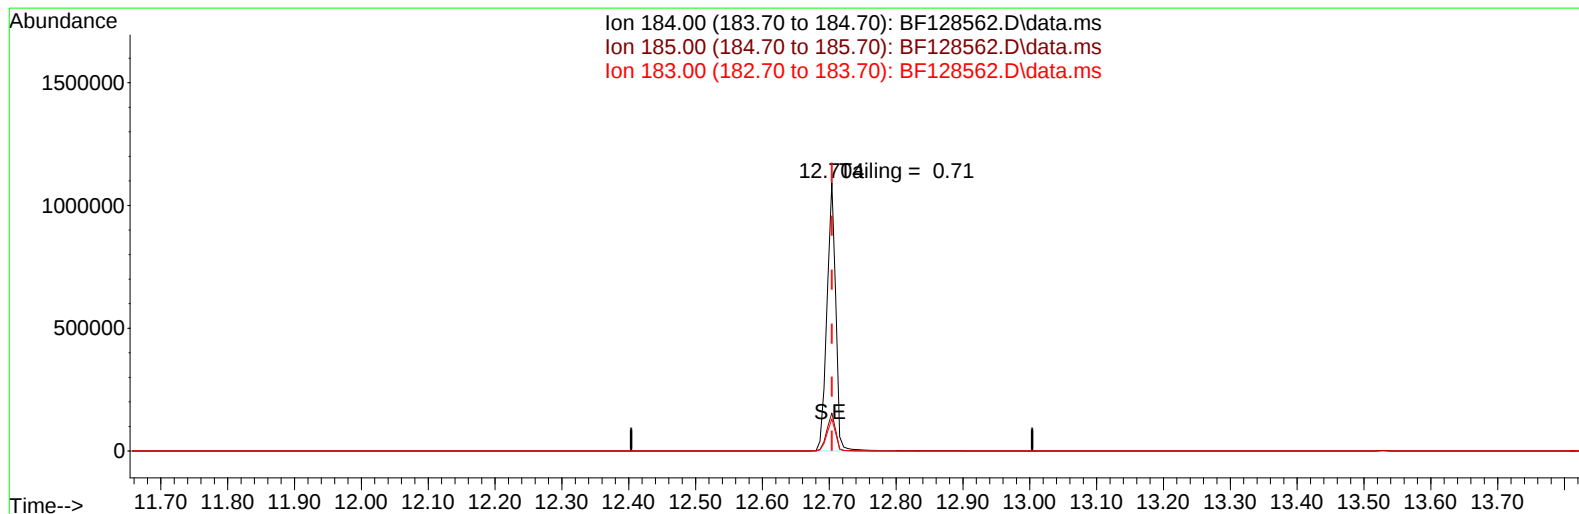

TIC: BF128562.D\data.ms

(77) Benzidine

12.704min (-0.000) 0.00 ng

response 1002983

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.18
183.00	11.60	11.98
0.00	0.00	0.00