

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
 Data File : BF128578.D
 Acq On : 29 May 2022 18:31
 Operator : CG\JU
 Sample : N2951-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P035-SS001-2430-01

Quant Time: May 30 00:52:12 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 27 01:51:59 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.840	152	110046	20.000	ng	0.00
21) Naphthalene-d8	8.116	136	380234	20.000	ng	-0.01
39) Acenaphthene-d10	9.875	164	180908	20.000	ng	0.00
64) Phenanthrene-d10	11.363	188	304817	20.000	ng	0.00
76) Chrysene-d12	14.004	240	291976	20.000	ng	# 0.00
86) Perylene-d12	15.468	264	274160	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.451	112	622925	93.762	ng	0.00
7) Phenol-d6	6.463	99	744372	87.874	ng	0.00
23) Nitrobenzene-d5	7.398	82	502116	76.180	ng	-0.01
42) 2,4,6-Tribromophenol	10.663	330	174626	101.412	ng	-0.01
45) 2-Fluorobiphenyl	9.198	172	848650	76.213	ng	0.00
79) Terphenyl-d14	12.951	244	828402	54.814	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
Data File : BF128578.D
Acq On : 29 May 2022 18:31
Operator : CG\JU
Sample : N2951-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P035-SS001-2430-01


Quant Time: May 30 00:52:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration

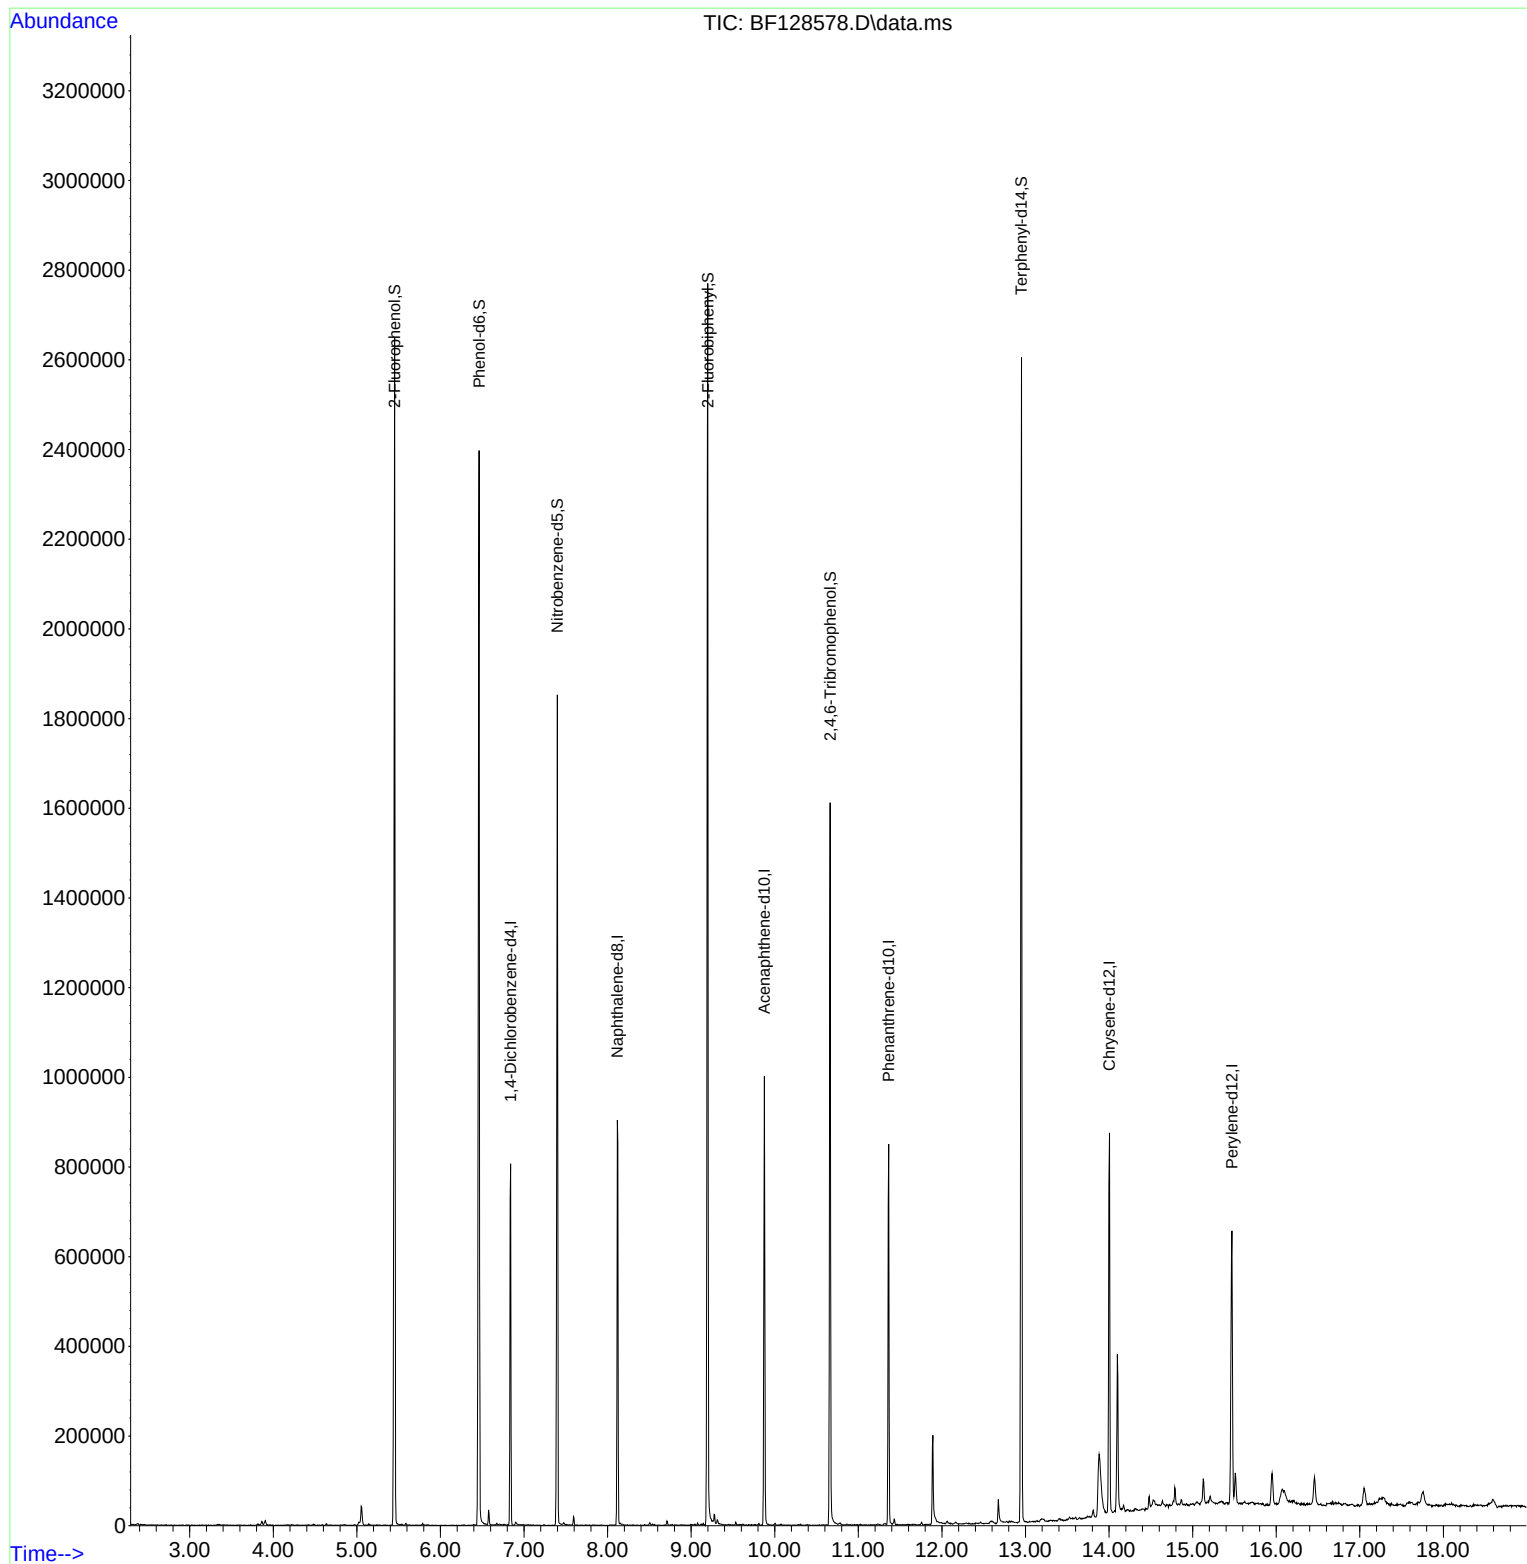



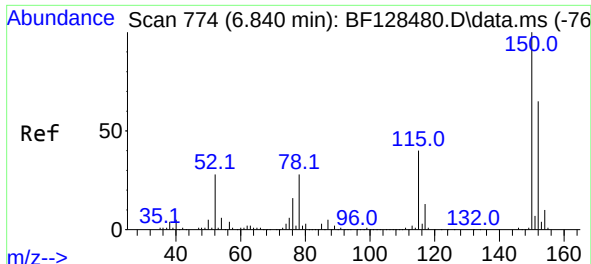


#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.840 min Scan# 71
Delta R.T. -0.000 min
Lab File: BF128578.D
Acq: 29 May 2022 18:31

Instrument :
BNA_F
ClientSampleId :
P035-SS001-2430-01







Tgt Ion:152 Resp: 110046
Ion Ratio Lower Upper
152 100
150 154.4 123.7 185.5
115 61.3 49.9 74.9

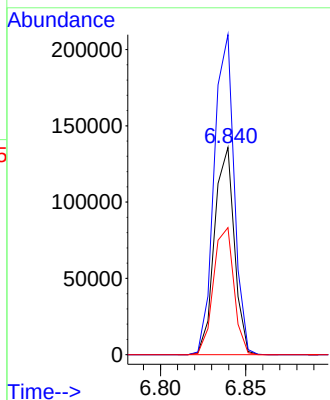

#5
2-Fluorophenol
Concen: 93.762 ng
RT: 5.451 min Scan# 538
Delta R.T. 0.000 min
Lab File: BF128578.D
Acq: 29 May 2022 18:31

Tgt Ion:112 Resp: 622925
Ion Ratio Lower Upper
112 100
64 69.3 53.3 79.9
63 37.9 28.0 42.0


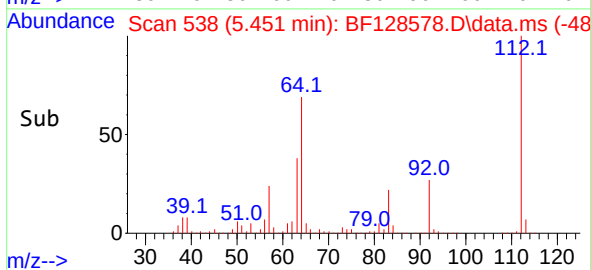
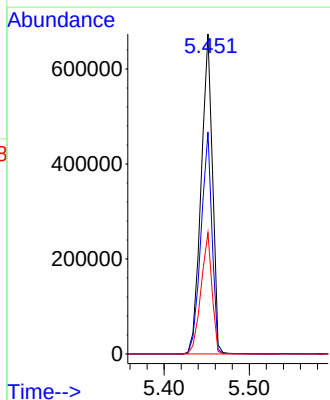
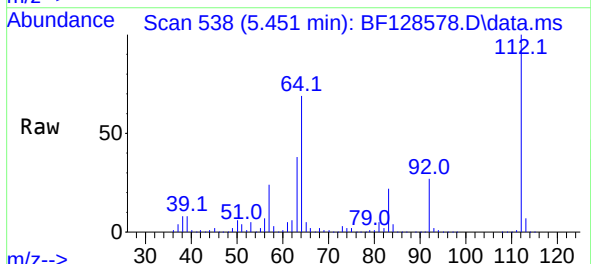


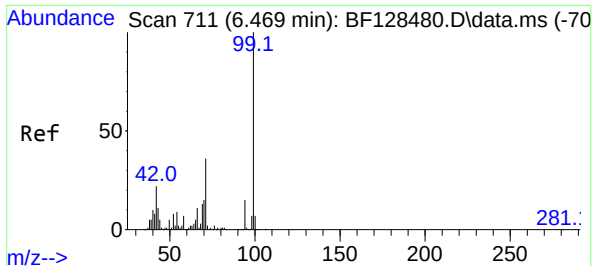

#7
Phenol-d6
Concen: 87.874 ng
RT: 6.463 min Scan# 711
Delta R.T. -0.006 min
Lab File: BF128578.D
Acq: 29 May 2022 18:31




Instrument :
BNA_F
ClientSampleId :
P035-SS001-2430-01


Tgt Ion: 99 Resp: 744372
Ion Ratio Lower Upper
99 100
42 22.6 17.3 25.9
71 40.3 28.9 43.3

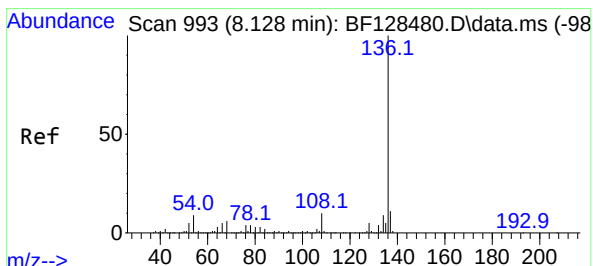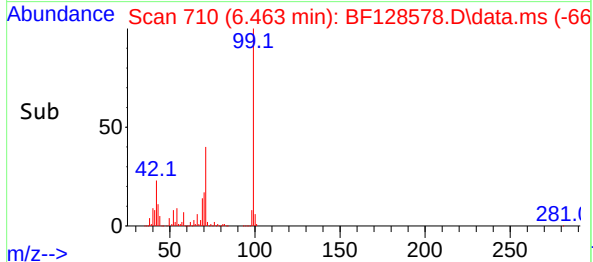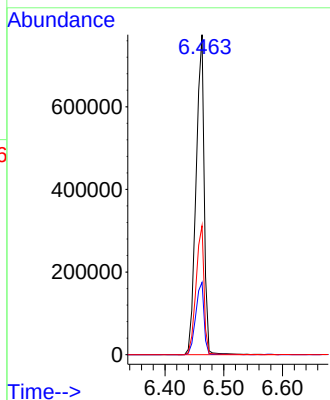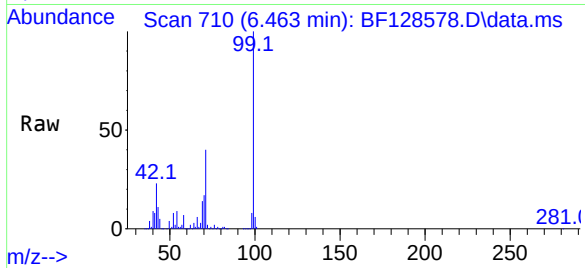

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.116 min Scan# 991
Delta R.T. -0.012 min
Lab File: BF128578.D
Acq: 29 May 2022 18:31

Tgt Ion: 136 Resp: 380234
Ion Ratio Lower Upper
136 100
137 10.8 8.8 13.2
54 10.5 7.5 11.3
68 6.0 4.7 7.1


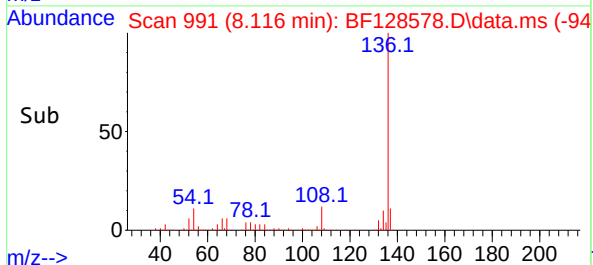
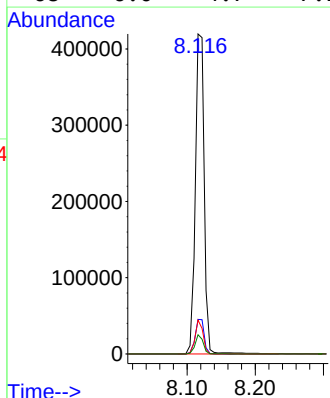
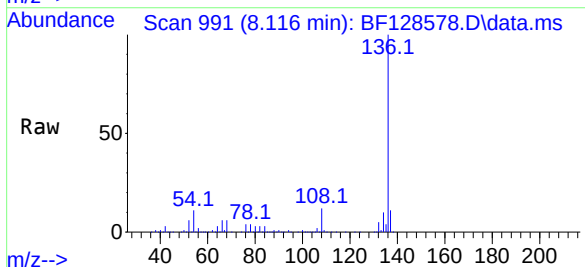


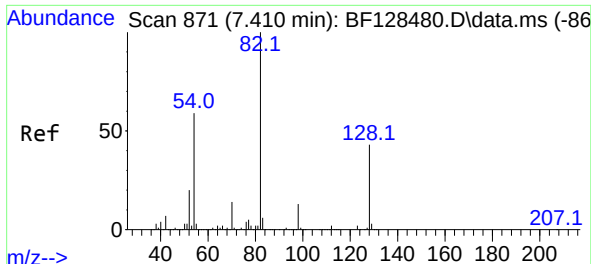

#23
Nitrobenzene-d5
Concen: 76.180 ng
RT: 7.398 min Scan# 80
Delta R.T. -0.012 min
Lab File: BF128578.D
Acq: 29 May 2022 18:31




Instrument :
BNA_F
ClientSampleId :
P035-SS001-2430-01


Tgt Ion: 82 Resp: 502116
Ion Ratio Lower Upper
82 100
128 41.4 34.0 51.0
54 59.7 46.9 70.3

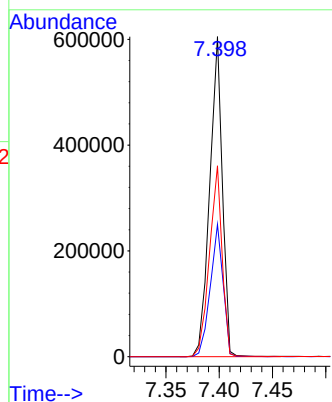

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.875 min Scan# 1290
Delta R.T. -0.006 min
Lab File: BF128578.D
Acq: 29 May 2022 18:31

Tgt Ion: 164 Resp: 180908
Ion Ratio Lower Upper
164 100
162 100.4 79.5 119.3
160 43.4 34.2 51.4

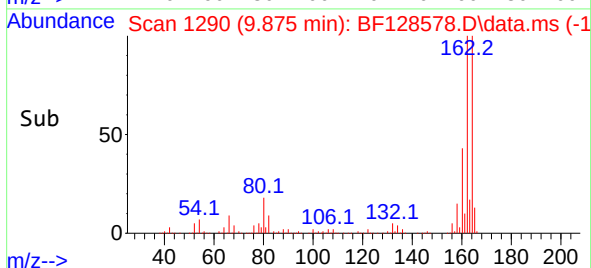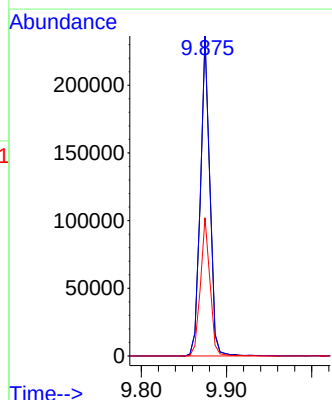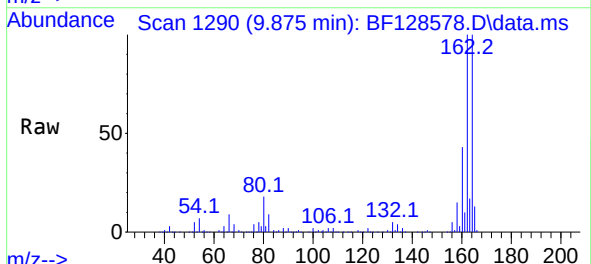



#42

2,4,6-Tribromophenol

Concen: 101.412 ng

RT: 10.663 min Scan# 1424

Delta R.T. -0.012 min

Lab File: BF128578.D


Acq: 29 May 2022 18:31

Instrument :

BNA_F

ClientSampleId :

P035-SS001-2430-01

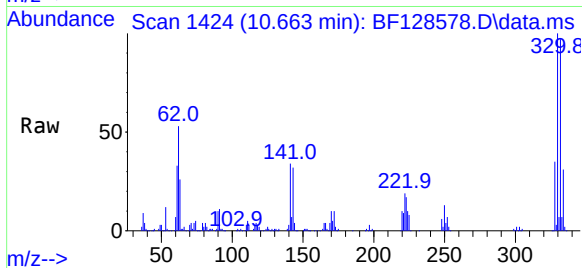




Tgt Ion:330 Resp: 174626

Ion Ratio Lower Upper

330 100

332 95.8 76.8 115.2

141 35.1 28.0 42.0

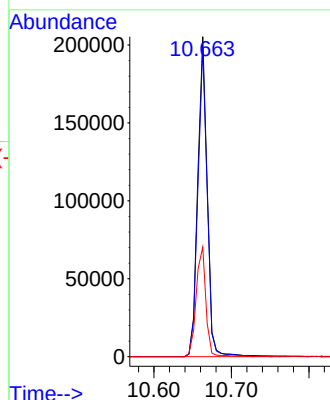

#45

2-Fluorobiphenyl

Concen: 76.213 ng

RT: 9.198 min Scan# 1175

Delta R.T. -0.006 min

Lab File: BF128578.D

Acq: 29 May 2022 18:31




Tgt Ion:172 Resp: 848650


Ion Ratio Lower Upper

172 100

171 35.1 28.8 43.2

170 23.6 19.8 29.8


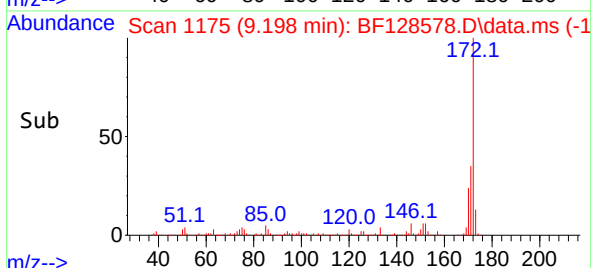
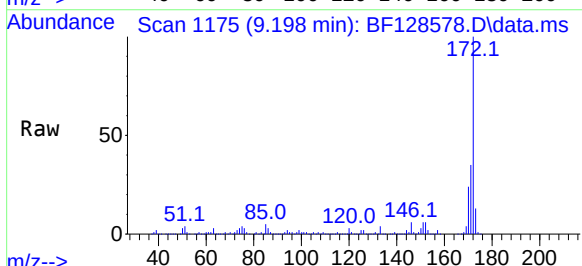
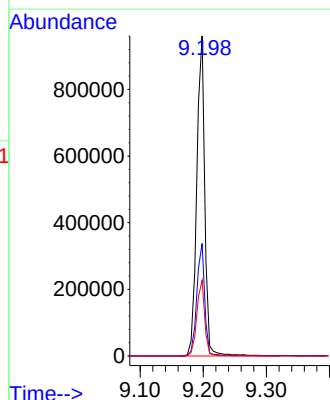




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.363 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF128578.D
Acq: 29 May 2022 18:31




Instrument :
BNA_F
ClientSampleId :
P035-SS001-2430-01


Tgt Ion:188 Resp: 304817
Ion Ratio Lower Upper
188 100
94 7.3 7.0 10.6
80 8.1 7.6 11.4

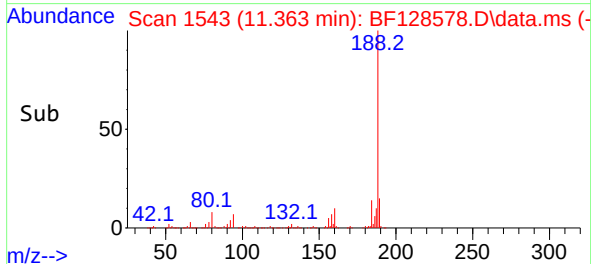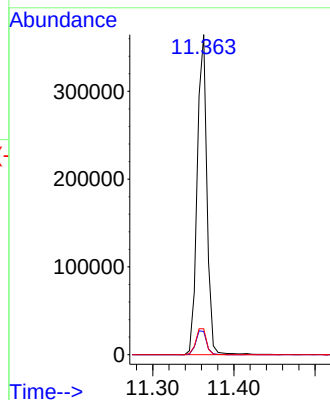

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.004 min Scan# 1992
Delta R.T. -0.006 min
Lab File: BF128578.D
Acq: 29 May 2022 18:31

Tgt Ion:240 Resp: 291976
Ion Ratio Lower Upper
240 100
120 8.3 8.9 13.3#
236 24.9 20.8 31.2


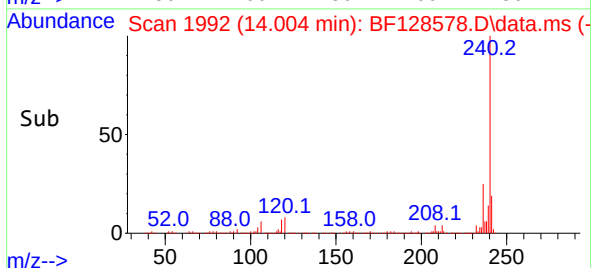
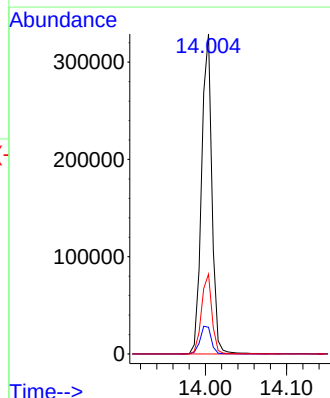
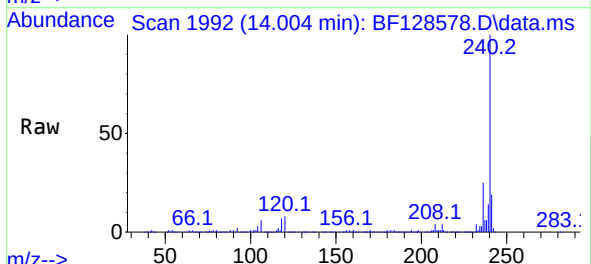




#79
Terphenyl-d14
Concen: 54.814 ng
RT: 12.951 min Scan# 1814
Delta R.T. -0.006 min
Lab File: BF128578.D
Acq: 29 May 2022 18:31

Instrument :
BNA_F
ClientSampleId :
P035-SS001-2430-01

Tgt Ion:244 Resp: 828402
Ion Ratio Lower Upper
244 100
212 7.3 6.1 9.1
122 9.7 8.8 13.2

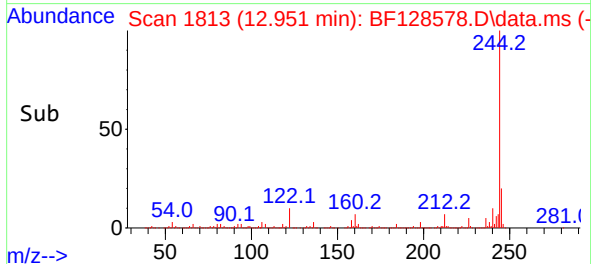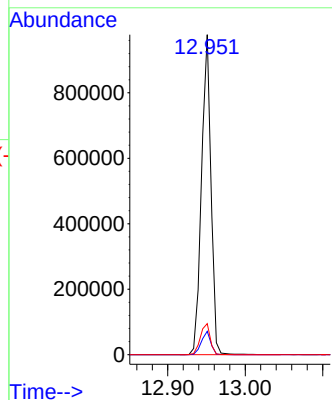

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.468 min Scan# 2241
Delta R.T. 0.000 min
Lab File: BF128578.D
Acq: 29 May 2022 18:31

Tgt Ion:264 Resp: 274160
Ion Ratio Lower Upper
264 100
260 23.7 18.4 27.6
265 19.8 17.2 25.8

