

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
 Data File : BF128564.D
 Acq On : 29 May 2022 11:36
 Operator : CG\JU
 Sample : PB145191BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB145191BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128564.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.463	534	540	543	rBV	4163459	4384671	75.87%	12.707%
2	6.463	704	710	713	rBV	3531450	4465360	77.27%	12.941%
3	6.834	770	773	777	rVB	1111472	939338	16.25%	2.722%
4	7.398	863	869	872	rBV	2806572	3054092	52.85%	8.851%
5	8.116	987	991	995	rBV	1361060	1224627	21.19%	3.549%
6	9.198	1169	1175	1178	rBV	5483875	5407923	93.58%	15.673%
7	9.875	1284	1290	1293	rBV	1655835	1423651	24.63%	4.126%
8	10.663	1418	1424	1428	rBV	3259273	3457203	59.82%	10.019%
9	11.363	1539	1543	1546	rBV	1762437	1482291	25.65%	4.296%
10	12.957	1808	1814	1817	rBV	5872943	5779153	100.00%	16.749%
11	14.004	1987	1992	1995	rBV	1442215	1392917	24.10%	4.037%
12	14.098	2003	2008	2017	rBV	212690	236220	4.09%	0.685%
13	15.469	2234	2241	2246	rBV	911506	1168832	20.22%	3.387%
14	16.921	2479	2488	2489	rBV5	40583	89069	1.54%	0.258%




Sum of corrected areas: 34505347

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
Data File : BF128564.D
Acq On : 29 May 2022 11:36
Operator : CG\JU
Sample : PB145191BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145191BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

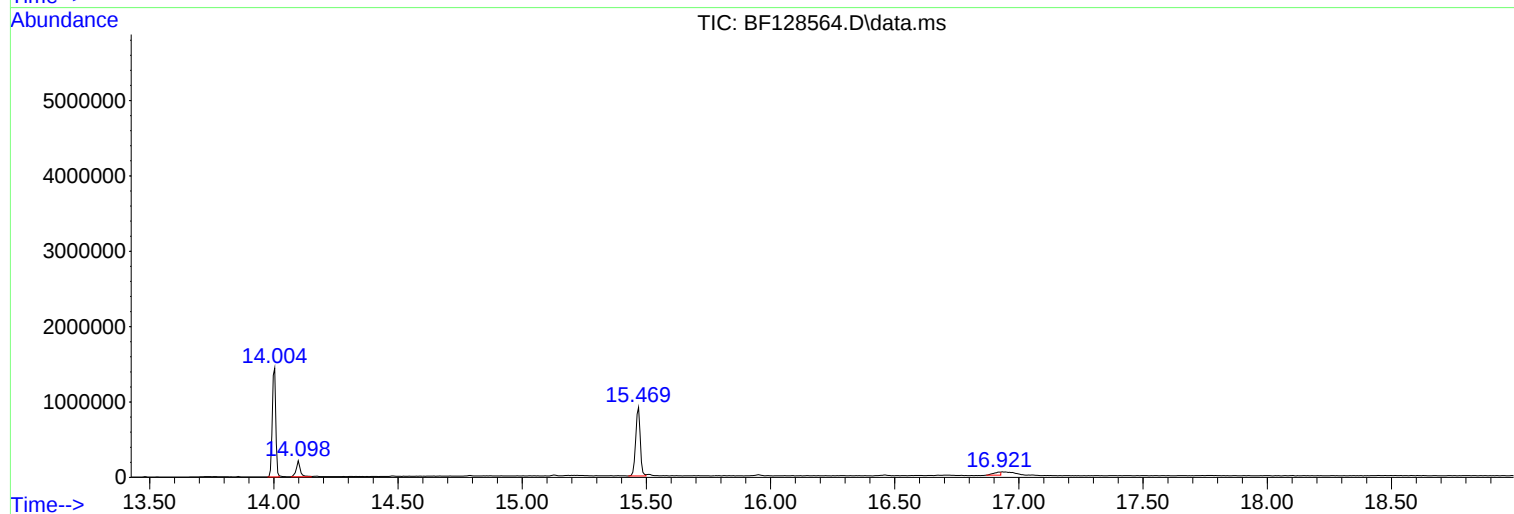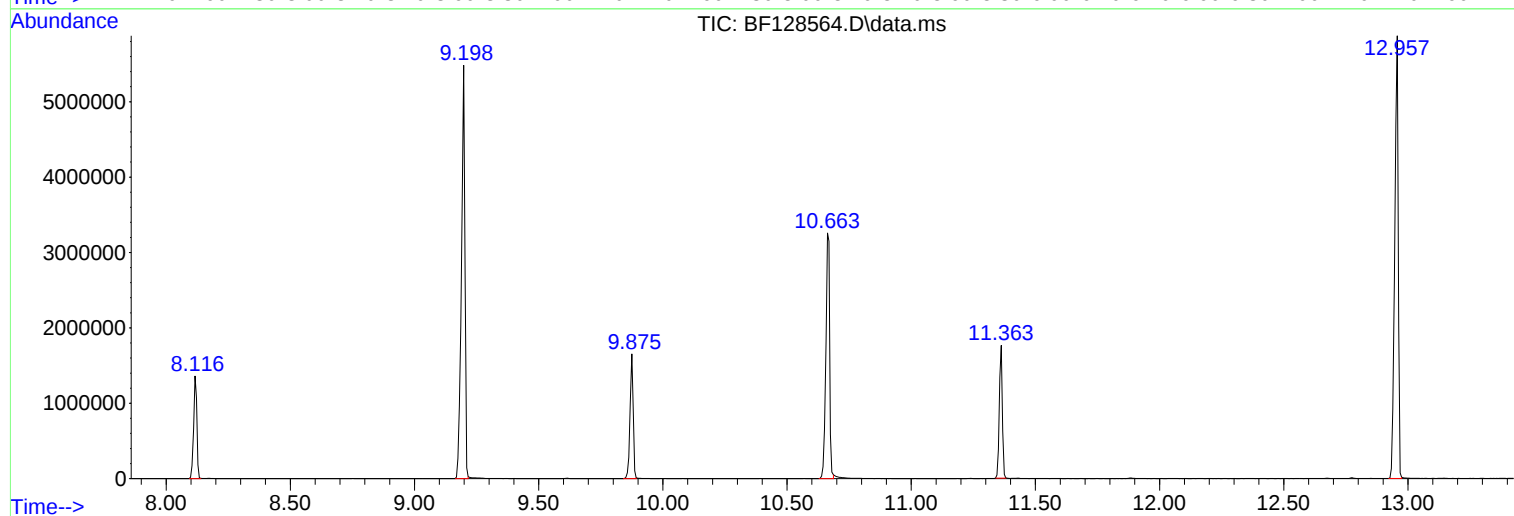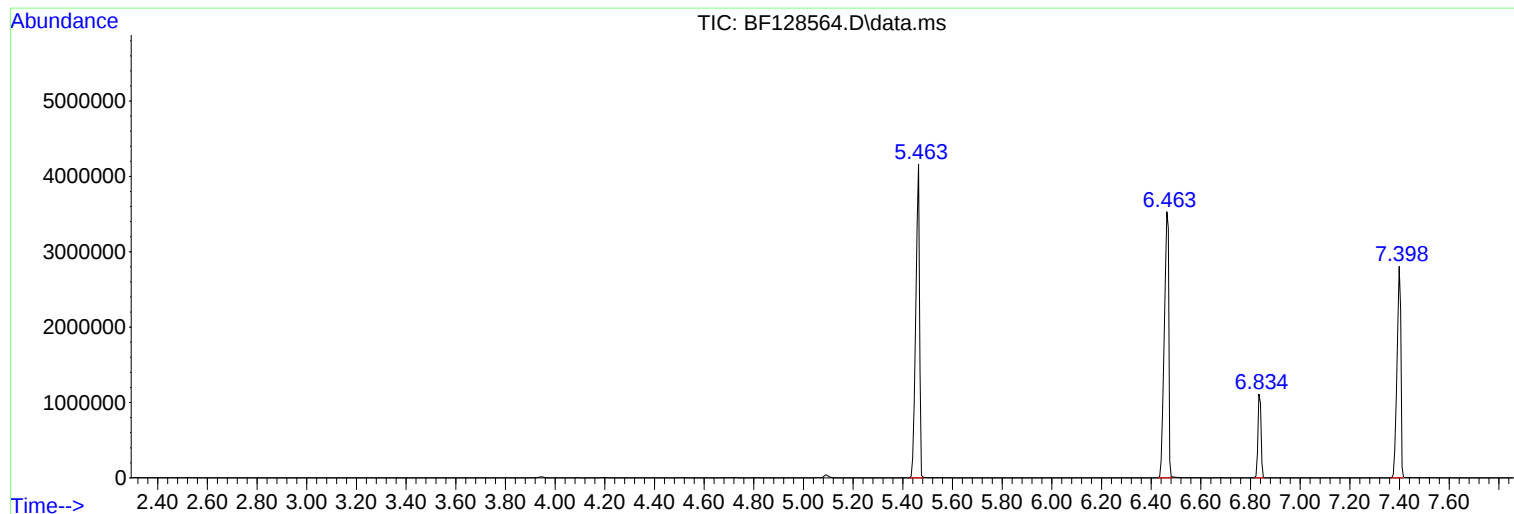

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
Data File : BF128564.D
Acq On : 29 May 2022 11:36
Operator : CG\JU
Sample : PB145191BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145191BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.098	3.39 ng	236220	Chrysene-d12	14.004

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	95
2			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19NO3S	1000483-83-4	70
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	50
4			2-Phenyl-6-(trifluoromethyl)-1H...	277	C15H10F3NO	1000387-59-3	47
5			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	47

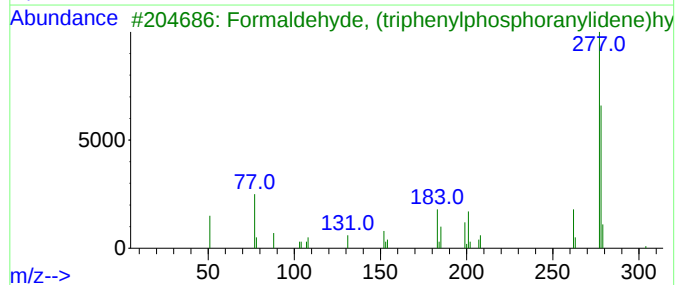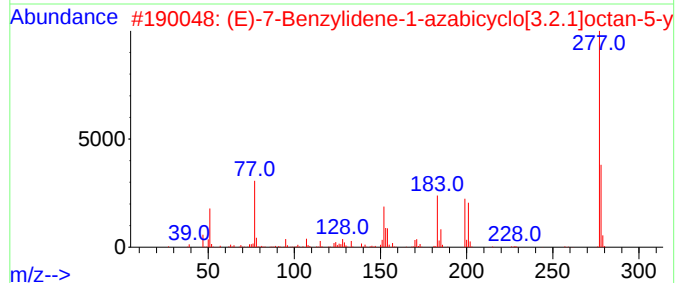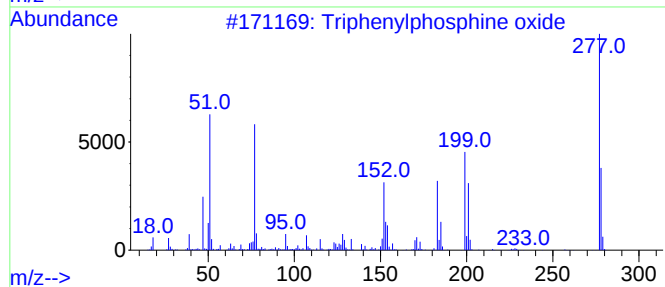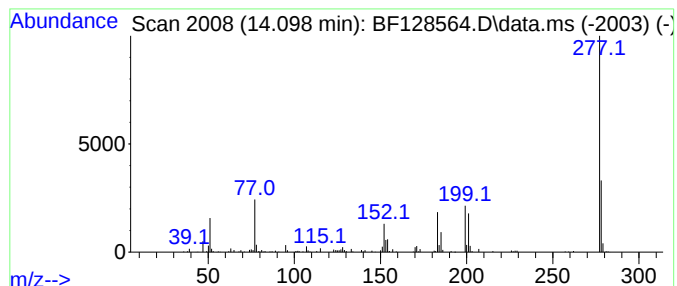

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
Data File : BF128564.D
Acq On : 29 May 2022 11:36
Operator : CG\JU
Sample : PB145191BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB145191BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
Triphenylphosph...	14.098	3.4	ng	236220	5	14.004	1392920	20.0