

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
 Data File : BF128576.D
 Acq On : 29 May 2022 17:32
 Operator : CG\JU
 Sample : N2951-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P035-SS001-0612-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128576.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.057	467	471	477	rVB	44158	53005	2.14%	0.297%
2	5.451	533	538	541	rBV	2562639	2369838	95.72%	13.259%
3	6.463	705	710	713	rBV	2361822	2255271	91.09%	12.618%
4	6.575	726	729	733	rVB	48528	38047	1.54%	0.213%
5	6.839	770	774	777	rBV	821266	683366	27.60%	3.823%
6	7.398	864	869	872	rBV	1808395	1518541	61.34%	8.496%
7	8.122	988	992	995	rBV	863666	782929	31.62%	4.380%
8	9.198	1170	1175	1178	rBV	2996058	2475765	100.00%	13.852%
9	9.875	1286	1290	1301	rBV	967166	774462	31.28%	4.333%
10	10.663	1420	1424	1427	rBV	1559494	1346041	54.37%	7.531%
11	11.363	1539	1543	1546	rBV	852661	724035	29.24%	4.051%
12	11.886	1629	1632	1638	rBV	106200	109104	4.41%	0.610%
13	12.674	1763	1766	1771	rBV2	30093	32022	1.29%	0.179%
14	12.951	1809	1813	1816	rBV	2720933	2246587	90.74%	12.569%
15	13.880	1965	1971	1982	rBV2	74701	216928	8.76%	1.214%
16	14.004	1987	1992	1995	rBV	803848	774055	31.27%	4.331%
17	14.098	2004	2008	2016	rBV	339112	379354	15.32%	2.122%
18	14.786	2123	2125	2130	rVB2	34623	36869	1.49%	0.206%
19	15.127	2180	2183	2187	rVB	49150	56469	2.28%	0.316%
20	15.468	2235	2241	2245	rBV	546697	698314	28.21%	3.907%
21	15.509	2245	2248	2255	rVB	61312	75782	3.06%	0.424%
22	15.951	2319	2323	2328	rVB	59268	80592	3.26%	0.451%
23	16.456	2405	2409	2418	rVB2	48658	90397	3.65%	0.506%
24	17.056	2506	2511	2515	rVB4	31145	55618	2.25%	0.311%




Sum of corrected areas: 17873391

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
Data File : BF128576.D
Acq On : 29 May 2022 17:32
Operator : CG\JU
Sample : N2951-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P035-SS001-0612-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

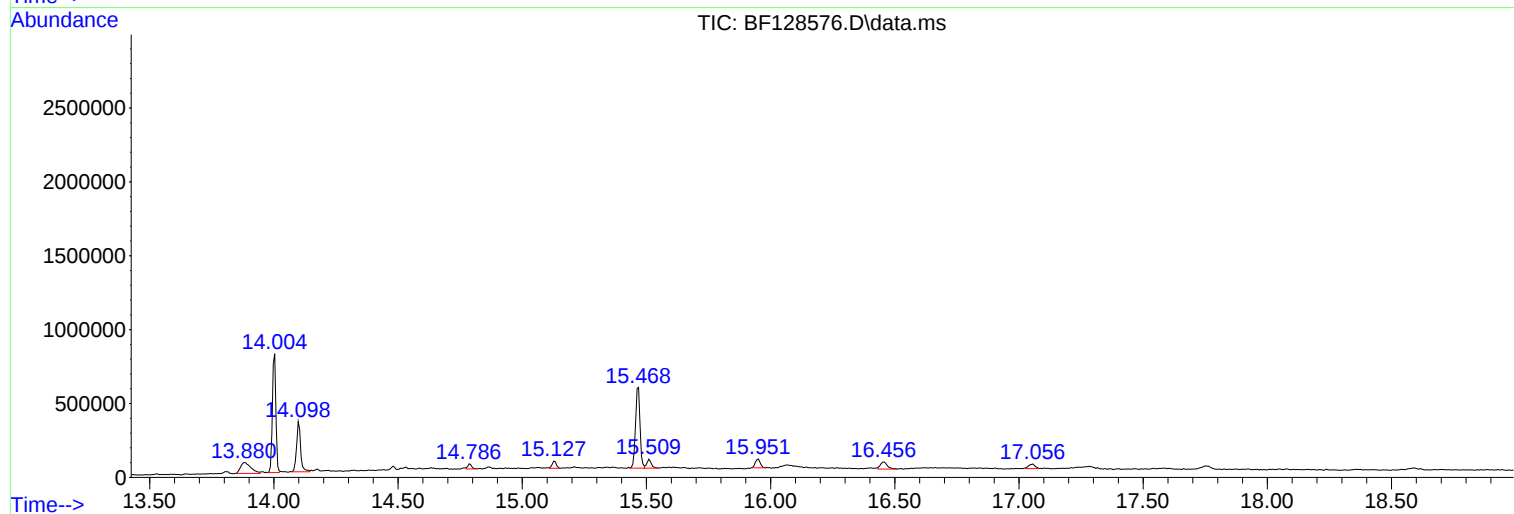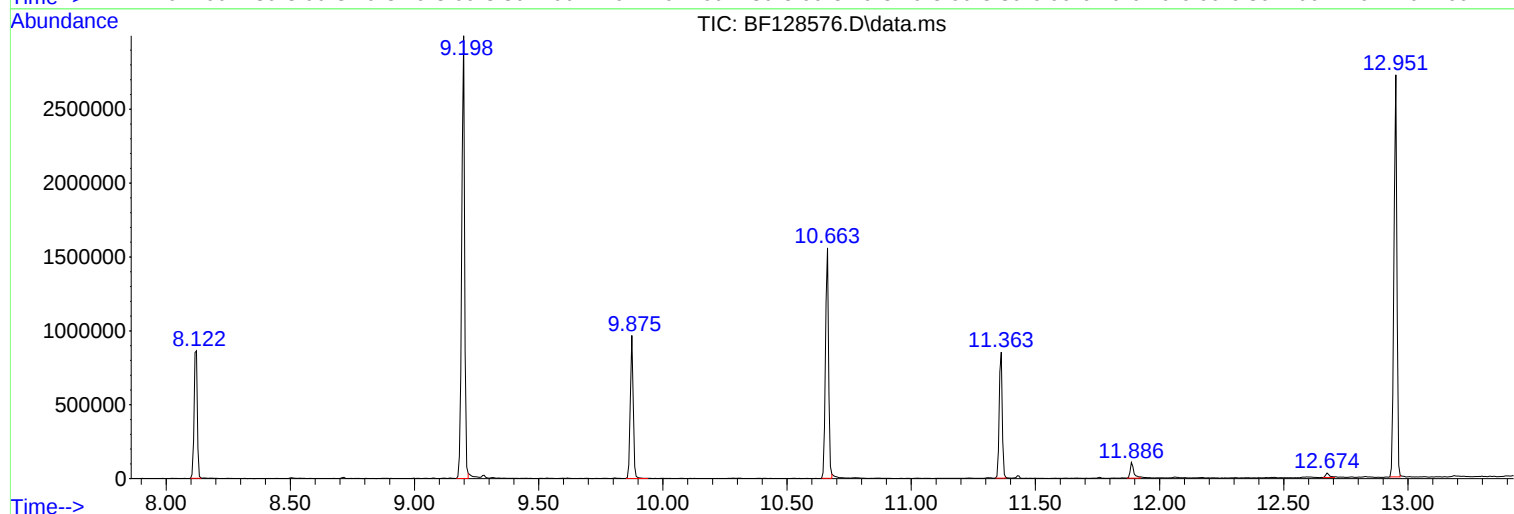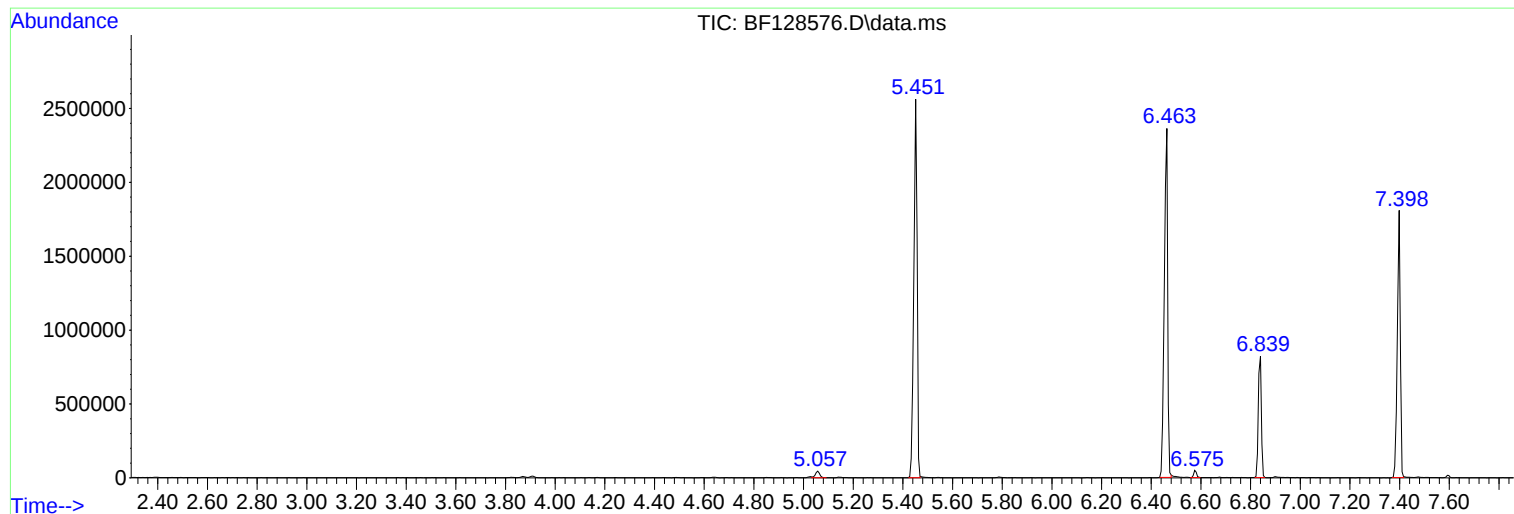

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
Data File : BF128576.D
Acq On : 29 May 2022 17:32
Operator : CG\JU
Sample : N2951-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P035-SS001-0612-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
Data File : BF128576.D
Acq On : 29 May 2022 17:32
Operator : CG\JU
Sample : N2951-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P035-SS001-0612-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------