

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
 Data File : BF128579.D
 Acq On : 29 May 2022 19:01
 Operator : CG\JU
 Sample : N2951-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P035-SS001-0006-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128579.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.069	469	473	479	rVB	53017	62693	1.76%	0.255%
2	5.457	533	539	542	rBV	3200428	3108608	87.16%	12.649%
3	6.463	705	710	713	rBV	2892617	3103703	87.03%	12.630%
4	6.575	726	729	737	rVB	52771	44674	1.25%	0.182%
5	6.839	770	774	777	rBV	1078653	889809	24.95%	3.621%
6	7.398	864	869	872	rBV	2196910	2116758	59.35%	8.613%
7	8.122	987	992	995	rBV	1139109	1067759	29.94%	4.345%
8	9.198	1169	1175	1178	rBV	4127462	3566369	100.00%	14.512%
9	9.316	1191	1195	1198	rVB	47099	46327	1.30%	0.189%
10	9.875	1284	1290	1294	rBV	1253925	1047583	29.37%	4.263%
11	10.663	1420	1424	1427	rBV	2123252	1821541	51.08%	7.412%
12	11.363	1539	1543	1546	rBV	1097203	925779	25.96%	3.767%
13	11.892	1629	1633	1650	rVB	423639	422282	11.84%	1.718%
14	12.063	1660	1662	1674	rVB2	26308	40984	1.15%	0.167%
15	12.616	1751	1756	1763	rVB	65872	100842	2.83%	0.410%
16	12.674	1763	1766	1773	rBV2	119064	126851	3.56%	0.516%
17	12.951	1808	1813	1816	rBV	3356304	3004727	84.25%	12.227%
18	13.810	1957	1959	1964	rVB	39735	40336	1.13%	0.164%
19	13.886	1968	1972	1981	rVB2	139382	292720	8.21%	1.191%
20	13.998	1987	1991	1997	rBV	888835	853943	23.94%	3.475%
21	14.098	2004	2008	2013	rBV	309812	333424	9.35%	1.357%
22	14.174	2018	2021	2024	rBV2	62668	62725	1.76%	0.255%
23	14.480	2070	2073	2076	rBV	61009	54349	1.52%	0.221%
24	14.533	2079	2082	2087	rVB5	37574	59999	1.68%	0.244%
25	14.786	2123	2125	2129	rVB	41846	42489	1.19%	0.173%
26	14.862	2135	2138	2141	rVB2	44745	41687	1.17%	0.170%
27	15.127	2180	2183	2187	rVB	88175	95328	2.67%	0.388%
28	15.468	2236	2241	2245	rBV	494257	595395	16.69%	2.423%
29	15.509	2245	2248	2254	rVB2	59237	72515	2.03%	0.295%
30	15.951	2319	2323	2329	rVB	82142	123713	3.47%	0.503%
31	16.751	2456	2459	2468	rVB5	59545	109471	3.07%	0.445%
32	17.286	2546	2550	2560	rVB5	143224	299567	8.40%	1.219%




Sum of corrected areas: 24574950

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
Data File : BF128579.D
Acq On : 29 May 2022 19:01
Operator : CG\JU
Sample : N2951-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P035-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

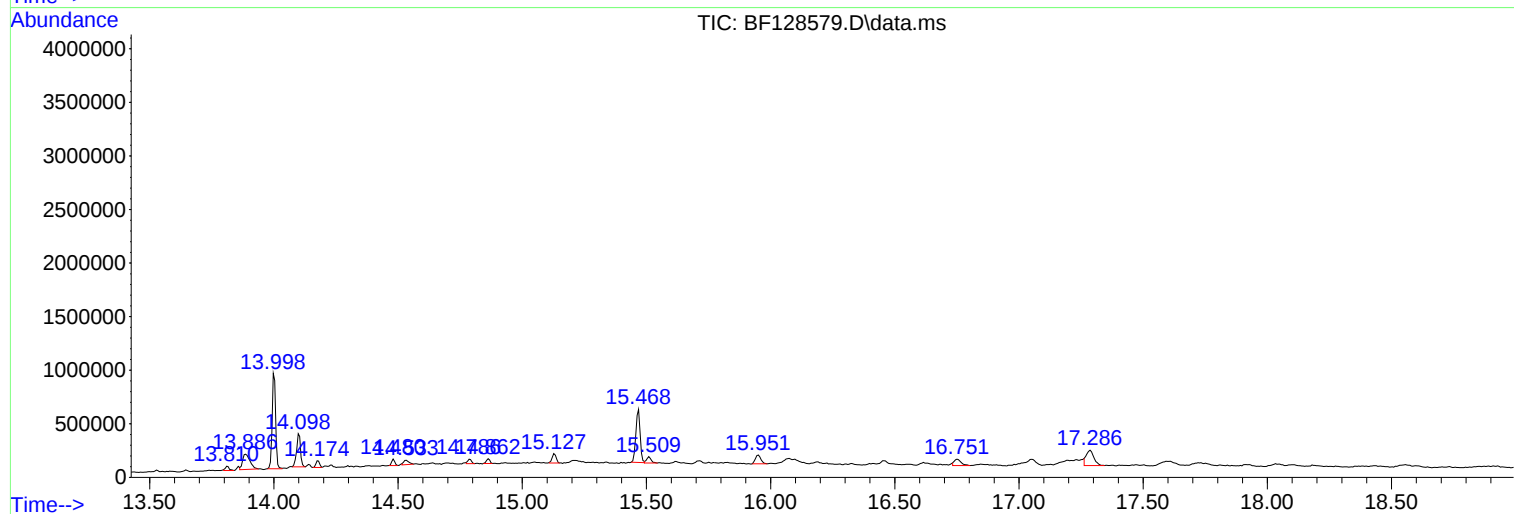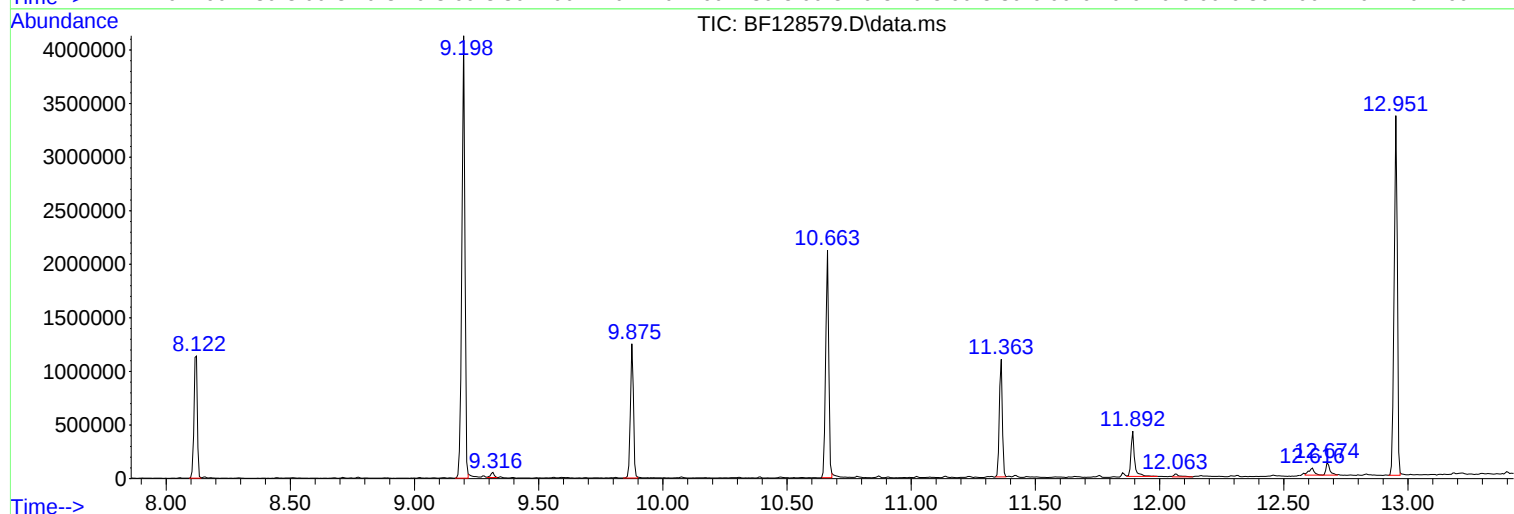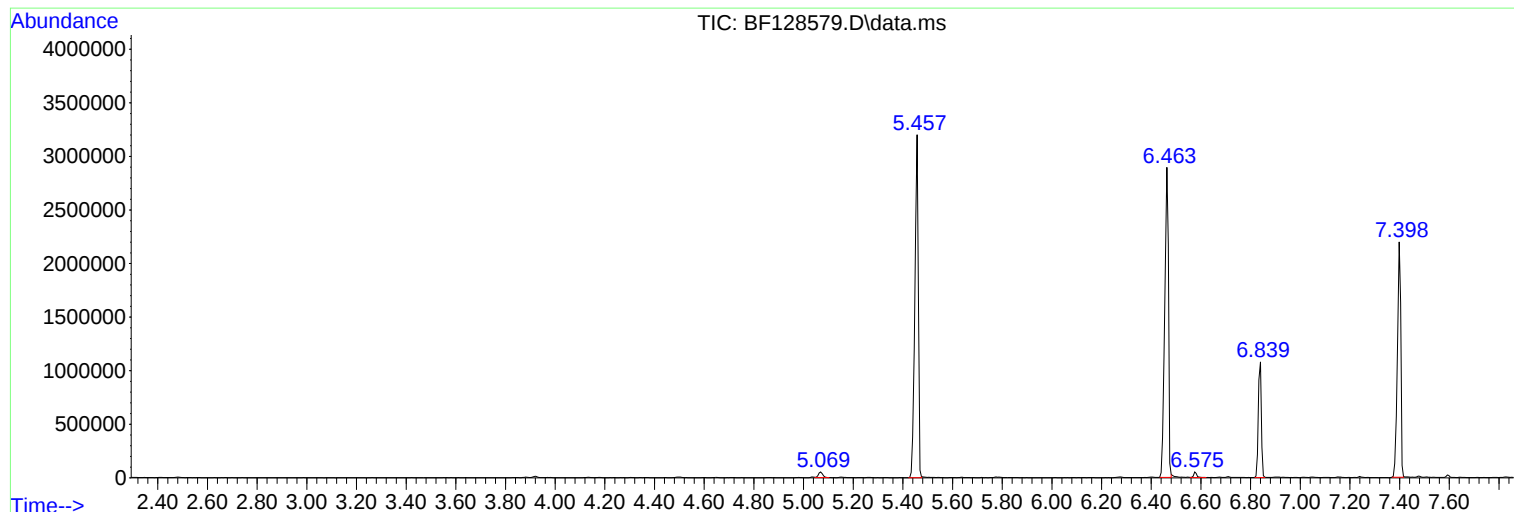

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
Data File : BF128579.D
Acq On : 29 May 2022 19:01
Operator : CG\JU
Sample : N2951-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P035-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
Data File : BF128579.D
Acq On : 29 May 2022 19:01
Operator : CG\JU
Sample : N2951-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P035-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------