

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
 Data File : BF128584.D
 Acq On : 29 May 2022 21:29
 Operator : CG\JU
 Sample : N2951-17
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P036-SS001-0006-01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF128584.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.045	466	469	477	rVB	39348	44005	2.42%	0.259%
2	5.451	533	538	541	rBV	1821622	1595535	87.79%	9.404%
3	6.463	706	710	713	rBV	1727170	1488456	81.90%	8.773%
4	6.581	727	730	738	rVB	22746	25441	1.40%	0.150%
5	6.839	770	774	777	rBV	773444	577579	31.78%	3.404%
6	7.398	865	869	872	rBV	1238082	981994	54.03%	5.788%
7	7.998	968	971	978	rBV2	18667	29117	1.60%	0.172%
8	8.122	988	992	995	rBV	833998	653053	35.93%	3.849%
9	8.880	1116	1121	1129	rBV	27142	39586	2.18%	0.233%
10	9.198	1170	1175	1178	rBV	2031178	1658095	91.23%	9.773%
11	9.316	1191	1195	1199	rVB	26355	24807	1.36%	0.146%
12	9.875	1286	1290	1294	rBV	824780	726188	39.96%	4.280%
13	10.663	1420	1424	1427	rBV	1334387	1110254	61.09%	6.544%
14	10.686	1427	1428	1433	rVB2	49087	37189	2.05%	0.219%
15	11.310	1531	1534	1538	rBV	48306	43029	2.37%	0.254%
16	11.363	1538	1543	1547	rBV	979073	798837	43.95%	4.708%
17	11.892	1629	1633	1637	rBV	461794	430848	23.71%	2.539%
18	11.927	1637	1639	1642	rVB	37615	34163	1.88%	0.201%
19	12.069	1660	1663	1667	rBV2	35605	36912	2.03%	0.218%
20	12.604	1751	1754	1762	rVB6	25292	47647	2.62%	0.281%
21	12.680	1763	1767	1775	rBV	204661	230605	12.69%	1.359%
22	12.827	1790	1792	1799	rVB4	17719	24118	1.33%	0.142%
23	12.951	1809	1813	1816	rBV	2121954	1817416	100.00%	10.712%
24	13.186	1850	1853	1856	rBV	64473	59277	3.26%	0.349%
25	13.398	1887	1889	1892	rBV3	27426	31487	1.73%	0.186%
26	13.427	1892	1894	1897	rVV	72043	66338	3.65%	0.391%
27	13.457	1897	1899	1902	rVB	31491	27390	1.51%	0.161%
28	13.527	1908	1911	1915	rBV	136004	118657	6.53%	0.699%
29	13.645	1929	1931	1936	rVB6	42319	48646	2.68%	0.287%
30	13.810	1956	1959	1962	rBV2	79304	90891	5.00%	0.536%
31	13.863	1964	1968	1970	rVV2	223537	242672	13.35%	1.430%
32	13.886	1970	1972	1978	rVB	219976	256972	14.14%	1.515%
33	14.004	1987	1992	1996	rBV2	792960	976904	53.75%	5.758%
34	14.104	2005	2009	2013	rBV	346971	318486	17.52%	1.877%
35	14.174	2018	2021	2025	rVB	363181	329447	18.13%	1.942%
36	14.480	2070	2073	2077	rBV	398306	367121	20.20%	2.164%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
Data File : BF128584.D
Acq On : 29 May 2022 21:29
Operator : CG\JU
Sample : N2951-17
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P036-SS001-0006-01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	14.792	2123	2126	2130	rVB	361424	331233	18.23%	1.952%
38	15.133	2180	2184	2189	rVB	308104	339653	18.69%	2.002%
39	15.474	2237	2242	2245	rBV	385873	470110	25.87%	2.771%
40	15.515	2245	2249	2255	rVB	194656	237898	13.09%	1.402%
41	15.957	2320	2324	2329	rVB	138232	198007	10.89%	1.167%




Sum of corrected areas: 16966063

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
Data File : BF128584.D
Acq On : 29 May 2022 21:29
Operator : CG\JU
Sample : N2951-17
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P036-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

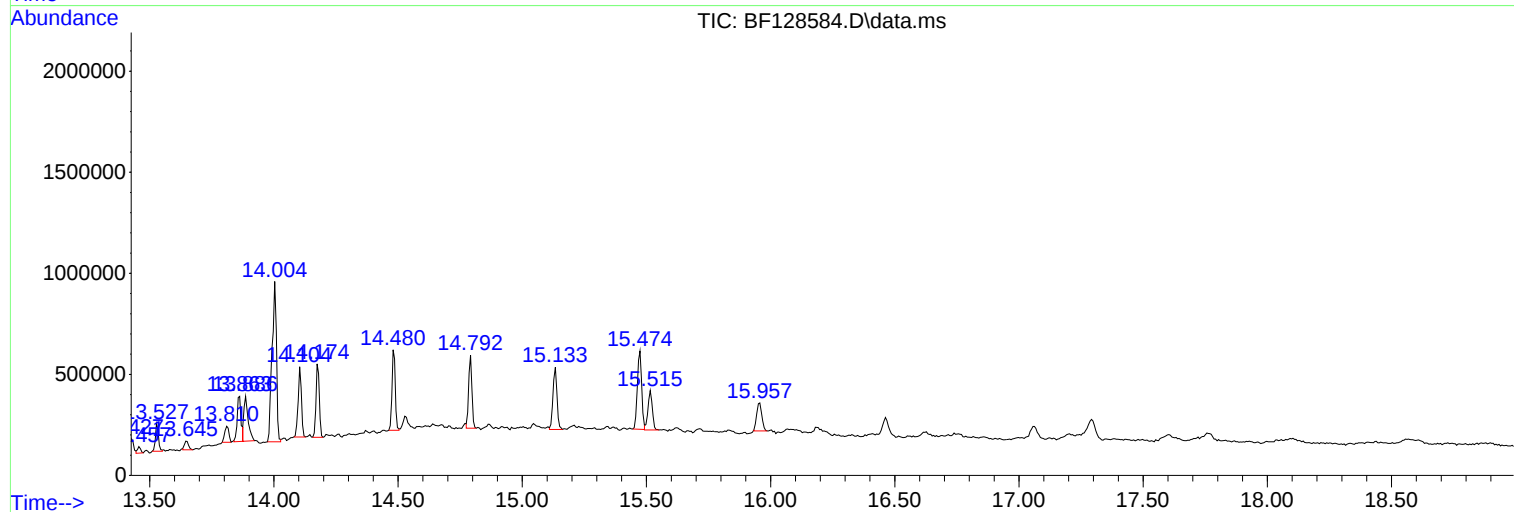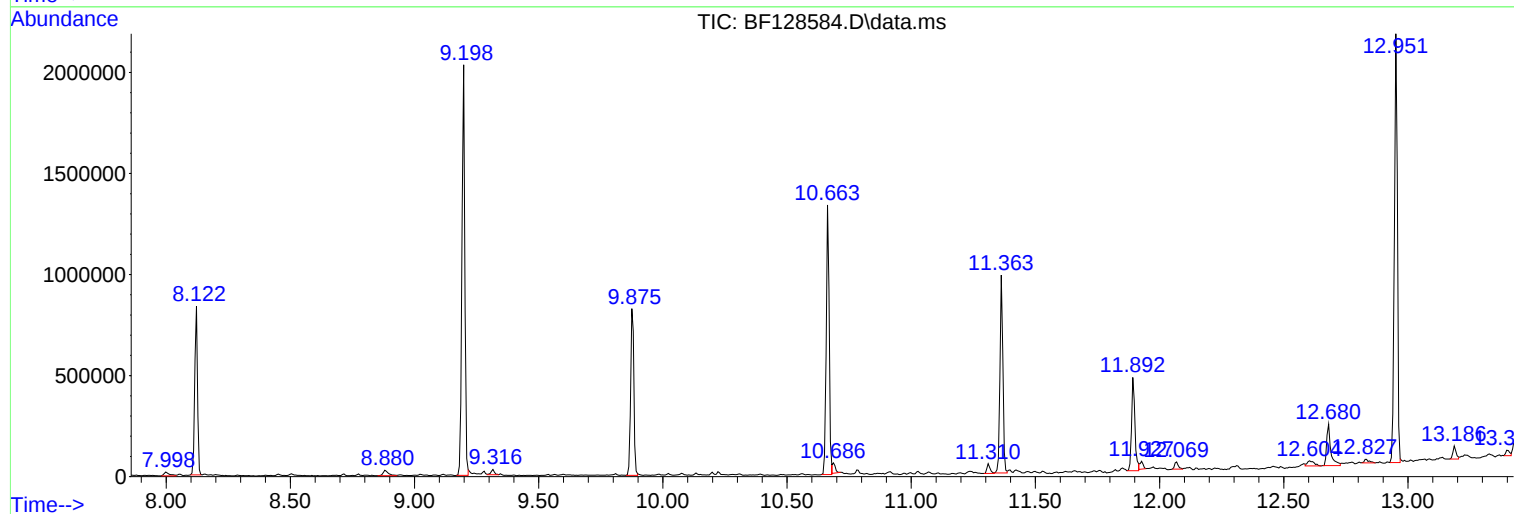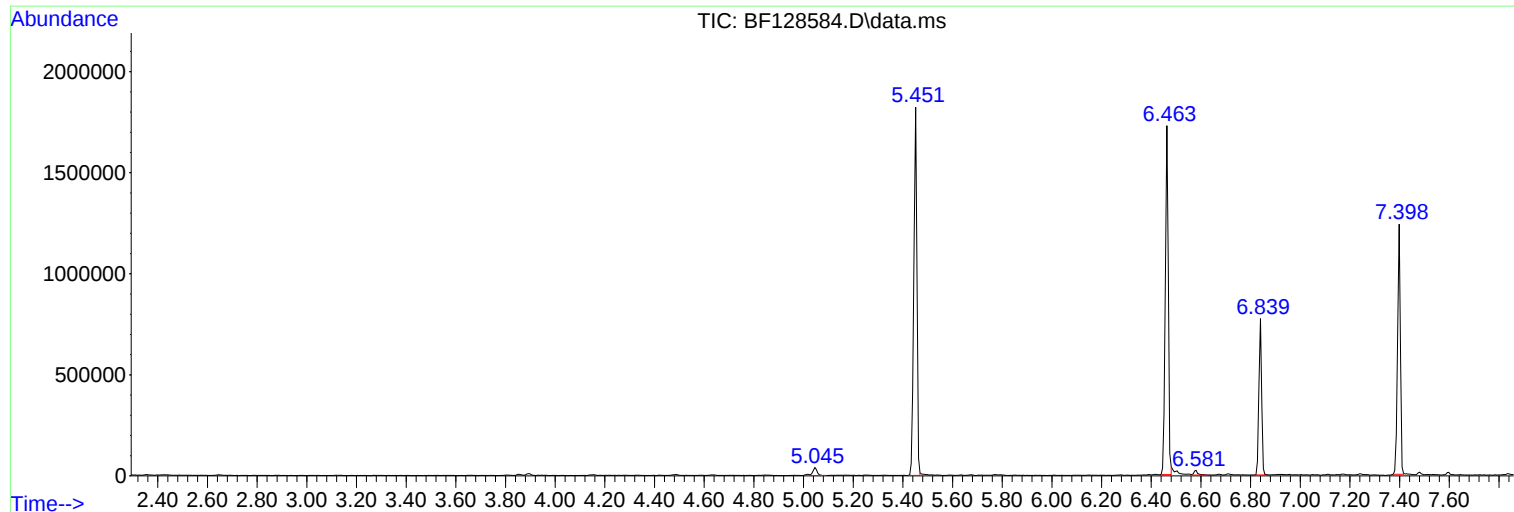

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
Data File : BF128584.D
Acq On : 29 May 2022 21:29
Operator : CG\JU
Sample : N2951-17
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P036-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
Data File : BF128584.D
Acq On : 29 May 2022 21:29
Operator : CG\JU
Sample : N2951-17
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P036-SS001-0006-01

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc