
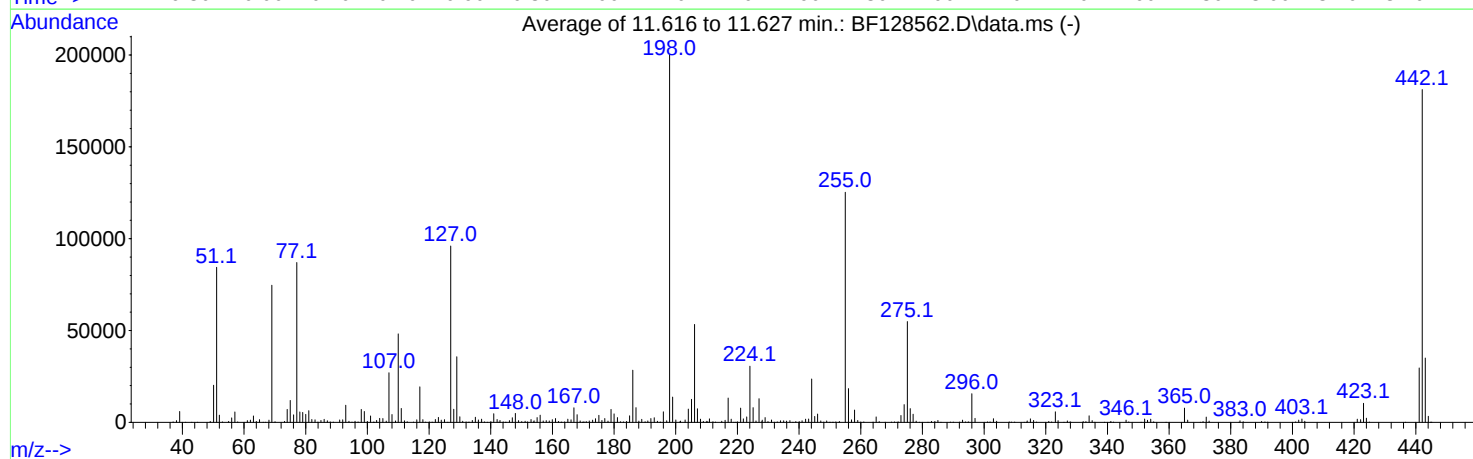


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
 Data File : BF128562.D
 Acq On : 29 May 2022 10:38
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 27 01:51:59 2022

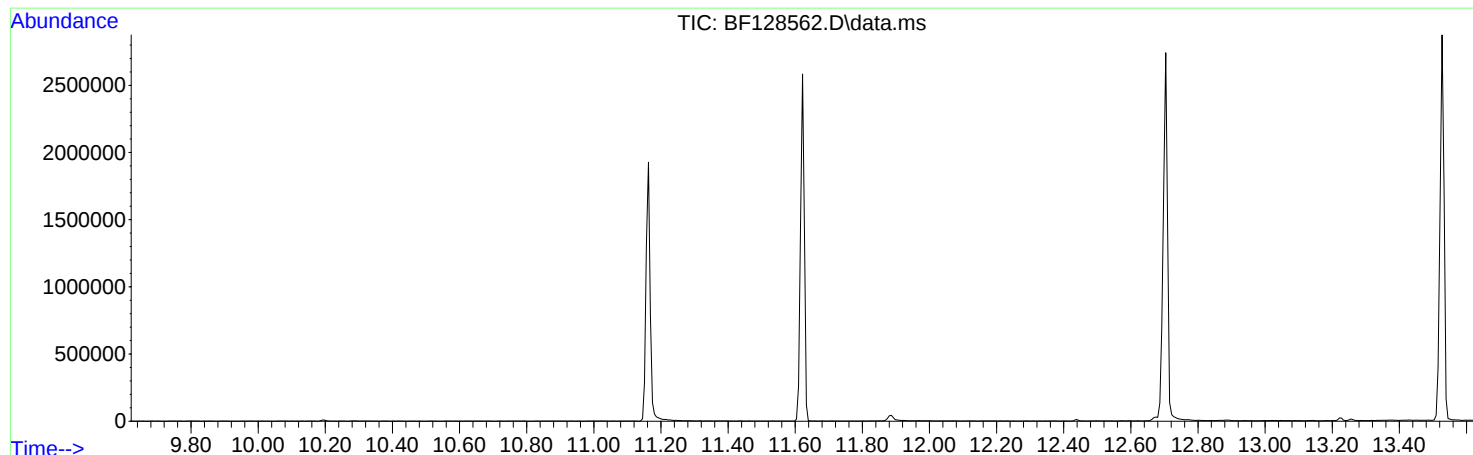

AutoFind: Scans 1586, 1587, 1588; Background Corrected with Scan 1581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	84421	PASS
68	69	0.00	2	1.6	1222	PASS
69	198	0.00	100	37.3	74701	PASS
70	69	0.00	2	0.5	338	PASS
127	198	10	80	47.9	95995	PASS
197	198	0.00	2	0.4	849	PASS
198	198	100	100	100.0	200299	PASS
199	198	5	9	6.9	13792	PASS
275	198	10	60	27.4	54896	PASS
365	198	1	100	3.9	7748	PASS
441	198	0.01	100	14.8	29609	PASS
442	442	50	100	100.0	181213	PASS
443	442	15	24	19.3	35026	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
5/29/2022	BNA_F	<u>BF128562.D</u>
Compound Name	Response	Retention Time
DDT	457760	13.527
DDD	6355	13.221
DDE	512	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6867	464627	1.48

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
Data File : BF128562.D
Acq On : 29 May 2022 10:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 30 01:54:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration

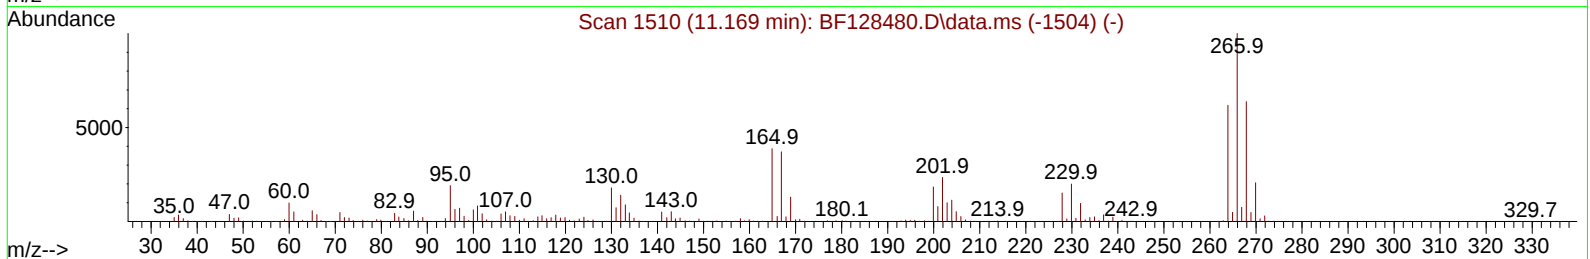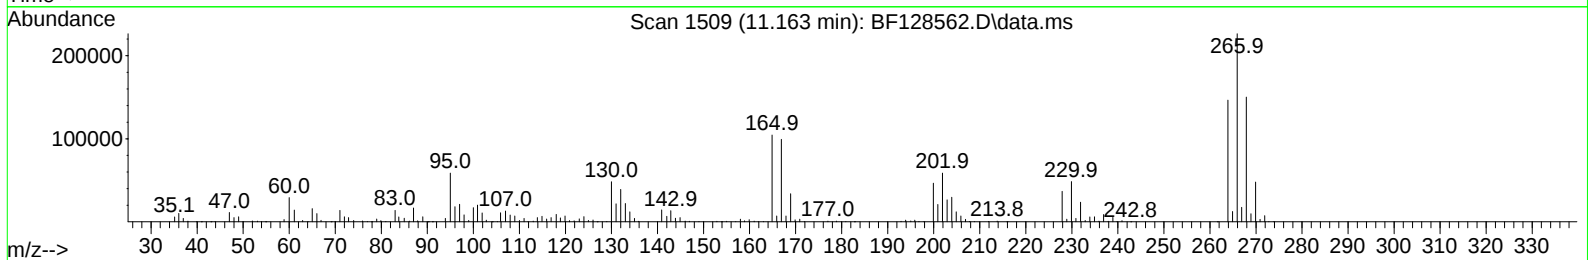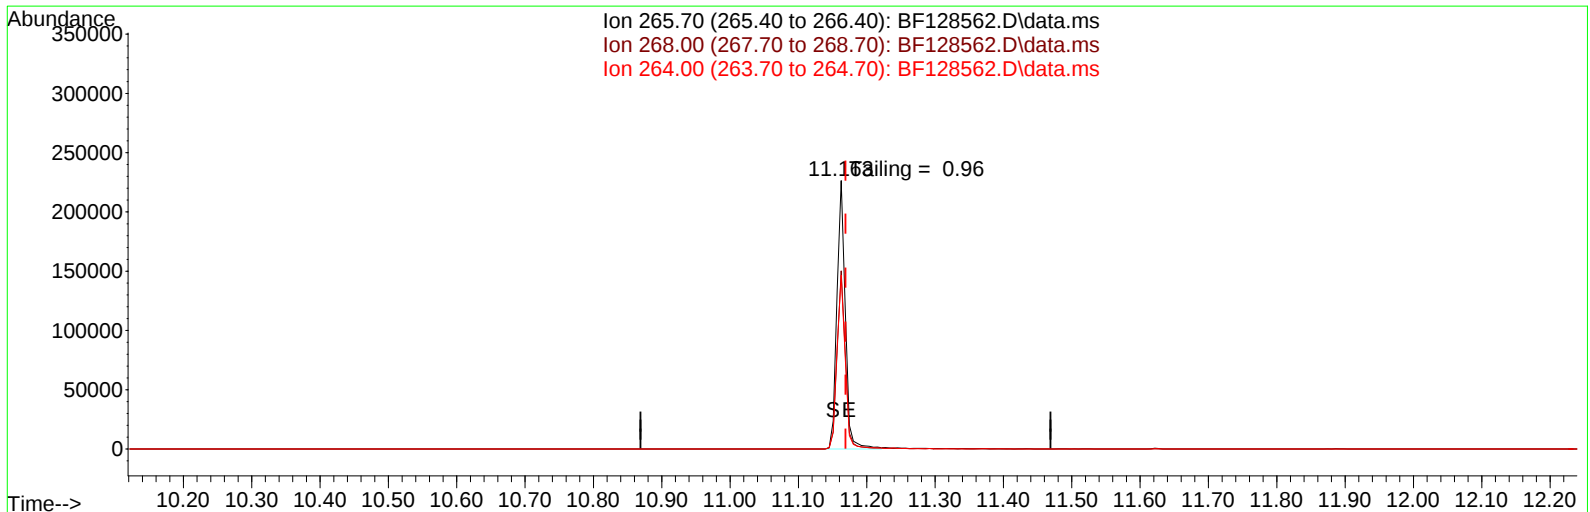

TIC: BF128562.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.006) 37714.22 ng


response 193255

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	66.37
264.00	61.80	64.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF052922\
Data File : BF128562.D
Acq On : 29 May 2022 10:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: May 30 01:54:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF052622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 27 01:51:59 2022
Response via : Initial Calibration

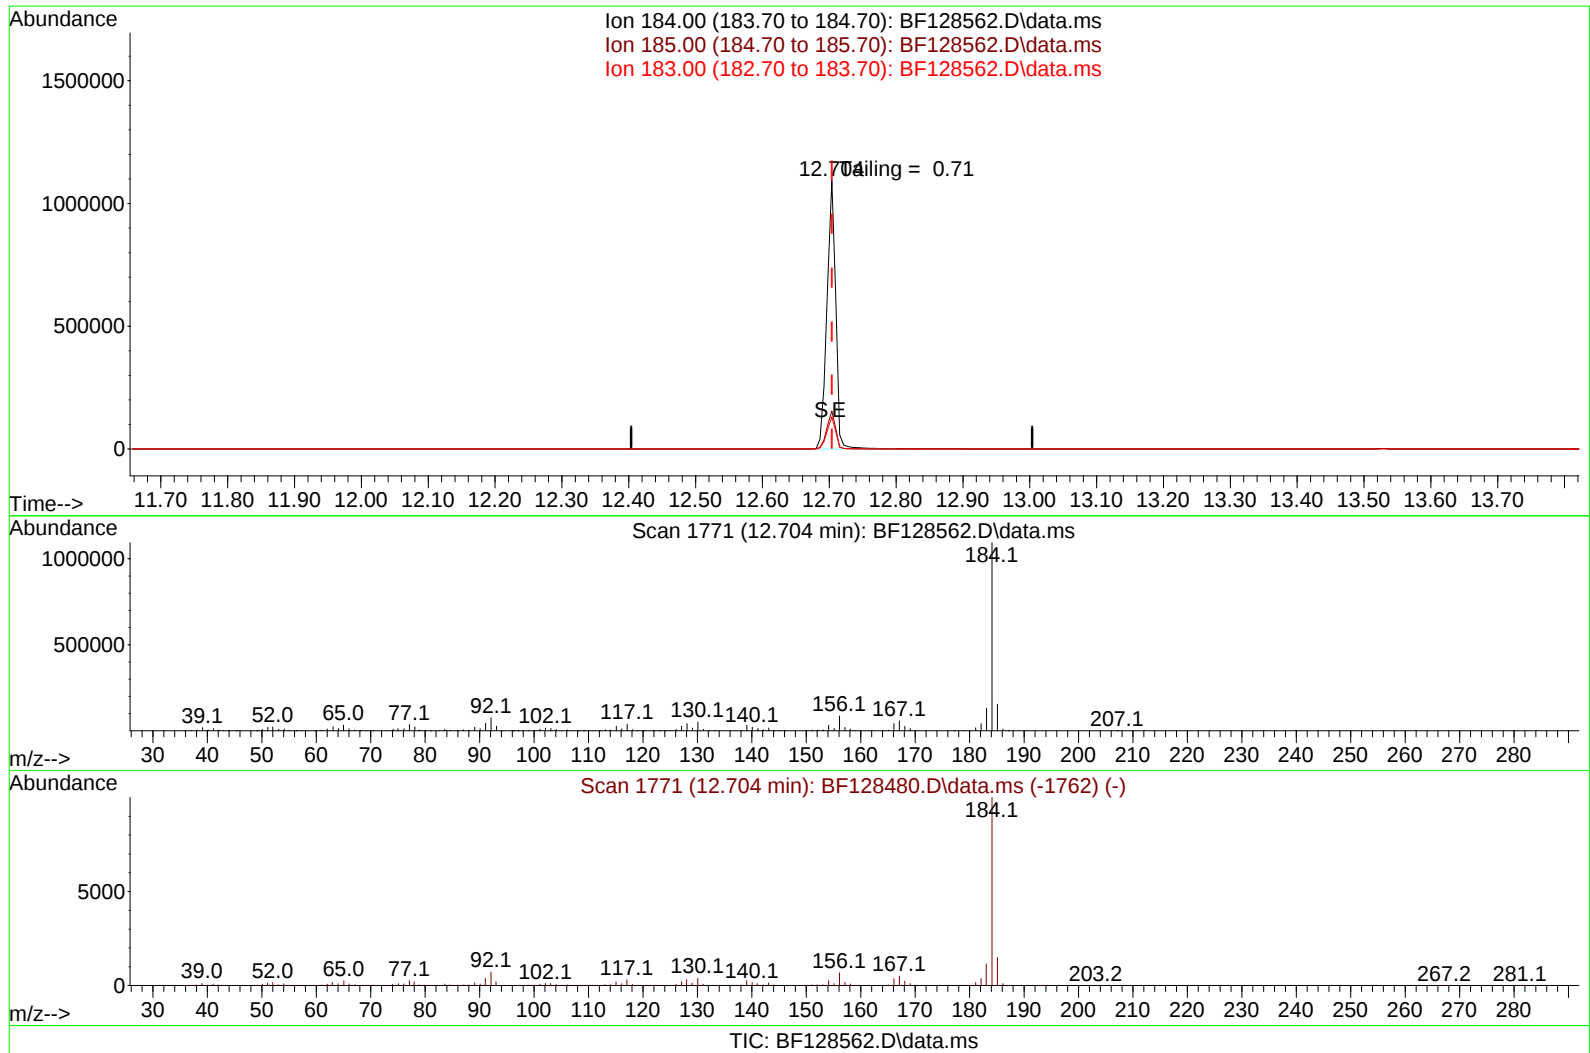

(77) Benzidine

12.704min (-0.000) 0.00 ng

response 1002983

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.18
183.00	11.60	11.98
0.00	0.00	0.00